

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV090624\
 Data File : VV037214.D
 Acq On : 06 Sep 2024 10:59
 Operator : SY/MD
 Sample : P3842-06
 Misc : 5.00mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082624WMA.M
 Title : VOC Analysis

Signal : TIC: VV037214.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.175	37	42	50	rBV	15161	21757	0.88%	0.124%
2	1.278	68	74	88	rVB	334229	362403	14.65%	2.059%
3	1.532	146	153	171	rVB	290100	346620	14.01%	1.970%
4	2.060	307	317	330	rBV	591014	857352	34.65%	4.872%
5	3.298	700	702	706	rBV4	1287	782	0.03%	0.004%
6	3.461	752	753	756	rBV3	724	470	0.02%	0.003%
7	3.548	776	780	784	rBV5	828	819	0.03%	0.005%
8	3.619	800	802	805	rVB4	983	442	0.02%	0.003%
9	3.683	819	822	823	rBV3	1071	375	0.02%	0.002%
10	3.693	823	825	827	rBV3	1199	626	0.03%	0.004%
11	3.744	837	841	844	rVB5	984	701	0.03%	0.004%
12	3.761	844	846	847	rBV2	1085	458	0.02%	0.003%
13	3.789	847	855	887	rBV	109406	304333	12.30%	1.729%
14	4.240	980	995	1020	rBV	392252	1004810	40.61%	5.710%
15	4.513	1078	1080	1083	rBV3	910	471	0.02%	0.003%
16	4.622	1112	1114	1116	rBV3	1258	629	0.03%	0.004%
17	4.664	1124	1127	1130	rBV4	1208	748	0.03%	0.004%
18	4.677	1130	1131	1135	rVV3	711	370	0.01%	0.002%
19	4.696	1135	1137	1141	rVV4	1235	903	0.04%	0.005%
20	4.719	1141	1144	1145	rVV2	863	498	0.02%	0.003%
21	4.748	1149	1153	1155	rVV3	974	625	0.03%	0.004%
22	4.851	1180	1185	1190	rBV8	1464	1864	0.08%	0.011%
23	4.947	1199	1215	1246	rBV2	974446	2474049	100.00%	14.059%
24	5.452	1370	1372	1376	rBV4	956	452	0.02%	0.003%
25	5.474	1376	1379	1382	rBV4	1181	758	0.03%	0.004%
26	5.526	1383	1395	1429	rBV	683049	1414513	57.17%	8.038%
27	5.982	1524	1537	1562	rBV	553698	1136391	45.93%	6.457%
28	6.240	1615	1617	1621	rVB5	2236	1048	0.04%	0.006%
29	6.404	1664	1668	1672	rVB7	1921	1612	0.07%	0.009%
30	6.442	1678	1680	1684	rBV3	1734	1067	0.04%	0.006%
31	6.503	1696	1699	1700	rBV3	1305	700	0.03%	0.004%
32	6.600	1727	1729	1733	rVB4	978	492	0.02%	0.003%
33	6.619	1733	1735	1739	rVB5	1085	527	0.02%	0.003%
34	6.638	1739	1741	1743	rBV3	866	552	0.02%	0.003%
35	6.776	1782	1784	1789	rVB6	1465	1030	0.04%	0.006%
36	6.802	1789	1792	1795	rBV4	1064	868	0.04%	0.005%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV090624\
 Data File : VV037214.D
 Acq On : 06 Sep 2024 10:59
 Operator : SY/MD
 Sample : P3842-06
 Misc : 5.00mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082624WMA.M
 Title : VOC Analysis

37	6.860	1803	1810	1813	rBV8	844	1113	0.04%	0.006%
38	6.908	1813	1825	1858	rBV	286903	566072	22.88%	3.217%
39	7.166	1903	1905	1907	rBV2	1301	591	0.02%	0.003%
40	7.236	1916	1927	1953	rBV	1085587	1921764	77.68%	10.920%
41	7.548	2015	2024	2046	rBV	185938	341769	13.81%	1.942%
42	7.857	2116	2120	2121	rBV3	1417	996	0.04%	0.006%
43	7.947	2146	2148	2151	rVV4	916	483	0.02%	0.003%
44	8.024	2163	2172	2209	rBV2	304407	679239	27.45%	3.860%
45	8.542	2330	2333	2337	rBV6	1630	1663	0.07%	0.009%
46	8.661	2368	2370	2371	rBV2	1001	382	0.02%	0.002%
47	8.722	2387	2389	2391	rBV3	1252	507	0.02%	0.003%
48	8.776	2395	2406	2435	rBV	1039368	1740054	70.33%	9.888%
49	9.207	2538	2540	2542	rBV3	921	443	0.02%	0.003%
50	9.320	2571	2575	2577	rBV4	982	629	0.03%	0.004%
51	9.333	2577	2579	2584	rVB5	709	598	0.02%	0.003%
52	9.397	2595	2599	2600	rBV3	618	439	0.02%	0.002%
53	9.468	2617	2621	2625	rBV5	966	804	0.03%	0.005%
54	9.487	2625	2627	2628	rBV2	967	385	0.02%	0.002%
55	9.577	2652	2655	2657	rBV4	994	601	0.02%	0.003%
56	9.590	2657	2659	2662	rVV2	1027	561	0.02%	0.003%
57	9.625	2666	2670	2672	rVV4	864	522	0.02%	0.003%
58	9.654	2677	2679	2682	rVB4	1071	456	0.02%	0.003%
59	9.696	2687	2692	2695	rBV5	1745	1620	0.07%	0.009%
60	9.715	2695	2698	2701	rBV3	723	471	0.02%	0.003%
61	9.731	2701	2703	2709	rBV8	967	1029	0.04%	0.006%
62	9.825	2729	2732	2735	rBV4	1847	1277	0.05%	0.007%
63	9.947	2768	2770	2773	rVV3	1260	910	0.04%	0.005%
64	9.985	2777	2782	2786	rBV8	1227	1284	0.05%	0.007%
65	10.053	2800	2803	2804	rBV	1075	530	0.02%	0.003%
66	10.075	2808	2810	2814	rBV4	639	482	0.02%	0.003%
67	10.146	2818	2832	2851	rBV	597155	944537	38.18%	5.367%
68	10.307	2880	2882	2885	rBV4	1469	1036	0.04%	0.006%
69	10.464	2929	2931	2933	rBV3	645	391	0.02%	0.002%
70	10.596	2967	2972	2973	rBV5	965	653	0.03%	0.004%
71	10.680	2995	2998	3000	rBV2	1114	734	0.03%	0.004%
72	10.738	3014	3016	3019	rBV4	985	802	0.03%	0.005%
73	10.818	3038	3041	3044	rBV4	1263	1091	0.04%	0.006%
74	10.870	3055	3057	3062	rVB6	1068	670	0.03%	0.004%
75	10.937	3073	3078	3080	rBV6	1101	983	0.04%	0.006%
76	10.969	3086	3088	3090	rBV3	836	370	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV090624\
 Data File : VV037214.D
 Acq On : 06 Sep 2024 10:59
 Operator : SY/MD
 Sample : P3842-06
 Misc : 5.00mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082624WMA.M
 Title : VOC Analysis

77	11.072	3115	3120	3123	rVB6	873	661	0.03%	0.004%
78	11.088	3123	3125	3127	rBV4	1286	669	0.03%	0.004%
79	11.178	3142	3153	3181	rBV	1038939	1665650	67.32%	9.465%
80	11.500	3250	3253	3256	rBV4	1189	931	0.04%	0.005%
81	11.554	3259	3270	3300	rVV	1087648	1755291	70.95%	9.974%
82	11.960	3394	3396	3399	rBV4	1571	650	0.03%	0.004%
83	12.037	3418	3420	3424	rBV6	881	826	0.03%	0.005%
84	12.133	3445	3450	3453	rBV4	1328	902	0.04%	0.005%
85	12.246	3482	3485	3489	rBV5	964	514	0.02%	0.003%
86	12.268	3489	3492	3495	rBV4	659	450	0.02%	0.003%
87	12.297	3499	3501	3506	rVV5	1263	854	0.03%	0.005%
88	12.657	3610	3613	3616	rVB4	1189	759	0.03%	0.004%
89	12.677	3616	3619	3621	rBV4	918	546	0.02%	0.003%
90	13.088	3744	3747	3750	rBV5	1350	1149	0.05%	0.007%
91	13.265	3800	3802	3804	rBV2	1040	520	0.02%	0.003%
92	13.307	3814	3815	3819	rBV3	965	667	0.03%	0.004%
93	13.358	3828	3831	3833	rBV3	1771	1175	0.05%	0.007%
94	13.426	3850	3852	3853	rBV	898	408	0.02%	0.002%
95	13.564	3893	3895	3897	rBV	1333	628	0.03%	0.004%
96	13.886	3991	3995	3997	rBV4	1240	846	0.03%	0.005%
97	14.265	4110	4113	4116	rBV3	1131	776	0.03%	0.004%
98	14.281	4116	4118	4121	rBV3	1061	806	0.03%	0.005%
99	14.320	4128	4130	4133	rBV3	1059	680	0.03%	0.004%
100	14.474	4176	4178	4180	rBV2	1315	673	0.03%	0.004%




Sum of corrected areas: 17598087

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV090624\
Data File : VV037214.D
Acq On : 06 Sep 2024 10:59
Operator : SY/MD
Sample : P3842-06
Misc : 5.00mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

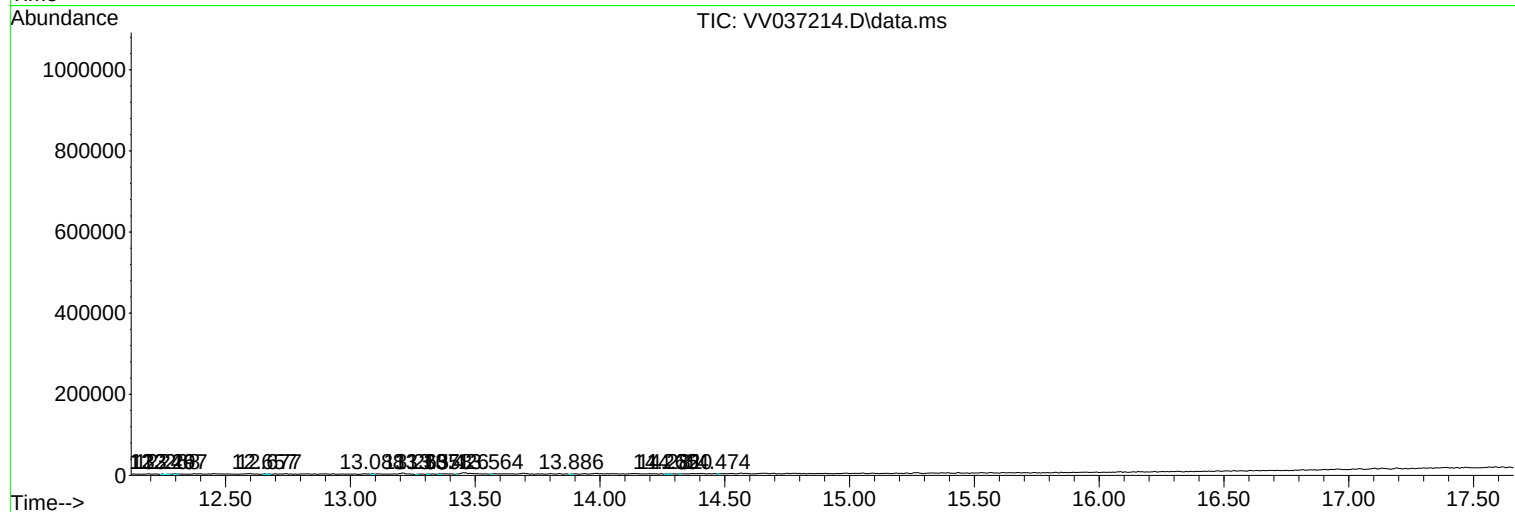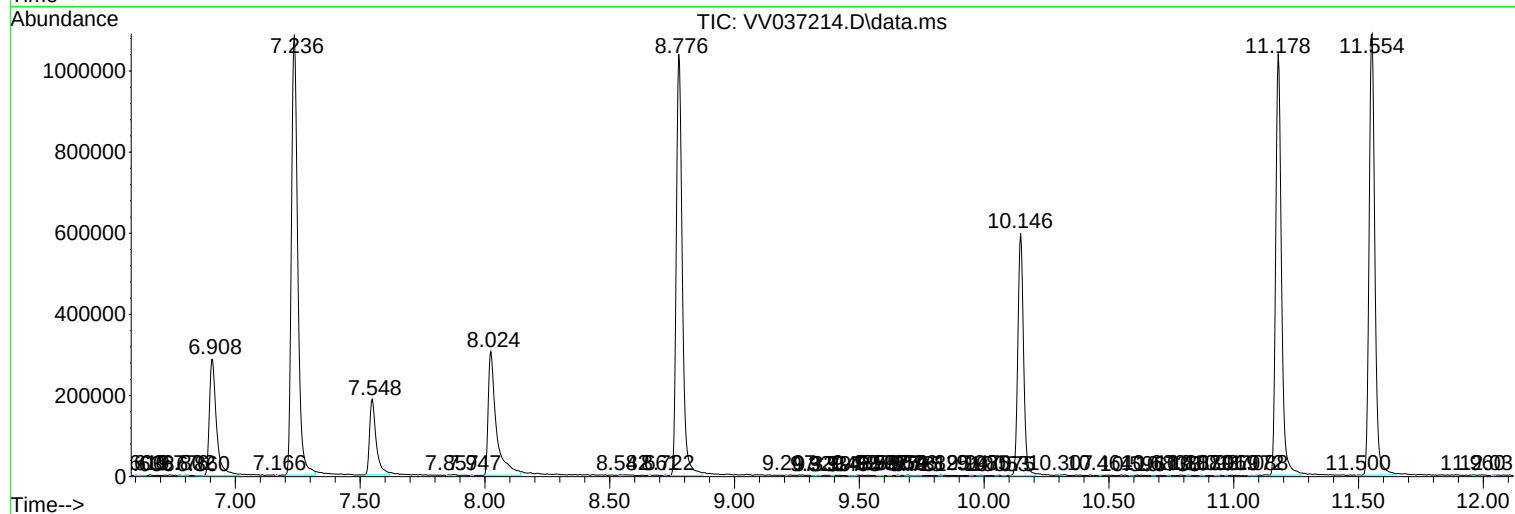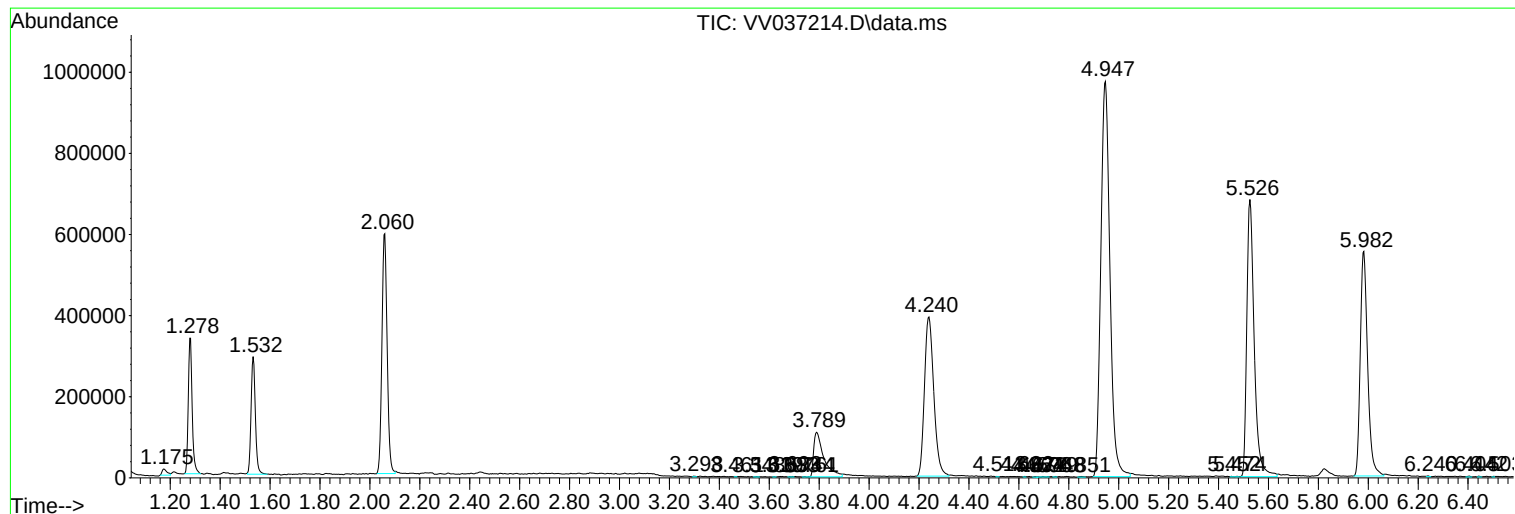

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV090624\
Data File : VV037214.D
Acq On : 06 Sep 2024 10:59
Operator : SY/MD
Sample : P3842-06
Misc : 5.00mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV090624\
Data File : VV037214.D
Acq On : 06 Sep 2024 10:59
Operator : SY/MD
Sample : P3842-06
Misc : 5.00mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------