

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV090624\
 Data File : VV037215.D
 Acq On : 06 Sep 2024 11:20
 Operator : SY/MD
 Sample : P3843-03
 Misc : 5.00mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BHJM6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082624WMA.M
 Title : VOC Analysis

Signal : TIC: VV037215.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.175	37	42	52	rBV	11586	19979	0.79%	0.105%
2	1.282	67	75	91	rVB	330511	360129	14.25%	1.894%
3	1.532	146	153	165	rBV	285485	344605	13.64%	1.812%
4	1.835	240	247	257	rBV2	16392	24744	0.98%	0.130%
5	2.060	308	317	328	rBV	590705	855807	33.86%	4.500%
6	2.114	328	334	356	rVB	63853	108806	4.31%	0.572%
7	3.301	700	703	708	rVV7	1853	2027	0.08%	0.011%
8	3.490	759	762	764	rBV5	1328	909	0.04%	0.005%
9	3.632	803	806	809	rBV5	1212	948	0.04%	0.005%
10	3.796	847	857	884	rBV	118834	326778	12.93%	1.718%
11	4.076	941	944	947	rVB4	1823	1141	0.05%	0.006%
12	4.246	979	997	1029	rBV	405349	1053472	41.68%	5.539%
13	4.513	1077	1080	1083	rBV4	1276	749	0.03%	0.004%
14	4.558	1088	1094	1097	rBV7	1142	1328	0.05%	0.007%
15	4.715	1140	1143	1146	rVB5	1271	927	0.04%	0.005%
16	4.809	1167	1172	1173	rBV4	933	823	0.03%	0.004%
17	4.867	1187	1190	1194	rBV6	1266	848	0.03%	0.004%
18	4.950	1200	1216	1242	rBV2	999246	2527326	100.00%	13.289%
19	5.317	1327	1330	1335	rBV7	1148	1045	0.04%	0.005%
20	5.342	1336	1338	1344	rVV9	1203	1276	0.05%	0.007%
21	5.375	1345	1348	1352	rVB4	2254	1528	0.06%	0.008%
22	5.529	1384	1396	1430	rBV	774835	1597443	63.21%	8.400%
23	5.825	1476	1488	1504	rBV4	24218	61131	2.42%	0.321%
24	5.899	1505	1511	1525	rVV3	25357	62960	2.49%	0.331%
25	5.982	1526	1537	1567	rVB	575713	1201447	47.54%	6.318%
26	6.423	1672	1674	1676	rBV3	1512	833	0.03%	0.004%
27	6.539	1706	1710	1715	rVB5	1245	1336	0.05%	0.007%
28	6.619	1732	1735	1739	rBV5	1306	846	0.03%	0.004%
29	6.641	1739	1742	1744	rBV4	1344	729	0.03%	0.004%
30	6.741	1770	1773	1777	rBV5	1320	1118	0.04%	0.006%
31	6.867	1807	1812	1814	rBV5	1412	1176	0.05%	0.006%
32	6.908	1815	1825	1864	rBV2	299636	576217	22.80%	3.030%
33	7.156	1900	1902	1906	rVB4	1499	951	0.04%	0.005%
34	7.239	1916	1928	1954	rBV	1110248	1991495	78.80%	10.472%
35	7.548	2016	2024	2047	rBV	190328	352962	13.97%	1.856%
36	7.873	2119	2125	2129	rVB7	1964	2154	0.09%	0.011%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV090624\
 Data File : VV037215.D
 Acq On : 06 Sep 2024 11:20
 Operator : SY/MD
 Sample : P3843-03
 Misc : 5.00mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BHJM6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082624WMA.M
 Title : VOC Analysis

37	7.915	2134	2138	2140	rBV3	1819	1761	0.07%	0.009%
38	7.966	2149	2154	2159	rVB7	1994	2183	0.09%	0.011%
39	8.024	2159	2172	2216	rBV2	338232	777754	30.77%	4.090%
40	8.336	2266	2269	2271	rBV4	1956	1252	0.05%	0.007%
41	8.420	2293	2295	2299	rVB5	1639	1003	0.04%	0.005%
42	8.780	2396	2407	2441	rVV	1185144	1972868	78.06%	10.374%
43	9.214	2535	2542	2544	rBV8	1044	1069	0.04%	0.006%
44	9.326	2575	2577	2579	rVB3	1607	741	0.03%	0.004%
45	9.355	2579	2586	2590	rBV7	1275	1450	0.06%	0.008%
46	9.535	2637	2642	2645	rBV5	1697	1673	0.07%	0.009%
47	9.577	2653	2655	2659	rVB4	1260	834	0.03%	0.004%
48	9.606	2659	2664	2666	rBV6	1627	1437	0.06%	0.008%
49	9.799	2722	2724	2727	rBV3	1268	754	0.03%	0.004%
50	9.902	2753	2756	2759	rBV3	816	830	0.03%	0.004%
51	9.960	2771	2774	2776	rBV3	1386	781	0.03%	0.004%
52	9.973	2776	2778	2782	rVB5	1233	756	0.03%	0.004%
53	10.146	2819	2832	2854	rBV	611205	977626	38.68%	5.141%
54	10.310	2879	2883	2886	rVV5	949	1102	0.04%	0.006%
55	10.387	2903	2907	2913	rVB7	1400	1509	0.06%	0.008%
56	10.432	2913	2921	2925	rVB9	1553	1837	0.07%	0.010%
57	10.773	3021	3027	3030	rBV8	1233	1314	0.05%	0.007%
58	10.895	3063	3065	3068	rVB4	1326	793	0.03%	0.004%
59	10.992	3088	3095	3098	rVB7	1273	1082	0.04%	0.006%
60	11.027	3101	3106	3107	rBV5	1250	1042	0.04%	0.005%
61	11.130	3134	3138	3139	rBV4	1479	866	0.03%	0.005%
62	11.178	3142	3153	3182	rBV	1191977	1897015	75.06%	9.975%
63	11.403	3221	3223	3226	rVB3	1753	734	0.03%	0.004%
64	11.439	3232	3234	3239	rVB5	1383	878	0.03%	0.005%
65	11.497	3239	3252	3259	rBV6	13210	29076	1.15%	0.153%
66	11.554	3259	3270	3294	rVV	1135959	1809640	71.60%	9.516%
67	11.860	3363	3365	3370	rVB6	1270	863	0.03%	0.005%
68	11.979	3399	3402	3405	rVB4	1918	1039	0.04%	0.005%
69	12.197	3468	3470	3474	rVV5	1212	786	0.03%	0.004%
70	12.214	3474	3475	3480	rVB4	1425	772	0.03%	0.004%
71	12.249	3482	3486	3488	rBV4	1476	974	0.04%	0.005%
72	12.400	3532	3533	3541	rVB6	1205	1162	0.05%	0.006%
73	12.455	3545	3550	3551	rBV3	942	796	0.03%	0.004%
74	12.468	3551	3554	3562	rVB9	1234	1380	0.05%	0.007%
75	12.545	3576	3578	3582	rVB6	1422	983	0.04%	0.005%
76	12.577	3582	3588	3591	rBV7	2255	1864	0.07%	0.010%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV090624\
Data File : VV037215.D
Acq On : 06 Sep 2024 11:20
Operator : SY/MD
Sample : P3843-03
Misc : 5.00mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BHJM6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082624WMA.M
Title : VOC Analysis

77	12.593	3591	3593	3597	rVV5	1787	1609	0.06%	0.008%
78	12.622	3600	3602	3607	rVB4	1363	1010	0.04%	0.005%
79	12.706	3621	3628	3631	rVV7	1211	1173	0.05%	0.006%
80	12.802	3655	3658	3663	rBV5	1908	1522	0.06%	0.008%
81	12.895	3684	3687	3691	rVB5	1465	1123	0.04%	0.006%
82	12.924	3695	3696	3701	rVB3	1360	796	0.03%	0.004%
83	12.976	3708	3712	3717	rVB7	1297	1527	0.06%	0.008%
84	13.005	3717	3721	3722	rBV4	1373	843	0.03%	0.004%
85	13.017	3723	3725	3730	rVB4	1673	1134	0.04%	0.006%
86	13.043	3730	3733	3734	rBV3	1457	907	0.04%	0.005%
87	13.095	3746	3749	3752	rBV5	924	840	0.03%	0.004%
88	13.214	3783	3786	3792	rVB8	1913	1630	0.06%	0.009%
89	13.644	3915	3920	3922	rBV4	1827	1752	0.07%	0.009%
90	13.680	3926	3931	3932	rBV5	1065	918	0.04%	0.005%
91	13.815	3969	3973	3975	rVB3	969	771	0.03%	0.004%
92	13.882	3992	3994	4000	rVB6	1962	1678	0.07%	0.009%
93	14.001	4027	4031	4035	rVB5	1089	1020	0.04%	0.005%
94	14.050	4044	4046	4049	rBV3	1068	800	0.03%	0.004%
95	14.133	4068	4072	4073	rBV3	1559	997	0.04%	0.005%
96	14.143	4073	4075	4083	rVB8	1339	1485	0.06%	0.008%
97	14.403	4153	4156	4158	rVB4	1510	913	0.04%	0.005%
98	14.490	4181	4183	4187	rVB3	1417	825	0.03%	0.004%
99	14.908	4309	4313	4315	rBV5	1329	1079	0.04%	0.006%
100	15.008	4342	4344	4349	rVB4	1529	930	0.04%	0.005%




Sum of corrected areas: 19017554

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV090624\
Data File : VV037215.D
Acq On : 06 Sep 2024 11:20
Operator : SY/MD
Sample : P3843-03
Misc : 5.00mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BHJM6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

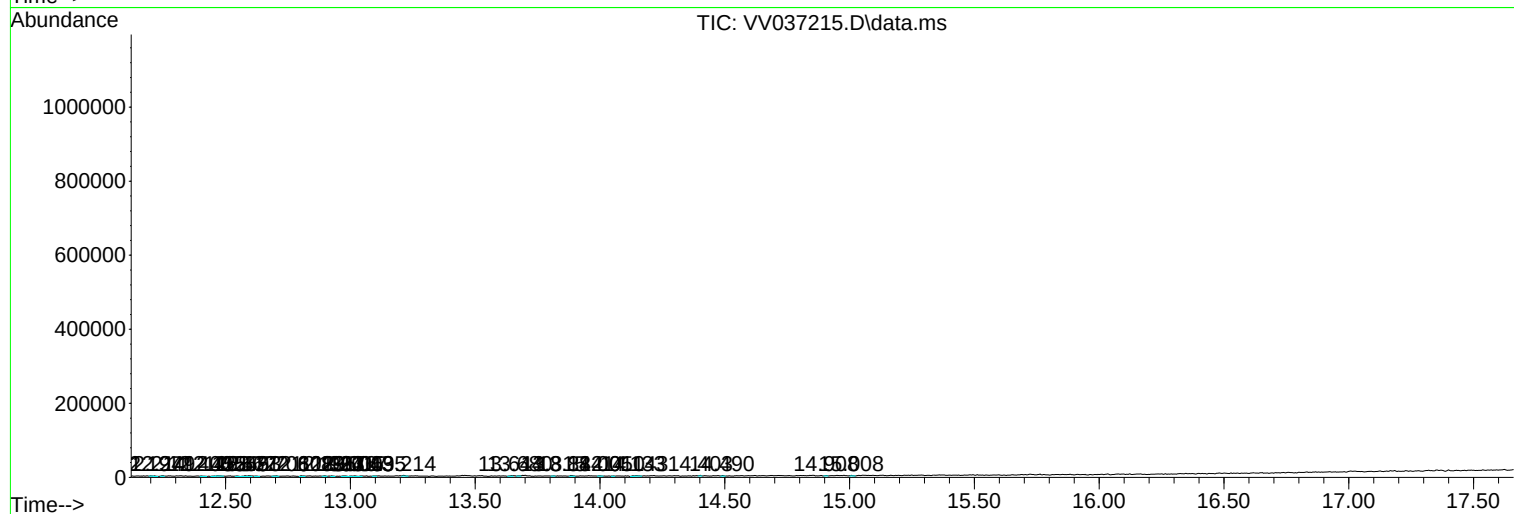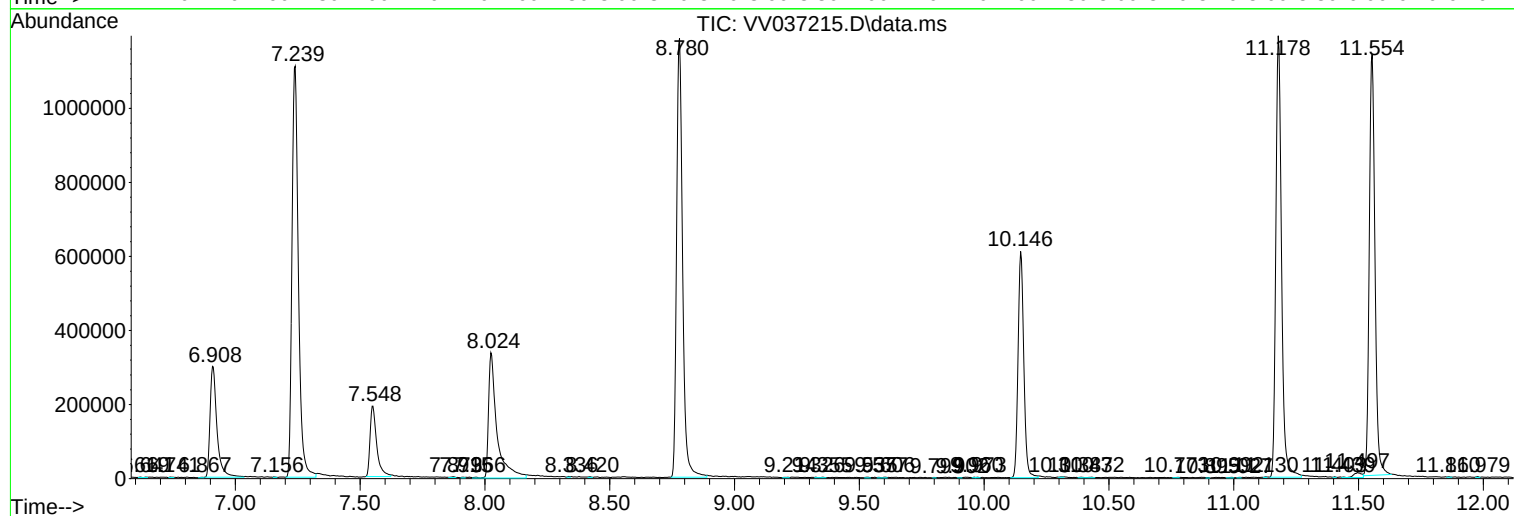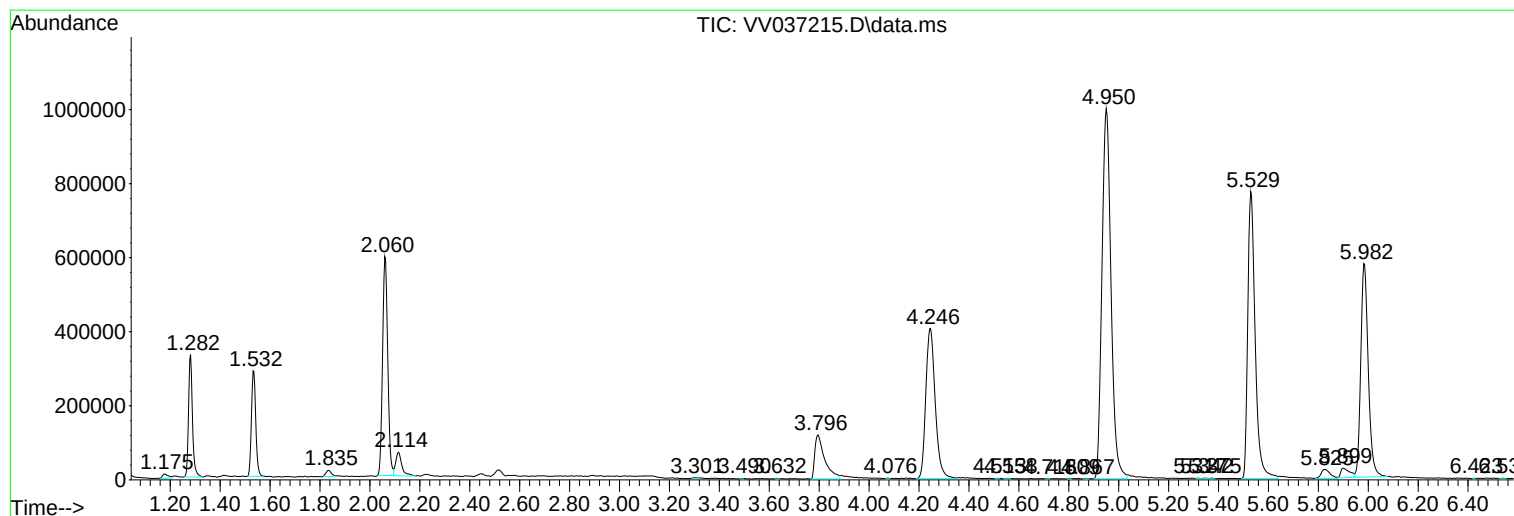

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV090624\
Data File : VV037215.D
Acq On : 06 Sep 2024 11:20
Operator : SY/MD
Sample : P3843-03
Misc : 5.00mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BHJM6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV090624\
Data File : VV037215.D
Acq On : 06 Sep 2024 11:20
Operator : SY/MD
Sample : P3843-03
Misc : 5.00mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BHJM6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------