

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV090624\
 Data File : VV037219.D
 Acq On : 06 Sep 2024 12:46
 Operator : SY/MD
 Sample : P3843-05
 Misc : 5.00mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BHJM2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082624WMA.M
 Title : VOC Analysis

Signal : TIC: VV037219.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	68	74	87	rVB	294570	314288	13.44%	1.796%
2	1.532	146	153	167	rVB	266862	311862	13.34%	1.783%
3	2.060	308	317	327	rBV	537055	765404	32.73%	4.375%
4	3.519	769	771	772	rBV3	862	315	0.01%	0.002%
5	3.622	800	803	805	rBV3	1142	638	0.03%	0.004%
6	3.664	813	816	818	rBV3	1042	550	0.02%	0.003%
7	3.690	821	824	828	rBV4	1017	894	0.04%	0.005%
8	3.796	848	857	882	rBV2	106611	296086	12.66%	1.692%
9	4.175	972	975	976	rBV3	1213	698	0.03%	0.004%
10	4.246	981	997	1028	rVV	378433	1018617	43.56%	5.822%
11	4.590	1100	1104	1106	rBV4	1004	632	0.03%	0.004%
12	4.622	1111	1114	1119	rVB6	1461	1287	0.06%	0.007%
13	4.658	1123	1125	1128	rVB4	1512	806	0.03%	0.005%
14	4.674	1128	1130	1132	rBV2	885	463	0.02%	0.003%
15	4.703	1135	1139	1143	rBV7	1384	1238	0.05%	0.007%
16	4.728	1143	1147	1149	rBV3	586	389	0.02%	0.002%
17	4.751	1149	1154	1158	rVB7	1482	1521	0.07%	0.009%
18	4.773	1158	1161	1163	rBV3	1116	801	0.03%	0.005%
19	4.950	1200	1216	1254	rBV2	917508	2338650	100.00%	13.367%
20	5.375	1345	1348	1351	rBV4	1367	870	0.04%	0.005%
21	5.529	1385	1396	1429	rBV	735971	1524469	65.19%	8.713%
22	5.899	1505	1511	1524	rBV2	28744	66415	2.84%	0.380%
23	5.985	1527	1538	1563	rVB	535561	1107656	47.36%	6.331%
24	6.625	1734	1737	1739	rBV2	935	664	0.03%	0.004%
25	6.866	1808	1812	1815	rBV5	964	920	0.04%	0.005%
26	6.911	1816	1826	1851	rVV	271837	520203	22.24%	2.973%
27	7.239	1917	1928	1956	rBV	1010608	1820578	77.85%	10.406%
28	7.551	2016	2025	2045	rBV	174157	324675	13.88%	1.856%
29	7.969	2153	2155	2156	rBB2	267	165	0.01%	0.001%
30	8.024	2164	2172	2212	rBV2	317907	704259	30.11%	4.025%
31	8.715	2385	2387	2390	rBV5	764	419	0.02%	0.002%
32	8.780	2396	2407	2437	rBV	1140800	1893910	80.98%	10.825%
33	9.162	2524	2526	2528	rBV3	1190	448	0.02%	0.003%
34	9.339	2577	2581	2584	rBV6	597	493	0.02%	0.003%
35	9.355	2584	2586	2588	rBV3	686	323	0.01%	0.002%
36	9.407	2599	2602	2605	rVB5	1105	481	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV090624\
 Data File : VV037219.D
 Acq On : 06 Sep 2024 12:46
 Operator : SY/MD
 Sample : P3843-05
 Misc : 5.00mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BHJM2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082624WMA.M
 Title : VOC Analysis

37	9.480	2623	2625	2629	rVB5	1801	1264	0.05%	0.007%
38	9.516	2631	2636	2642	rBV7	1522	1563	0.07%	0.009%
39	9.612	2665	2666	2668	rBV	708	270	0.01%	0.002%
40	9.712	2694	2697	2702	rVB7	1333	1160	0.05%	0.007%
41	9.741	2704	2706	2710	rVB5	922	429	0.02%	0.002%
42	9.802	2723	2725	2726	rBV	515	214	0.01%	0.001%
43	9.828	2731	2733	2738	rVB5	1064	643	0.03%	0.004%
44	9.853	2738	2741	2745	rBV5	544	462	0.02%	0.003%
45	9.886	2749	2751	2754	rBV4	1169	516	0.02%	0.003%
46	9.902	2754	2756	2758	rBV3	766	453	0.02%	0.003%
47	9.934	2762	2766	2769	rVB5	1605	1145	0.05%	0.007%
48	9.998	2784	2786	2787	rBV2	734	384	0.02%	0.002%
49	10.021	2791	2793	2795	rBV3	756	236	0.01%	0.001%
50	10.030	2795	2796	2797	rVB	1011	195	0.01%	0.001%
51	10.040	2797	2799	2800	rBV2	681	353	0.02%	0.002%
52	10.079	2809	2811	2812	rBV2	372	164	0.01%	0.001%
53	10.146	2821	2832	2851	rBV	590721	939731	40.18%	5.371%
54	10.394	2905	2909	2911	rBV3	1092	808	0.03%	0.005%
55	10.435	2919	2922	2925	rBV3	421	263	0.01%	0.002%
56	10.461	2925	2930	2931	rBV3	866	702	0.03%	0.004%
57	10.480	2934	2936	2938	rBV2	1075	519	0.02%	0.003%
58	10.522	2946	2949	2951	rBV3	951	591	0.03%	0.003%
59	10.574	2963	2965	2968	rVB3	516	275	0.01%	0.002%
60	10.599	2972	2973	2974	rVB	339	65	0.00%	0.000%
61	10.615	2974	2978	2981	rBV4	838	711	0.03%	0.004%
62	10.632	2981	2983	2985	rBV2	1024	569	0.02%	0.003%
63	10.644	2985	2987	2988	rBV2	963	306	0.01%	0.002%
64	10.686	2998	3000	3001	rBV2	1330	603	0.03%	0.003%
65	10.760	3020	3023	3027	rBV3	1418	1115	0.05%	0.006%
66	10.786	3027	3031	3035	rBV6	2871	2492	0.11%	0.014%
67	10.841	3045	3048	3049	rBV3	929	407	0.02%	0.002%
68	10.889	3060	3063	3066	rVB4	1261	844	0.04%	0.005%
69	10.924	3072	3074	3075	rBV2	860	372	0.02%	0.002%
70	10.976	3087	3090	3091	rBV2	824	449	0.02%	0.003%
71	11.027	3103	3106	3110	rBV4	970	876	0.04%	0.005%
72	11.104	3127	3130	3131	rBV3	850	534	0.02%	0.003%
73	11.117	3131	3134	3135	rBV3	1160	573	0.02%	0.003%
74	11.178	3143	3153	3187	rBV	1132493	1809528	77.37%	10.343%
75	11.490	3243	3250	3252	rBV3	12634	15715	0.67%	0.090%
76	11.554	3260	3270	3297	rVB	1035746	1674399	71.60%	9.570%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV090624\
 Data File : VV037219.D
 Acq On : 06 Sep 2024 12:46
 Operator : SY/MD
 Sample : P3843-05
 Misc : 5.00mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BHJM2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082624WMA.M

Title : VOC Analysis

77	12.172	3460	3462	3465	rBV4	1365	982	0.04%	0.006%
78	12.323	3507	3509	3515	rBV5	973	798	0.03%	0.005%
79	12.564	3577	3584	3589	rBV9	1633	2088	0.09%	0.012%
80	12.586	3589	3591	3592	rBV3	1507	663	0.03%	0.004%
81	12.641	3606	3608	3611	rBV4	757	453	0.02%	0.003%
82	12.705	3625	3628	3634	rBV7	1065	1075	0.05%	0.006%
83	12.869	3678	3679	3682	rBV2	702	309	0.01%	0.002%
84	12.934	3695	3699	3702	rBV4	1357	1313	0.06%	0.008%
85	13.152	3764	3767	3770	rBV4	1206	841	0.04%	0.005%
86	13.204	3777	3783	3785	rBV5	2458	2239	0.10%	0.013%
87	13.824	3974	3976	3977	rBV2	868	280	0.01%	0.002%
88	14.162	4079	4081	4084	rBV2	985	670	0.03%	0.004%




Sum of corrected areas: 17495696

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV090624\
Data File : VV037219.D
Acq On : 06 Sep 2024 12:46
Operator : SY/MD
Sample : P3843-05
Misc : 5.00mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BHJM2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

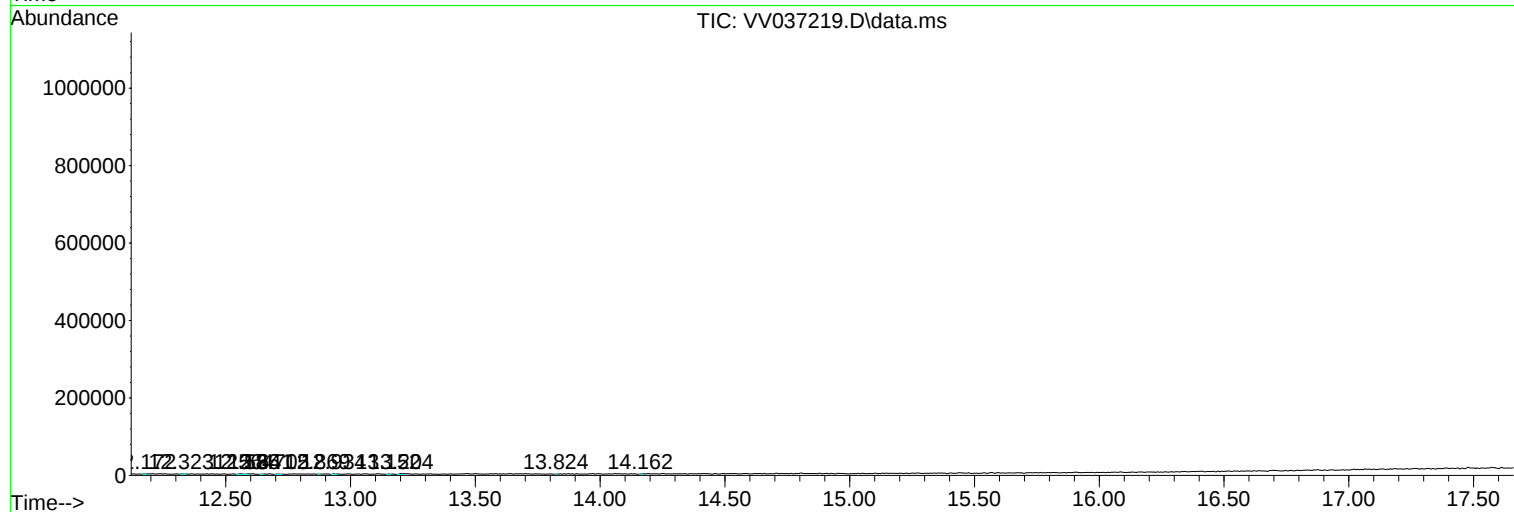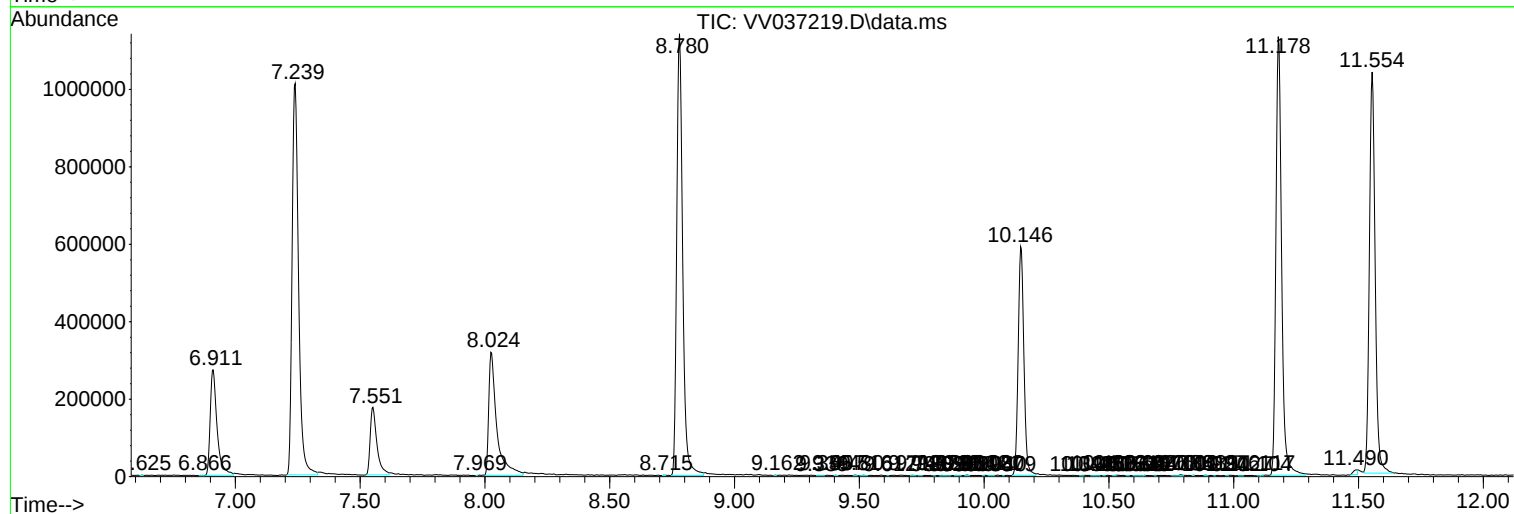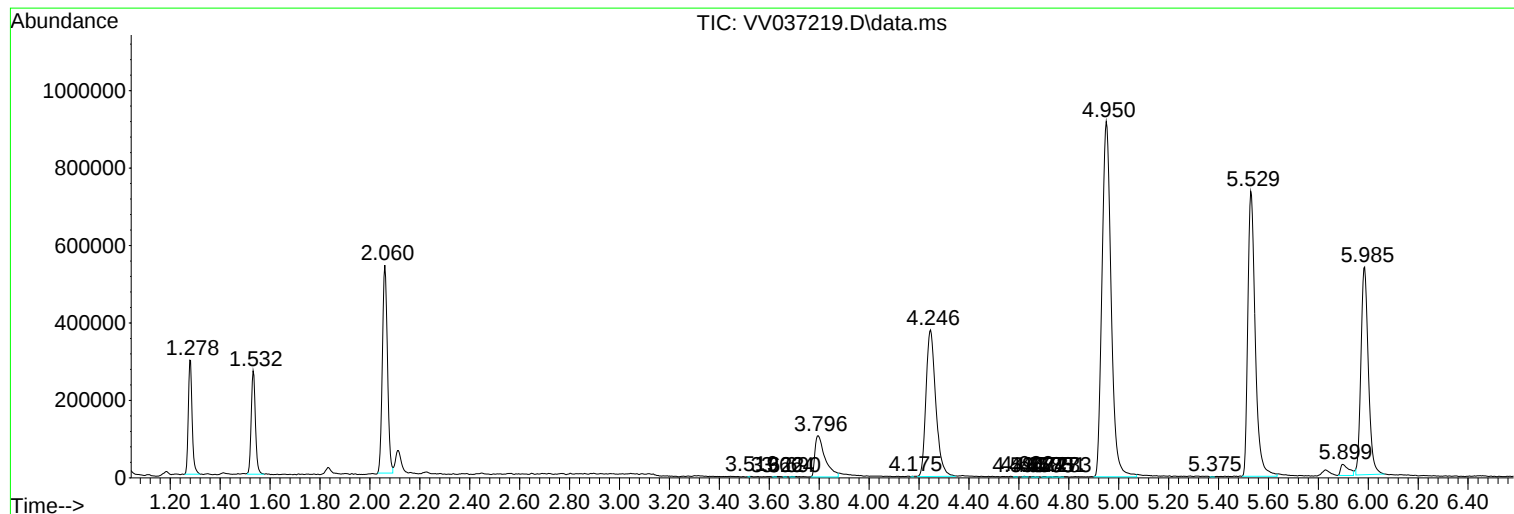

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV090624\
Data File : VV037219.D
Acq On : 06 Sep 2024 12:46
Operator : SY/MD
Sample : P3843-05
Misc : 5.00mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BHJM2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV090624\
Data File : VV037219.D
Acq On : 06 Sep 2024 12:46
Operator : SY/MD
Sample : P3843-05
Misc : 5.00mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BHJM2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------