

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV090624\
 Data File : VV037220.D
 Acq On : 06 Sep 2024 13:07
 Operator : SY/MD
 Sample : P3843-12
 Misc : 5.00mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BHJM7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082624WMA.M

Title : VOC Analysis

Signal : TIC: VV037220.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.179	36	43	50	rBV	5370	9041	0.47%	0.062%
2	1.278	67	74	90	rVV	251292	268745	13.99%	1.851%
3	1.349	90	96	108	rVB	34522	40495	2.11%	0.279%
4	1.532	146	153	171	rVB	222759	262101	13.65%	1.806%
5	2.060	307	317	329	rBV	448755	648606	33.77%	4.468%
6	3.298	701	702	706	rVB3	1096	740	0.04%	0.005%
7	3.413	735	738	740	rBV2	1375	1004	0.05%	0.007%
8	3.442	745	747	749	rVV3	1485	771	0.04%	0.005%
9	3.465	749	754	756	rVB6	1251	1053	0.05%	0.007%
10	3.523	768	772	776	rVV6	1309	960	0.05%	0.007%
11	3.613	798	800	804	rVV4	1393	912	0.05%	0.006%
12	3.796	849	857	897	rVV2	86436	254510	13.25%	1.753%
13	4.246	978	997	1026	rBV3	334711	1028626	53.56%	7.086%
14	4.545	1088	1090	1096	rVB6	1142	769	0.04%	0.005%
15	4.613	1107	1111	1113	rVB3	1845	1206	0.06%	0.008%
16	4.632	1113	1117	1120	rBV5	1305	1175	0.06%	0.008%
17	4.767	1155	1159	1163	rBV3	1283	905	0.05%	0.006%
18	4.802	1168	1170	1175	rVV5	1000	835	0.04%	0.006%
19	4.834	1175	1180	1183	rVV7	817	770	0.04%	0.005%
20	4.950	1200	1216	1250	rBV2	752900	1920423	100.00%	13.230%
21	5.198	1291	1293	1298	rVB5	1767	1265	0.07%	0.009%
22	5.532	1385	1397	1427	rBV	558122	1161266	60.47%	8.000%
23	5.828	1479	1489	1502	rBV4	14585	35039	1.82%	0.241%
24	5.912	1508	1515	1524	rBV5	13062	27036	1.41%	0.186%
25	5.986	1527	1538	1566	rVB	437334	907083	47.23%	6.249%
26	6.211	1605	1608	1614	rVB7	1994	1167	0.06%	0.008%
27	6.304	1635	1637	1641	rVB4	1356	902	0.05%	0.006%
28	6.436	1667	1678	1697	rBV2	40529	82970	4.32%	0.572%
29	6.709	1760	1763	1766	rBV5	1513	1186	0.06%	0.008%
30	6.834	1800	1802	1806	rBV5	1238	1054	0.05%	0.007%
31	6.912	1815	1826	1854	rBV	221733	432185	22.50%	2.977%
32	7.240	1916	1928	1961	rBV	833959	1485287	77.34%	10.232%
33	7.551	2016	2025	2046	rBV	142182	267464	13.93%	1.843%
34	7.892	2128	2131	2133	rBV4	1557	1168	0.06%	0.008%
35	7.931	2140	2143	2146	rBV4	1145	788	0.04%	0.005%
36	8.027	2164	2173	2211	rBV2	252333	570232	29.69%	3.928%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV090624\
Data File : VV037220.D
Acq On : 06 Sep 2024 13:07
Operator : SY/MD
Sample : P3843-12
Misc : 5.00mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BHJM7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082624WMA.M
Title : VOC Analysis

37	8.378	2280	2282	2286	rBV4	1104	902	0.05%	0.006%
38	8.468	2306	2310	2314	rBV6	1313	1072	0.06%	0.007%
39	8.513	2321	2324	2327	rBV4	1059	827	0.04%	0.006%
40	8.677	2372	2375	2378	rBV4	1090	783	0.04%	0.005%
41	8.780	2395	2407	2431	rBV	864779	1445810	75.29%	9.960%
42	9.034	2483	2486	2488	rBV3	1225	951	0.05%	0.007%
43	9.198	2535	2537	2541	rVB4	2582	1741	0.09%	0.012%
44	9.227	2541	2546	2548	rBV4	2381	2225	0.12%	0.015%
45	9.532	2638	2641	2644	rVB4	1415	1112	0.06%	0.008%
46	9.555	2646	2648	2651	rBV3	1256	905	0.05%	0.006%
47	9.612	2664	2666	2669	rBV4	1225	801	0.04%	0.006%
48	9.673	2679	2685	2690	rVB8	1829	2618	0.14%	0.018%
49	9.773	2711	2716	2717	rBV4	1083	765	0.04%	0.005%
50	9.879	2747	2749	2752	rBV3	1096	726	0.04%	0.005%
51	9.969	2773	2777	2778	rBV3	1363	855	0.04%	0.006%
52	10.040	2797	2799	2803	rVB5	1290	952	0.05%	0.007%
53	10.146	2821	2832	2852	rBV	461766	762854	39.72%	5.255%
54	10.416	2914	2916	2921	rVB6	1684	1162	0.06%	0.008%
55	10.481	2933	2936	2940	rBV6	1168	797	0.04%	0.005%
56	10.850	3047	3051	3056	rBV7	844	811	0.04%	0.006%
57	10.927	3070	3075	3077	rBV4	1101	1017	0.05%	0.007%
58	11.104	3125	3130	3131	rBV5	1055	824	0.04%	0.006%
59	11.127	3134	3137	3141	rVB6	1480	1018	0.05%	0.007%
60	11.181	3141	3154	3182	rBV	865971	1408455	73.34%	9.703%
61	11.371	3211	3213	3219	rVB6	1836	1453	0.08%	0.010%
62	11.439	3230	3234	3236	rBV4	1635	1363	0.07%	0.009%
63	11.497	3243	3252	3257	rBV4	11412	19164	1.00%	0.132%
64	11.554	3260	3270	3299	rVB	858431	1376168	71.66%	9.480%
65	11.976	3399	3401	3406	rBV5	1387	1326	0.07%	0.009%
66	12.043	3418	3422	3423	rBV2	1813	978	0.05%	0.007%
67	12.101	3436	3440	3441	rBV2	1362	895	0.05%	0.006%
68	12.188	3463	3467	3471	rVV7	1865	1530	0.08%	0.011%
69	12.249	3484	3486	3490	rVB5	1623	1078	0.06%	0.007%
70	12.281	3490	3496	3498	rBV5	1121	1033	0.05%	0.007%
71	12.316	3504	3507	3512	rBV6	2099	1478	0.08%	0.010%
72	12.461	3549	3552	3555	rBV4	1004	745	0.04%	0.005%
73	12.542	3574	3577	3579	rBV3	1182	731	0.04%	0.005%
74	12.583	3586	3590	3593	rBV5	774	751	0.04%	0.005%
75	12.651	3608	3611	3615	rBV5	1194	868	0.05%	0.006%
76	12.792	3653	3655	3658	rBV3	1539	1017	0.05%	0.007%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV090624\
Data File : VV037220.D
Acq On : 06 Sep 2024 13:07
Operator : SY/MD
Sample : P3843-12
Misc : 5.00mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BHJM7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082624WMA.M
Title : VOC Analysis

77	12.898	3685	3688	3690	rBV4	1735	1229	0.06%	0.008%
78	12.963	3703	3708	3709	rBV5	1260	907	0.05%	0.006%
79	13.098	3748	3750	3755	rBV4	1260	930	0.05%	0.006%
80	13.207	3779	3784	3787	rBV6	1792	1572	0.08%	0.011%
81	13.281	3804	3807	3813	rBV6	1091	862	0.04%	0.006%
82	13.410	3844	3847	3851	rVB4	1304	775	0.04%	0.005%
83	13.455	3857	3861	3863	rBV4	995	807	0.04%	0.006%
84	13.587	3897	3902	3903	rBV4	1183	900	0.05%	0.006%
85	13.606	3906	3908	3912	rVV4	1043	907	0.05%	0.006%
86	13.654	3920	3923	3927	rVV6	1133	899	0.05%	0.006%
87	13.683	3927	3932	3937	rVV8	1574	2033	0.11%	0.014%
88	13.731	3944	3947	3954	rVV8	1840	2130	0.11%	0.015%
89	13.779	3957	3962	3963	rVV5	1355	1196	0.06%	0.008%
90	13.799	3966	3968	3974	rVB7	1742	1294	0.07%	0.009%
91	13.902	3994	4000	4001	rBV5	1399	1152	0.06%	0.008%
92	13.911	4001	4003	4008	rVB5	912	783	0.04%	0.005%
93	14.046	4041	4045	4050	rBV8	1521	1761	0.09%	0.012%
94	14.181	4085	4087	4090	rVB4	1420	725	0.04%	0.005%
95	14.503	4185	4187	4192	rVB5	1602	1282	0.07%	0.009%
96	14.599	4213	4217	4222	rBV7	1527	1378	0.07%	0.009%
97	14.895	4306	4309	4313	rVB6	1810	968	0.05%	0.007%
98	15.210	4405	4407	4413	rBV6	1568	1535	0.08%	0.011%
99	15.262	4420	4423	4428	rBV5	1442	1349	0.07%	0.009%
100	15.439	4474	4478	4489	rVB	20124	18162	0.95%	0.125%




Sum of corrected areas: 14515836

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV090624\
Data File : VV037220.D
Acq On : 06 Sep 2024 13:07
Operator : SY/MD
Sample : P3843-12
Misc : 5.00mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BHJM7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

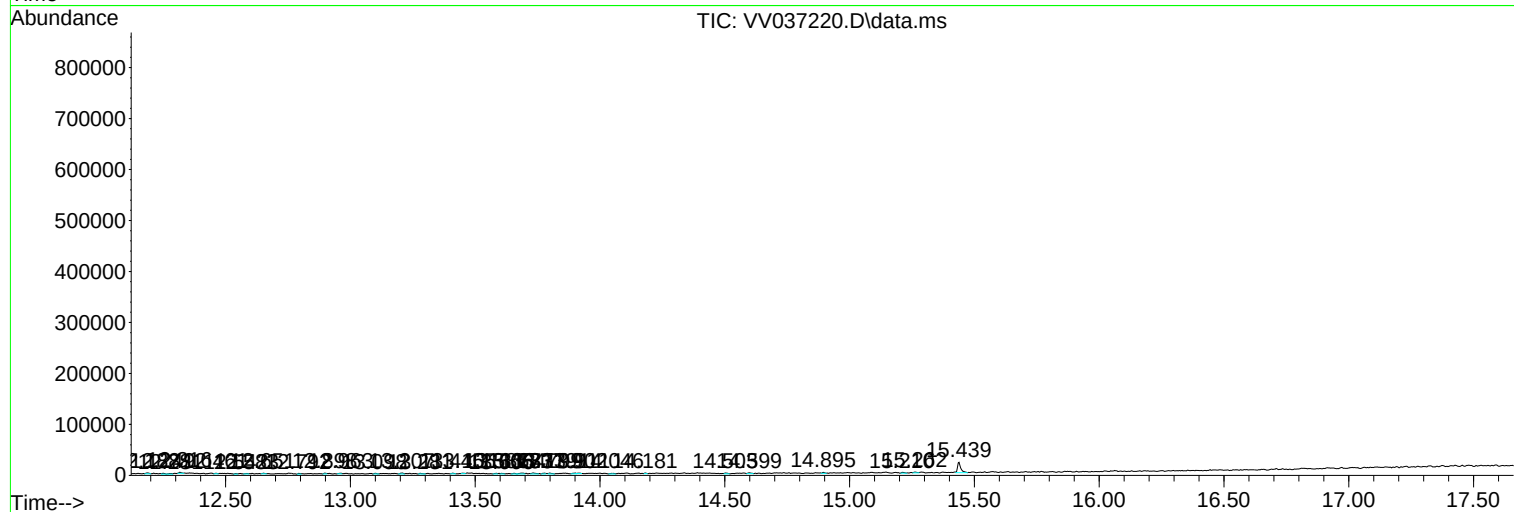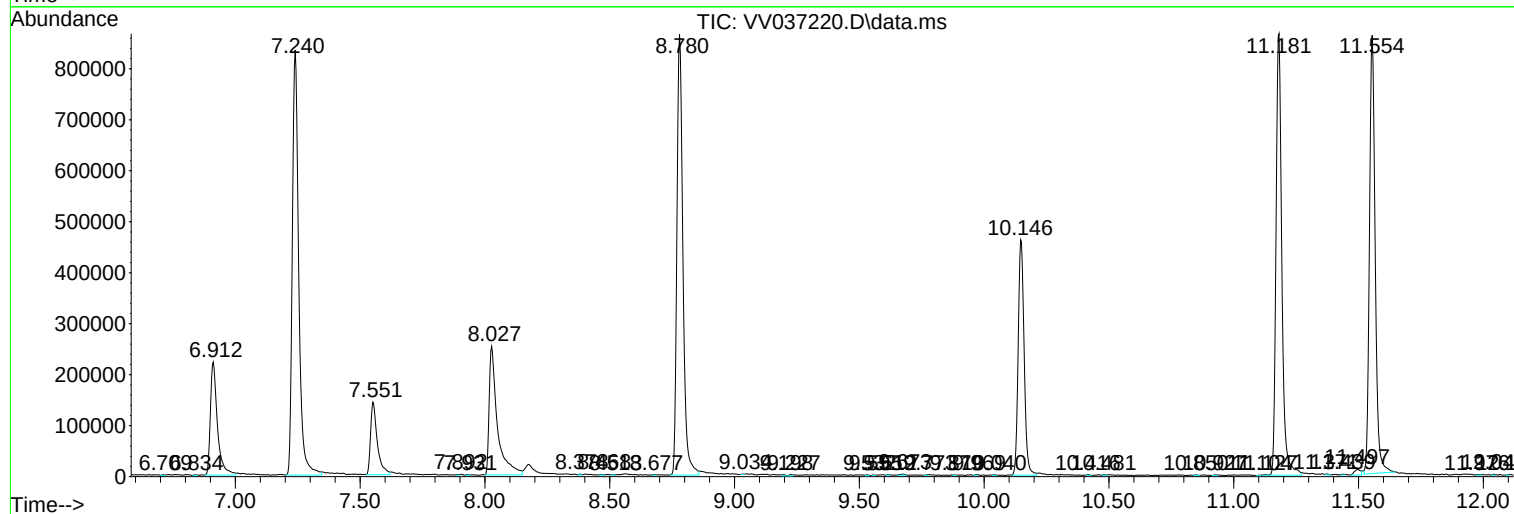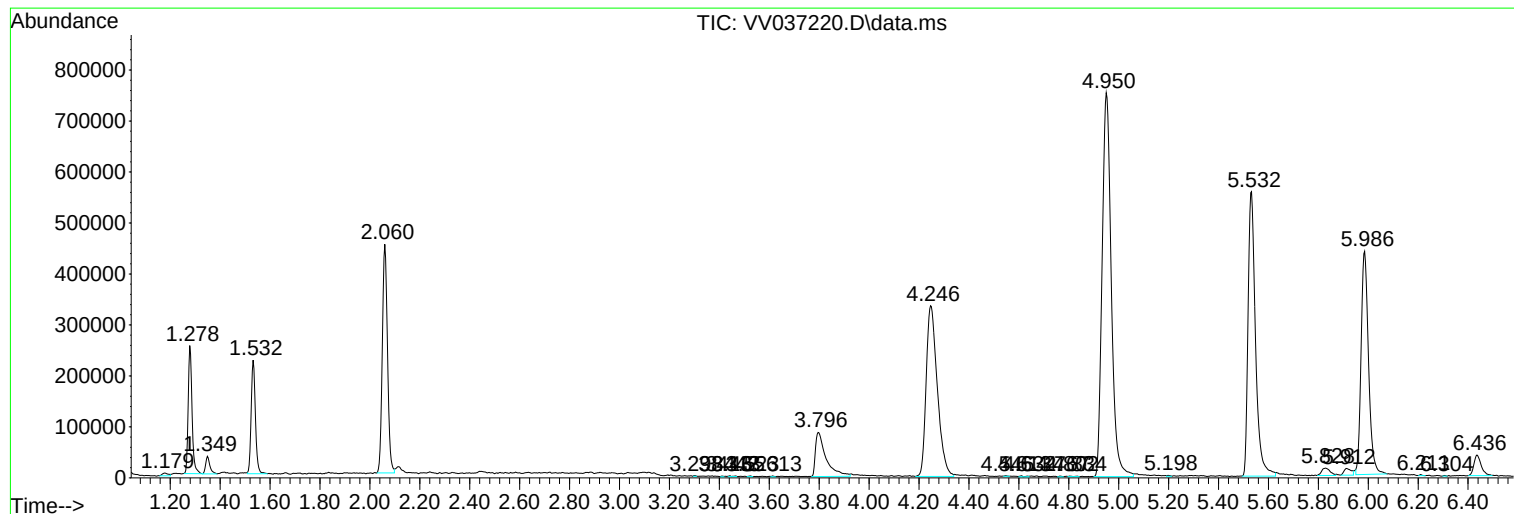

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV090624\
Data File : VV037220.D
Acq On : 06 Sep 2024 13:07
Operator : SY/MD
Sample : P3843-12
Misc : 5.00mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BHJM7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV090624\
Data File : VV037220.D
Acq On : 06 Sep 2024 13:07
Operator : SY/MD
Sample : P3843-12
Misc : 5.00mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BHJM7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc