

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV090624\
 Data File : VV037221.D
 Acq On : 06 Sep 2024 13:29
 Operator : SY/MD
 Sample : P3843-07
 Misc : 5.00mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BHJL8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082624WMA.M
 Title : VOC Analysis

Signal : TIC: VV037221.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	68	74	93	rVB	297277	308606	13.75%	1.881%
2	1.532	146	153	165	rVB	257483	297551	13.26%	1.814%
3	2.060	308	317	329	rBV	523663	744753	33.18%	4.540%
4	3.256	683	689	691	rBV8	1771	1444	0.06%	0.009%
5	3.477	756	758	761	rVB2	1286	559	0.02%	0.003%
6	3.555	778	782	787	rBV5	955	907	0.04%	0.006%
7	3.577	787	789	791	rBV4	780	433	0.02%	0.003%
8	3.680	815	821	825	rBV6	1726	2052	0.09%	0.013%
9	3.748	840	842	843	rBV2	756	306	0.01%	0.002%
10	3.757	843	845	847	rVB3	567	240	0.01%	0.001%
11	3.796	847	857	892	rBV2	102812	302379	13.47%	1.843%
12	4.246	982	997	1026	rBV	355763	912133	40.63%	5.560%
13	4.535	1085	1087	1088	rBV2	841	342	0.02%	0.002%
14	4.564	1093	1096	1098	rBV5	1215	762	0.03%	0.005%
15	4.638	1117	1119	1123	rBV5	908	702	0.03%	0.004%
16	4.735	1147	1149	1152	rVB4	1251	663	0.03%	0.004%
17	4.764	1155	1158	1161	rBV4	1153	910	0.04%	0.006%
18	4.799	1166	1169	1170	rBV2	502	192	0.01%	0.001%
19	4.821	1171	1176	1180	rVB7	1375	930	0.04%	0.006%
20	4.838	1180	1181	1183	rVB2	662	195	0.01%	0.001%
21	4.850	1183	1185	1187	rVB2	490	186	0.01%	0.001%
22	4.870	1187	1191	1192	rBV2	1081	666	0.03%	0.004%
23	4.950	1200	1216	1247	rBV2	873795	2244767	100.00%	13.683%
24	5.436	1366	1367	1370	rBV3	834	431	0.02%	0.003%
25	5.529	1385	1396	1431	rBV	639582	1332119	59.34%	8.120%
26	5.902	1506	1512	1524	rBV3	23332	51734	2.30%	0.315%
27	5.985	1527	1538	1573	rVB	515934	1078919	48.06%	6.577%
28	6.809	1792	1794	1796	rBV3	1128	553	0.02%	0.003%
29	6.911	1815	1826	1854	rBV	263872	510267	22.73%	3.110%
30	7.239	1917	1928	1962	rBV	982185	1744651	77.72%	10.635%
31	7.551	2014	2025	2049	rBV	169936	323702	14.42%	1.973%
32	7.979	2154	2158	2162	rVB6	1530	1257	0.06%	0.008%
33	8.027	2162	2173	2209	rBV2	306770	684526	30.49%	4.173%
34	8.519	2320	2326	2330	rBV7	1845	2086	0.09%	0.013%
35	8.780	2396	2407	2442	rBV	991573	1668886	74.35%	10.173%
36	9.120	2512	2513	2516	rBV3	774	380	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV090624\
 Data File : VV037221.D
 Acq On : 06 Sep 2024 13:29
 Operator : SY/MD
 Sample : P3843-07
 Misc : 5.00mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BHJL8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082624WMA.M
 Title : VOC Analysis

37	9.194	2530	2536	2542	rBV9	1307	2018	0.09%	0.012%
38	9.223	2543	2545	2547	rVB2	1134	367	0.02%	0.002%
39	9.236	2547	2549	2551	rBV3	949	420	0.02%	0.003%
40	9.378	2592	2593	2594	rBV	620	165	0.01%	0.001%
41	9.407	2599	2602	2603	rBV2	723	397	0.02%	0.002%
42	9.452	2614	2616	2618	rVB2	987	416	0.02%	0.003%
43	9.468	2618	2621	2622	rBV2	743	492	0.02%	0.003%
44	9.474	2622	2623	2626	rVV2	609	384	0.02%	0.002%
45	9.538	2639	2643	2646	rBV4	1380	991	0.04%	0.006%
46	9.554	2646	2648	2651	rBV3	861	492	0.02%	0.003%
47	9.574	2651	2654	2658	rVB5	1512	951	0.04%	0.006%
48	9.599	2660	2662	2663	rBV2	1296	589	0.03%	0.004%
49	9.760	2709	2712	2715	rVB5	1103	636	0.03%	0.004%
50	9.779	2715	2718	2720	rBV3	1112	788	0.04%	0.005%
51	9.850	2737	2740	2742	rBV2	728	567	0.03%	0.003%
52	9.924	2761	2763	2766	rBV3	1260	698	0.03%	0.004%
53	9.985	2779	2782	2784	rBV4	898	416	0.02%	0.003%
54	10.046	2797	2801	2802	rBV2	588	413	0.02%	0.003%
55	10.056	2802	2804	2806	rVV2	1151	542	0.02%	0.003%
56	10.146	2819	2832	2858	rBV	576668	920277	41.00%	5.610%
57	10.461	2924	2930	2932	rBV4	1054	1121	0.05%	0.007%
58	10.503	2942	2943	2946	rVB2	663	300	0.01%	0.002%
59	10.551	2956	2958	2959	rBV2	1360	618	0.03%	0.004%
60	10.583	2966	2968	2974	rBV5	912	712	0.03%	0.004%
61	10.657	2986	2991	2993	rBV4	1034	1004	0.04%	0.006%
62	10.705	3001	3006	3007	rBV4	1276	993	0.04%	0.006%
63	10.731	3011	3014	3016	rBV4	1323	800	0.04%	0.005%
64	10.789	3025	3032	3034	rBV7	1559	1453	0.06%	0.009%
65	10.921	3070	3073	3076	rVB3	1453	764	0.03%	0.005%
66	10.943	3078	3080	3084	rVB3	1191	764	0.03%	0.005%
67	10.969	3084	3088	3090	rBV4	1188	900	0.04%	0.005%
68	11.001	3096	3098	3099	rVB2	712	234	0.01%	0.001%
69	11.011	3099	3101	3103	rBV3	684	361	0.02%	0.002%
70	11.033	3106	3108	3111	rVV3	493	262	0.01%	0.002%
71	11.178	3143	3153	3186	rBV	982403	1583180	70.53%	9.650%
72	11.490	3240	3250	3259	rBV5	13879	31752	1.41%	0.194%
73	11.554	3260	3270	3301	rVB	1007590	1619789	72.16%	9.874%
74	12.191	3464	3468	3472	rBV6	1384	1421	0.06%	0.009%
75	12.442	3544	3546	3550	rVB5	1205	662	0.03%	0.004%
76	12.522	3570	3571	3572	rBV	757	166	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV090624\
Data File : VV037221.D
Acq On : 06 Sep 2024 13:29
Operator : SY/MD
Sample : P3843-07
Misc : 5.00mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BHJL8

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082624WMA.M
Title : VOC Analysis

77	12.541	3575	3577	3579	rBV2	767	395	0.02%	0.002%
78	12.683	3615	3621	3624	rBV5	1450	1563	0.07%	0.010%
79	12.734	3632	3637	3638	rBV4	1493	1339	0.06%	0.008%
80	13.149	3764	3766	3769	rVB3	1649	795	0.04%	0.005%
81	13.889	3994	3996	3999	rBV3	1063	829	0.04%	0.005%


Sum of corrected areas: 16405385

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV090624\
Data File : VV037221.D
Acq On : 06 Sep 2024 13:29
Operator : SY/MD
Sample : P3843-07
Misc : 5.00mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BHJL8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

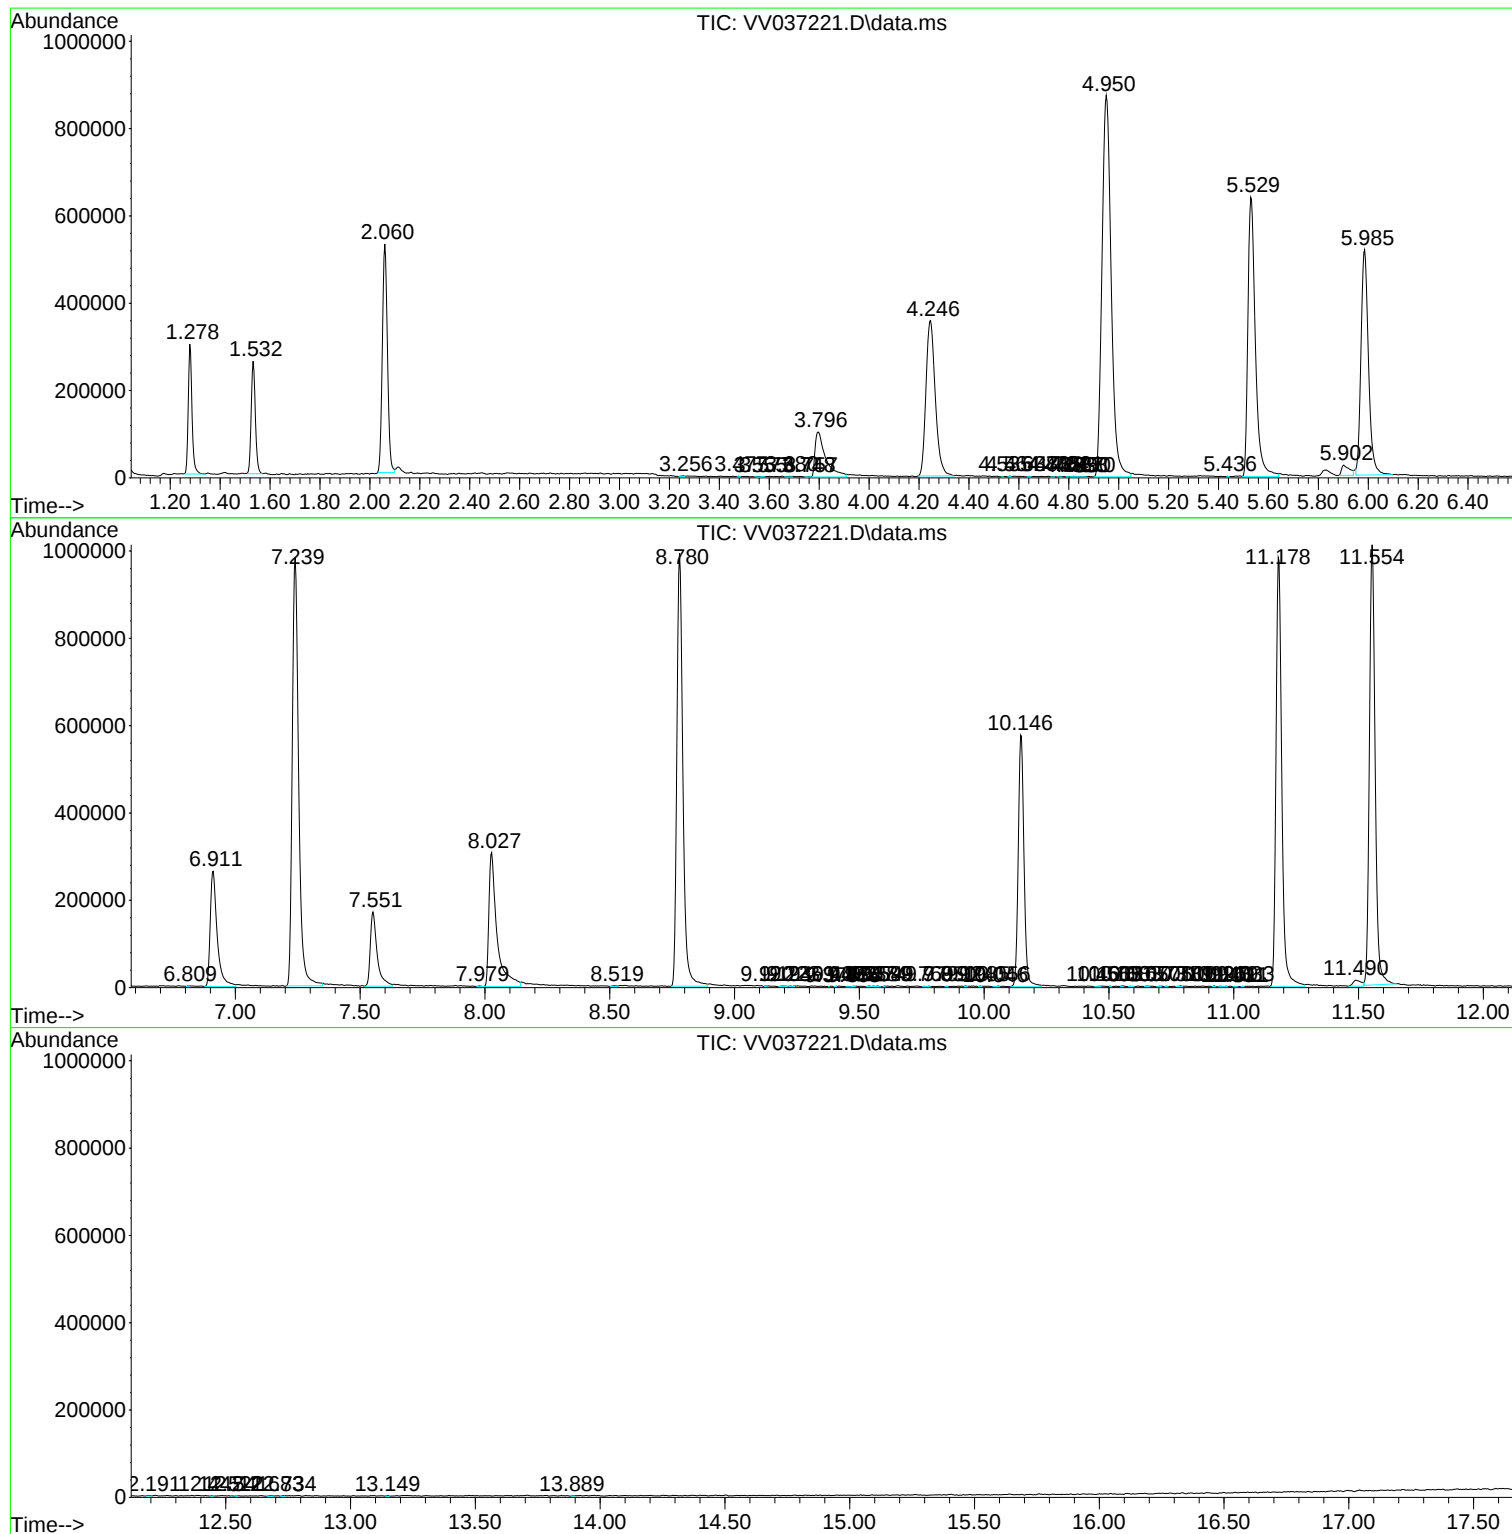

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV090624\
Data File : VV037221.D
Acq On : 06 Sep 2024 13:29
Operator : SY/MD
Sample : P3843-07
Misc : 5.00mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BHJL8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV090624\
Data File : VV037221.D
Acq On : 06 Sep 2024 13:29
Operator : SY/MD
Sample : P3843-07
Misc : 5.00mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BHJL8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc