

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV090624\
 Data File : VV037222.D
 Acq On : 06 Sep 2024 13:50
 Operator : SY/MD
 Sample : P3843-10
 Misc : 5.00mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BHJL9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082624WMA.M
 Title : VOC Analysis

Signal : TIC: VV037222.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	68	74	92	rVB	303731	320387	14.08%	1.880%
2	1.532	146	153	169	rVB	265689	307618	13.52%	1.805%
3	2.060	308	317	329	rBV	533167	763707	33.56%	4.482%
4	3.339	712	715	717	rBV4	1327	642	0.03%	0.004%
5	3.362	720	722	723	rBV2	1112	416	0.02%	0.002%
6	3.410	734	737	743	rVB6	1445	1475	0.06%	0.009%
7	3.439	743	746	748	rBV3	819	599	0.03%	0.004%
8	3.465	751	754	757	rBV4	1326	800	0.04%	0.005%
9	3.616	799	801	805	rVB4	1369	775	0.03%	0.005%
10	3.732	834	837	838	rBV3	536	299	0.01%	0.002%
11	3.738	838	839	841	rVB2	805	248	0.01%	0.001%
12	3.796	848	857	885	rBV2	108063	299897	13.18%	1.760%
13	4.076	942	944	946	rBV2	1381	648	0.03%	0.004%
14	4.162	968	971	972	rBV3	1101	660	0.03%	0.004%
15	4.243	982	996	1024	rBV	361437	921933	40.51%	5.411%
16	4.523	1081	1083	1085	rBV2	617	254	0.01%	0.001%
17	4.555	1091	1093	1095	rBV3	742	361	0.02%	0.002%
18	4.587	1099	1103	1106	rBV5	1370	1159	0.05%	0.007%
19	4.629	1115	1116	1119	rBV3	911	434	0.02%	0.003%
20	4.661	1123	1126	1129	rBV4	1141	954	0.04%	0.006%
21	4.719	1140	1144	1146	rBV4	1547	1006	0.04%	0.006%
22	4.748	1151	1153	1155	rBV2	565	281	0.01%	0.002%
23	4.806	1169	1171	1175	rVB4	933	580	0.03%	0.003%
24	4.831	1175	1179	1182	rBV6	1047	903	0.04%	0.005%
25	4.857	1182	1187	1190	rBV6	1414	962	0.04%	0.006%
26	4.950	1200	1216	1246	rBV2	891086	2275960	100.00%	13.357%
27	5.420	1359	1362	1367	rBV7	1757	1215	0.05%	0.007%
28	5.529	1385	1396	1426	rBV	721040	1483293	65.17%	8.705%
29	5.905	1507	1513	1525	rBV4	21726	51304	2.25%	0.301%
30	5.982	1528	1537	1564	rVB	508995	1064335	46.76%	6.246%
31	6.577	1719	1722	1725	rBV4	1588	969	0.04%	0.006%
32	6.725	1765	1768	1770	rBV5	1589	1012	0.04%	0.006%
33	6.818	1789	1797	1799	rBV8	1012	1438	0.06%	0.008%
34	6.908	1815	1825	1853	rBV	265983	510315	22.42%	2.995%
35	7.239	1917	1928	1952	rBV	987683	1753668	77.05%	10.292%
36	7.551	2015	2025	2053	rBV	172667	332479	14.61%	1.951%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV090624\
 Data File : VV037222.D
 Acq On : 06 Sep 2024 13:50
 Operator : SY/MD
 Sample : P3843-10
 Misc : 5.00mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BHJL9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082624WMA.M
 Title : VOC Analysis

37	7.934	2142	2144	2145	rBV	716	301	0.01%	0.002%
38	7.973	2153	2156	2157	rBV3	785	400	0.02%	0.002%
39	8.024	2164	2172	2205	rBV2	315993	696311	30.59%	4.087%
40	8.667	2367	2372	2374	rBV4	1258	1282	0.06%	0.008%
41	8.780	2396	2407	2434	rBV	1119330	1848903	81.24%	10.851%
42	9.201	2536	2538	2541	rVB4	1185	480	0.02%	0.003%
43	9.304	2569	2570	2572	rVB2	698	208	0.01%	0.001%
44	9.326	2574	2577	2580	rVV5	1174	766	0.03%	0.004%
45	9.358	2585	2587	2589	rVV3	1147	510	0.02%	0.003%
46	9.378	2590	2593	2598	rVV5	1041	1093	0.05%	0.006%
47	9.400	2598	2600	2602	rVV2	1146	622	0.03%	0.004%
48	9.423	2605	2607	2609	rVB3	671	250	0.01%	0.001%
49	9.448	2611	2615	2617	rBV3	937	512	0.02%	0.003%
50	9.474	2621	2623	2626	rBV3	488	237	0.01%	0.001%
51	9.709	2692	2696	2697	rBV4	1023	691	0.03%	0.004%
52	9.770	2712	2715	2716	rBV3	918	575	0.03%	0.003%
53	9.837	2734	2736	2740	rVB4	404	243	0.01%	0.001%
54	9.860	2740	2743	2748	rBV6	1435	1417	0.06%	0.008%
55	9.882	2748	2750	2752	rBV2	700	323	0.01%	0.002%
56	9.915	2757	2760	2763	rBV4	981	524	0.02%	0.003%
57	9.931	2763	2765	2767	rVB3	645	216	0.01%	0.001%
58	9.960	2770	2774	2777	rBV5	819	606	0.03%	0.004%
59	10.011	2788	2790	2794	rVB4	629	479	0.02%	0.003%
60	10.091	2813	2815	2816	rBV	661	325	0.01%	0.002%
61	10.146	2821	2832	2849	rVV	580733	924618	40.63%	5.426%
62	10.426	2916	2919	2925	rBV7	1060	879	0.04%	0.005%
63	10.455	2925	2928	2931	rBV4	924	729	0.03%	0.004%
64	10.481	2934	2936	2940	rVB4	717	487	0.02%	0.003%
65	10.506	2940	2944	2947	rBV5	1284	1114	0.05%	0.007%
66	10.519	2947	2948	2951	rBV3	909	355	0.02%	0.002%
67	10.564	2960	2962	2965	rVB2	729	331	0.01%	0.002%
68	10.583	2965	2968	2969	rBV3	804	554	0.02%	0.003%
69	10.632	2980	2983	2986	rVB5	1336	837	0.04%	0.005%
70	10.648	2986	2988	2991	rVB3	544	286	0.01%	0.002%
71	10.664	2991	2993	2995	rBV3	936	457	0.02%	0.003%
72	10.686	2998	3000	3002	rBV3	919	495	0.02%	0.003%
73	10.699	3002	3004	3007	rVB4	655	385	0.02%	0.002%
74	10.715	3007	3009	3012	rBV4	894	652	0.03%	0.004%
75	10.763	3020	3024	3026	rBV4	904	650	0.03%	0.004%
76	10.789	3030	3032	3038	rVB7	1578	984	0.04%	0.006%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV090624\
 Data File : VV037222.D
 Acq On : 06 Sep 2024 13:50
 Operator : SY/MD
 Sample : P3843-10
 Misc : 5.00mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BHJL9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082624WMA.M
 Title : VOC Analysis

77	10.841	3046	3048	3049	rVB2	636	222	0.01%	0.001%
78	10.863	3053	3055	3058	rVB4	844	335	0.01%	0.002%
79	10.882	3058	3061	3063	rVB4	828	503	0.02%	0.003%
80	10.899	3063	3066	3067	rBV3	717	351	0.02%	0.002%
81	10.953	3078	3083	3085	rBV5	1216	1009	0.04%	0.006%
82	10.992	3091	3095	3096	rBV2	1037	691	0.03%	0.004%
83	11.034	3105	3108	3112	rVB4	1333	1087	0.05%	0.006%
84	11.059	3112	3116	3117	rBV3	621	439	0.02%	0.003%
85	11.095	3125	3127	3129	rBV3	1014	496	0.02%	0.003%
86	11.178	3142	3153	3186	rBV	1108728	1778252	78.13%	10.436%
87	11.490	3242	3250	3258	rBV4	17120	30365	1.33%	0.178%
88	11.554	3260	3270	3296	rVB	1018862	1623289	71.32%	9.527%
89	12.017	3411	3414	3416	rBV3	1325	852	0.04%	0.005%
90	12.297	3498	3501	3506	rBV7	1505	1117	0.05%	0.007%
91	12.349	3515	3517	3519	rBV3	1206	575	0.03%	0.003%
92	12.474	3554	3556	3558	rBV3	930	403	0.02%	0.002%
93	12.490	3558	3561	3562	rVV3	885	323	0.01%	0.002%
94	12.625	3601	3603	3606	rBV3	770	454	0.02%	0.003%
95	12.976	3710	3712	3713	rBV3	747	281	0.01%	0.002%
96	13.136	3758	3762	3767	rVB5	997	980	0.04%	0.006%
97	13.162	3768	3770	3771	rBV	662	212	0.01%	0.001%
98	13.210	3780	3785	3787	rBV6	1722	1586	0.07%	0.009%
99	13.644	3918	3920	3926	rVB6	1280	955	0.04%	0.006%
100	14.082	4054	4056	4058	rBV4	914	316	0.01%	0.002%




Sum of corrected areas: 17039166

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV090624\
Data File : VV037222.D
Acq On : 06 Sep 2024 13:50
Operator : SY/MD
Sample : P3843-10
Misc : 5.00mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BHJL9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

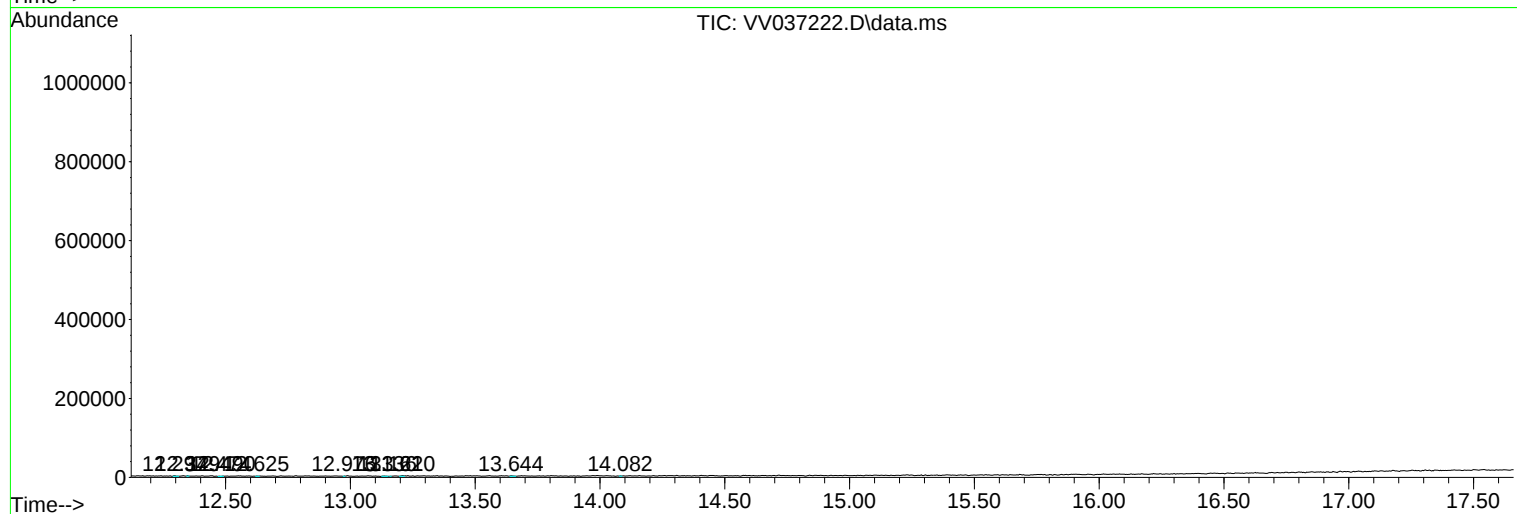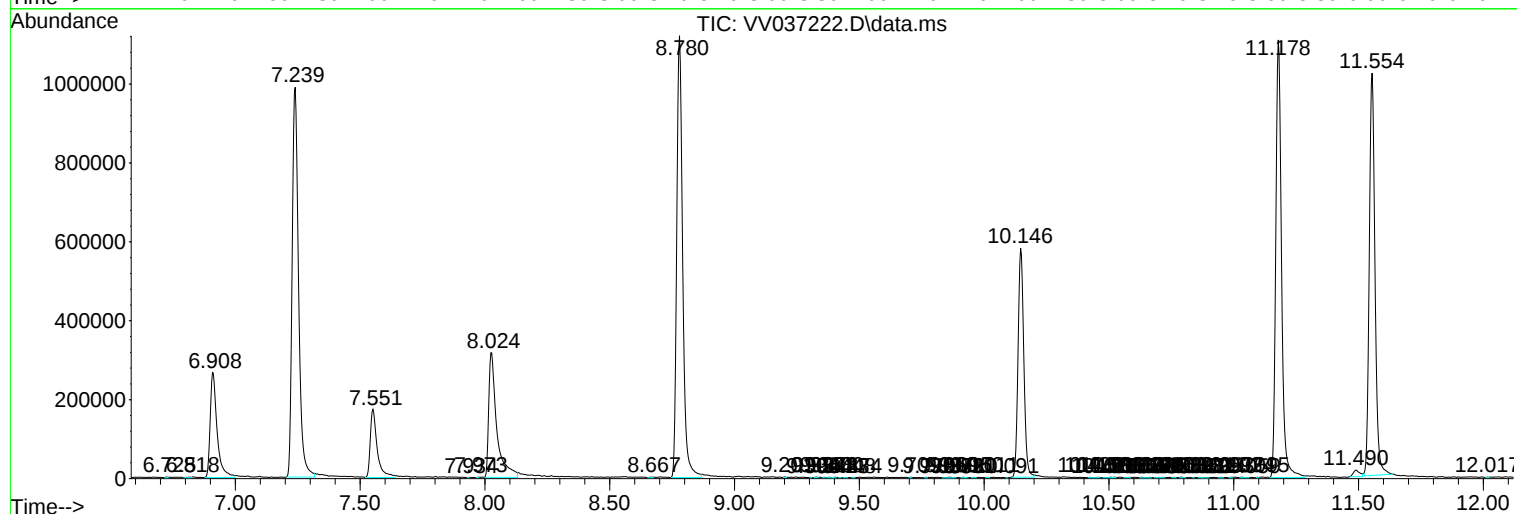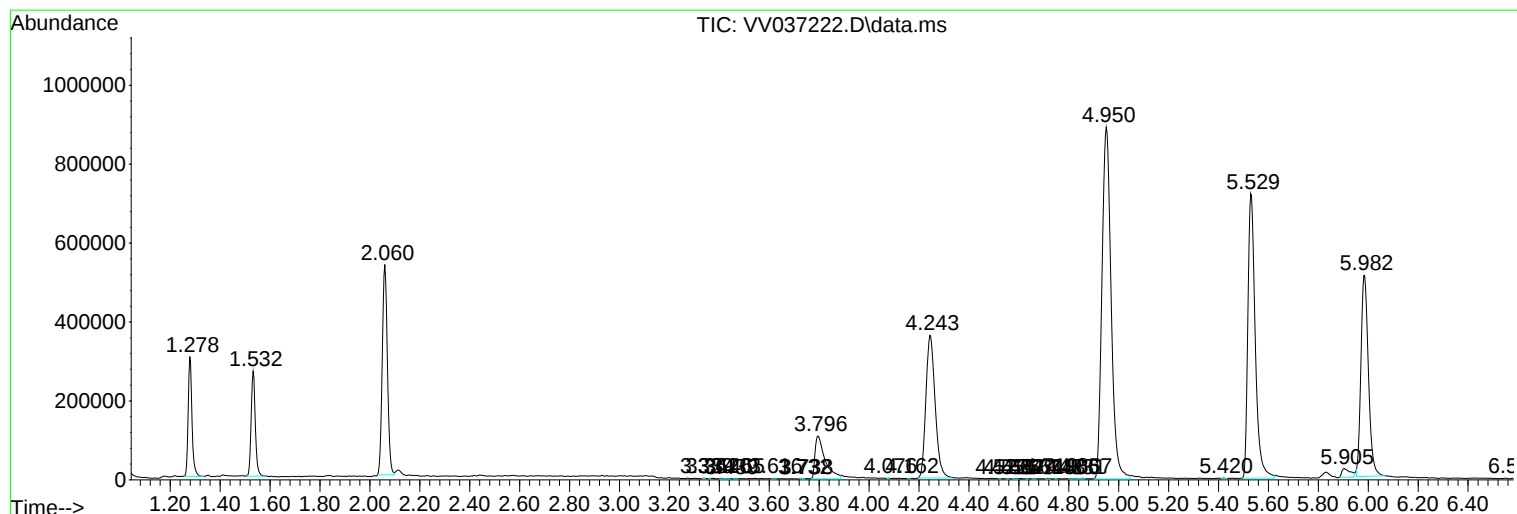

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV090624\
Data File : VV037222.D
Acq On : 06 Sep 2024 13:50
Operator : SY/MD
Sample : P3843-10
Misc : 5.00mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BHJL9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV090624\
Data File : VV037222.D
Acq On : 06 Sep 2024 13:50
Operator : SY/MD
Sample : P3843-10
Misc : 5.00mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BHJL9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------