

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV090624\
 Data File : VV037223.D
 Acq On : 06 Sep 2024 14:12
 Operator : SY/MD
 Sample : P3843-11
 Misc : 5.00mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BHJM3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082624WMA.M

Title : VOC Analysis

Signal : TIC: VV037223.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.111	18	22	32	rVB	16972	18677	0.82%	0.109%
2	1.185	37	45	51	rBV3	20565	27238	1.19%	0.158%
3	1.278	67	74	89	rBV	289437	312162	13.68%	1.815%
4	1.532	146	153	169	rVB	255576	301293	13.21%	1.752%
5	2.060	308	317	327	rBV	526460	747798	32.78%	4.348%
6	3.262	686	691	692	rBV5	1901	1414	0.06%	0.008%
7	3.394	730	732	734	rVB3	1086	440	0.02%	0.003%
8	3.471	753	756	757	rBV3	823	397	0.02%	0.002%
9	3.526	770	773	776	rBV5	1062	824	0.04%	0.005%
10	3.609	790	799	803	rBV9	1439	1829	0.08%	0.011%
11	3.635	803	807	811	rVB6	1010	886	0.04%	0.005%
12	3.687	820	823	829	rVV8	1319	1150	0.05%	0.007%
13	3.732	833	837	842	rBV6	1286	1353	0.06%	0.008%
14	3.796	848	857	887	rBV	113381	316212	13.86%	1.839%
15	4.137	959	963	965	rBV5	1386	1081	0.05%	0.006%
16	4.246	981	997	1028	rBV	371091	999114	43.80%	5.809%
17	4.523	1080	1083	1089	rVB5	1403	1499	0.07%	0.009%
18	4.638	1117	1119	1123	rBV4	779	408	0.02%	0.002%
19	4.670	1123	1129	1132	rBV7	1590	1484	0.07%	0.009%
20	4.860	1182	1188	1190	rBV5	1154	1325	0.06%	0.008%
21	4.950	1200	1216	1249	rBV2	896001	2281241	100.00%	13.264%
22	5.432	1362	1366	1368	rBV5	1506	1051	0.05%	0.006%
23	5.455	1371	1373	1376	rBV4	718	359	0.02%	0.002%
24	5.529	1385	1396	1426	rBV	701632	1451284	63.62%	8.438%
25	5.828	1480	1489	1504	rVB6	13976	30525	1.34%	0.177%
26	5.899	1506	1511	1524	rBV2	27055	59637	2.61%	0.347%
27	5.982	1527	1537	1562	rVB	515428	1073965	47.08%	6.244%
28	6.847	1804	1806	1809	rBV2	1135	758	0.03%	0.004%
29	6.908	1813	1825	1859	rBV	265629	518289	22.72%	3.013%
30	7.239	1914	1928	1965	rBV	988238	1782291	78.13%	10.363%
31	7.551	2016	2025	2051	rBV	170074	318429	13.96%	1.851%
32	7.828	2109	2111	2116	rVB5	1378	872	0.04%	0.005%
33	7.918	2137	2139	2141	rBV2	1245	605	0.03%	0.004%
34	7.956	2149	2151	2153	rVB3	877	318	0.01%	0.002%
35	7.973	2154	2156	2158	rBV2	1050	530	0.02%	0.003%
36	8.024	2163	2172	2210	rBV	335211	723994	31.74%	4.209%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV090624\
 Data File : VV037223.D
 Acq On : 06 Sep 2024 14:12
 Operator : SY/MD
 Sample : P3843-11
 Misc : 5.00mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BHJM3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082624WMA.M
 Title : VOC Analysis

37	8.709	2383	2385	2388	rBV3	770	408	0.02%	0.002%
38	8.780	2395	2407	2436	rBV	1106274	1818314	79.71%	10.572%
39	9.297	2565	2568	2569	rBV2	775	311	0.01%	0.002%
40	9.407	2597	2602	2603	rBV3	968	761	0.03%	0.004%
41	9.445	2611	2614	2615	rBV2	1078	556	0.02%	0.003%
42	9.471	2621	2622	2624	rBV	893	424	0.02%	0.002%
43	9.558	2646	2649	2653	rBV5	1630	1380	0.06%	0.008%
44	9.596	2657	2661	2664	rBV3	864	637	0.03%	0.004%
45	9.644	2671	2676	2677	rBV4	1712	1463	0.06%	0.009%
46	9.683	2686	2688	2691	rVB2	1192	719	0.03%	0.004%
47	9.747	2702	2708	2709	rBV5	977	755	0.03%	0.004%
48	9.763	2709	2713	2716	rVB6	1133	978	0.04%	0.006%
49	9.786	2716	2720	2723	rBV5	957	1007	0.04%	0.006%
50	9.850	2737	2740	2746	rVB6	841	855	0.04%	0.005%
51	9.889	2748	2752	2753	rBV4	950	705	0.03%	0.004%
52	9.963	2770	2775	2778	rVB7	973	922	0.04%	0.005%
53	9.985	2780	2782	2783	rBV3	789	436	0.02%	0.003%
54	10.040	2797	2799	2802	rBV3	1080	769	0.03%	0.004%
55	10.088	2810	2814	2818	rBV5	865	854	0.04%	0.005%
56	10.146	2818	2832	2855	rBV	592316	952764	41.77%	5.540%
57	10.410	2913	2914	2917	rBV2	842	475	0.02%	0.003%
58	10.461	2927	2930	2932	rBV4	1171	769	0.03%	0.004%
59	10.487	2935	2938	2939	rBV3	905	489	0.02%	0.003%
60	10.529	2948	2951	2955	rBV6	1764	1323	0.06%	0.008%
61	10.648	2982	2988	2990	rBV5	926	765	0.03%	0.004%
62	10.664	2991	2993	3001	rVB9	1570	1642	0.07%	0.010%
63	10.696	3001	3003	3006	rVB4	697	396	0.02%	0.002%
64	10.725	3009	3012	3013	rBV2	716	366	0.02%	0.002%
65	10.773	3025	3027	3029	rBV3	1379	732	0.03%	0.004%
66	10.821	3040	3042	3044	rBV2	796	422	0.02%	0.002%
67	10.857	3050	3053	3055	rVB2	1377	826	0.04%	0.005%
68	10.873	3055	3058	3061	rBV4	1250	726	0.03%	0.004%
69	10.895	3063	3065	3068	rVB4	930	529	0.02%	0.003%
70	10.934	3072	3077	3079	rBV5	758	739	0.03%	0.004%
71	10.985	3090	3093	3097	rVB6	1326	927	0.04%	0.005%
72	11.050	3109	3113	3116	rVB6	1062	849	0.04%	0.005%
73	11.085	3122	3124	3130	rBV6	730	589	0.03%	0.003%
74	11.111	3130	3132	3135	rBV2	883	627	0.03%	0.004%
75	11.178	3142	3153	3183	rBV	1074062	1732961	75.97%	10.076%
76	11.490	3244	3250	3259	rBV4	11190	23513	1.03%	0.137%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV090624\
 Data File : VV037223.D
 Acq On : 06 Sep 2024 14:12
 Operator : SY/MD
 Sample : P3843-11
 Misc : 5.00mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BHJM3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082624WMA.M
 Title : VOC Analysis

77	11.554	3260	3270	3300	rVB	1017507	1645800	72.14%	9.569%
78	12.024	3414	3416	3420	rVB4	1395	836	0.04%	0.005%
79	12.107	3440	3442	3444	rBV2	755	446	0.02%	0.003%
80	12.130	3447	3449	3451	rBV2	949	436	0.02%	0.003%
81	12.159	3456	3458	3460	rBV3	1119	588	0.03%	0.003%
82	12.278	3492	3495	3497	rBV4	1547	832	0.04%	0.005%
83	12.509	3565	3567	3571	rBV4	788	659	0.03%	0.004%
84	12.580	3587	3589	3592	rBV4	1019	563	0.02%	0.003%
85	12.702	3625	3627	3629	rVB3	828	381	0.02%	0.002%
86	12.718	3630	3632	3637	rBV6	652	666	0.03%	0.004%
87	12.812	3658	3661	3662	rBV2	1139	639	0.03%	0.004%
88	12.898	3686	3688	3691	rBV3	1367	853	0.04%	0.005%
89	12.914	3691	3693	3696	rVV4	737	450	0.02%	0.003%
90	13.011	3721	3723	3730	rVB5	1402	1303	0.06%	0.008%
91	13.043	3730	3733	3735	rBV3	939	760	0.03%	0.004%
92	13.201	3780	3782	3787	rBV6	1396	1047	0.05%	0.006%
93	13.365	3829	3833	3836	rBV4	1354	967	0.04%	0.006%
94	13.435	3852	3855	3856	rBV2	1147	650	0.03%	0.004%
95	13.490	3869	3872	3874	rBV3	1192	561	0.02%	0.003%
96	13.506	3874	3877	3880	rBV4	1371	882	0.04%	0.005%
97	13.586	3900	3902	3904	rBV3	1164	735	0.03%	0.004%
98	14.027	4037	4039	4045	rBV7	1369	982	0.04%	0.006%
99	14.107	4061	4064	4068	rBV5	1761	1209	0.05%	0.007%
100	14.194	4089	4091	4097	rVB7	1618	1507	0.07%	0.009%




Sum of corrected areas: 17199167

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV090624\
Data File : VV037223.D
Acq On : 06 Sep 2024 14:12
Operator : SY/MD
Sample : P3843-11
Misc : 5.00mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BHJM3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

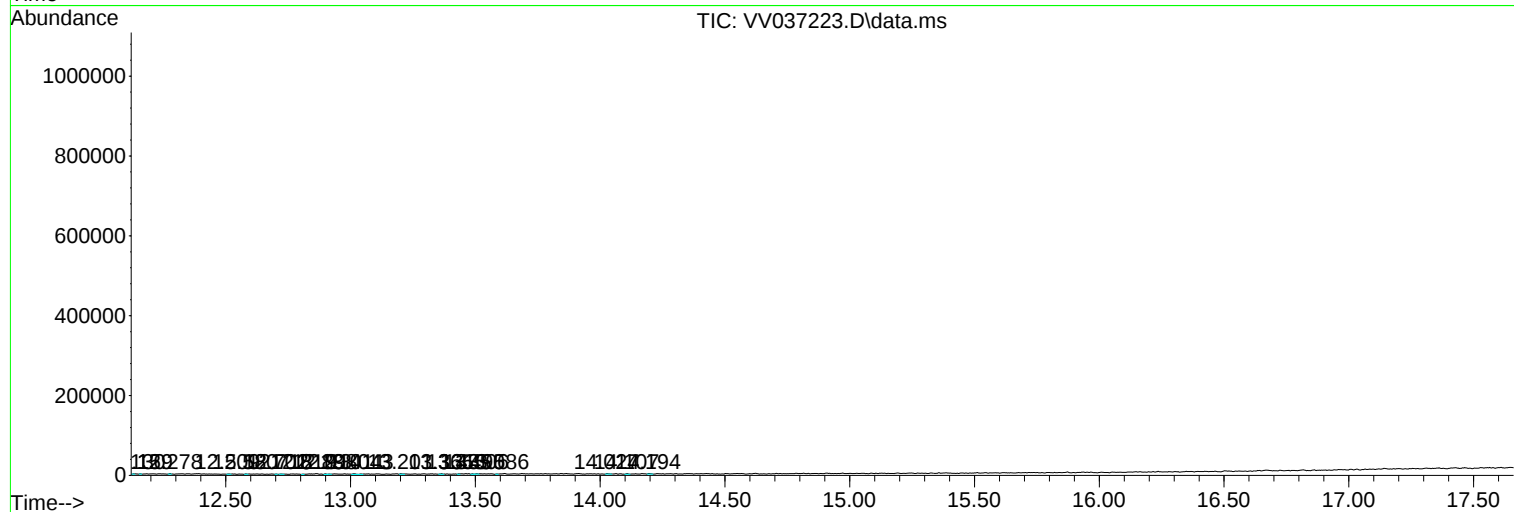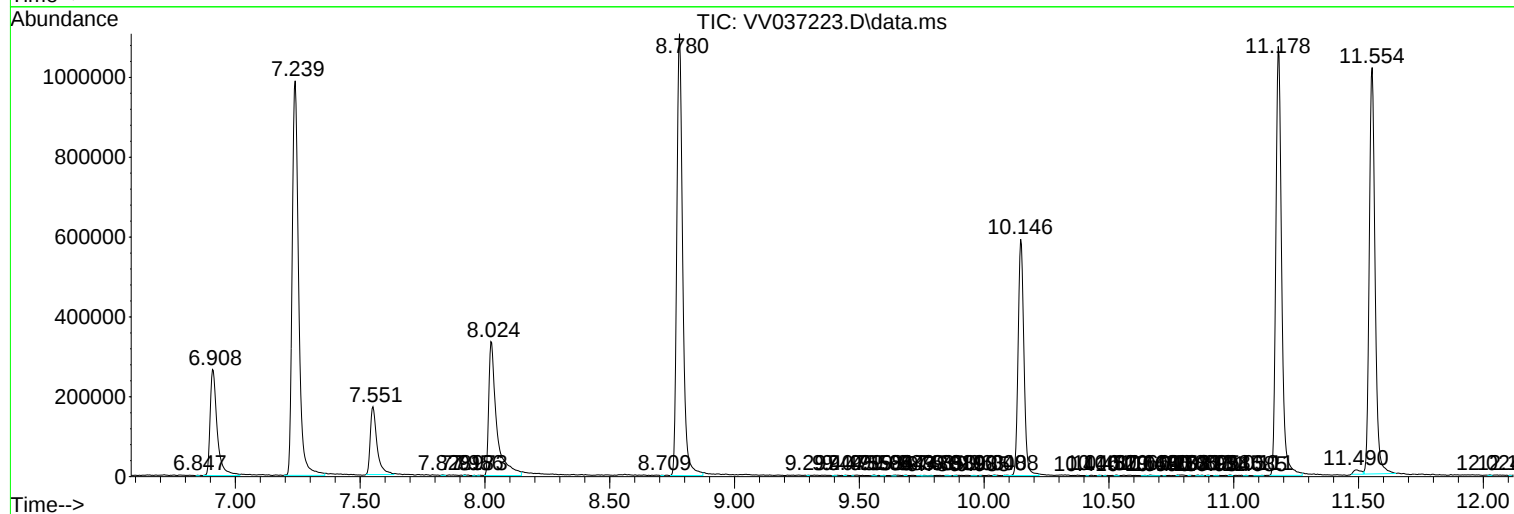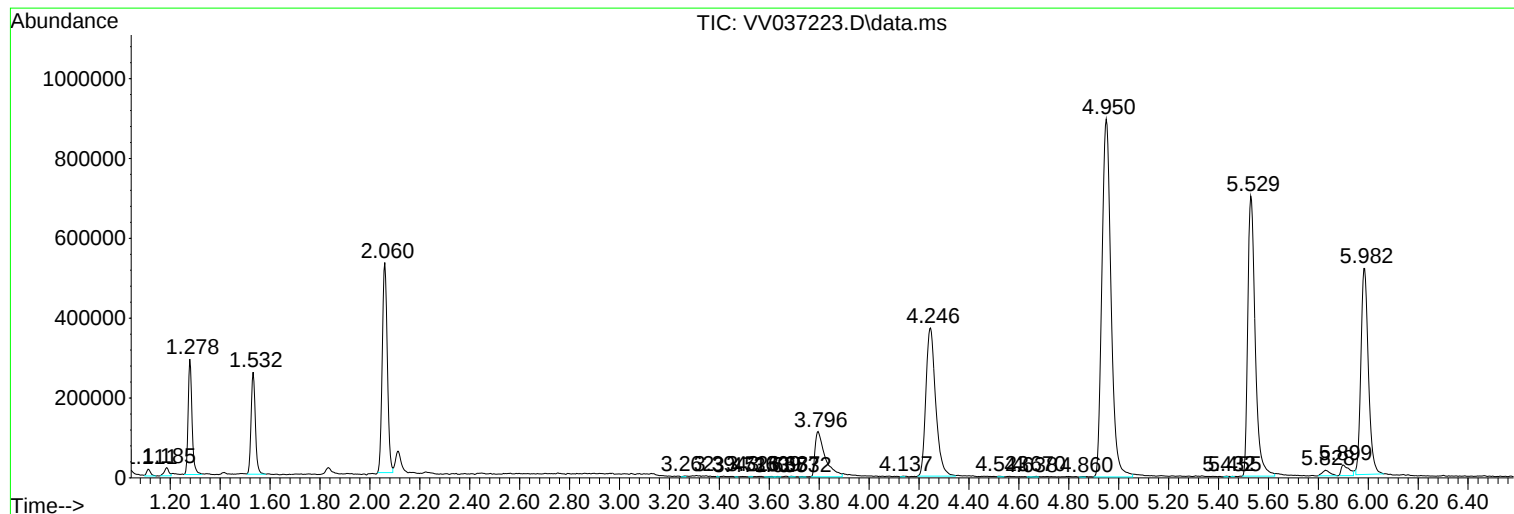

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV090624\
Data File : VV037223.D
Acq On : 06 Sep 2024 14:12
Operator : SY/MD
Sample : P3843-11
Misc : 5.00mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BHJM3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV090624\
Data File : VV037223.D
Acq On : 06 Sep 2024 14:12
Operator : SY/MD
Sample : P3843-11
Misc : 5.00mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BHJM3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------