

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV090624\
 Data File : VV037224.D
 Acq On : 06 Sep 2024 14:33
 Operator : SY/MD
 Sample : P3843-13
 Misc : 5.00mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BHJM4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082624WMA.M

Title : VOC Analysis

Signal : TIC: VV037224.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	68	74	89	rVB	301350	321455	13.93%	1.864%
2	1.532	146	153	169	rVB	267895	318824	13.81%	1.849%
3	2.060	308	317	329	rBV	544166	776287	33.63%	4.501%
4	3.413	736	738	740	rVB	1265	448	0.02%	0.003%
5	3.429	740	743	746	rBV5	711	504	0.02%	0.003%
6	3.535	774	776	779	rBV2	1160	557	0.02%	0.003%
7	3.600	793	796	799	rBV3	1090	730	0.03%	0.004%
8	3.616	799	801	803	rVV3	824	487	0.02%	0.003%
9	3.629	803	805	806	rVV2	718	282	0.01%	0.002%
10	3.638	806	808	811	rVB3	1113	611	0.03%	0.004%
11	3.712	828	831	834	rBV5	750	520	0.02%	0.003%
12	3.728	834	836	838	rVB3	695	313	0.01%	0.002%
13	3.741	838	840	842	rVB2	192	63	0.00%	0.000%
14	3.761	842	846	848	rBV5	814	644	0.03%	0.004%
15	3.793	848	856	886	rBV	109914	308598	13.37%	1.789%
16	4.246	981	997	1024	rBV	372163	1012027	43.85%	5.868%
17	4.471	1065	1067	1070	rBV4	895	402	0.02%	0.002%
18	4.542	1086	1089	1091	rBV4	1239	998	0.04%	0.006%
19	4.574	1096	1099	1102	rVB4	1198	839	0.04%	0.005%
20	4.596	1102	1106	1107	rBV4	631	356	0.02%	0.002%
21	4.638	1116	1119	1121	rBV3	1447	862	0.04%	0.005%
22	4.741	1147	1151	1154	rVB3	1048	774	0.03%	0.004%
23	4.770	1154	1160	1163	rBV5	1557	1483	0.06%	0.009%
24	4.950	1197	1216	1245	rBV2	910604	2308114	100.00%	13.384%
25	5.471	1375	1378	1380	rBV4	1327	921	0.04%	0.005%
26	5.529	1385	1396	1433	rVV	715866	1490377	64.57%	8.642%
27	5.912	1509	1515	1519	rBV5	13290	19410	0.84%	0.113%
28	5.982	1527	1537	1565	rVB	526698	1080042	46.79%	6.263%
29	6.584	1722	1724	1728	rVB4	1086	638	0.03%	0.004%
30	6.844	1803	1805	1809	rVB3	1029	559	0.02%	0.003%
31	6.860	1809	1810	1813	rBV2	709	450	0.02%	0.003%
32	6.908	1816	1825	1851	rBV	268641	504332	21.85%	2.924%
33	7.156	1898	1902	1903	rBV3	1423	963	0.04%	0.006%
34	7.239	1917	1928	1959	rBV	1004906	1785999	77.38%	10.356%
35	7.551	2016	2025	2055	rBV	171533	327820	14.20%	1.901%
36	8.024	2164	2172	2209	rBV2	330530	721168	31.24%	4.182%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV090624\
 Data File : VV037224.D
 Acq On : 06 Sep 2024 14:33
 Operator : SY/MD
 Sample : P3843-13
 Misc : 5.00mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BHJM4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082624WMA.M
 Title : VOC Analysis

37	8.693	2377	2380	2381	rBV2	1061	569	0.02%	0.003%
38	8.780	2396	2407	2436	rBV	1121692	1834456	79.48%	10.637%
39	9.384	2592	2595	2598	rBV4	928	676	0.03%	0.004%
40	9.416	2601	2605	2607	rBV4	890	589	0.03%	0.003%
41	9.516	2634	2636	2638	rVB3	1108	483	0.02%	0.003%
42	9.529	2638	2640	2642	rBV2	1228	629	0.03%	0.004%
43	9.554	2646	2648	2649	rBV3	826	302	0.01%	0.002%
44	9.699	2689	2693	2697	rBV6	1175	866	0.04%	0.005%
45	9.834	2733	2735	2738	rBV4	810	490	0.02%	0.003%
46	9.854	2738	2741	2743	rBV3	1216	670	0.03%	0.004%
47	9.915	2759	2760	2761	rBV	785	293	0.01%	0.002%
48	9.960	2772	2774	2775	rBV	466	124	0.01%	0.001%
49	10.040	2795	2799	2803	rBV6	1587	1328	0.06%	0.008%
50	10.059	2803	2805	2806	rBV3	607	168	0.01%	0.001%
51	10.146	2821	2832	2855	rBV	594312	956620	41.45%	5.547%
52	10.423	2917	2918	2920	rBV	671	292	0.01%	0.002%
53	10.468	2931	2932	2935	rVB3	1402	558	0.02%	0.003%
54	10.599	2969	2973	2976	rVV5	1378	796	0.03%	0.005%
55	10.622	2979	2980	2984	rVB3	909	264	0.01%	0.002%
56	10.641	2984	2986	2987	rBV2	829	255	0.01%	0.001%
57	10.677	2995	2997	2999	rBV3	819	355	0.02%	0.002%
58	10.689	2999	3001	3004	rBV3	899	469	0.02%	0.003%
59	10.706	3004	3006	3008	rVV3	834	454	0.02%	0.003%
60	10.731	3012	3014	3017	rBV4	959	674	0.03%	0.004%
61	10.747	3017	3019	3021	rBV2	1017	434	0.02%	0.003%
62	10.850	3048	3051	3054	rBV4	1422	924	0.04%	0.005%
63	10.902	3063	3067	3071	rVB6	2032	1397	0.06%	0.008%
64	10.995	3093	3096	3097	rBV3	808	362	0.02%	0.002%
65	11.072	3118	3120	3123	rVB3	816	348	0.02%	0.002%
66	11.091	3123	3126	3130	rBV4	973	625	0.03%	0.004%
67	11.120	3133	3135	3136	rBV2	765	350	0.02%	0.002%
68	11.178	3142	3153	3185	rBV	1090423	1763512	76.40%	10.226%
69	11.503	3243	3254	3259	rBV6	8923	18801	0.81%	0.109%
70	11.554	3260	3270	3301	rVB	1010985	1662080	72.01%	9.638%
71	12.249	3483	3486	3487	rBV3	983	500	0.02%	0.003%
72	12.294	3497	3500	3501	rBV2	1252	624	0.03%	0.004%
73	12.574	3584	3587	3591	rBV4	1472	1432	0.06%	0.008%
74	13.268	3801	3803	3806	rBV2	1073	769	0.03%	0.004%
75	13.667	3922	3927	3929	rBV4	1642	1196	0.05%	0.007%
76	14.059	4047	4049	4051	rBV2	1009	641	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV090624\
Data File : VV037224.D
Acq On : 06 Sep 2024 14:33
Operator : SY/MD
Sample : P3843-13
Misc : 5.00mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BHJM4

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082624WMA.M
Title : VOC Analysis




Sum of corrected areas: 17245232

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV090624\
Data File : VV037224.D
Acq On : 06 Sep 2024 14:33
Operator : SY/MD
Sample : P3843-13
Misc : 5.00mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BHJM4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

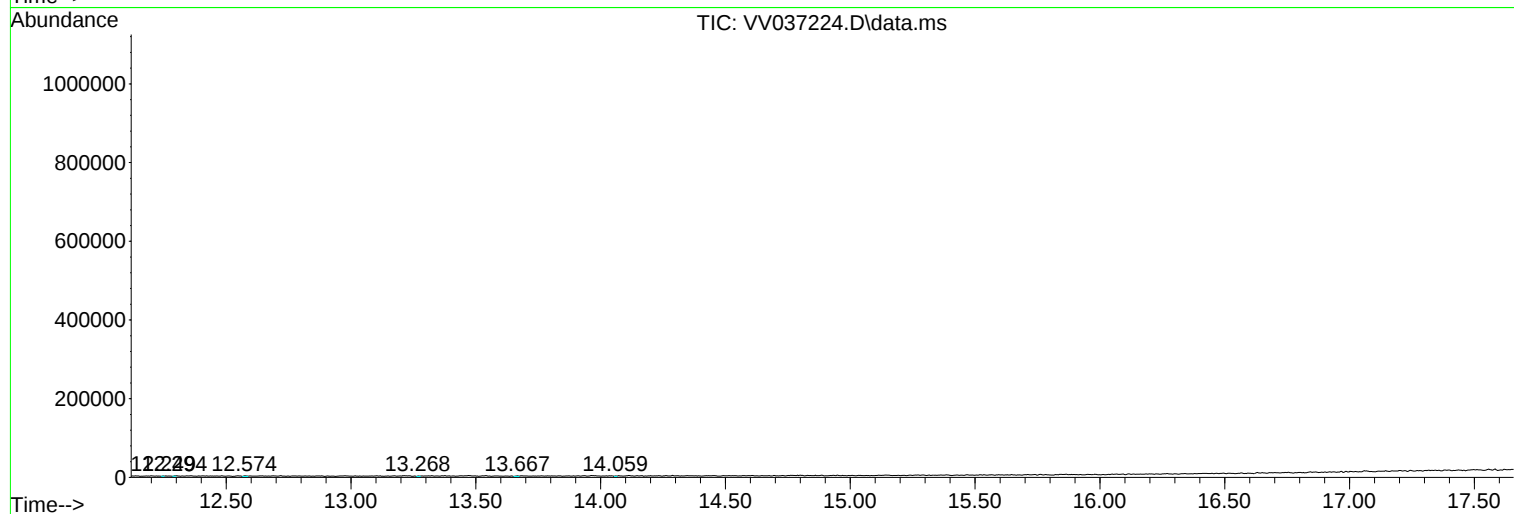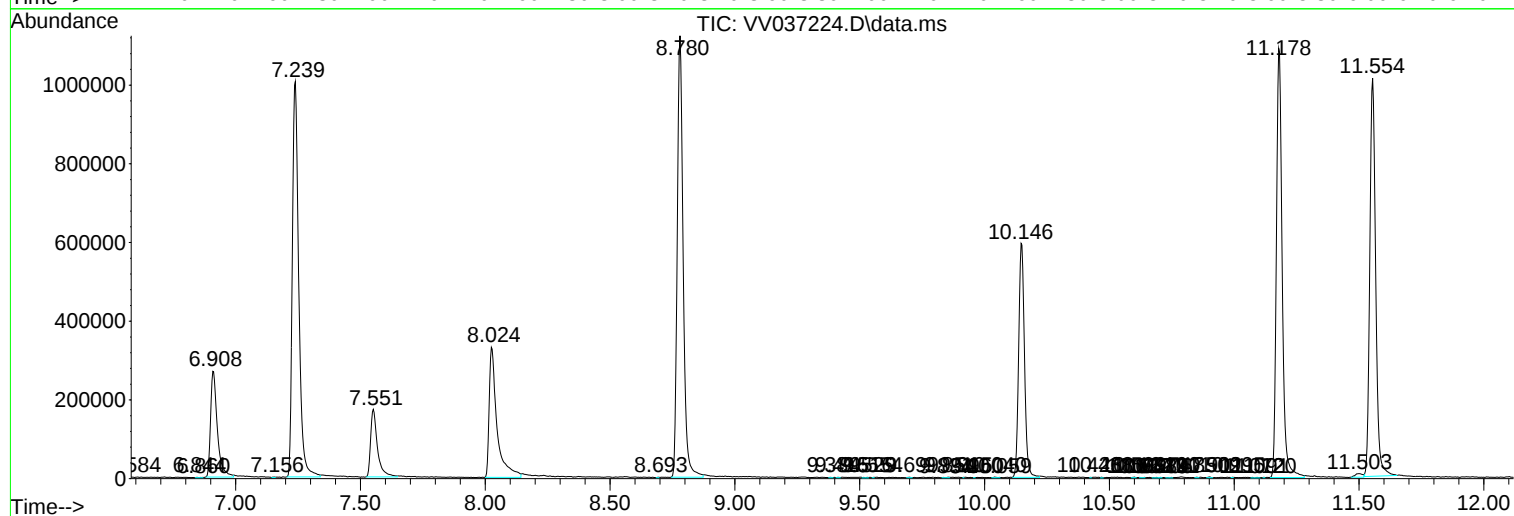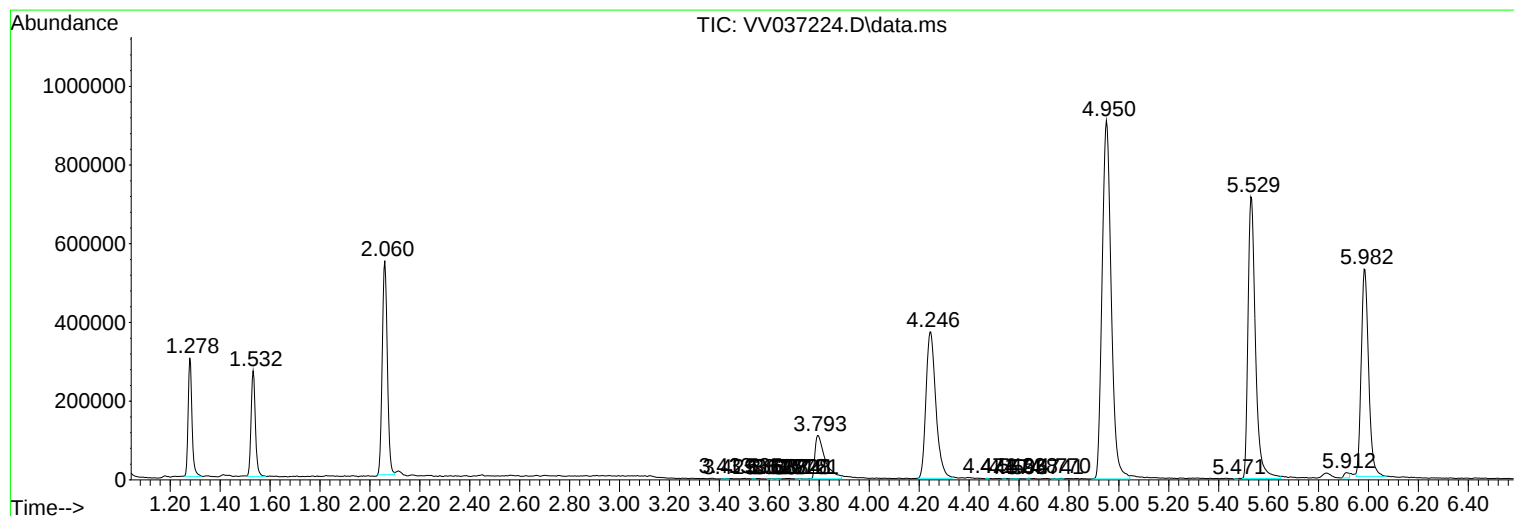

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV090624\
Data File : VV037224.D
Acq On : 06 Sep 2024 14:33
Operator : SY/MD
Sample : P3843-13
Misc : 5.00mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BHJM4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV090624\
Data File : VV037224.D
Acq On : 06 Sep 2024 14:33
Operator : SY/MD
Sample : P3843-13
Misc : 5.00mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BHJM4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------