

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV090624\
 Data File : VV037226.D
 Acq On : 06 Sep 2024 15:16
 Operator : SY/MD
 Sample : P3843-06
 Misc : 5.00mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082624WMA.M

Title : VOC Analysis

Signal : TIC: VV037226.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	68	74	90	rVB	271881	291250	13.75%	1.903%
2	1.532	146	153	168	rVB	242620	285072	13.45%	1.862%
3	2.060	308	317	339	rVB	489598	714346	33.71%	4.667%
4	3.523	769	772	775	rBV3	1025	759	0.04%	0.005%
5	3.571	785	787	789	rBV3	947	554	0.03%	0.004%
6	3.600	793	796	798	rBV4	832	640	0.03%	0.004%
7	3.629	804	805	807	rVB2	829	299	0.01%	0.002%
8	3.687	821	823	827	rBV5	670	310	0.01%	0.002%
9	3.757	842	845	848	rBV7	914	682	0.03%	0.004%
10	3.796	848	857	900	rBV2	103136	303298	14.31%	1.982%
11	4.243	980	996	1024	rBV	338848	868997	41.01%	5.677%
12	4.626	1114	1115	1119	rVB4	679	368	0.02%	0.002%
13	4.693	1134	1136	1140	rBV4	1292	820	0.04%	0.005%
14	4.709	1140	1141	1143	rBV2	507	187	0.01%	0.001%
15	4.751	1152	1154	1155	rBV2	614	213	0.01%	0.001%
16	4.950	1201	1216	1247	rBV2	830656	2118912	100.00%	13.844%
17	5.529	1385	1396	1428	rBV	589555	1247813	58.89%	8.152%
18	5.986	1526	1538	1571	rBV	477050	983965	46.44%	6.429%
19	6.478	1687	1691	1694	rBV6	1334	1184	0.06%	0.008%
20	6.587	1723	1725	1730	rBV4	1635	1379	0.07%	0.009%
21	6.654	1743	1746	1747	rBV3	894	384	0.02%	0.003%
22	6.680	1752	1754	1757	rVB5	1342	725	0.03%	0.005%
23	6.712	1762	1764	1769	rVB5	1299	847	0.04%	0.006%
24	6.748	1774	1775	1777	rBV2	1113	435	0.02%	0.003%
25	6.802	1791	1792	1794	rVB2	1022	228	0.01%	0.001%
26	6.815	1794	1796	1799	rVB4	1399	808	0.04%	0.005%
27	6.838	1799	1803	1806	rBV4	1460	1175	0.06%	0.008%
28	6.912	1816	1826	1847	rBV	237297	458221	21.63%	2.994%
29	7.240	1917	1928	1960	rBV	909970	1618173	76.37%	10.572%
30	7.552	2016	2025	2048	rBV	157396	296696	14.00%	1.938%
31	7.973	2155	2156	2159	rBV2	497	224	0.01%	0.001%
32	7.989	2159	2161	2164	rBV4	1060	572	0.03%	0.004%
33	8.027	2164	2173	2213	rBV2	294336	660330	31.16%	4.314%
34	8.458	2305	2307	2310	rVB4	1312	678	0.03%	0.004%
35	8.690	2377	2379	2380	rBV2	647	218	0.01%	0.001%
36	8.780	2397	2407	2433	rBV	933693	1539043	72.63%	10.055%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV090624\
 Data File : VV037226.D
 Acq On : 06 Sep 2024 15:16
 Operator : SY/MD
 Sample : P3843-06
 Misc : 5.00mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082624WMA.M
 Title : VOC Analysis

37	9.121	2508	2513	2515	rBV5	1380	1180	0.06%	0.008%
38	9.236	2547	2549	2551	rVB3	1438	622	0.03%	0.004%
39	9.423	2605	2607	2608	rBV2	1023	428	0.02%	0.003%
40	9.445	2612	2614	2618	rBV4	957	688	0.03%	0.004%
41	9.474	2621	2623	2624	rBV2	1498	825	0.04%	0.005%
42	9.535	2640	2642	2644	rVB3	1307	467	0.02%	0.003%
43	9.584	2654	2657	2662	rVB7	1239	948	0.04%	0.006%
44	9.609	2663	2665	2667	rBV3	865	321	0.02%	0.002%
45	9.622	2667	2669	2672	rBV3	861	561	0.03%	0.004%
46	9.680	2683	2687	2688	rBV3	865	476	0.02%	0.003%
47	9.744	2705	2707	2708	rBV2	1039	351	0.02%	0.002%
48	9.870	2744	2746	2750	rBV4	622	326	0.02%	0.002%
49	9.889	2750	2752	2758	rVB6	904	586	0.03%	0.004%
50	9.937	2764	2767	2768	rBV3	1256	609	0.03%	0.004%
51	10.008	2787	2789	2792	rBV4	1071	612	0.03%	0.004%
52	10.047	2799	2801	2803	rBV4	445	193	0.01%	0.001%
53	10.104	2817	2819	2821	rVB3	803	356	0.02%	0.002%
54	10.146	2821	2832	2853	rBV	552600	884797	41.76%	5.781%
55	10.307	2880	2882	2884	rBV3	1290	794	0.04%	0.005%
56	10.336	2889	2891	2892	rBV2	919	344	0.02%	0.002%
57	10.407	2909	2913	2915	rBV4	1509	1008	0.05%	0.007%
58	10.436	2920	2922	2923	rBV	641	251	0.01%	0.002%
59	10.461	2929	2930	2933	rVB2	1364	363	0.02%	0.002%
60	10.487	2933	2938	2940	rBV4	1459	1390	0.07%	0.009%
61	10.593	2968	2971	2973	rBV4	1331	752	0.04%	0.005%
62	10.645	2983	2987	2988	rBV2	995	583	0.03%	0.004%
63	10.696	3001	3003	3007	rBV5	939	376	0.02%	0.002%
64	10.780	3028	3029	3032	rBV4	1117	701	0.03%	0.005%
65	10.899	3064	3066	3070	rVB4	1287	712	0.03%	0.005%
66	10.918	3070	3072	3074	rVB	1078	513	0.02%	0.003%
67	10.934	3074	3077	3079	rBV2	708	606	0.03%	0.004%
68	10.957	3079	3084	3091	rBV8	1613	2029	0.10%	0.013%
69	11.043	3108	3111	3112	rBV2	920	479	0.02%	0.003%
70	11.133	3129	3139	3141	rBV2	1350	1661	0.08%	0.011%
71	11.178	3141	3153	3192	rBV	903639	1475967	69.66%	9.643%
72	11.493	3245	3251	3255	rVB7	1501	1584	0.07%	0.010%
73	11.555	3259	3270	3298	rVV	949262	1512030	71.36%	9.879%
74	12.040	3417	3421	3428	rVB6	1157	1342	0.06%	0.009%
75	12.075	3428	3432	3436	rBV5	1273	884	0.04%	0.006%
76	12.310	3502	3505	3508	rVB5	1605	1025	0.05%	0.007%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV090624\
Data File : VV037226.D
Acq On : 06 Sep 2024 15:16
Operator : SY/MD
Sample : P3843-06
Misc : 5.00mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082624WMA.M

Title : VOC Analysis

77	12.506	3564	3566	3567	rBV2	888	290	0.01%	0.002%
78	12.567	3581	3585	3589	rBV4	1711	1991	0.09%	0.013%
79	12.715	3629	3631	3633	rBV3	806	481	0.02%	0.003%
80	12.834	3665	3668	3670	rBV3	1572	870	0.04%	0.006%
81	12.973	3709	3711	3714	rBV2	1228	896	0.04%	0.006%
82	13.272	3802	3804	3809	rVB5	1244	837	0.04%	0.005%
83	13.294	3809	3811	3812	rBV2	830	300	0.01%	0.002%
84	13.664	3924	3926	3932	rBV7	1396	904	0.04%	0.006%




Sum of corrected areas: 15306114

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV090624\
Data File : VV037226.D
Acq On : 06 Sep 2024 15:16
Operator : SY/MD
Sample : P3843-06
Misc : 5.00mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

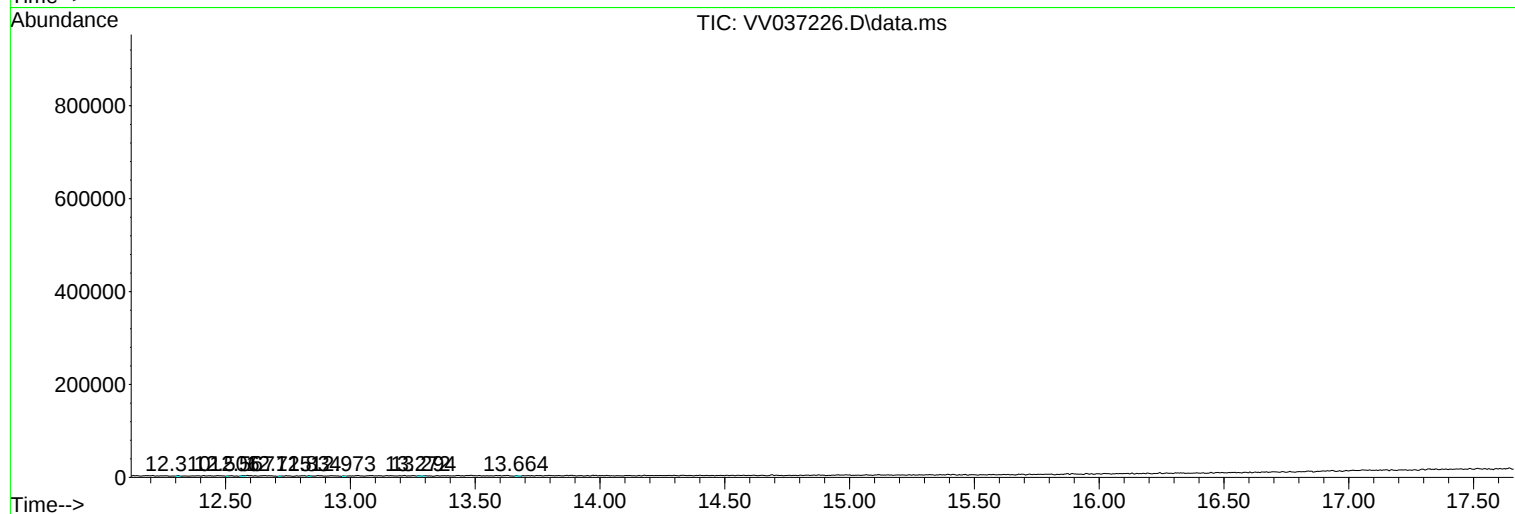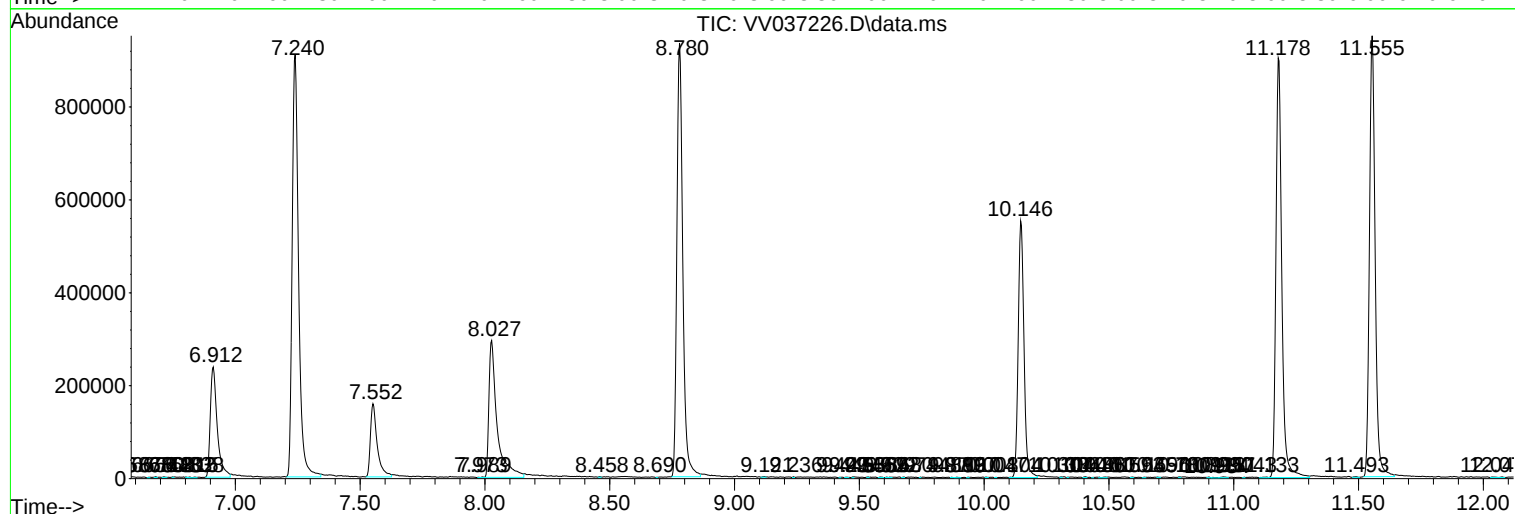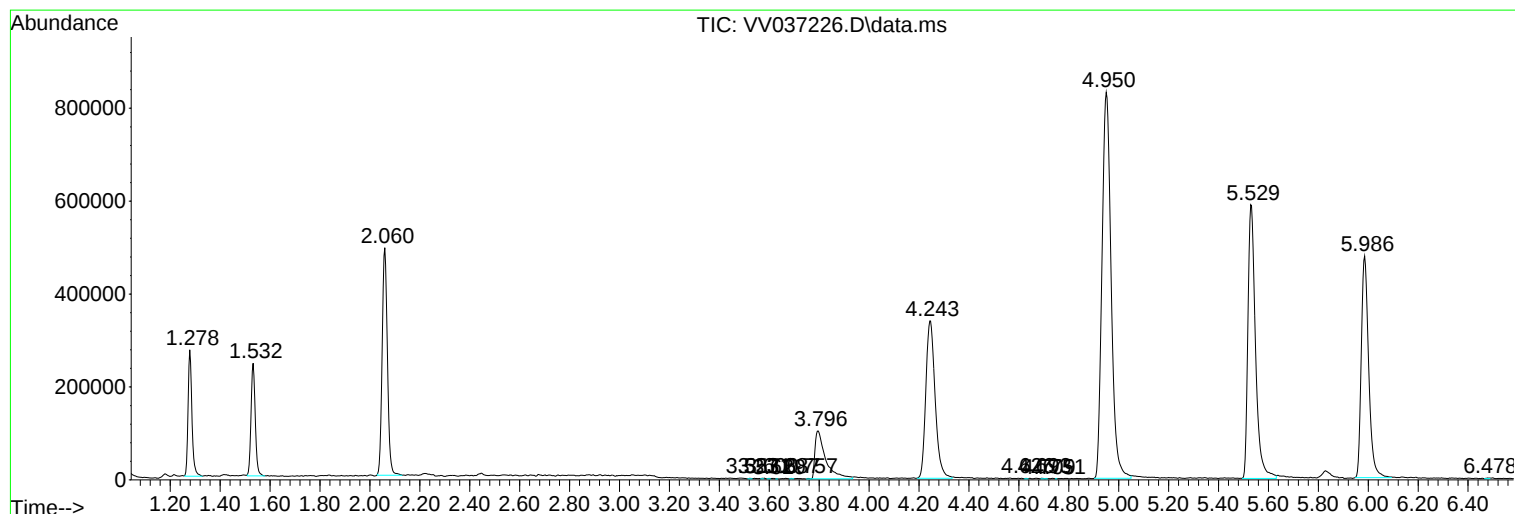

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV090624\
Data File : VV037226.D
Acq On : 06 Sep 2024 15:16
Operator : SY/MD
Sample : P3843-06
Misc : 5.00mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV090624\
Data File : VV037226.D
Acq On : 06 Sep 2024 15:16
Operator : SY/MD
Sample : P3843-06
Misc : 5.00mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc