
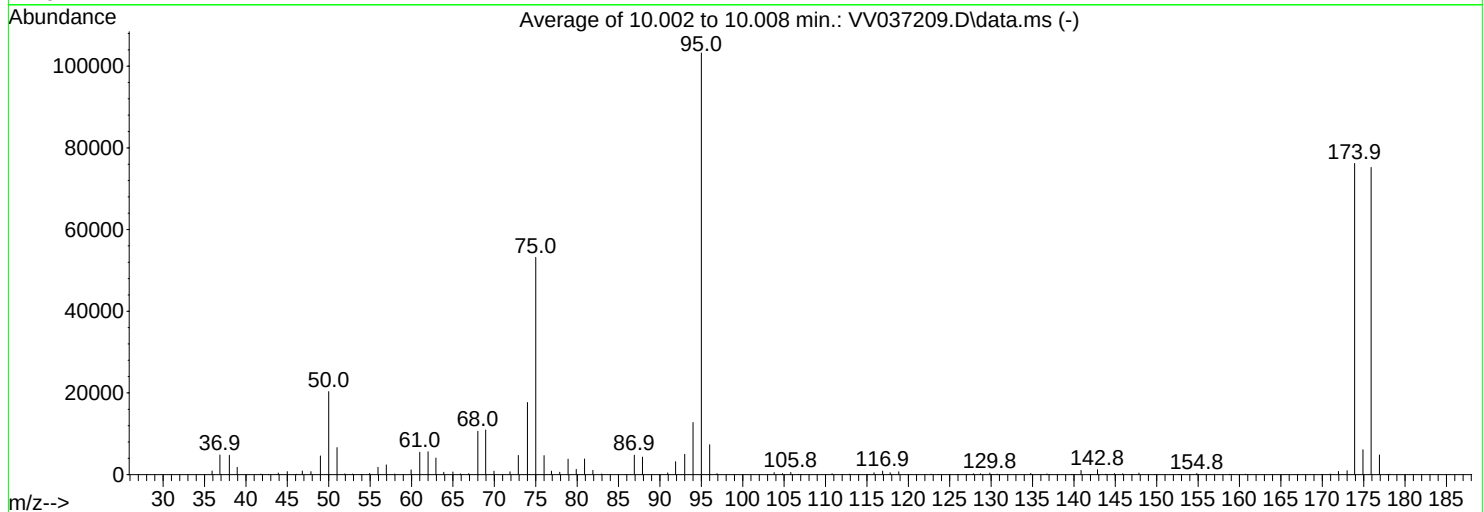


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV090624\
Data File : VV037209.D
Acq On : 06 Sep 2024 08:07
Operator : SY/MD
Sample : BFB375
Misc : 5.00mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB375

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082624WMA.M
Title : VOC Analysis
Last Update : Fri Sep 06 23:21:35 2024

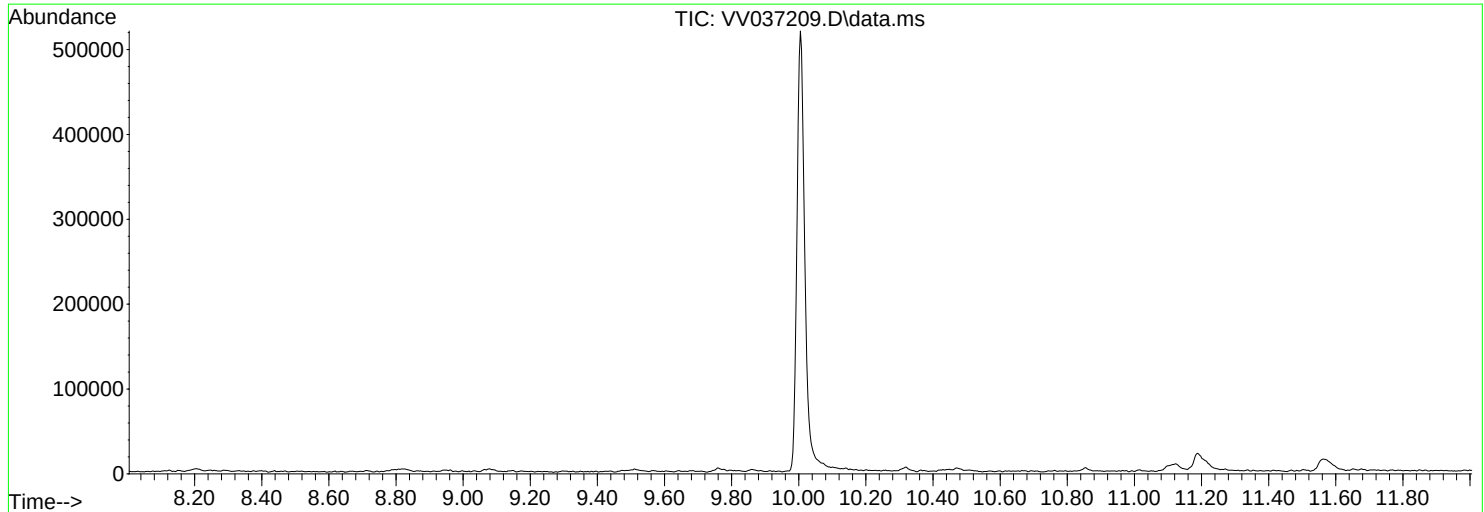

AutoFind: Scans 2787, 2788, 2789; Background Corrected with Scan 2776

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.7	20341	PASS
75	95	30	80	51.5	53176	PASS
95	95	100	100	100.0	103261	PASS
96	95	5	9	7.1	7315	PASS
173	174	0.00	2	1.3	999	PASS
174	95	50	120	73.8	76184	PASS
175	174	5	9	8.0	6127	PASS
176	174	95	105	98.7	75197	PASS
177	176	5	10	6.4	4800	PASS

m/z	Abundance
36.70	103.0
37.80	102.0
38.20	118.0
38.80	206.0
40.00	443.0
40.80	154.0
42.90	103.0
43.90	934.0
45.10	134.0
46.70	121.0
48.30	121.0
54.60	107.0
55.00	114.0
57.00	123.0
68.90	154.0
70.90	125.0
72.80	157.0
77.20	118.0
81.10	109.0
142.00	102.0

Instrument :
MSVOA_V
ClientSampleId :
BFB375

m/z	Abundance
35.90	830.0
36.90	4978.0
38.00	5061.0
39.00	2060.0
39.90	372.0
41.90	178.0
42.80	145.0
44.00	1362.0
45.00	818.0
46.20	192.0
46.80	1037.0
47.80	680.0
49.00	4386.0
50.00	20648.0
51.00	6483.0
52.00	162.0
53.00	186.0
54.90	423.0
56.00	1797.0
57.00	2420.0
57.90	123.0
59.90	1249.0
61.00	5236.0
62.00	5553.0
62.90	4224.0
63.90	640.0
65.00	662.0
65.90	185.0
67.00	232.0
68.00	10743.0
69.00	10769.0
69.90	746.0
71.90	638.0
73.00	4768.0
74.00	17424.0
75.00	52248.0
76.00	4600.0
76.90	777.0
77.90	528.0
78.90	3908.0
79.90	1378.0
80.90	3762.0
81.90	978.0
82.90	162.0
85.80	112.0
86.90	5110.0
87.90	4048.0
90.90	460.0
91.90	3081.0
93.00	4724.0
94.00	12695.0
95.00	102648.0
96.00	7137.0
96.90	268.0
103.80	527.0
104.80	252.0
105.80	527.0
106.70	133.0
107.10	105.0
110.70	231.0
112.10	124.0
112.90	114.0
115.90	453.0
116.90	834.0
117.80	471.0
118.90	781.0
122.80	104.0
127.80	279.0
128.70	189.0
129.90	405.0
130.90	127.0
134.80	296.0
136.70	247.0
140.80	1051.0
141.90	155.0
142.90	1229.0
144.90	284.0
145.90	255.0
146.90	145.0
147.80	341.0
150.00	121.0
154.90	342.0
156.90	149.0
158.80	150.0
160.80	166.0
170.90	150.0
172.00	760.0
173.00	934.0
173.90	72496.0
174.90	5935.0
175.90	69712.0
176.90	4689.0

Instrument :
MSVOA_V
ClientSampleId :
BFB375

177.80

141.0

Instrument :
MSVOA_V
ClientSampleId :
BFB375

m/z	Abundance
35.90	860.0
36.90	5186.0
38.00	5220.0
39.00	2068.0
39.90	391.0
41.80	169.0
42.70	124.0
43.90	1393.0
45.00	870.0
46.00	151.0
46.80	1038.0
47.80	759.0
49.00	4699.0
50.00	21200.0
51.00	6894.0
52.00	198.0
52.90	135.0
53.80	104.0
55.00	470.0
55.90	1901.0
56.90	2531.0
58.00	151.0
60.00	1206.0
61.00	5778.0
62.00	5812.0
62.90	4165.0
63.90	624.0
65.00	671.0
65.90	204.0
66.90	254.0
68.00	10849.0
69.00	11573.0
70.00	917.0
71.90	746.0
73.00	5031.0
74.00	18184.0
75.00	55032.0
76.00	4772.0
76.90	856.0
77.90	585.0
78.90	3929.0
79.90	1308.0
80.90	4040.0
81.90	1128.0
82.90	155.0
86.90	4879.0
87.90	4434.0
90.90	429.0
91.90	3294.0
93.00	5134.0
94.00	13132.0
95.00	107008.0
96.00	7589.0
96.90	279.0
103.80	527.0
104.80	309.0
105.80	567.0
106.80	123.0
110.80	246.0
112.10	110.0
112.90	115.0
115.90	475.0
116.90	932.0
117.80	468.0
118.90	755.0
122.80	121.0
125.90	117.0
127.20	119.0
127.90	246.0
128.70	233.0
129.80	397.0
130.70	122.0
134.80	307.0
136.70	210.0
139.70	116.0
140.80	1074.0
141.80	146.0
142.90	1269.0
143.80	132.0
144.90	282.0
145.90	265.0
147.90	430.0
149.90	112.0
152.70	118.0
154.90	315.0
157.00	143.0
158.80	125.0
160.70	118.0
171.00	159.0
172.00	843.0
173.00	1023.0
173.90	78768.0

Instrument :
MSVOA_V
ClientSampleId :
BFB375

174.90	6490.0
175.90	77840.0
176.90	4947.0
178.00	158.0

Instrument :
MSVOA_V
ClientSampleId :
BFB375

m/z	Abundance
35.90	970.0
36.90	4601.0
38.00	4569.0
39.00	1857.0
39.90	455.0
41.00	122.0
41.70	118.0
42.60	114.0
44.00	1268.0
45.00	992.0
45.80	168.0
46.90	1045.0
47.90	746.0
49.00	4669.0
50.00	19176.0
51.00	6499.0
51.90	233.0
52.80	157.0
55.00	408.0
55.90	1757.0
57.00	2562.0
58.00	173.0
60.00	1078.0
61.00	5479.0
62.00	5428.0
63.00	3864.0
63.90	560.0
65.00	702.0
65.90	163.0
66.80	247.0
68.00	10248.0
69.00	10908.0
70.00	926.0
71.90	750.0
72.90	4736.0
74.00	17376.0
75.00	52248.0
76.00	4649.0
76.90	904.0
77.90	640.0
78.90	3622.0
79.90	1216.0
80.90	4042.0
81.90	1088.0
83.00	191.0
86.90	4361.0
87.90	4461.0
91.00	384.0
91.90	3204.0
93.00	5113.0
94.00	12509.0
95.00	100128.0
96.00	7220.0
96.90	288.0
103.80	499.0
104.80	320.0
105.80	586.0
110.90	212.0
112.90	129.0
115.10	101.0
115.80	454.0
116.90	819.0
117.80	458.0
118.80	616.0
122.70	132.0
123.60	113.0
125.90	106.0
127.90	236.0
128.70	243.0
129.90	371.0
130.70	127.0
134.80	286.0
136.80	164.0
137.10	167.0
139.80	110.0
140.90	1001.0
141.70	172.0
142.80	1179.0
143.90	192.0
144.90	241.0
145.90	218.0
147.90	399.0
149.70	134.0
152.70	136.0
154.80	246.0
157.00	116.0
159.00	106.0
160.70	111.0
171.00	152.0
171.90	812.0
173.00	1039.0
173.90	77288.0

Instrument :
MSVOA_V
ClientSampleId :
BFB375

174.90	5955.0
175.90	78040.0
176.90	4763.0
178.10	203.0

Instrument :
MSVOA_V
ClientSampleId :
BFB375