

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV090924\
 Data File : VV037231.D
 Acq On : 09 Sep 2024 09:54
 Operator : SY/MD
 Sample : VV0909MBL01
 Misc : 5.00mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :

Quant Time: Sep 09 22:03:13 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082624WMA.M
 Quant Title : VOC Analysis
 QLast Update : Mon Sep 09 22:02:35 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.529	114	671576	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.779	117	655928	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.178	152	308558	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.278	65	274372	44.662	ug/L	0.00
Spiked Amount	50.000	Range 60 - 135	Recovery	=	89.320%	
7) Chloroethane-d5	1.532	69	217013	45.707	ug/L	0.00
Spiked Amount	50.000	Range 70 - 130	Recovery	=	91.420%	
11) 1,1-Dichloroethene-d2	2.059	65	114794	44.459	ug/L	0.00
Spiked Amount	50.000	Range 60 - 125	Recovery	=	88.920%	
21) 2-Butanone-d5	3.789	46	196574	82.629	ug/L	0.00
Spiked Amount	100.000	Range 40 - 130	Recovery	=	82.630%	
24) Chloroform-d	4.239	84	451067	46.914	ug/L	0.00
Spiked Amount	50.000	Range 70 - 125	Recovery	=	93.820%	
26) 1,2-Dichloroethane-d4	4.934	65	282430	46.645	ug/L	0.00
Spiked Amount	50.000	Range 70 - 125	Recovery	=	93.280%	
32) Benzene-d6	4.950	84	942629	47.580	ug/L	0.00
Spiked Amount	50.000	Range 70 - 125	Recovery	=	95.160%	
36) 1,2-Dichloropropane-d6	5.982	67	299097	48.201	ug/L	0.00
Spiked Amount	50.000	Range 70 - 120	Recovery	=	96.400%	
41) Toluene-d8	7.236	98	820477	45.888	ug/L	0.00
Spiked Amount	50.000	Range 80 - 120	Recovery	=	91.780%	
43) trans-1,3-Dichloroprop...	7.548	79	129090	44.966	ug/L	0.00
Spiked Amount	50.000	Range 60 - 125	Recovery	=	89.940%	
47) 2-Hexanone-d5	8.024	63	122427	72.291	ug/L	0.00
Spiked Amount	100.000	Range 45 - 130	Recovery	=	72.290%	
56) 1,1,2,2-Tetrachloroeth...	10.146	84	320465	42.582	ug/L	0.00
Spiked Amount	50.000	Range 65 - 120	Recovery	=	85.160%	
66) 1,2-Dichlorobenzene-d4	11.554	152	295128	47.757	ug/L	0.00
Spiked Amount	50.000	Range 80 - 120	Recovery	=	95.520%	
Target Compounds						
10) 1,1,2-Trichloro-1,2,2-...	2.056	101	3810	0.819	ug/L	Qvalue # 24


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV090924\
Data File : VV037231.D
Acq On : 09 Sep 2024 09:54
Operator : SY/MD
Sample : VV0909MBL01
Misc : 5.00mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :


Quant Time: Sep 09 22:03:13 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082624WMA.M
Quant Title : VOC Analysis
QLast Update : Mon Sep 09 22:02:35 2024
Response via : Initial Calibration

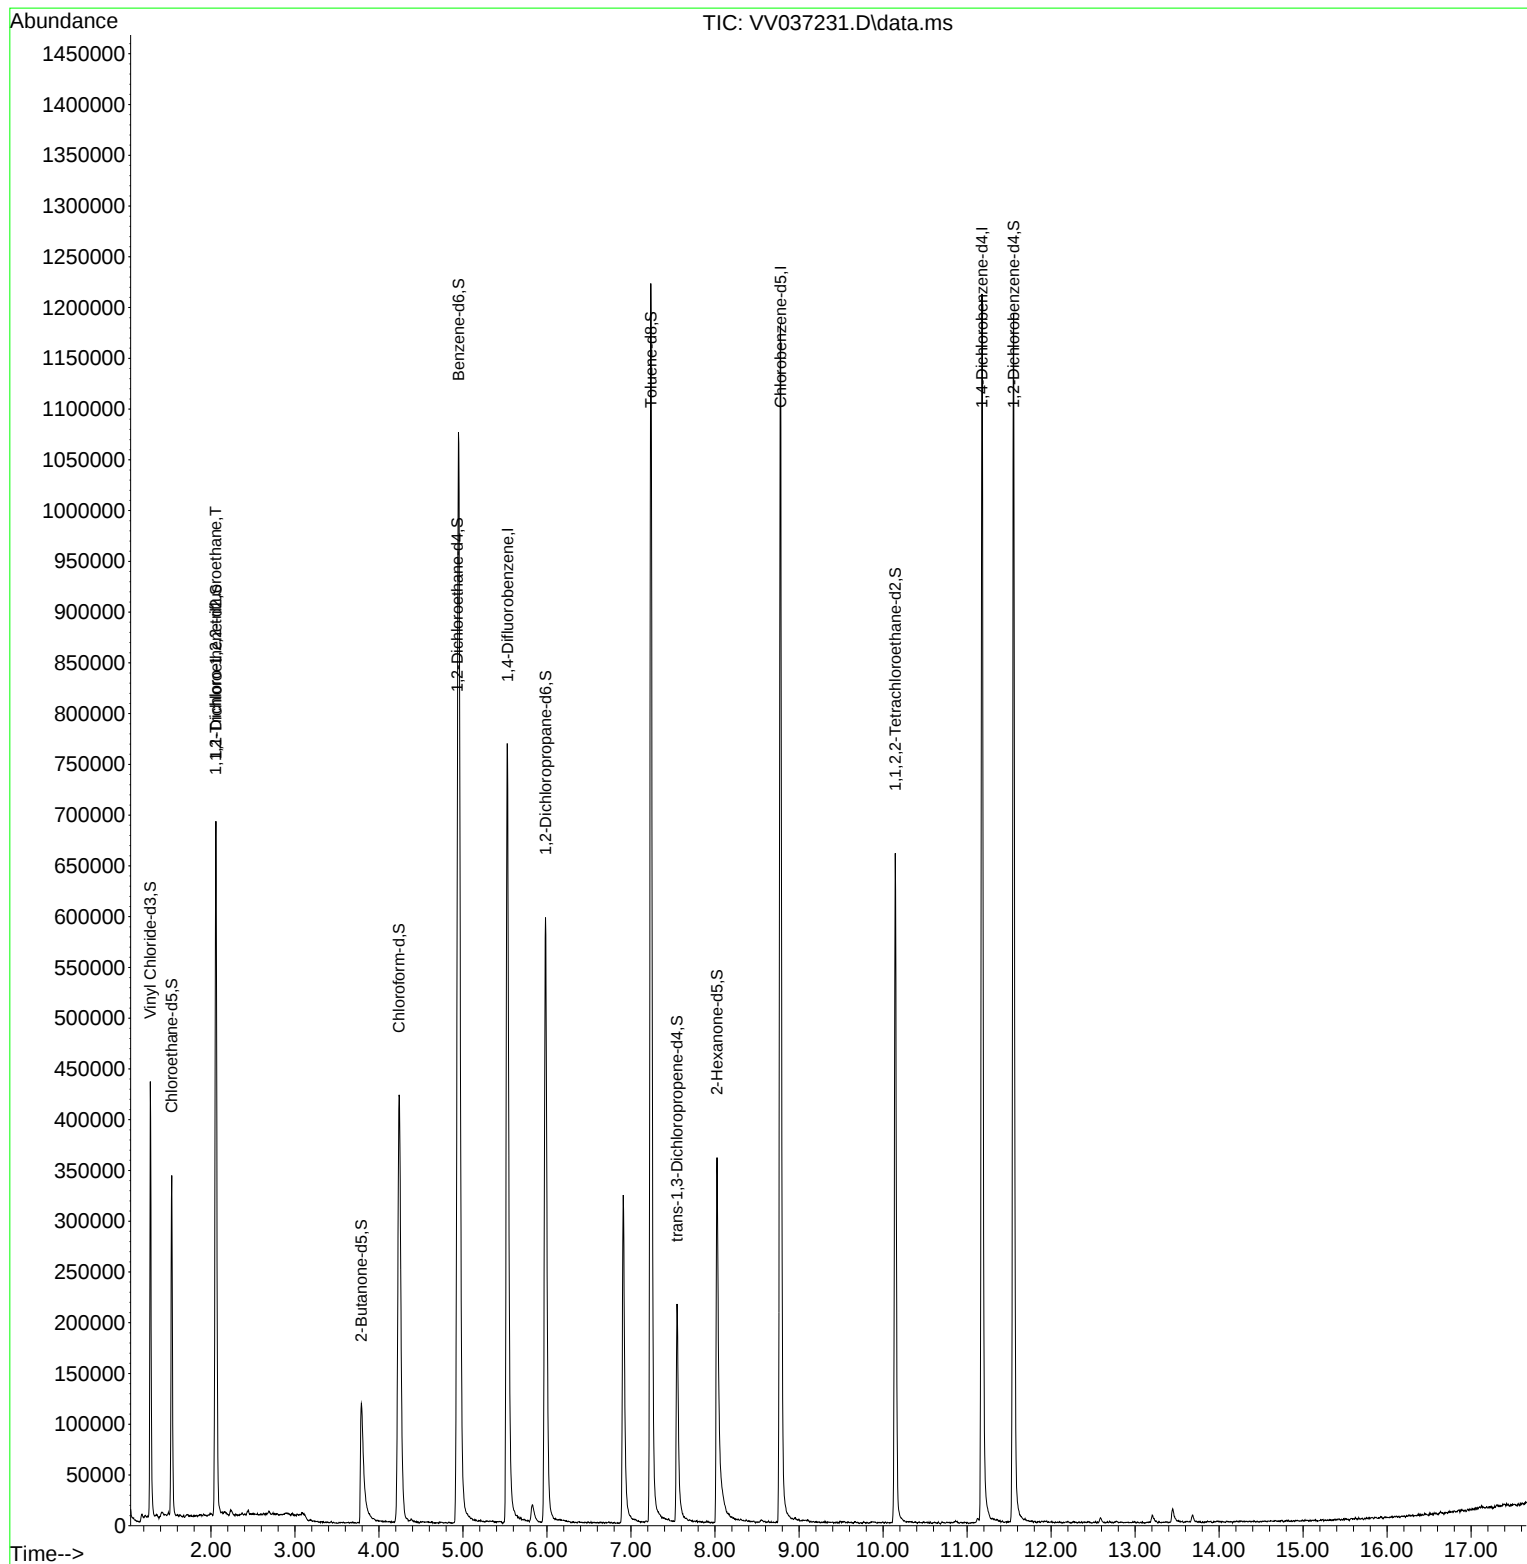

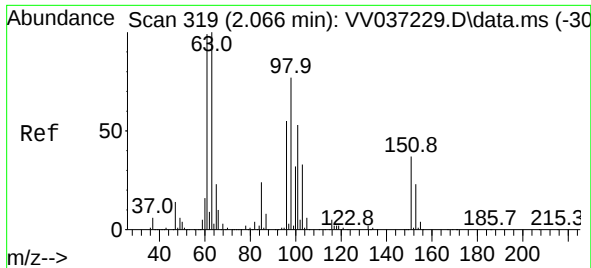

#10
 1,1,2-Trichloro-1,2,2-trifluoroethane
 Concen: 0.819 ug/L
 RT: 2.056 min Scan# 316
 Delta R.T. -0.010 min
 Lab File: VV037231.D
 Acq: 09 Sep 2024 09:54

Instrument :
 MSVOA_V
 ClientSampleId :

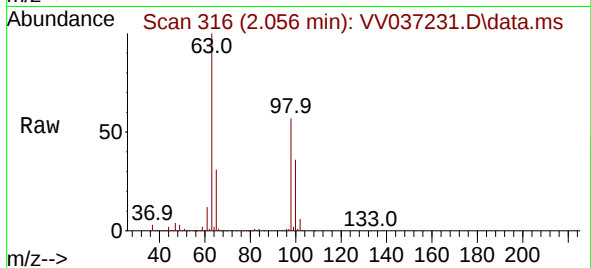

Tgt Ion:	101	Resp:	3810
Ion	Ratio	Lower	Upper
101	100		
85	2.8	35.6	53.4#
151	1.2	55.0	82.4#

