

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV090924\
 Data File : VV037234.D
 Acq On : 09 Sep 2024 12:45
 Operator : SY/MD
 Sample : P3808-02
 Misc : 5.00mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 X0B25

Quant Time: Sep 09 22:03:53 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082624WMA.M
 Quant Title : VOC Analysis
 QLast Update : Mon Sep 09 22:02:35 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	5.526	114	705018	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.776	117	681731	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.178	152	349808	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.278	65	247092	38.313	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	76.620%
7) Chloroethane-d5	1.532	69	198994	39.924	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	79.840%
11) 1,1-Dichloroethene-d2	2.057	65	103612	38.224	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	76.440%
21) 2-Butanone-d5	3.790	46	171053	68.491	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	68.490%
24) Chloroform-d	4.240	84	457078	45.284	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	90.560%
26) 1,2-Dichloroethane-d4	4.934	65	260754	41.022	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	82.040%
32) Benzene-d6	4.950	84	843037	40.942	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	81.880%
36) 1,2-Dichloropropane-d6	5.979	67	273688	42.437	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	84.880%
41) Toluene-d8	7.236	98	749832	40.349	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	80.700%
43) trans-1,3-Dichloroprop...	7.548	79	119765	40.139	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	80.280%
47) 2-Hexanone-d5	8.021	63	117751	66.898	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	66.900%
56) 1,1,2,2-Tetrachloroeth...	10.146	84	299750	38.322	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	76.640%
66) 1,2-Dichlorobenzene-d4	11.551	152	283028	40.398	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	80.800%
Target Compounds						
					Qvalue	
9) Trichlorofluoromethane	1.712	101	629883	76.738	ug/L	99
12) 1,1-Dichloroethene	2.069	96	138948	30.209	ug/L	92
13) Acetone	2.111	43	197320	73.669	ug/L	99
16) Methylene chloride	2.442	84	225047	43.365	ug/L	99
17) trans-1,2-Dichloroethene	2.687	96	151211	31.668	ug/L	98
18) Methyl tert-butyl Ether	2.700	73	826988	55.057	ug/L	100
19) 1,1-Dichloroethane	3.101	63	170861	18.018	ug/L	99
25) Chloroform	4.265	83	869707	90.561	ug/L	100
27) 1,2-Dichloroethane	5.031	62	577303	81.950	ug/L	99
31) Carbon tetrachloride	4.722	117	362611	54.783	ug/L	100
33) Benzene	4.998	78	2356999	119.801	ug/L	100
34) Trichloroethene	5.822	95	450382	86.731	ug/L	97
37) 1,2-Dichloropropane	6.085	63	123256	23.368	ug/L	# 92
38) Bromodichloromethane	6.426	83	251179	37.155	ug/L	99
39) cis-1,3-Dichloropropene	6.947	75	183889	22.093	ug/L	97
42) Toluene	7.307	91	675979	33.000	ug/L	99
44) trans-1,3-Dichloropropene	7.577	75	96322	12.947	ug/L	99
45) 1,1,2-Trichloroethane	7.760	97	606679	123.560	ug/L	99
46) Tetrachloroethene	7.896	164	132884	35.665	ug/L	97

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV090924\
 Data File : VV037234.D
 Acq On : 09 Sep 2024 12:45
 Operator : SY/MD
 Sample : P3808-02
 Misc : 5.00mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 X0B25

Quant Time: Sep 09 22:03:53 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082624WMA.M
 Quant Title : VOC Analysis
 QLast Update : Mon Sep 09 22:02:35 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


48) 2-Hexanone	8.072	43	154842	37.338	ug/L	98
49) Dibromochloromethane	8.169	129	260135	52.911	ug/L	99
50) 1,2-Dibromoethane	8.278	107	82142	16.533	ug/L	97
51) Chlorobenzene	8.809	112	256203	18.892	ug/L	99
53) m,p-Xylene	9.066	106	271323	31.649	ug/L	100
54) o-Xylene	9.471	106	200563	23.894	ug/L	97
55) Styrene	9.487	104	1375574	94.445	ug/L	99
57) 1,1,2,2-Tetrachloroethane	10.169	83	590007	81.135	ug/L	98
59) Bromoform	9.657	173	279261	85.733	ug/L	99
61) 1,2,3-Trichloropropane	10.201	75	514509	94.550	ug/L	100
62) 1,3,5-Trimethylbenzene	10.468	105	851032	45.868	ug/L	99
63) 1,2,4-Trimethylbenzene	10.844	105	1280797	69.172	ug/L	99
64) 1,3-Dichlorobenzene	11.111	146	137287	13.110	ug/L	99
65) 1,4-Dichlorobenzene	11.201	146	253549	23.657	ug/L	99
67) 1,2-Dichlorobenzene	11.571	146	314983	30.591	ug/L	98
68) 1,2-Dibromo-3-chloropr...	12.355	75	161869	119.278	ug/L	97
70) 1,2,4-trichlorobenzene	13.191	180	113479	16.539	ug/L	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV090924\
Data File : VV037234.D
Acq On : 09 Sep 2024 12:45
Operator : SY/MD
Sample : P3808-02
Misc : 5.00mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
X0B25

Quant Time: Sep 09 22:03:53 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082624WMA.M
Quant Title : VOC Analysis
QLast Update : Mon Sep 09 22:02:35 2024
Response via : Initial Calibration




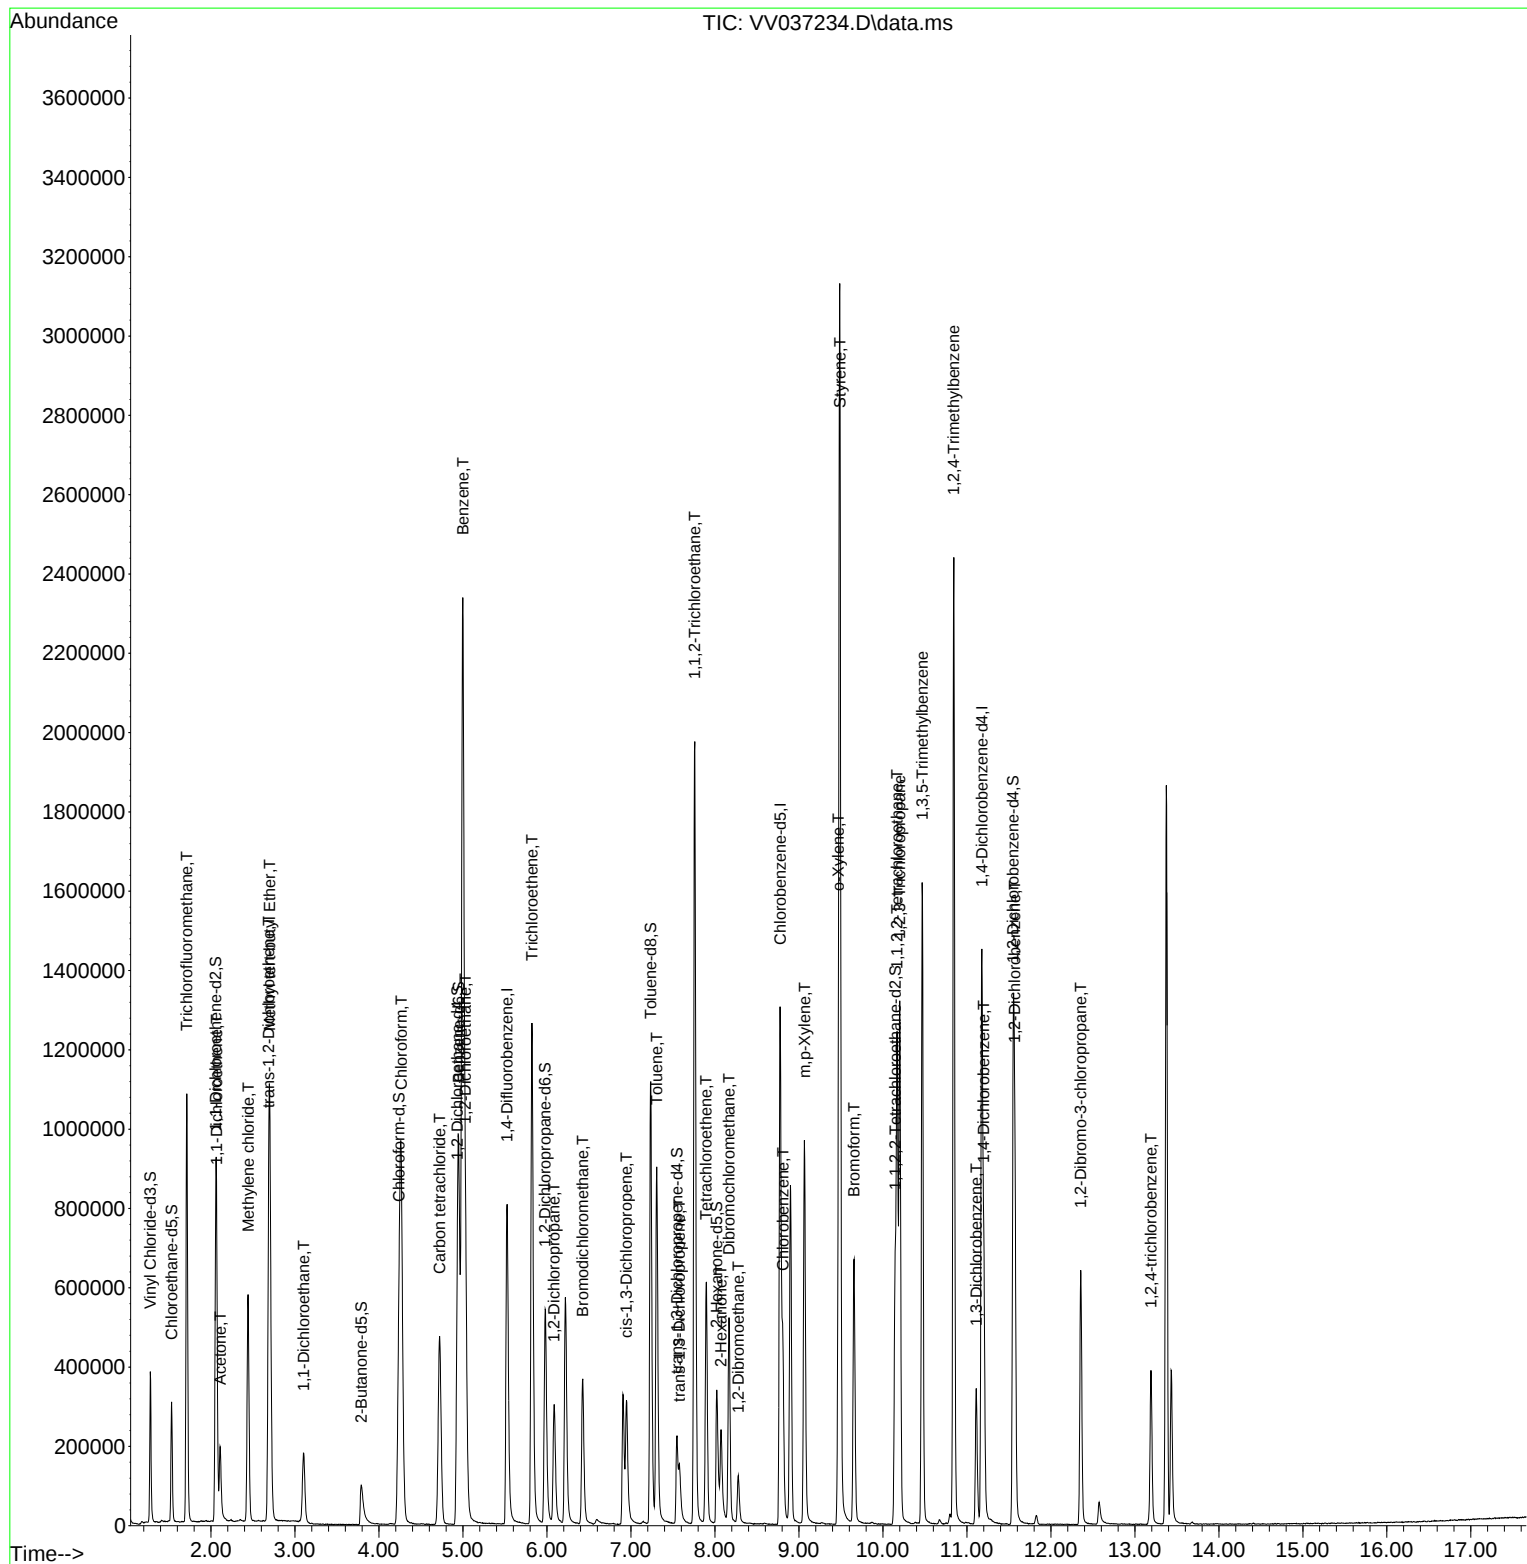




#9
 Trichlorofluoromethane
 Concen: 76.738 ug/L
 RT: 1.712 min Scan# 209
 Delta R.T. 0.000 min
 Lab File: VV037234.D
 Acq: 09 Sep 2024 12:45




Instrument :
 MSVOA_V
 ClientSampleId :
 X0B25


Tgt Ion:101 Resp: 629883
 Ion Ratio Lower Upper
 101 100
 103 63.9 51.7 77.5

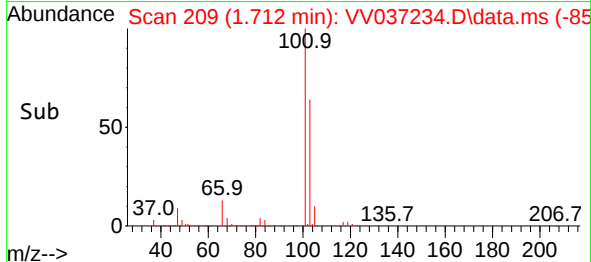

#12
 1,1-Dichloroethene
 Concen: 30.209 ug/L
 RT: 2.069 min Scan# 320
 Delta R.T. 0.000 min
 Lab File: VV037234.D
 Acq: 09 Sep 2024 12:45

Tgt Ion: 96 Resp: 138948
 Ion Ratio Lower Upper
 96 100
 61 176.9 123.8 229.8
 63 160.3 96.5 179.1

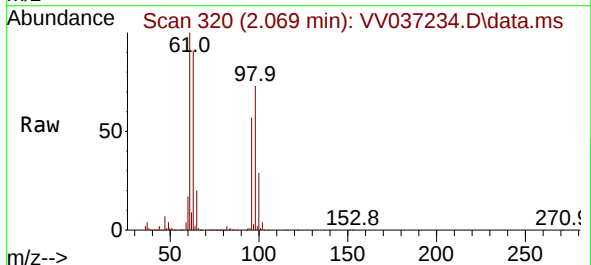



#13

Acetone

Concen: 73.669 ug/L

RT: 2.111 min Scan# 31

Delta R.T. 0.000 min

Lab File: VV037234.D

Acq: 09 Sep 2024 12:45

Instrument :

MSVOA_V

ClientSampleId :





X0B25

Tgt Ion: 43 Resp: 197320

Ion Ratio Lower Upper

43 100

58 32.9 0.0 64.8

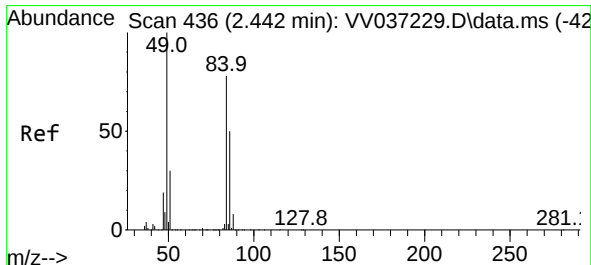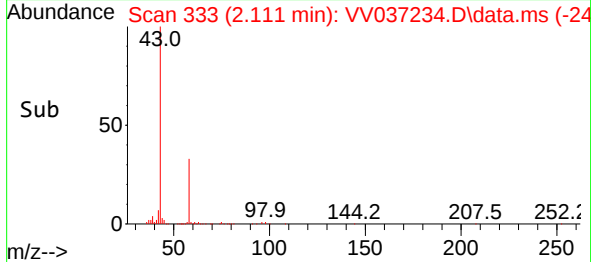

#16

Methylene chloride

Concen: 43.365 ug/L

RT: 2.442 min Scan# 436

Delta R.T. 0.000 min

Lab File: VV037234.D

Acq: 09 Sep 2024 12:45




Tgt Ion: 84 Resp: 225047


Ion Ratio Lower Upper

84 100

86 64.6 44.7 82.9

49 128.6 91.4 169.8



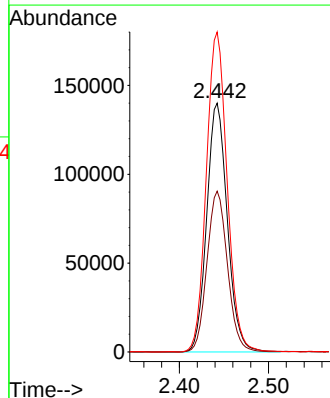
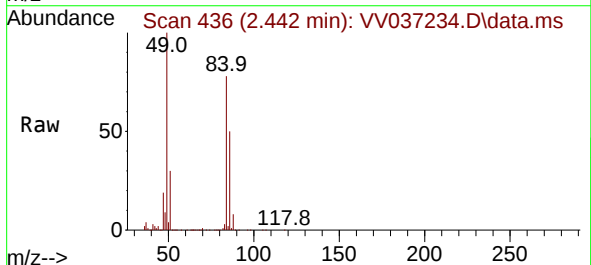




#17
trans-1,2-Dichloroethene
Concen: 31.668 ug/L
RT: 2.687 min Scan# 513
Delta R.T. -0.003 min
Lab File: VV037234.D
Acq: 09 Sep 2024 12:45




Instrument :
MSVOA_V
ClientSampleId :
X0B25


Tgt Ion: 96 Resp: 151211
Ion Ratio Lower Upper
96 100
61 142.2 102.3 189.9
98 63.4 44.8 83.2

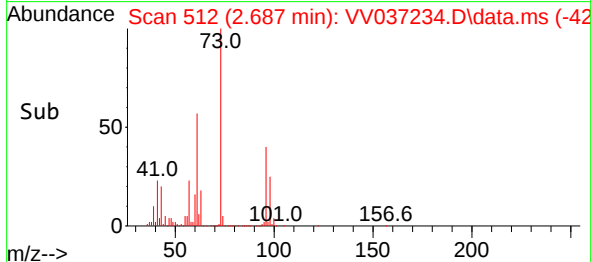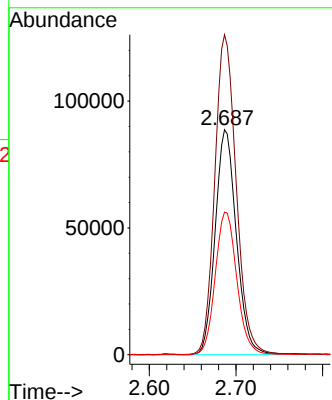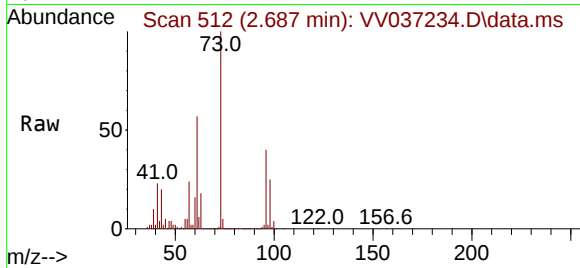

#18
Methyl tert-butyl Ether
Concen: 55.057 ug/L
RT: 2.700 min Scan# 516
Delta R.T. -0.003 min
Lab File: VV037234.D
Acq: 09 Sep 2024 12:45

Tgt Ion: 73 Resp: 826988
Ion Ratio Lower Upper
73 100
43 19.4 15.8 23.6
57 22.7 18.1 27.1

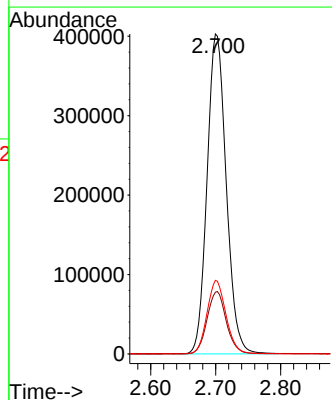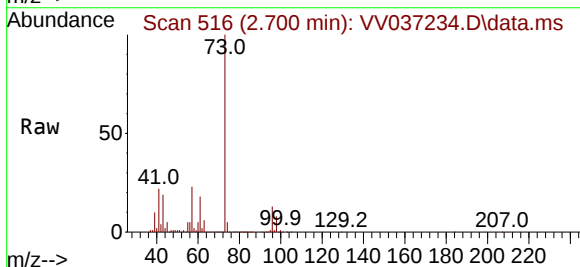



#19

1,1-Dichloroethane

Concen: 18.018 ug/L

RT: 3.101 min Scan# 64

Delta R.T. -0.003 min

Lab File: VV037234.D

Acq: 09 Sep 2024 12:45

Instrument :

MSVOA_V

ClientSampleId :

X0B25





Tgt Ion: 63 Resp: 170861

Ion Ratio Lower Upper

63 100

65 31.3 22.0 41.0

83 14.1 9.2 17.0

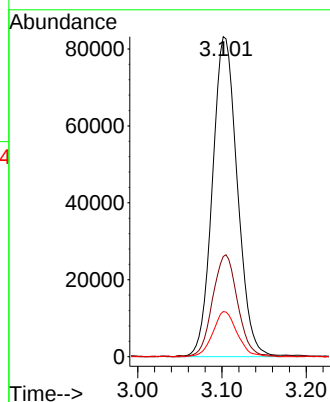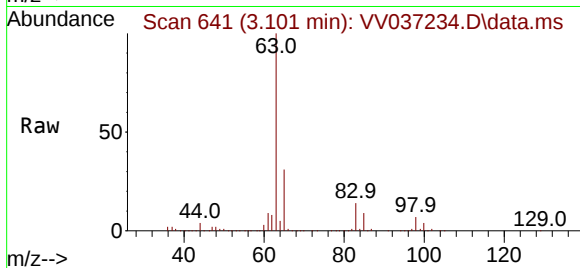

#25

Chloroform

Concen: 90.561 ug/L

RT: 4.265 min Scan# 1003

Delta R.T. -0.003 min

Lab File: VV037234.D




Acq: 09 Sep 2024 12:45


Tgt Ion: 83 Resp: 869707

Ion Ratio Lower Upper

83 100

85 64.7 45.1 83.7

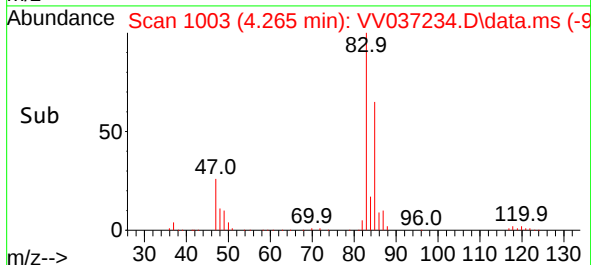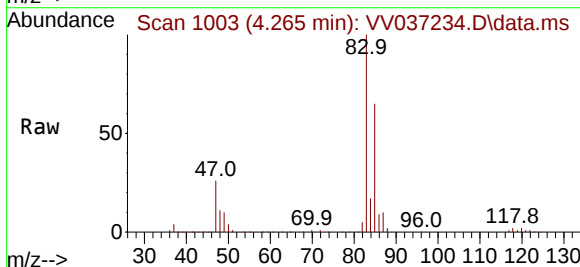



#27

1,2-Dichloroethane

Concen: 81.950 ug/L

RT: 5.031 min Scan# 11

Delta R.T. -0.003 min

Lab File: VV037234.D

Acq: 09 Sep 2024 12:45

Instrument :

MSVOA_V

ClientSampleId :





X0B25

Tgt Ion: 62 Resp: 577303

Ion Ratio Lower Upper

62 100

98 9.7 8.0 12.0

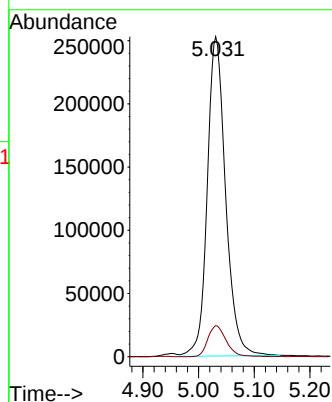

#31

Carbon tetrachloride

Concen: 54.783 ug/L

RT: 4.722 min Scan# 1145

Delta R.T. -0.003 min

Lab File: VV037234.D




Acq: 09 Sep 2024 12:45


Tgt Ion: 117 Resp: 362611

Ion Ratio Lower Upper

117 100

119 95.1 75.8 113.6

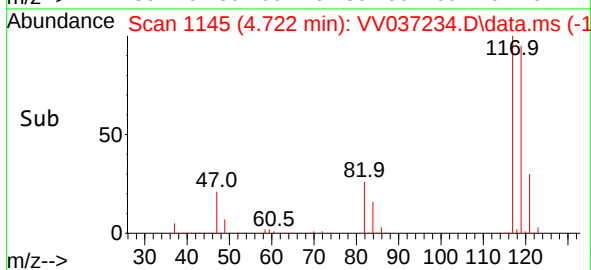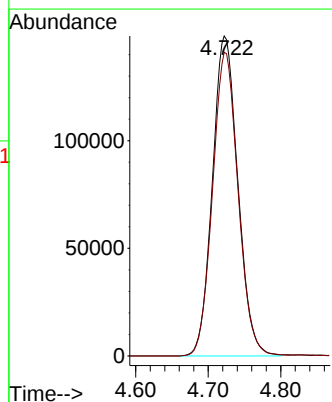



#33

Benzene

Concen: 119.801 ug/L

RT: 4.998 min Scan# 1

Delta R.T. -0.003 min

Lab File: VV037234.D

Acq: 09 Sep 2024 12:45





Instrument :

MSVOA_V

ClientSampleId :

X0B25

Tgt Ion: 78 Resp: 2356999



#34

Trichloroethene

Concen: 86.731 ug/L

RT: 5.822 min Scan# 1487

Delta R.T. -0.003 min

Lab File: VV037234.D

Acq: 09 Sep 2024 12:45

Tgt Ion: 95 Resp: 450382




Ion Ratio Lower Upper


95 100

97 65.6 44.4 82.5

132 95.8 64.9 120.5

130 97.5 69.4 129.0

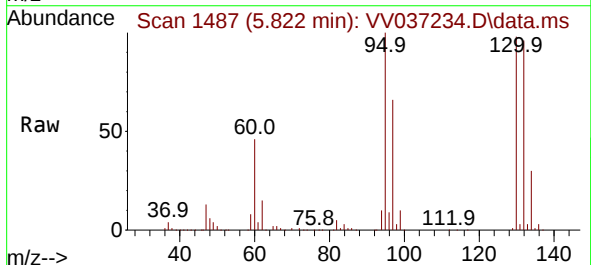



#37

1,2-Dichloropropane

Concen: 23.368 ug/L

RT: 6.085 min Scan# 1

Delta R.T. 0.000 min

Lab File: VV037234.D

Acq: 09 Sep 2024 12:45

Instrument :

MSVOA_V

ClientSampleId :





X0B25

Tgt Ion: 63 Resp: 123256

Ion Ratio Lower Upper

63 100

112 1.6 3.5 5.3#

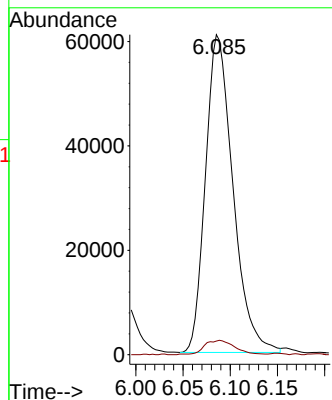

#38

Bromodichloromethane

Concen: 37.155 ug/L

RT: 6.426 min Scan# 1675

Delta R.T. 0.000 min

Lab File: VV037234.D

Acq: 09 Sep 2024 12:45




Tgt Ion: 83 Resp: 251179


Ion Ratio Lower Upper

83 100

85 64.0 44.5 82.7

127 7.5 6.1 9.1

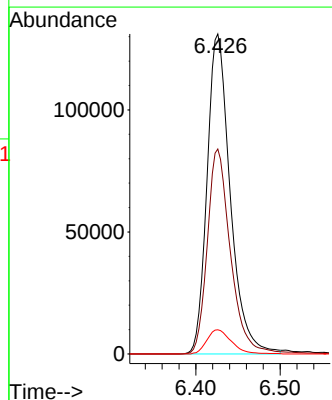



#39

cis-1,3-Dichloropropene

Concen: 22.093 ug/L

RT: 6.947 min Scan# 1837

Delta R.T. 0.000 min

Lab File: VV037234.D

Acq: 09 Sep 2024 12:45

Instrument :

MSVOA_V

ClientSampleId :





X0B25

Tgt Ion: 75 Resp: 183889

Ion Ratio Lower Upper

75 100

77 32.4 21.7 40.3

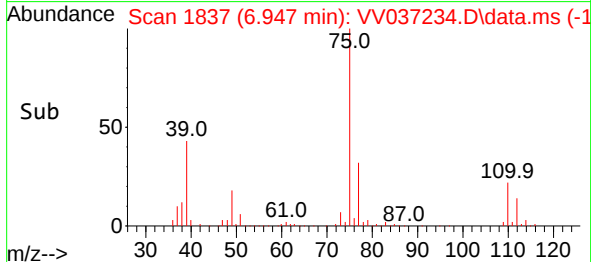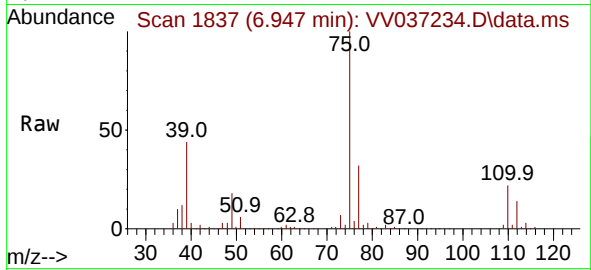

#42

Toluene

Concen: 33.000 ug/L

RT: 7.307 min Scan# 1949

Delta R.T. 0.000 min

Lab File: VV037234.D




Acq: 09 Sep 2024 12:45


Tgt Ion: 91 Resp: 675979

Ion Ratio Lower Upper

91 100

92 57.4 40.8 75.8

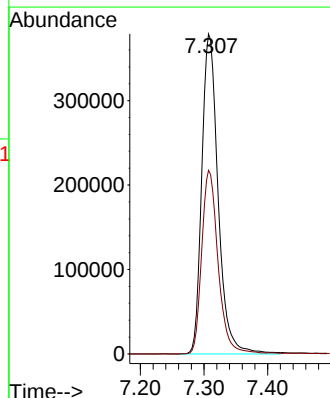

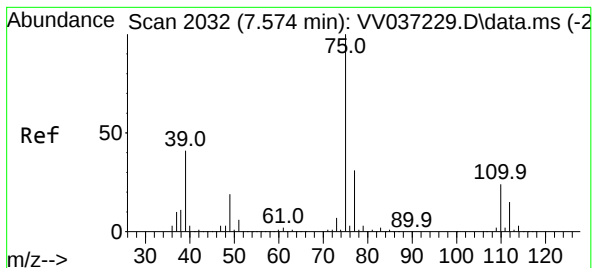

#44

trans-1,3-Dichloropropene

Concen: 12.947 ug/L

RT: 7.577 min Scan# 2032

Delta R.T. 0.003 min

Lab File: VV037234.D

Acq: 09 Sep 2024 12:45

Instrument :

MSVOA_V

ClientSampleId :





X0B25

Tgt Ion: 75 Resp: 96322

Ion Ratio Lower Upper

75 100

77 30.7 22.0 40.8

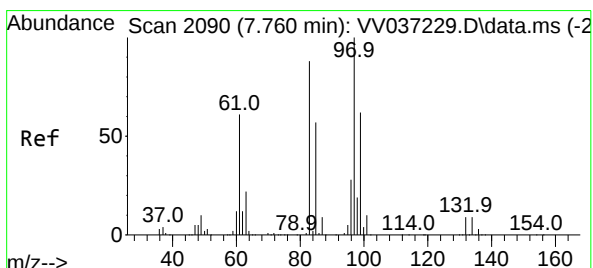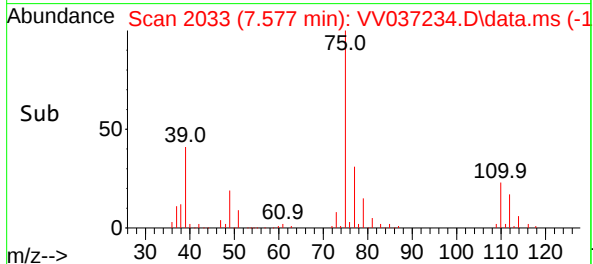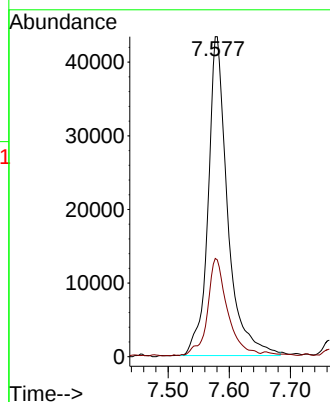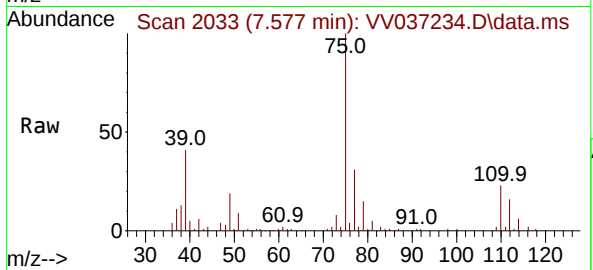

#45

1,1,2-Trichloroethane

Concen: 123.560 ug/L

RT: 7.760 min Scan# 2090

Delta R.T. 0.000 min

Lab File: VV037234.D

Acq: 09 Sep 2024 12:45

Tgt Ion: 97 Resp: 606679




Ion Ratio Lower Upper


97 100

99 61.2 42.6 79.0

83 86.9 60.5 112.3


85 55.3 38.2 71.0

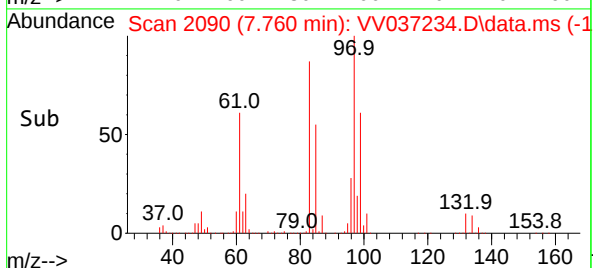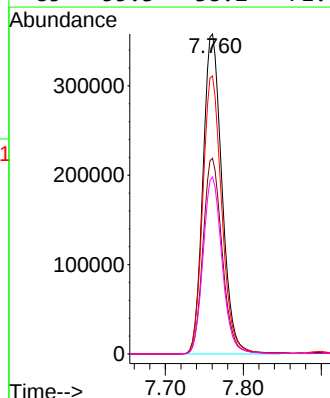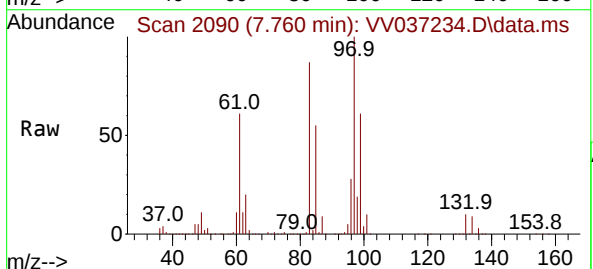






#46
Tetrachloroethene
Concen: 35.665 ug/L
RT: 7.896 min Scan# 2133
Delta R.T. -0.003 min
Lab File: VV037234.D
Acq: 09 Sep 2024 12:45


Instrument :
MSVOA_V
ClientSampleId :
X0B25





Tgt Ion:164 Resp: 132884
Ion Ratio Lower Upper
164 100
129 99.6 67.1 124.7
131 92.6 67.0 124.4
166 126.3 86.2 160.2

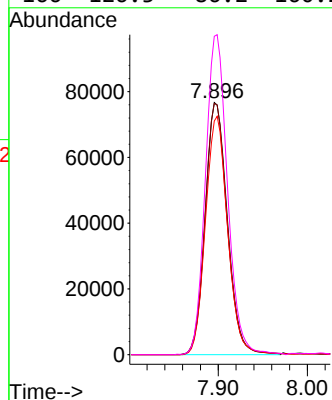


#48
2-Hexanone
Concen: 37.338 ug/L
RT: 8.072 min Scan# 2187
Delta R.T. 0.000 min
Lab File: VV037234.D
Acq: 09 Sep 2024 12:45



Tgt Ion: 43 Resp: 154842
Ion Ratio Lower Upper
43 100
58 58.7 46.0 69.0
57 18.7 15.6 23.4
100 12.8 10.6 16.0



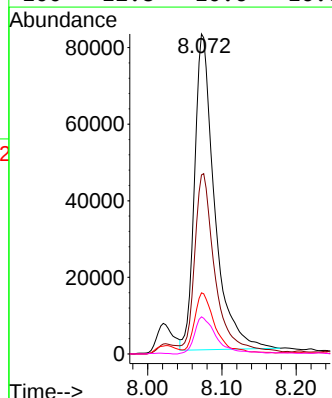
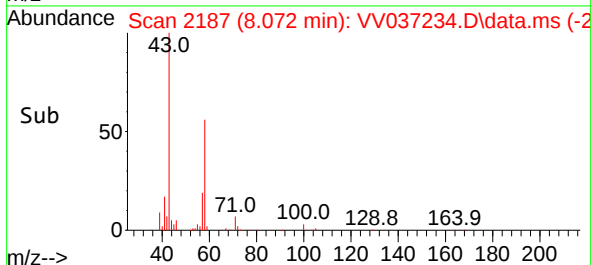




#49
Dibromochloromethane
Concen: 52.911 ug/L
RT: 8.169 min Scan# 21
Delta R.T. 0.000 min
Lab File: VV037234.D
Acq: 09 Sep 2024 12:45




Instrument :
MSVOA_V
ClientSampleId :
X0B25


Tgt Ion:129 Resp: 260135
Ion Ratio Lower Upper
129 100
127 77.4 54.7 101.7

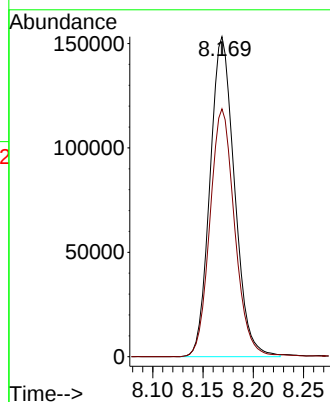

#50
1,2-Dibromoethane
Concen: 16.533 ug/L
RT: 8.278 min Scan# 2251
Delta R.T. 0.003 min
Lab File: VV037234.D
Acq: 09 Sep 2024 12:45

Tgt Ion:107 Resp: 82142
Ion Ratio Lower Upper
107 100
109 91.7 66.6 123.6
188 3.4 2.6 3.8


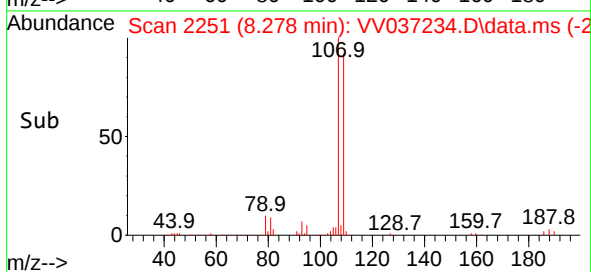
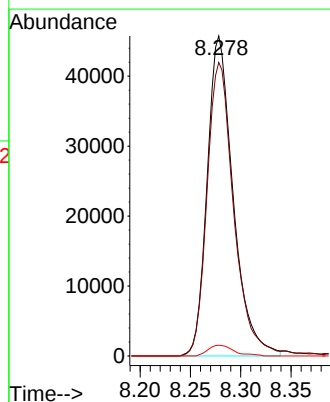





#51
Chlorobenzene
Concen: 18.892 ug/L
RT: 8.809 min Scan# 2415
Delta R.T. 0.003 min
Lab File: VV037234.D
Acq: 09 Sep 2024 12:45




Instrument :
MSVOA_V
ClientSampleId :
X0B25


Tgt Ion:112 Resp: 256203
Ion Ratio Lower Upper
112 100
114 31.6 22.3 41.5
77 59.4 47.8 71.8

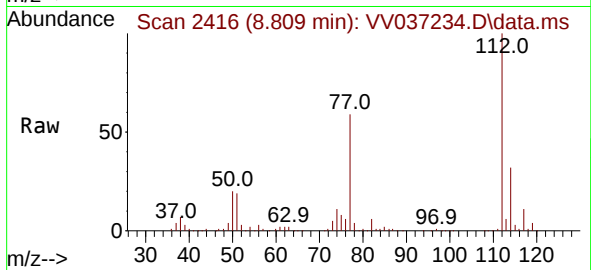

#53
m,p-Xylene
Concen: 31.649 ug/L
RT: 9.066 min Scan# 2496
Delta R.T. 0.000 min
Lab File: VV037234.D
Acq: 09 Sep 2024 12:45

Tgt Ion:106 Resp: 271323
Ion Ratio Lower Upper
106 100
91 204.4 143.0 265.6









#54
o-Xylene
Concen: 23.894 ug/L
RT: 9.471 min Scan# 2622
Delta R.T. 0.000 min
Lab File: VV037234.D
Acq: 09 Sep 2024 12:45




Instrument :
MSVOA_V
ClientSampleId :
X0B25


Tgt Ion:106 Resp: 200563
Ion Ratio Lower Upper
106 100
91 214.1 153.2 284.6

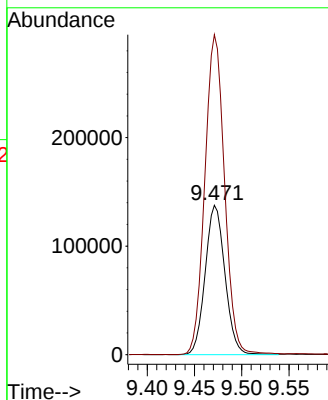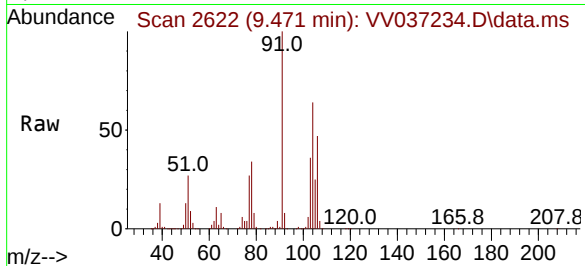

#55
Styrene
Concen: 94.445 ug/L
RT: 9.487 min Scan# 2627
Delta R.T. 0.000 min
Lab File: VV037234.D
Acq: 09 Sep 2024 12:45

Tgt Ion:104 Resp: 1375574
Ion Ratio Lower Upper
104 100
78 43.3 30.9 57.5

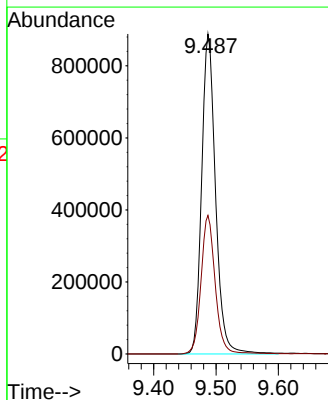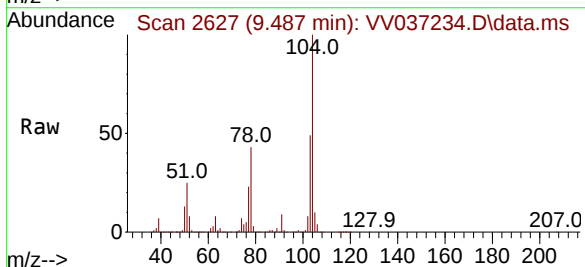



#57

1,1,2,2-Tetrachloroethane

Concen: 81.135 ug/L

RT: 10.169 min Scan# 21

Delta R.T. -0.003 min

Lab File: VV037234.D

Acq: 09 Sep 2024 12:45

Instrument :

MSVOA_V

ClientSampleId :

X0B25





Tgt Ion: 83 Resp: 590007

Ion Ratio Lower Upper

83 100

85 65.9 45.1 83.7

131 9.5 7.4 11.0

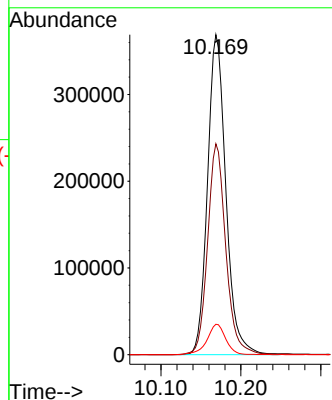

#59

Bromoform

Concen: 85.733 ug/L

RT: 9.657 min Scan# 2680

Delta R.T. 0.000 min

Lab File: VV037234.D

Acq: 09 Sep 2024 12:45




Tgt Ion: 173 Resp: 279261


Ion Ratio Lower Upper

173 100

175 48.1 38.7 58.1

254 7.9 6.8 10.2

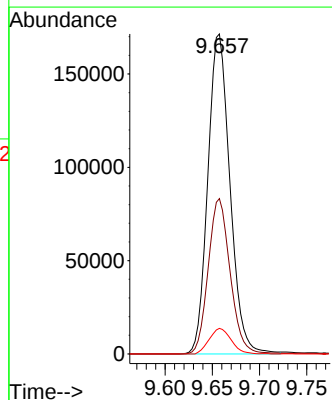



#61

1,2,3-Trichloropropane

Concen: 94.550 ug/L

RT: 10.201 min Scan# 2849

Delta R.T. 0.000 min

Lab File: VV037234.D

Acq: 09 Sep 2024 12:45

Instrument :

MSVOA_V

ClientSampleId :

X0B25





Tgt Ion: 75 Resp: 514509

Ion Ratio Lower Upper

75 100

77 32.0 25.2 37.8

110 38.8 31.1 46.7

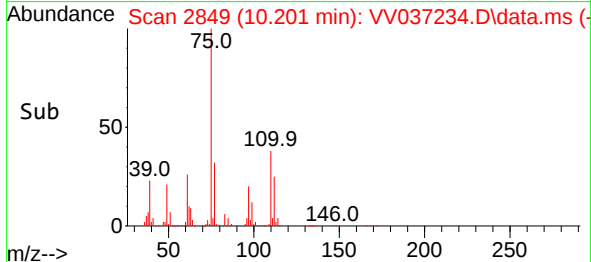

#62

1,3,5-Trimethylbenzene

Concen: 45.868 ug/L

RT: 10.468 min Scan# 2932

Delta R.T. 0.000 min

Lab File: VV037234.D




Acq: 09 Sep 2024 12:45


Tgt Ion: 105 Resp: 851032

Ion Ratio Lower Upper

105 100

120 48.3 38.3 57.5

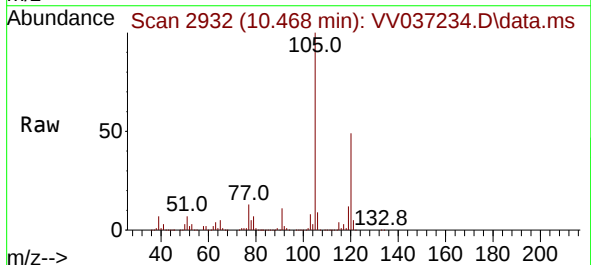

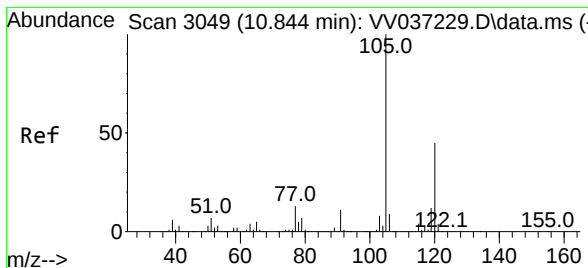

#63

1,2,4-Trimethylbenzene

Concen: 69.172 ug/L

RT: 10.844 min Scan# 3049

Delta R.T. 0.000 min

Lab File: VV037234.D

Acq: 09 Sep 2024 12:45

Instrument :

MSVOA_V

ClientSampleId :





X0B25

Tgt Ion:105 Resp: 1280797

Ion Ratio Lower Upper

105 100

120 45.1 35.8 53.6

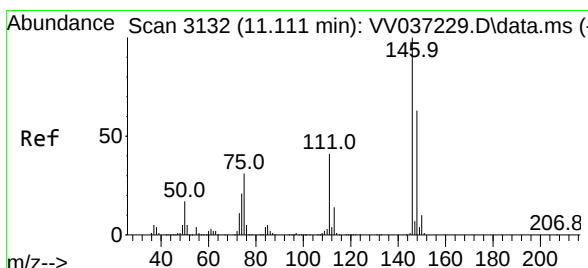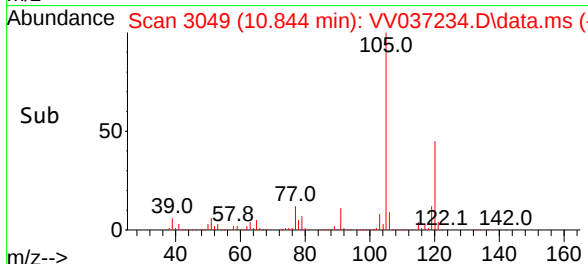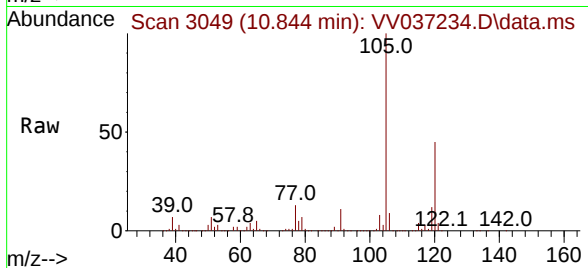

#64

1,3-Dichlorobenzene

Concen: 13.110 ug/L

RT: 11.111 min Scan# 3132

Delta R.T. 0.000 min

Lab File: VV037234.D

Acq: 09 Sep 2024 12:45




Tgt Ion:146 Resp: 137287


Ion Ratio Lower Upper

146 100

111 42.5 29.7 55.1

148 62.5 44.8 83.2

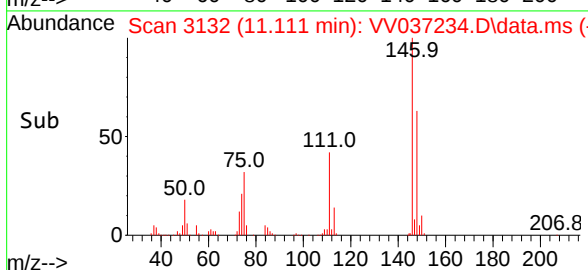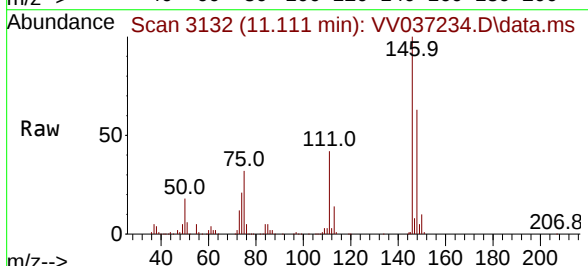



#65

1,4-Dichlorobenzene

Concen: 23.657 ug/L

RT: 11.201 min Scan# 3160

Delta R.T. 0.000 min

Lab File: VV037234.D

Acq: 09 Sep 2024 12:45

Instrument :

MSVOA_V

ClientSampleId :

X0B25





Tgt Ion:146 Resp: 253549

Ion Ratio Lower Upper

146 100

111 40.5 28.1 52.1

148 63.8 44.2 82.0

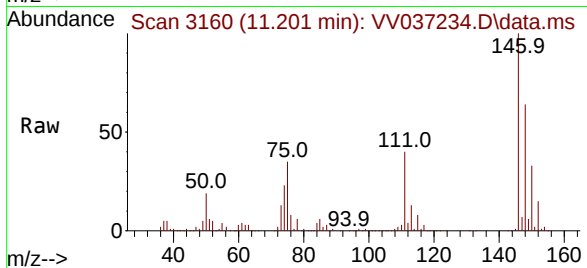

#67

1,2-Dichlorobenzene

Concen: 30.591 ug/L

RT: 11.571 min Scan# 3275

Delta R.T. 0.000 min

Lab File: VV037234.D

Acq: 09 Sep 2024 12:45




Tgt Ion:146 Resp: 314983


Ion Ratio Lower Upper

146 100

111 43.8 34.6 51.8

148 64.4 50.2 75.4


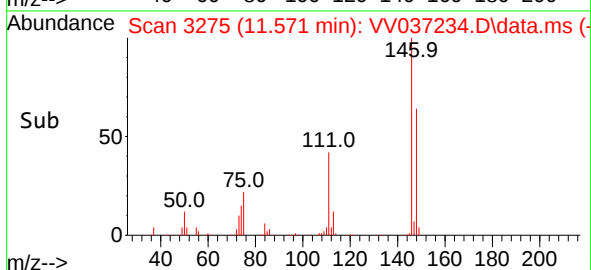

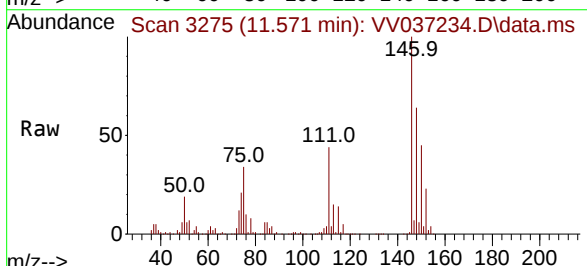


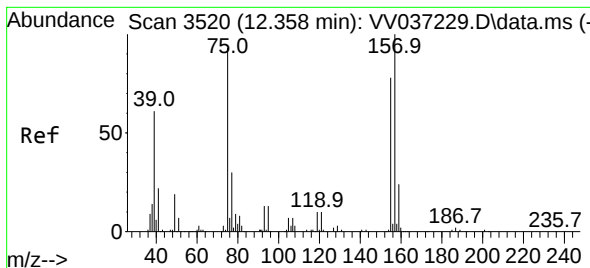

#68
1,2-Dibromo-3-chloropropane
Concen: 119.278 ug/L
RT: 12.355 min Scan# 3520
Delta R.T. -0.003 min
Lab File: VV037234.D
Acq: 09 Sep 2024 12:45

Instrument :
MSVOA_V
ClientSampleId :
X0B25

Tgt Ion: 75 Resp: 161869
Ion Ratio Lower Upper
75 100
155 80.8 61.8 92.6
157 106.1 82.5 123.7

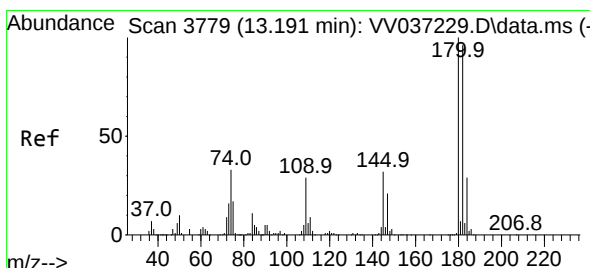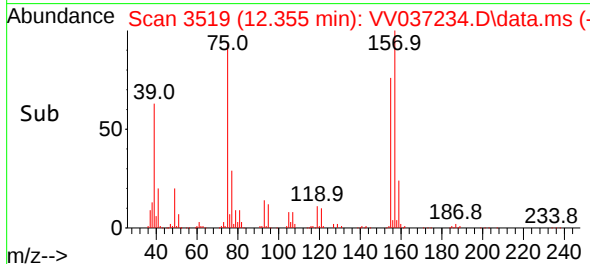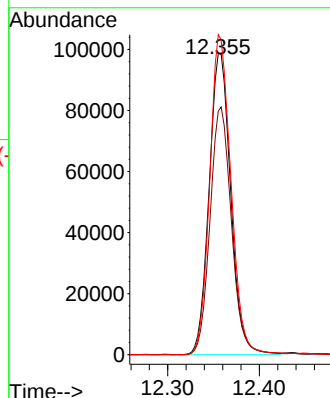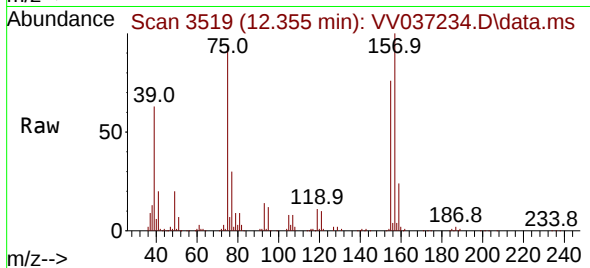

#70
1,2,4-trichlorobenzene
Concen: 16.539 ug/L
RT: 13.191 min Scan# 3779
Delta R.T. 0.000 min
Lab File: VV037234.D
Acq: 09 Sep 2024 12:45

Tgt Ion:180 Resp: 113479
Ion Ratio Lower Upper
180 100
182 97.1 75.7 113.5
145 31.5 26.0 39.0

