

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV090924\
 Data File : VV037232.D
 Acq On : 09 Sep 2024 10:20
 Operator : SY/MD
 Sample : P3843-12
 Misc : 5.00mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BHJM7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082624WMA.M
 Title : VOC Analysis

Signal : TIC: VV037232.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.176	35	42	49	rBV	9830	16302	0.59%	0.084%
2	1.278	67	74	88	rBV	414678	439000	15.95%	2.256%
3	1.349	90	96	108	rVB	36943	44895	1.63%	0.231%
4	1.532	145	153	170	rVB	335843	403708	14.67%	2.075%
5	2.060	306	317	330	rBV	695670	1009984	36.70%	5.190%
6	3.217	671	677	681	rVV8	2017	1897	0.07%	0.010%
7	3.240	681	684	690	rVB6	1956	1534	0.06%	0.008%
8	3.327	708	711	716	rBV5	1115	871	0.03%	0.004%
9	3.536	774	776	781	rVV6	1179	762	0.03%	0.004%
10	3.581	786	790	792	rBV4	1164	875	0.03%	0.004%
11	3.683	820	822	825	rVB4	1600	923	0.03%	0.005%
12	3.709	825	830	832	rBV5	1124	1193	0.04%	0.006%
13	3.790	846	855	891	rBV	119183	342094	12.43%	1.758%
14	4.069	940	942	948	rVB6	1645	1111	0.04%	0.006%
15	4.243	979	996	1027	rBV2	462725	1348078	48.98%	6.927%
16	4.751	1152	1154	1158	rVB4	1702	887	0.03%	0.005%
17	4.783	1158	1164	1168	rBV9	1621	1824	0.07%	0.009%
18	4.947	1199	1215	1252	rVV2	1083423	2752290	100.00%	14.143%
19	5.256	1309	1311	1313	rVB3	1677	739	0.03%	0.004%
20	5.304	1316	1326	1327	rBV8	1568	1801	0.07%	0.009%
21	5.478	1378	1380	1384	rBV4	977	883	0.03%	0.005%
22	5.529	1384	1396	1425	rBV	640568	1335798	48.53%	6.864%
23	5.828	1477	1489	1502	rBV4	19264	45171	1.64%	0.232%
24	5.915	1510	1516	1517	rBV5	7526	6293	0.23%	0.032%
25	5.982	1525	1537	1558	rBV	605549	1219365	44.30%	6.266%
26	6.378	1655	1660	1664	rBV7	1626	1598	0.06%	0.008%
27	6.433	1666	1677	1698	rVV	45071	94968	3.45%	0.488%
28	6.648	1742	1744	1750	rVB7	1183	954	0.03%	0.005%
29	6.722	1764	1767	1770	rBV4	1036	767	0.03%	0.004%
30	6.908	1814	1825	1851	rBV	329642	628527	22.84%	3.230%
31	7.043	1865	1867	1873	rVB7	2008	1669	0.06%	0.009%
32	7.236	1915	1927	1962	rBV	1233833	2202917	80.04%	11.320%
33	7.506	2007	2011	2013	rBV5	1338	1124	0.04%	0.006%
34	7.548	2015	2024	2053	rVV	212138	395237	14.36%	2.031%
35	7.870	2116	2124	2129	rBV9	3497	4286	0.16%	0.022%
36	7.915	2136	2138	2142	rVB5	1353	794	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV090924\
 Data File : VV037232.D
 Acq On : 09 Sep 2024 10:20
 Operator : SY/MD
 Sample : P3843-12
 Misc : 5.00mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BHJM7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082624WMA.M
 Title : VOC Analysis

37	8.024	2160	2172	2202	rBV2	364544	789025	28.67%	4.055%
38	8.490	2315	2317	2321	rVB5	1257	739	0.03%	0.004%
39	8.548	2329	2335	2337	rBV6	1918	1732	0.06%	0.009%
40	8.677	2371	2375	2380	rBV6	780	953	0.03%	0.005%
41	8.776	2395	2406	2435	rBV	1010777	1675326	60.87%	8.609%
42	9.085	2496	2502	2503	rBV5	1843	1878	0.07%	0.010%
43	9.217	2541	2543	2549	rVB5	1601	1181	0.04%	0.006%
44	9.313	2570	2573	2577	rVB4	1367	784	0.03%	0.004%
45	9.339	2577	2581	2585	rVB7	1191	1045	0.04%	0.005%
46	9.365	2585	2589	2592	rVB6	1357	1002	0.04%	0.005%
47	9.465	2614	2620	2622	rBV6	1122	1103	0.04%	0.006%
48	9.657	2677	2680	2681	rBV3	1318	848	0.03%	0.004%
49	9.857	2740	2742	2744	rBV4	1081	758	0.03%	0.004%
50	9.937	2762	2767	2770	rVB5	1362	1335	0.05%	0.007%
51	9.963	2770	2775	2777	rBV6	1793	1050	0.04%	0.005%
52	10.043	2797	2800	2806	rBV7	871	1142	0.04%	0.006%
53	10.146	2820	2832	2858	rBV	652020	1045837	38.00%	5.374%
54	10.313	2879	2884	2893	rBV8	2993	4268	0.16%	0.022%
55	10.423	2913	2918	2919	rBV3	1327	869	0.03%	0.004%
56	10.548	2955	2957	2960	rVB4	1459	782	0.03%	0.004%
57	10.571	2960	2964	2968	rVB6	1704	1327	0.05%	0.007%
58	10.629	2977	2982	2985	rBV5	918	871	0.03%	0.004%
59	10.645	2985	2987	2994	rVB7	985	854	0.03%	0.004%
60	10.690	2997	3001	3006	rBV8	1230	1473	0.05%	0.008%
61	10.780	3026	3029	3031	rBV4	1595	1207	0.04%	0.006%
62	10.825	3038	3043	3045	rVB6	1439	1343	0.05%	0.007%
63	10.850	3045	3051	3053	rBV5	2529	2423	0.09%	0.012%
64	10.940	3076	3079	3082	rVB4	1783	1151	0.04%	0.006%
65	11.117	3130	3134	3135	rVV3	1549	871	0.03%	0.004%
66	11.127	3135	3137	3139	rVV3	2571	1635	0.06%	0.008%
67	11.178	3143	3153	3185	rVV	1007065	1614409	58.66%	8.296%
68	11.442	3227	3235	3239	rBV10	2399	2611	0.09%	0.013%
69	11.471	3240	3244	3246	rBV5	1713	1216	0.04%	0.006%
70	11.510	3248	3256	3258	rBV6	3740	5056	0.18%	0.026%
71	11.555	3258	3270	3302	rVV	1182746	1912905	69.50%	9.830%
72	11.812	3348	3350	3354	rVB5	1765	1124	0.04%	0.006%
73	11.854	3361	3363	3367	rVB5	1141	855	0.03%	0.004%
74	12.079	3429	3433	3438	rVV7	1472	1924	0.07%	0.010%
75	12.191	3464	3468	3469	rBV2	1497	909	0.03%	0.005%
76	12.310	3501	3505	3506	rVV4	1441	900	0.03%	0.005%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV090924\
Data File : VV037232.D
Acq On : 09 Sep 2024 10:20
Operator : SY/MD
Sample : P3843-12
Misc : 5.00mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BHJM7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082624WMA.M
Title : VOC Analysis

77	12.558	3578	3582	3584	rBV6	1222	995	0.04%	0.005%
78	12.583	3585	3590	3594	rBV7	3341	3630	0.13%	0.019%
79	12.709	3626	3629	3632	rVB3	1107	764	0.03%	0.004%
80	12.831	3663	3667	3670	rVB4	1321	1074	0.04%	0.006%
81	12.879	3678	3682	3685	rVV4	1268	1083	0.04%	0.006%
82	12.940	3698	3701	3705	rVV5	988	792	0.03%	0.004%
83	12.960	3705	3707	3712	rVB6	1462	1195	0.04%	0.006%
84	12.985	3712	3715	3718	rBV4	1397	848	0.03%	0.004%
85	13.079	3741	3744	3747	rVB4	1102	838	0.03%	0.004%
86	13.101	3747	3751	3753	rBV3	1069	861	0.03%	0.004%
87	13.156	3765	3768	3772	rVB5	1384	1006	0.04%	0.005%
88	13.204	3776	3783	3791	rBV9	5634	7820	0.28%	0.040%
89	13.394	3838	3842	3845	rBV6	1417	1062	0.04%	0.005%
90	13.448	3850	3859	3877	rVV2	8728	21592	0.78%	0.111%
91	13.529	3879	3884	3886	rVB5	1025	1014	0.04%	0.005%
92	13.683	3925	3932	3941	rBV5	6652	9619	0.35%	0.049%
93	13.815	3971	3973	3980	rVB7	1474	1419	0.05%	0.007%
94	13.943	4011	4013	4018	rVB4	1294	786	0.03%	0.004%
95	14.062	4047	4050	4051	rBV2	1811	1110	0.04%	0.006%
96	14.452	4168	4171	4175	rBV6	872	826	0.03%	0.004%
97	14.709	4249	4251	4255	rBV4	1125	839	0.03%	0.004%
98	14.786	4273	4275	4277	rBV3	1396	823	0.03%	0.004%
99	15.062	4357	4361	4362	rBV4	1767	1143	0.04%	0.006%
100	15.294	4431	4433	4438	rBV5	1520	1093	0.04%	0.006%


Sum of corrected areas: 19460072

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV090924\
Data File : VV037232.D
Acq On : 09 Sep 2024 10:20
Operator : SY/MD
Sample : P3843-12
Misc : 5.00mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BHJM7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

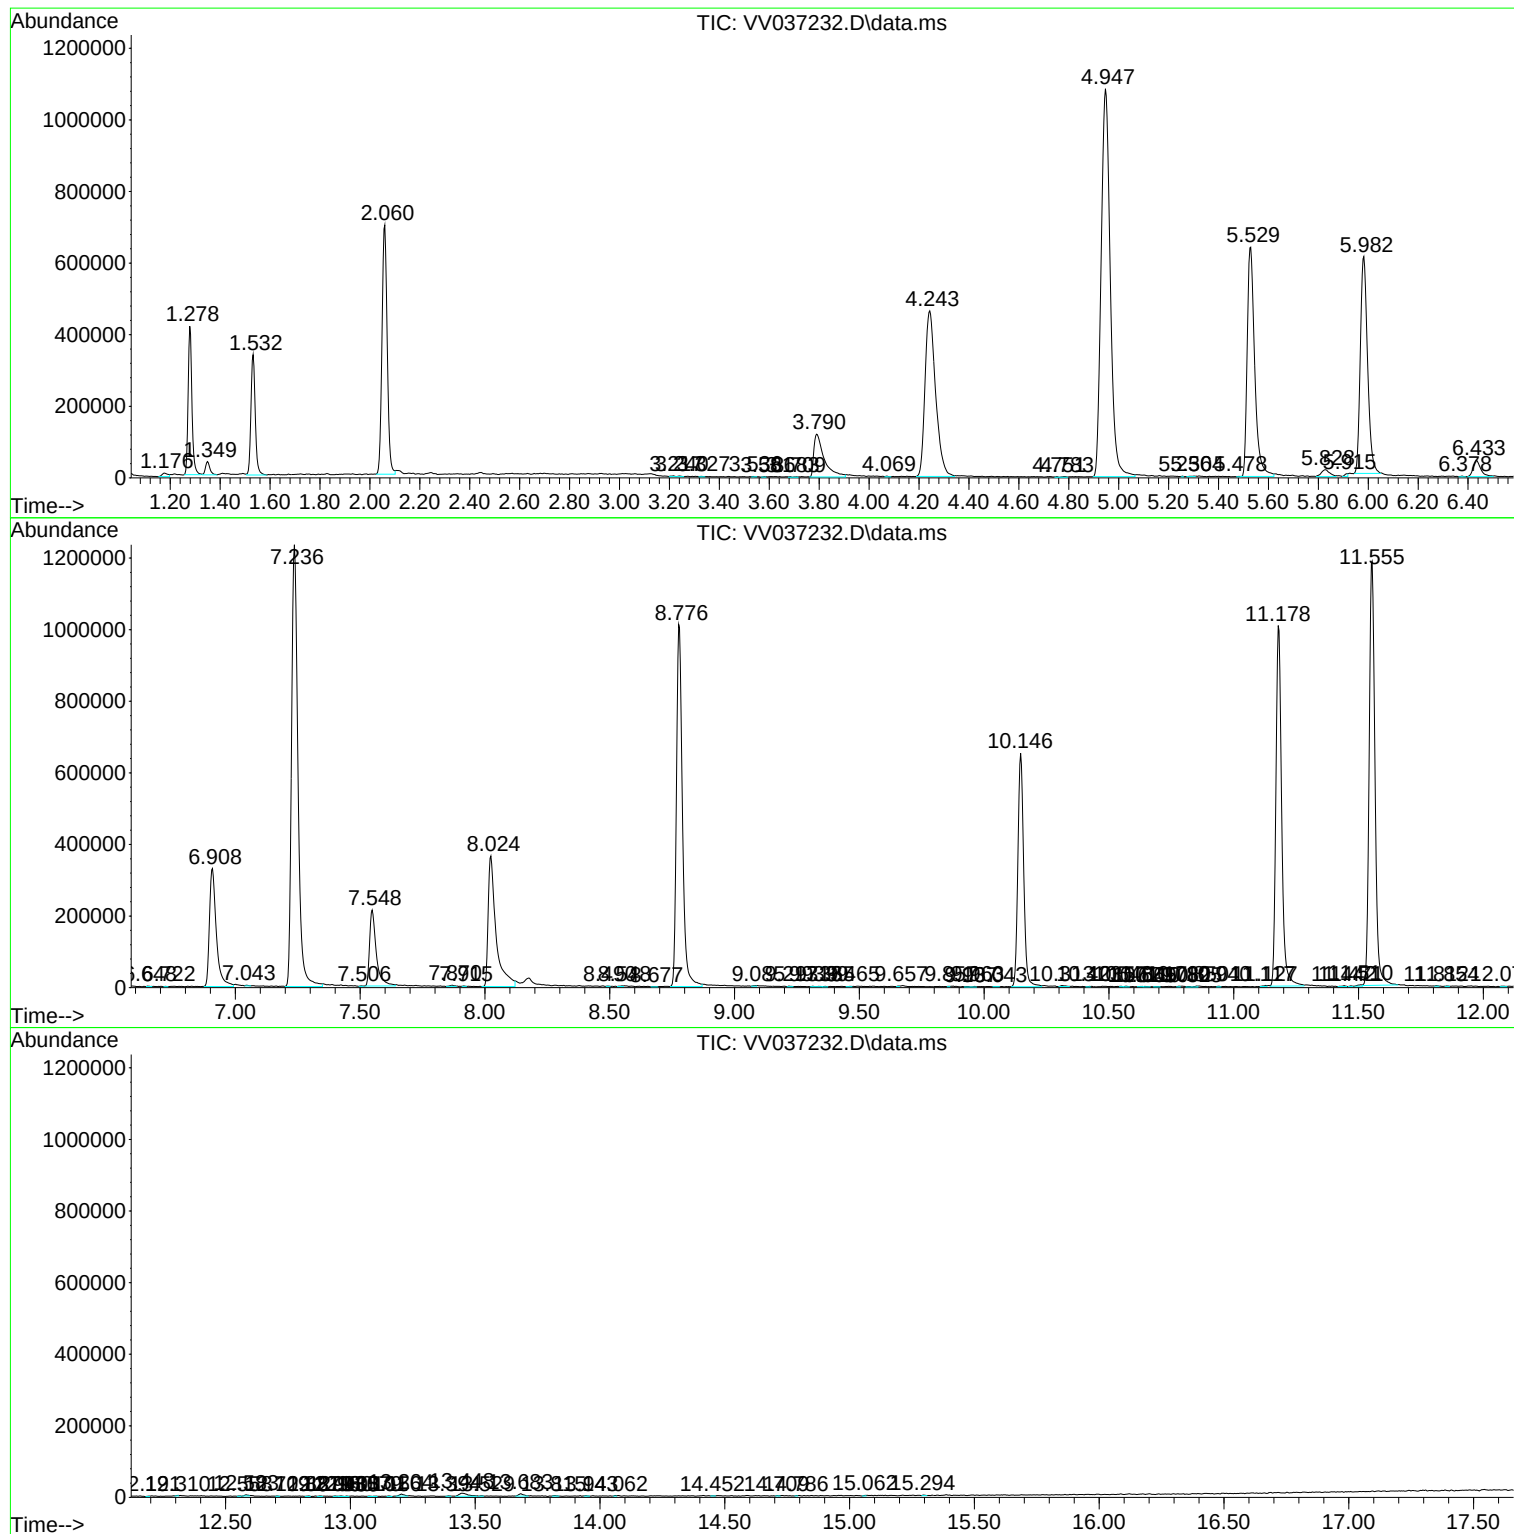

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV090924\
Data File : VV037232.D
Acq On : 09 Sep 2024 10:20
Operator : SY/MD
Sample : P3843-12
Misc : 5.00mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BHJM7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV090924\
Data File : VV037232.D
Acq On : 09 Sep 2024 10:20
Operator : SY/MD
Sample : P3843-12
Misc : 5.00mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BHJM7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------