

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV090924\
 Data File : VV037235.D
 Acq On : 09 Sep 2024 13:37
 Operator : SY/MD
 Sample : VIBLK376
 Misc : 5.00mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK376

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082624WMA.M
 Title : VOC Analysis

Signal : TIC: VV037235.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	68	74	90	rVB	373235	395971	16.08%	2.201%
2	1.532	146	153	168	rVB	309876	358362	14.55%	1.992%
3	2.056	307	316	335	rBV	612332	893098	36.26%	4.965%
4	3.455	749	751	754	rBV5	937	337	0.01%	0.002%
5	3.651	811	812	815	rVB2	977	387	0.02%	0.002%
6	3.735	836	838	839	rBV	605	171	0.01%	0.001%
7	3.789	847	855	880	rBV	99083	277436	11.27%	1.542%
8	4.240	979	995	1028	rBV	385309	987936	40.12%	5.493%
9	4.436	1053	1056	1058	rBV4	1027	542	0.02%	0.003%
10	4.458	1058	1063	1065	rBV4	1707	1455	0.06%	0.008%
11	4.571	1095	1098	1101	rBV4	1137	830	0.03%	0.005%
12	4.780	1159	1163	1164	rBV3	1074	686	0.03%	0.004%
13	4.944	1199	1214	1247	rBV2	958951	2462749	100.00%	13.692%
14	5.465	1372	1376	1378	rBV5	1359	969	0.04%	0.005%
15	5.526	1384	1395	1431	rBV	729744	1521391	61.78%	8.459%
16	5.979	1524	1536	1570	rBV	536594	1119226	45.45%	6.223%
17	6.301	1633	1636	1638	rBV4	1260	857	0.03%	0.005%
18	6.394	1661	1665	1669	rVB4	716	500	0.02%	0.003%
19	6.593	1725	1727	1729	rBV3	1123	490	0.02%	0.003%
20	6.719	1762	1766	1768	rBV4	1364	950	0.04%	0.005%
21	6.751	1774	1776	1780	rBV4	1363	894	0.04%	0.005%
22	6.776	1780	1784	1786	rBV4	1168	813	0.03%	0.005%
23	6.818	1795	1797	1798	rVB2	404	87	0.00%	0.000%
24	6.857	1806	1809	1814	rVB5	863	835	0.03%	0.005%
25	6.905	1814	1824	1848	rBV	285290	550717	22.36%	3.062%
26	7.236	1915	1927	1953	rBV	1089994	1933878	78.53%	10.752%
27	7.548	2015	2024	2055	rBV	184120	344704	14.00%	1.916%
28	7.956	2149	2151	2154	rBV5	805	555	0.02%	0.003%
29	7.973	2154	2156	2160	rVB5	1166	577	0.02%	0.003%
30	8.024	2163	2172	2212	rBV2	306325	680341	27.63%	3.783%
31	8.718	2385	2388	2390	rBV3	1428	950	0.04%	0.005%
32	8.776	2396	2406	2437	rBV	1122377	1850956	75.16%	10.291%
33	9.252	2552	2554	2557	rBV3	871	474	0.02%	0.003%
34	9.371	2587	2591	2593	rBV3	1330	1020	0.04%	0.006%
35	9.477	2622	2624	2628	rBV4	1832	1799	0.07%	0.010%
36	9.625	2668	2670	2672	rBV3	1333	744	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV090924\
 Data File : VV037235.D
 Acq On : 09 Sep 2024 13:37
 Operator : SY/MD
 Sample : VIBLK376
 Misc : 5.00mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK376

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082624WMA.M
 Title : VOC Analysis

37	9.664	2680	2682	2684	rBV3	1135	587	0.02%	0.003%
38	9.728	2700	2702	2705	rBV4	970	523	0.02%	0.003%
39	9.747	2705	2708	2710	rVV4	1161	744	0.03%	0.004%
40	9.773	2714	2716	2719	rVB3	1042	575	0.02%	0.003%
41	9.789	2719	2721	2723	rBV2	722	384	0.02%	0.002%
42	9.821	2727	2731	2737	rVB8	1226	1130	0.05%	0.006%
43	9.853	2737	2741	2743	rBV4	1198	919	0.04%	0.005%
44	9.927	2762	2764	2765	rBV2	423	172	0.01%	0.001%
45	10.050	2798	2802	2804	rBV3	1395	949	0.04%	0.005%
46	10.098	2816	2817	2819	rBV2	743	390	0.02%	0.002%
47	10.146	2821	2832	2847	rVV	584897	910492	36.97%	5.062%
48	10.397	2907	2910	2915	rVV6	838	741	0.03%	0.004%
49	10.432	2918	2921	2926	rBV4	1080	584	0.02%	0.003%
50	10.596	2970	2972	2974	rBV3	1194	560	0.02%	0.003%
51	10.641	2984	2986	2987	rBV3	358	93	0.00%	0.001%
52	10.651	2987	2989	2991	rVB3	830	283	0.01%	0.002%
53	10.667	2991	2994	2995	rBV2	690	300	0.01%	0.002%
54	10.860	3046	3054	3064	rVB4	7056	11866	0.48%	0.066%
55	10.921	3069	3073	3076	rBV4	973	782	0.03%	0.004%
56	10.969	3084	3088	3092	rBV6	1211	1243	0.05%	0.007%
57	10.995	3094	3096	3098	rBV3	450	231	0.01%	0.001%
58	11.040	3109	3110	3112	rBV	652	358	0.01%	0.002%
59	11.082	3121	3123	3125	rBV2	820	275	0.01%	0.002%
60	11.101	3125	3129	3130	rBV3	1423	940	0.04%	0.005%
61	11.133	3132	3139	3142	rVV8	3711	4877	0.20%	0.027%
62	11.178	3142	3153	3188	rVV	1129931	1825411	74.12%	10.149%
63	11.464	3240	3242	3243	rBV	1131	425	0.02%	0.002%
64	11.554	3258	3270	3299	rBV	1037556	1718482	69.78%	9.554%
65	11.905	3377	3379	3380	rBV	1237	521	0.02%	0.003%
66	11.976	3398	3401	3404	rBV4	1128	669	0.03%	0.004%
67	12.005	3408	3410	3411	rBV2	784	330	0.01%	0.002%
68	12.220	3475	3477	3480	rBV4	954	525	0.02%	0.003%
69	12.239	3481	3483	3485	rBV2	1130	461	0.02%	0.003%
70	12.287	3497	3498	3500	rBV2	645	224	0.01%	0.001%
71	12.310	3503	3505	3508	rBV4	757	457	0.02%	0.003%
72	12.349	3513	3517	3518	rBV3	736	520	0.02%	0.003%
73	12.554	3577	3581	3582	rBV4	1292	934	0.04%	0.005%
74	12.586	3586	3591	3594	rBV6	2439	2874	0.12%	0.016%
75	12.943	3698	3702	3705	rBV6	1395	1237	0.05%	0.007%
76	13.053	3733	3736	3738	rBV2	1300	832	0.03%	0.005%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV090924\
Data File : VV037235.D
Acq On : 09 Sep 2024 13:37
Operator : SY/MD
Sample : VIBLK376
Misc : 5.00mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK376

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082624WMA.M

Title : VOC Analysis

77	13.078	3742	3744	3746	rVV3	1116	561	0.02%	0.003%
78	13.091	3746	3748	3754	rVB5	1461	1265	0.05%	0.007%
79	13.204	3775	3783	3794	rBV7	9179	16876	0.69%	0.094%
80	13.374	3828	3836	3846	rVB3	26340	40311	1.64%	0.224%
81	13.445	3849	3858	3874	rBV2	19041	39891	1.62%	0.222%




Sum of corrected areas: 17986491

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV090924\
Data File : VV037235.D
Acq On : 09 Sep 2024 13:37
Operator : SY/MD
Sample : VIBLK376
Misc : 5.00mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK376

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

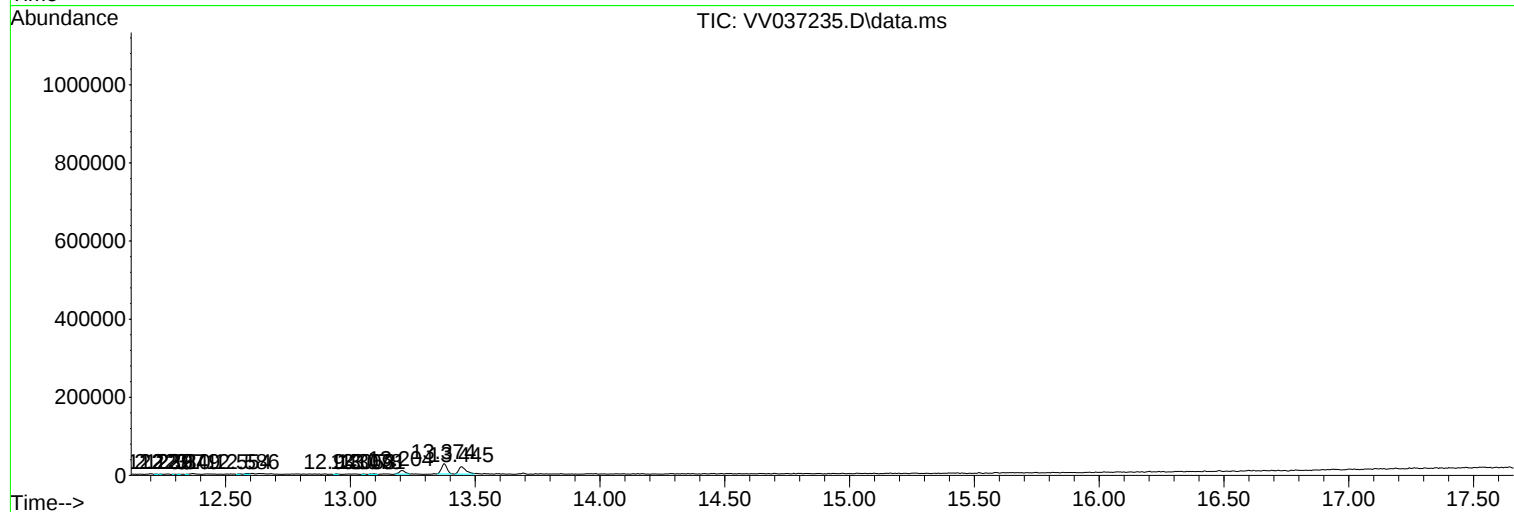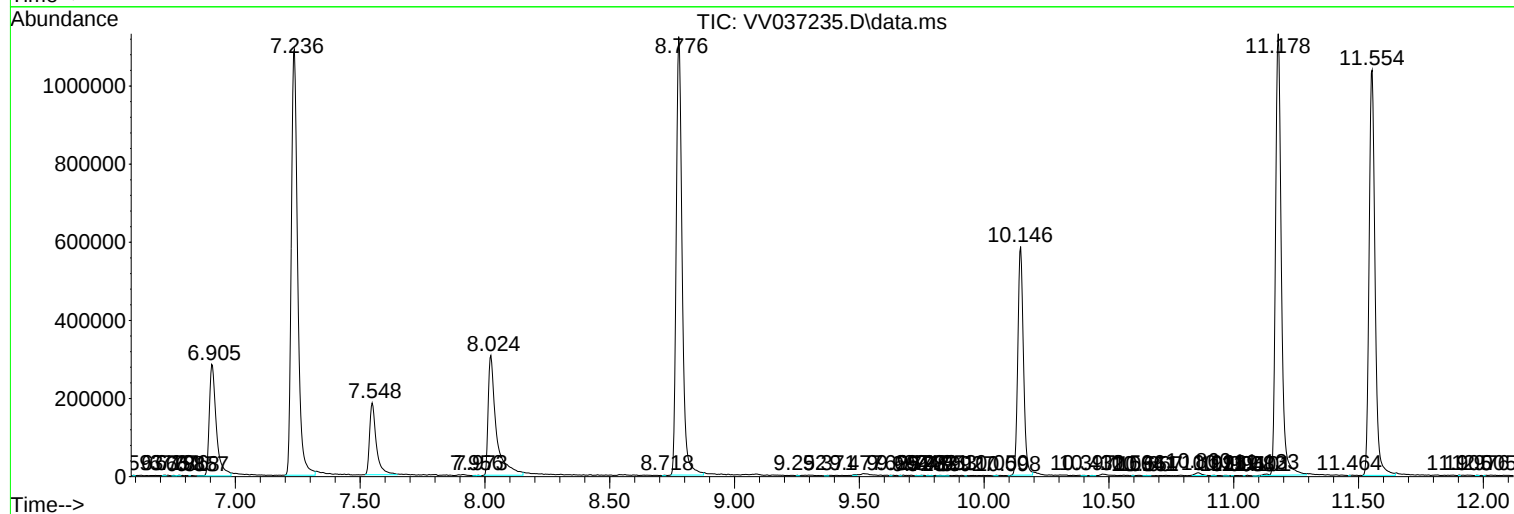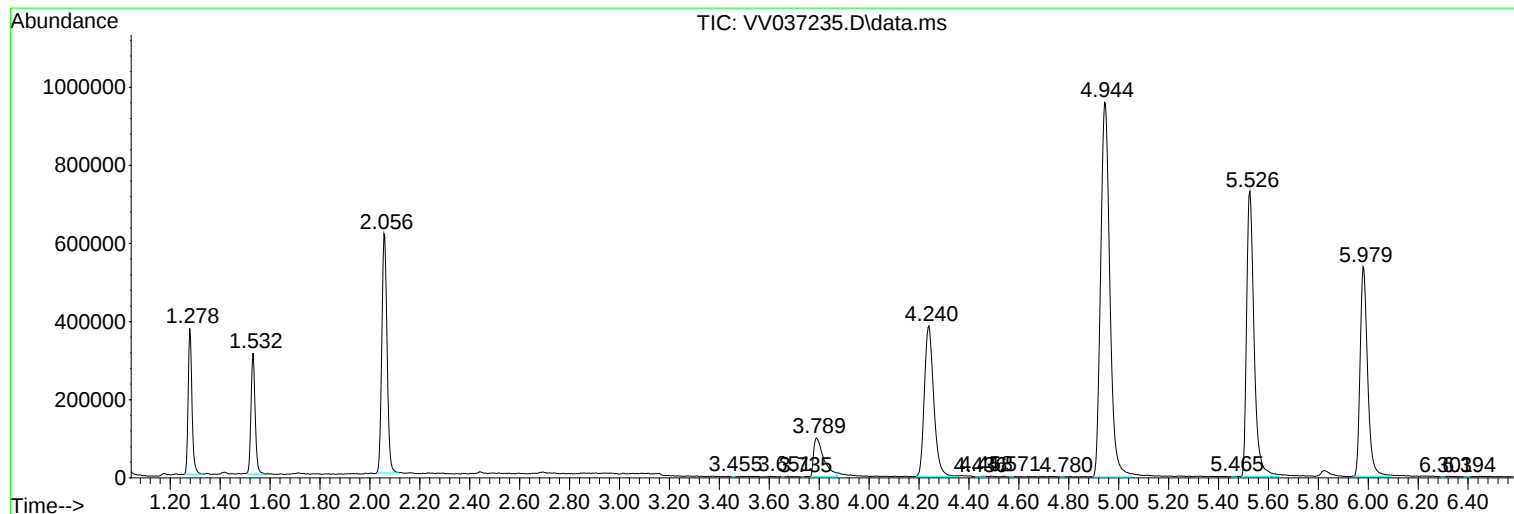

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV090924\
Data File : VV037235.D
Acq On : 09 Sep 2024 13:37
Operator : SY/MD
Sample : VIBLK376
Misc : 5.00mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK376

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV090924\
Data File : VV037235.D
Acq On : 09 Sep 2024 13:37
Operator : SY/MD
Sample : VIBLK376
Misc : 5.00mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK376

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc