

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV090924\
 Data File : VV037236.D
 Acq On : 09 Sep 2024 14:50
 Operator : SY/MD
 Sample : VIBLK377
 Misc : 5.00mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK377

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082624WMA.M
 Title : VOC Analysis

Signal : TIC: VV037236.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.172	37	41	50	rBV	7091	12452	0.54%	0.076%
2	1.278	68	74	88	rVB	346524	368118	15.88%	2.239%
3	1.532	146	153	168	rVB	284900	335848	14.48%	2.043%
4	2.056	307	316	333	rBV	576759	836841	36.09%	5.090%
5	3.526	771	773	777	rBV4	920	527	0.02%	0.003%
6	3.664	814	816	819	rVB2	1040	682	0.03%	0.004%
7	3.680	819	821	823	rBV3	718	482	0.02%	0.003%
8	3.735	835	838	844	rVB6	1073	1046	0.05%	0.006%
9	3.789	844	855	881	rBV	99842	275825	11.90%	1.678%
10	4.240	979	995	1024	rBV	367433	930913	40.15%	5.662%
11	4.596	1105	1106	1108	rBV	598	321	0.01%	0.002%
12	4.645	1117	1121	1123	rBV4	1141	700	0.03%	0.004%
13	4.686	1132	1134	1137	rVB4	801	474	0.02%	0.003%
14	4.715	1140	1143	1144	rBV2	1238	592	0.03%	0.004%
15	4.793	1164	1167	1168	rBV3	1161	500	0.02%	0.003%
16	4.844	1180	1183	1185	rBV3	823	545	0.02%	0.003%
17	4.876	1191	1193	1195	rBV3	587	250	0.01%	0.002%
18	4.947	1199	1215	1255	rVV2	908804	2318796	100.00%	14.103%
19	5.420	1360	1362	1367	rBV6	1239	905	0.04%	0.006%
20	5.526	1384	1395	1425	rBV	621216	1285621	55.44%	7.819%
21	5.982	1524	1537	1564	rBV	504929	1041629	44.92%	6.335%
22	6.326	1641	1644	1648	rBV5	950	778	0.03%	0.005%
23	6.600	1722	1729	1731	rBV6	1406	1685	0.07%	0.010%
24	6.664	1748	1749	1753	rBV3	776	453	0.02%	0.003%
25	6.696	1757	1759	1760	rBV2	724	180	0.01%	0.001%
26	6.831	1799	1801	1802	rBV2	1036	510	0.02%	0.003%
27	6.866	1810	1812	1813	rBV2	724	305	0.01%	0.002%
28	6.908	1814	1825	1857	rVV	263753	522037	22.51%	3.175%
29	7.124	1889	1892	1894	rVB4	1379	829	0.04%	0.005%
30	7.137	1894	1896	1898	rBV3	942	561	0.02%	0.003%
31	7.236	1915	1927	1959	rBV	1012071	1814048	78.23%	11.033%
32	7.548	2013	2024	2054	rBV	174902	338535	14.60%	2.059%
33	8.024	2162	2172	2212	rBV3	293069	673315	29.04%	4.095%
34	8.600	2347	2351	2353	rBV3	1041	776	0.03%	0.005%
35	8.638	2361	2363	2364	rBV2	805	429	0.02%	0.003%
36	8.776	2396	2406	2438	rBV	949680	1592076	68.66%	9.683%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV090924\
 Data File : VV037236.D
 Acq On : 09 Sep 2024 14:50
 Operator : SY/MD
 Sample : VIBLK377
 Misc : 5.00mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK377

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082624WMA.M
 Title : VOC Analysis

37	9.252	2549	2554	2559	rBV8	1291	1495	0.06%	0.009%
38	9.349	2581	2584	2585	rBV2	832	529	0.02%	0.003%
39	9.423	2605	2607	2609	rBV3	798	357	0.02%	0.002%
40	9.622	2666	2669	2672	rBV4	997	847	0.04%	0.005%
41	9.722	2698	2700	2701	rBV2	255	113	0.00%	0.001%
42	9.741	2703	2706	2707	rBV2	873	454	0.02%	0.003%
43	9.802	2723	2725	2729	rVB5	950	464	0.02%	0.003%
44	9.821	2729	2731	2734	rBV6	795	575	0.02%	0.003%
45	9.863	2741	2744	2745	rBV3	1166	637	0.03%	0.004%
46	9.895	2752	2754	2760	rBV4	680	560	0.02%	0.003%
47	9.921	2760	2762	2765	rBV4	1025	572	0.02%	0.003%
48	9.960	2771	2774	2775	rBV2	987	571	0.02%	0.003%
49	10.072	2802	2809	2810	rBV3	1391	1204	0.05%	0.007%
50	10.104	2817	2819	2820	rBV	596	291	0.01%	0.002%
51	10.146	2820	2832	2852	rBV	550685	879043	37.91%	5.346%
52	10.352	2894	2896	2899	rBV4	863	425	0.02%	0.003%
53	10.394	2907	2909	2914	rVB3	1464	869	0.04%	0.005%
54	10.516	2945	2947	2949	rBV3	886	374	0.02%	0.002%
55	10.644	2985	2987	2988	rBV2	967	417	0.02%	0.003%
56	10.686	2997	3000	3001	rBV2	1288	791	0.03%	0.005%
57	10.760	3020	3023	3025	rBV5	1014	590	0.03%	0.004%
58	10.853	3046	3052	3055	rBV6	3080	3208	0.14%	0.020%
59	10.976	3085	3090	3092	rBV4	1024	721	0.03%	0.004%
60	10.998	3095	3097	3100	rBV2	778	515	0.02%	0.003%
61	11.043	3109	3111	3113	rVB4	730	354	0.02%	0.002%
62	11.059	3113	3116	3118	rBV3	1124	783	0.03%	0.005%
63	11.085	3121	3124	3126	rBV3	622	416	0.02%	0.003%
64	11.111	3126	3132	3134	rBV5	1720	1712	0.07%	0.010%
65	11.178	3142	3153	3181	rBV	961805	1552651	66.96%	9.444%
66	11.554	3259	3270	3297	rBV	977789	1601816	69.08%	9.743%
67	11.895	3373	3376	3378	rBV4	1138	689	0.03%	0.004%
68	11.950	3391	3393	3396	rBV3	1145	609	0.03%	0.004%
69	12.104	3437	3441	3442	rBV3	800	483	0.02%	0.003%
70	12.162	3457	3459	3464	rVB6	1154	702	0.03%	0.004%
71	12.188	3464	3467	3469	rBV4	1177	705	0.03%	0.004%
72	12.204	3469	3472	3474	rBV4	762	478	0.02%	0.003%
73	12.268	3490	3492	3494	rBV2	581	204	0.01%	0.001%
74	12.320	3506	3508	3511	rBV4	1116	494	0.02%	0.003%
75	12.416	3536	3538	3542	rBV4	998	707	0.03%	0.004%
76	12.574	3584	3587	3588	rBV2	1164	692	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV090924\
Data File : VV037236.D
Acq On : 09 Sep 2024 14:50
Operator : SY/MD
Sample : VIBLK377
Misc : 5.00mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK377

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082624WMA.M

Title : VOC Analysis

77	12.670	3615	3617	3619	rVB	818	224	0.01%	0.001%
78	12.686	3619	3622	3624	rBV4	1126	836	0.04%	0.005%
79	12.709	3628	3629	3630	rBV	816	296	0.01%	0.002%
80	12.741	3637	3639	3643	rVB4	1268	510	0.02%	0.003%
81	12.927	3692	3697	3698	rBV4	1339	1276	0.06%	0.008%
82	13.043	3729	3733	3734	rBV4	1490	977	0.04%	0.006%
83	13.095	3747	3749	3750	rBV2	1242	432	0.02%	0.003%
84	13.349	3825	3828	3829	rBV2	749	479	0.02%	0.003%
85	13.377	3829	3837	3844	rVV9	10167	14976	0.65%	0.091%
86	13.783	3958	3963	3964	rBV4	1779	1590	0.07%	0.010%
87	14.033	4039	4041	4043	rBV4	881	502	0.02%	0.003%
88	14.795	4276	4278	4279	rBV2	1397	672	0.03%	0.004%


Sum of corrected areas: 16441471

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV090924\
Data File : VV037236.D
Acq On : 09 Sep 2024 14:50
Operator : SY/MD
Sample : VIBLK377
Misc : 5.00mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK377

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

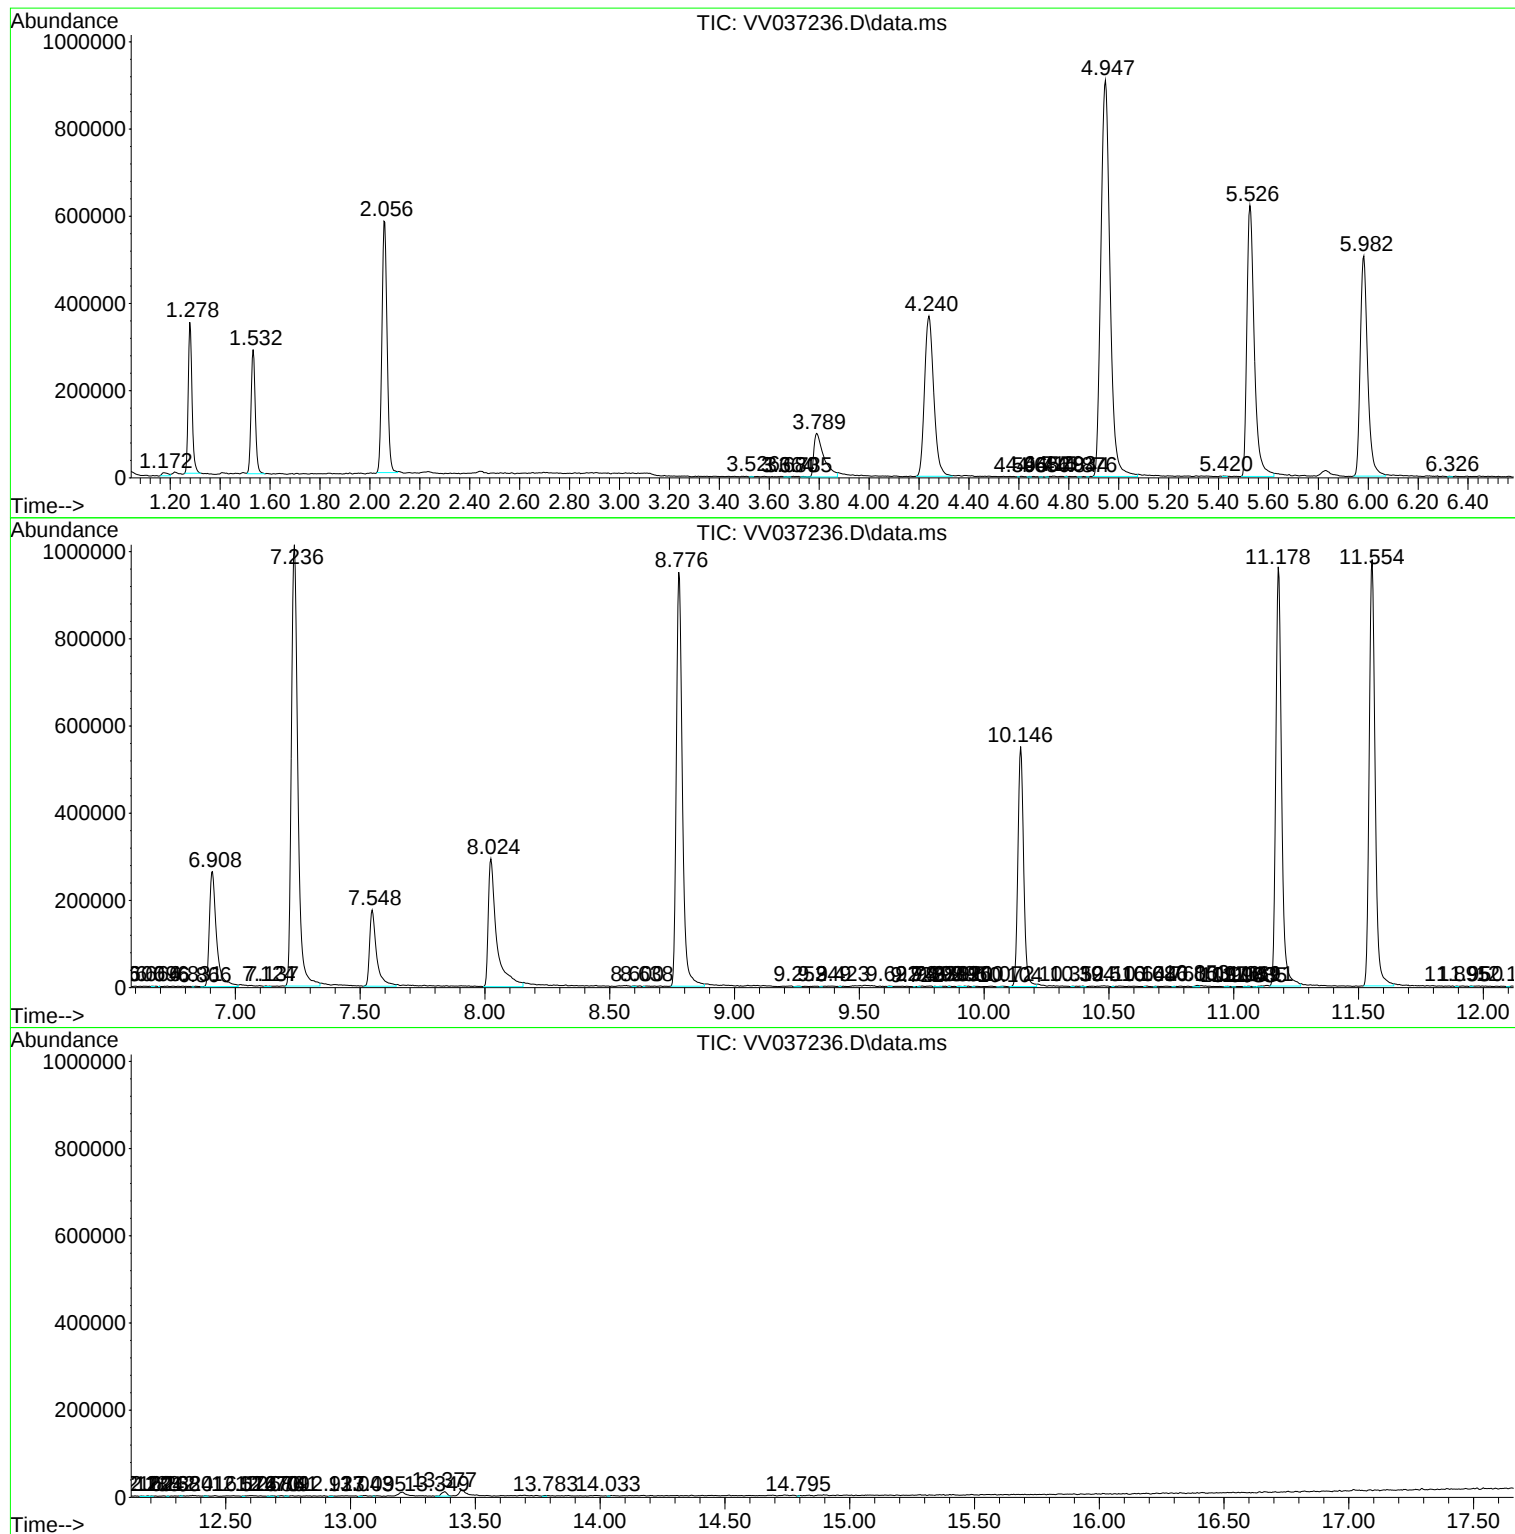

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV090924\
Data File : VV037236.D
Acq On : 09 Sep 2024 14:50
Operator : SY/MD
Sample : VIBLK377
Misc : 5.00mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK377

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV090924\
Data File : VV037236.D
Acq On : 09 Sep 2024 14:50
Operator : SY/MD
Sample : VIBLK377
Misc : 5.00mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK377

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc