
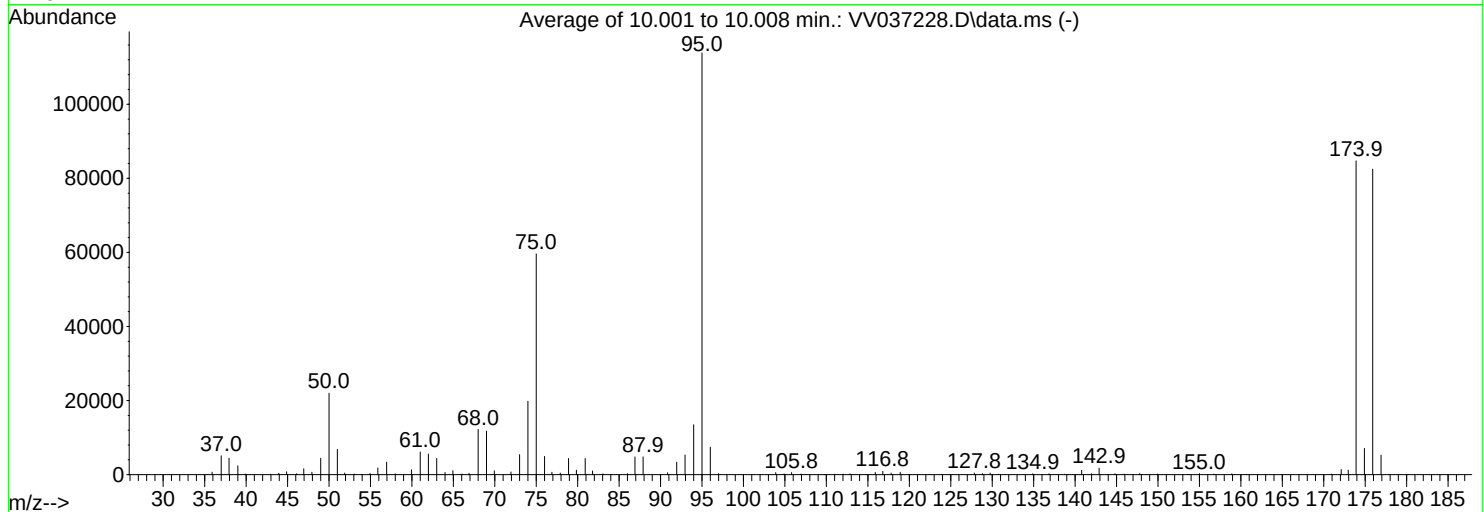


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV090924\
Data File : VV037228.D
Acq On : 09 Sep 2024 07:55
Operator : SY/MD
Sample : BFB376
Misc : 5.00mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB376

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082624WMA.M
Title : VOC Analysis
Last Update : Mon Sep 09 22:02:35 2024

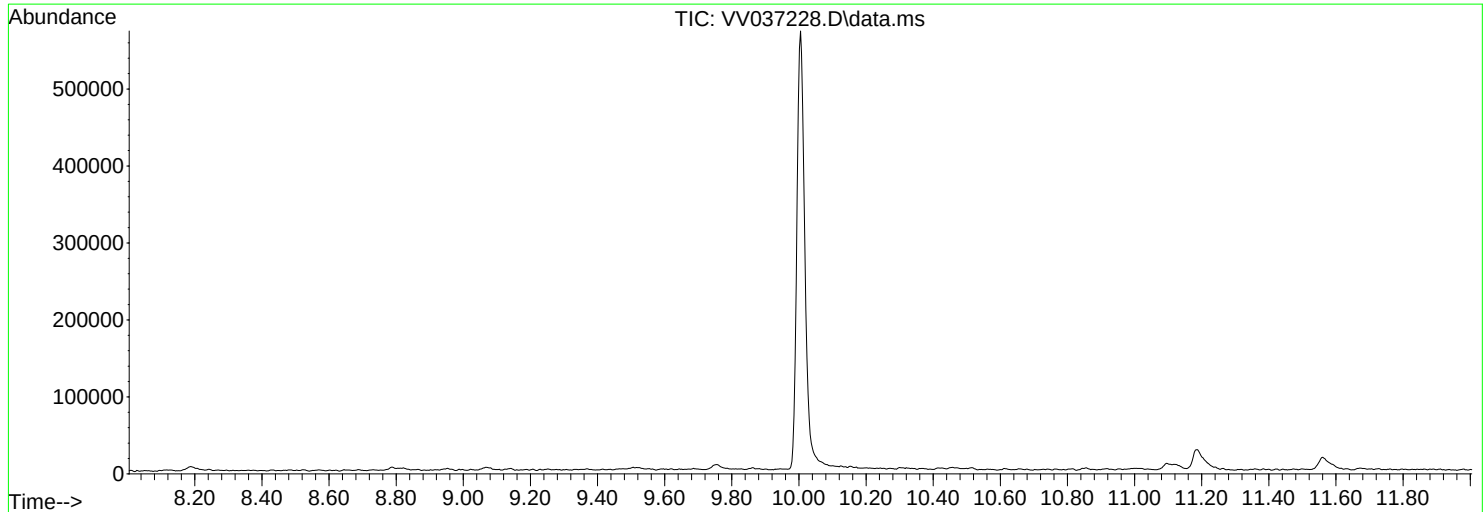

AutoFind: Scans 2787, 2788, 2789; Background Corrected with Scan 2776

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	19.3	22011	PASS
75	95	30	80	52.4	59616	PASS
95	95	100	100	100.0	113875	PASS
96	95	5	9	6.5	7443	PASS
173	174	0.00	2	1.5	1229	PASS
174	95	50	120	74.4	84707	PASS
175	174	5	9	8.4	7080	PASS
176	174	95	105	97.4	82483	PASS
177	176	5	10	6.4	5287	PASS

m/z	Abundance
35.90	1954.0
37.90	837.0
39.10	184.0
40.00	272.0
40.90	207.0
41.80	161.0
42.90	199.0
43.90	830.0
44.90	147.0
48.30	112.0
49.00	116.0
52.80	176.0
54.80	141.0
55.90	111.0
57.10	113.0
68.10	159.0
76.90	113.0
78.00	163.0
79.70	131.0

Instrument :
MSVOA_V
ClientSampleId :
BFB376

m/z	Abundance
36.00	2664.0
37.00	4933.0
38.00	5388.0
39.00	2633.0
39.90	418.0
41.00	216.0
43.00	369.0
44.00	1296.0
44.90	991.0
46.20	289.0
46.90	1605.0
48.00	669.0
49.00	4594.0
50.00	22200.0
51.00	6660.0
51.90	469.0
53.10	231.0
53.90	119.0
55.00	449.0
55.90	1921.0
57.00	3396.0
58.00	187.0
60.00	1267.0
61.00	6039.0
62.00	5821.0
63.00	4291.0
64.00	560.0
64.90	1074.0
66.10	192.0
66.90	507.0
68.00	12640.0
69.00	11747.0
69.90	1025.0
72.00	861.0
73.00	5124.0
74.00	20216.0
75.00	59112.0
76.00	4797.0
77.00	808.0
77.90	485.0
78.90	4282.0
79.90	1447.0
80.90	4480.0
81.80	979.0
83.00	243.0
86.10	231.0
86.90	4876.0
87.90	5009.0
90.90	560.0
92.00	3432.0
92.90	5358.0
94.00	13514.0
95.00	113264.0
96.00	7326.0
97.00	201.0
103.90	525.0
104.90	257.0
105.80	622.0
106.90	151.0
109.80	115.0
111.00	153.0
112.00	144.0
112.90	203.0
115.90	571.0
116.80	917.0
117.80	376.0
118.90	635.0
127.90	449.0
128.80	305.0
129.70	345.0
130.80	121.0
134.90	227.0
136.90	291.0
138.70	177.0
139.20	118.0
140.00	106.0
140.80	1120.0
142.00	285.0
142.90	1529.0
143.90	113.0
144.80	290.0
145.90	239.0
147.80	365.0
150.00	200.0
155.00	309.0
156.70	185.0
159.00	160.0
160.80	179.0
171.00	181.0
172.10	1309.0
173.00	1330.0
173.90	82600.0

Instrument :
MSVOA_V
ClientSampleId :
BFB376

174.90	6945.0
175.90	79352.0
176.90	5295.0
177.90	139.0

Instrument :
MSVOA_V
ClientSampleId :
BFB376

m/z	Abundance
36.00	2612.0
37.00	5243.0
38.00	5355.0
39.00	2666.0
39.90	462.0
40.90	171.0
43.00	333.0
44.00	1221.0
44.90	945.0
46.10	257.0
47.00	1703.0
48.00	627.0
49.00	4636.0
50.00	22896.0
51.00	7087.0
51.90	427.0
53.10	200.0
53.90	117.0
55.00	481.0
56.00	2028.0
56.90	3628.0
58.00	233.0
60.00	1339.0
61.00	6450.0
62.00	5673.0
63.00	4382.0
64.00	632.0
64.90	1149.0
66.10	157.0
66.90	376.0
68.00	12806.0
69.00	12062.0
69.90	1059.0
72.00	746.0
73.00	5582.0
74.00	20272.0
75.00	61424.0
76.00	4975.0
77.00	773.0
77.90	606.0
78.90	4475.0
79.90	1411.0
80.90	4505.0
81.80	1014.0
83.10	243.0
86.00	272.0
86.90	4924.0
87.90	4920.0
90.80	518.0
91.90	3431.0
93.00	5506.0
94.00	13730.0
95.00	117632.0
96.00	7560.0
97.00	279.0
103.90	593.0
104.90	252.0
105.80	569.0
106.90	176.0
109.70	105.0
110.90	132.0
112.00	162.0
112.90	221.0
115.90	616.0
116.80	914.0
117.80	449.0
118.90	682.0
123.80	120.0
127.90	441.0
128.80	346.0
129.80	397.0
130.80	131.0
134.90	311.0
136.80	295.0
138.80	166.0
140.10	107.0
140.80	1200.0
142.00	216.0
142.90	1917.0
144.80	285.0
145.90	191.0
147.80	344.0
149.90	205.0
153.00	103.0
153.60	104.0
155.00	308.0
156.80	177.0
158.80	159.0
159.10	153.0
160.60	139.0
171.00	172.0
172.10	1444.0

Instrument :
MSVOA_V
ClientSampleId :
BFB376

172.90	1259.0
173.90	87384.0
174.90	7334.0
175.90	85368.0
176.90	5395.0
177.80	103.0

Instrument :
MSVOA_V
ClientSampleId :
BFB376

m/z	Abundance
36.00	2617.0
37.00	5152.0
38.00	5097.0
39.00	2324.0
39.90	440.0
40.80	153.0
41.60	101.0
43.00	319.0
44.00	1197.0
44.90	819.0
46.00	211.0
47.00	1494.0
47.90	655.0
49.00	4285.0
50.00	20936.0
51.00	6792.0
51.90	361.0
53.00	152.0
55.00	465.0
56.00	1855.0
56.90	3442.0
58.00	259.0
59.90	1293.0
61.00	5986.0
62.00	5213.0
63.00	4391.0
64.00	628.0
65.00	1024.0
66.00	132.0
66.90	318.0
68.00	11673.0
69.00	11400.0
70.00	1057.0
71.90	652.0
73.00	5453.0
74.00	18992.0
75.00	58312.0
76.00	5026.0
76.90	720.0
77.90	684.0
78.90	4317.0
79.90	1229.0
80.90	4106.0
81.80	965.0
83.10	214.0
84.10	122.0
85.90	243.0
86.90	4612.0
87.90	4490.0
90.80	439.0
92.00	3199.0
92.90	5100.0
94.00	13241.0
95.00	110728.0
96.00	7442.0
97.00	357.0
103.90	545.0
104.90	190.0
105.80	487.0
107.00	168.0
110.90	136.0
112.10	145.0
112.80	206.0
114.80	125.0
115.90	606.0
116.80	910.0
117.80	457.0
118.90	656.0
122.60	133.0
123.90	140.0
127.80	383.0
128.80	252.0
129.80	495.0
130.80	128.0
134.90	311.0
136.80	237.0
138.80	107.0
140.80	1225.0
141.90	156.0
142.90	1879.0
144.80	251.0
145.80	138.0
147.80	270.0
149.90	145.0
153.80	120.0
155.00	272.0
156.80	198.0
158.80	140.0
159.20	107.0
170.80	165.0
172.10	1349.0
172.90	1099.0

Instrument :
MSVOA_V
ClientSampleId :
BFB376

173.90	84136.0
174.90	6960.0
175.90	82728.0
176.90	5171.0

Instrument :
MSVOA_V
ClientSampleId :
BFB376