
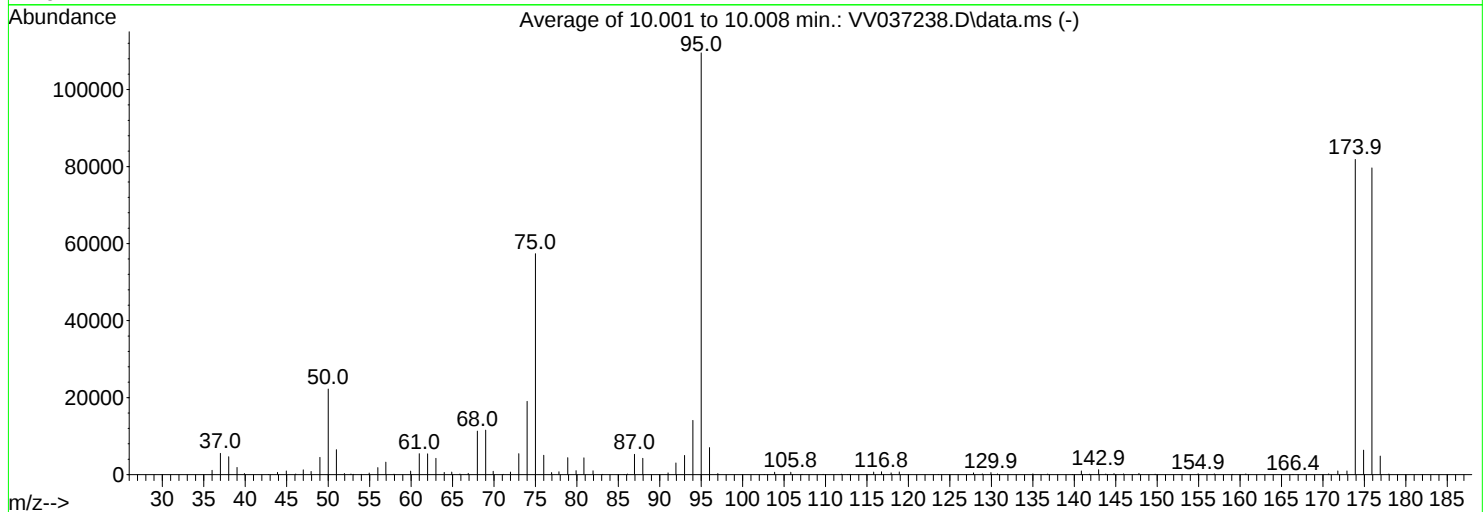


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091024\
Data File : VV037238.D
Acq On : 10 Sep 2024 08:04
Operator : SY/MD
Sample : BFB273
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB273

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR091024WMA.M
Title : TRACE VOA SFAM1.0
Last Update : Wed Sep 11 04:56:42 2024

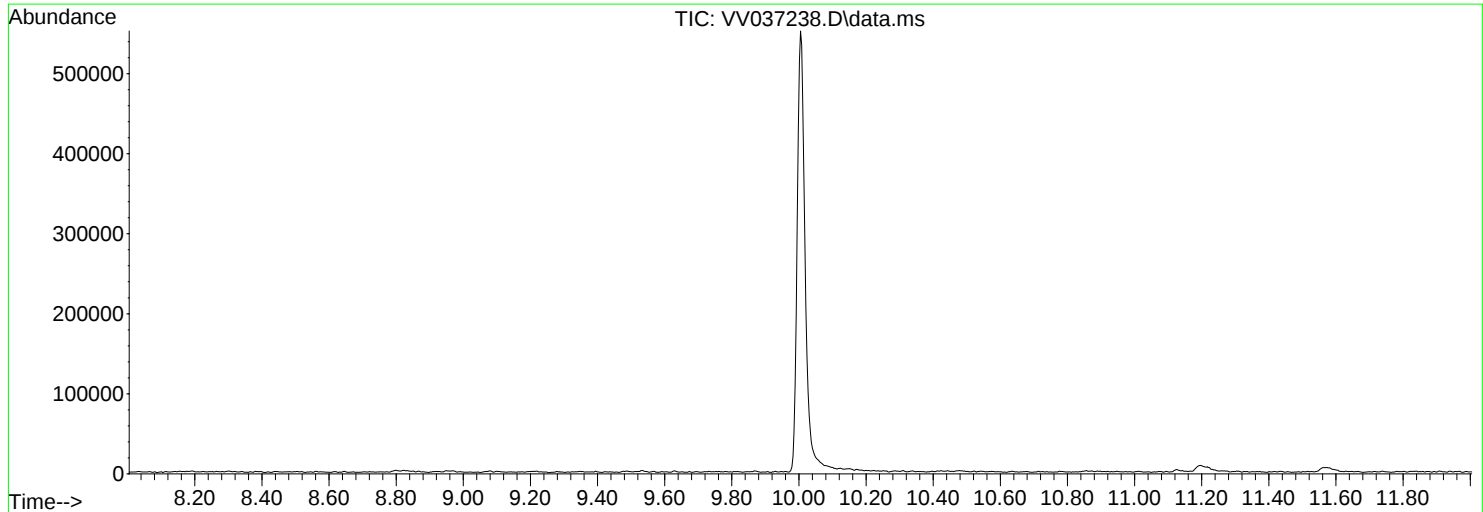

AutoFind: Scans 2787, 2788, 2789; Background Corrected with Scan 2776

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.3	22235	PASS
75	95	30	80	52.4	57397	PASS
95	95	100	100	100.0	109528	PASS
96	95	5	9	6.4	7021	PASS
173	174	0.00	2	1.2	967	PASS
174	95	50	120	74.7	81853	PASS
175	174	5	9	7.8	6357	PASS
176	174	95	105	97.3	79669	PASS
177	176	5	10	6.1	4823	PASS

m/z	Abundance
37.70	150.0
38.40	116.0
39.00	128.0
40.00	245.0
41.00	153.0
42.00	180.0
42.80	124.0
44.00	626.0
45.60	118.0
59.10	119.0
60.00	105.0
76.80	177.0
109.70	117.0
207.00	110.0

Instrument :
MSVOA_V
ClientSampleId :
BFB273

m/z	Abundance
36.00	985.0
37.00	5504.0
38.00	4530.0
39.00	2089.0
39.90	492.0
41.10	102.0
42.80	154.0
43.90	1070.0
44.90	1008.0
46.10	197.0
47.00	1089.0
47.90	724.0
49.00	4432.0
50.00	21520.0
51.00	6710.0
52.00	287.0
52.70	128.0
53.10	133.0
54.90	419.0
56.00	1778.0
56.90	3321.0
57.90	102.0
60.00	1004.0
61.00	5522.0
62.00	5040.0
63.00	4358.0
64.00	618.0
64.90	747.0
66.00	130.0
66.90	316.0
68.00	10985.0
69.00	11456.0
69.90	858.0
72.00	611.0
73.00	5648.0
74.00	18712.0
75.00	55120.0
76.00	4975.0
77.10	820.0
77.90	637.0
78.90	4211.0
79.90	1074.0
80.90	4169.0
82.00	947.0
83.10	162.0
86.10	169.0
86.90	4979.0
87.90	4244.0
91.00	418.0
91.90	3068.0
93.00	4520.0
94.00	13618.0
95.00	106272.0
96.00	7070.0
97.00	258.0
102.60	105.0
103.80	602.0
105.80	621.0
109.70	198.0
111.90	118.0
113.00	144.0
114.90	124.0
115.80	615.0
116.80	776.0
117.90	411.0
118.90	679.0
123.60	115.0
127.90	404.0
128.90	163.0
129.90	512.0
130.70	225.0
135.00	201.0
136.70	133.0
139.80	118.0
140.90	829.0
141.80	109.0
143.00	1194.0
143.80	144.0
144.80	249.0
146.00	192.0
147.80	339.0
149.70	134.0
154.90	214.0
156.90	232.0
159.10	110.0
160.70	185.0
170.70	191.0
171.80	788.0
172.90	948.0
173.90	77496.0
174.90	6061.0
175.90	76120.0

Instrument :
MSVOA_V
ClientSampleId :
BFB273

176.904543.0

177.90109.0

Instrument :
MSVOA_V
ClientSampleId :
BFB273

m/z	Abundance
36.00	1146.0
37.00	5690.0
38.00	4826.0
39.00	2077.0
39.90	538.0
41.00	109.0
42.80	163.0
43.90	1213.0
44.90	947.0
46.10	160.0
47.00	1275.0
47.90	865.0
49.00	4616.0
50.00	23192.0
51.00	6739.0
51.90	319.0
52.70	128.0
53.00	140.0
54.00	122.0
54.90	435.0
56.00	1905.0
57.00	3366.0
58.00	141.0
59.90	1022.0
61.00	5701.0
62.00	5706.0
63.00	4307.0
64.00	560.0
64.90	667.0
65.90	156.0
66.90	343.0
68.00	11576.0
69.00	11854.0
69.90	891.0
71.10	102.0
72.00	700.0
73.00	5649.0
74.00	19728.0
75.00	59672.0
76.00	5251.0
77.00	721.0
77.80	765.0
78.90	4634.0
79.90	1084.0
80.90	4513.0
81.90	984.0
83.10	150.0
86.10	175.0
86.90	5599.0
88.00	4219.0
91.00	486.0
92.00	3140.0
93.00	5299.0
94.00	14632.0
95.00	113496.0
96.00	7356.0
97.00	297.0
103.90	665.0
105.80	667.0
107.10	120.0
109.70	240.0
111.90	150.0
112.90	131.0
114.90	121.0
115.80	735.0
116.80	749.0
117.90	362.0
118.90	750.0
127.80	472.0
128.90	213.0
129.90	572.0
130.80	204.0
135.00	225.0
136.80	163.0
140.80	955.0
141.90	152.0
142.90	1360.0
143.80	171.0
144.80	330.0
146.00	251.0
147.80	333.0
149.80	151.0
153.10	140.0
154.90	242.0
156.90	228.0
159.10	123.0
160.70	222.0
170.70	250.0
171.80	999.0
172.90	979.0
173.90	84200.0
174.90	6588.0

Instrument :
MSVOA_V
ClientSampleId :
BFB273

175.90	82392.0
176.90	5026.0
177.90	153.0

Instrument :
MSVOA_V
ClientSampleId :
BFB273

m/z	Abundance
36.00	1185.0
37.00	5391.0
38.00	4659.0
39.00	1855.0
39.90	554.0
41.00	122.0
42.90	144.0
43.90	1362.0
45.00	926.0
46.10	177.0
47.00	1398.0
48.00	878.0
49.00	4485.0
50.00	21992.0
51.00	5964.0
51.90	336.0
52.80	187.0
54.00	115.0
55.00	395.0
56.00	1835.0
57.00	3073.0
58.00	182.0
59.90	1019.0
61.00	5176.0
62.00	5509.0
63.00	4096.0
64.00	542.0
64.90	567.0
65.80	168.0
66.90	356.0
68.00	11340.0
69.00	11308.0
69.90	874.0
71.10	112.0
72.00	655.0
73.00	5077.0
74.00	18680.0
75.00	57400.0
76.00	4908.0
76.90	671.0
77.80	839.0
78.90	4428.0
79.90	1027.0
80.80	4459.0
81.90	1012.0
85.70	123.0
86.10	188.0
87.00	5315.0
88.00	4208.0
91.00	507.0
92.00	2955.0
93.00	5201.0
94.00	14049.0
95.00	108816.0
96.00	6636.0
97.00	316.0
103.90	623.0
105.20	125.0
105.80	648.0
107.20	136.0
109.70	235.0
111.90	144.0
112.70	126.0
115.80	703.0
116.70	767.0
117.70	312.0
118.00	316.0
118.90	719.0
127.80	499.0
128.90	265.0
130.00	550.0
130.80	195.0
135.00	216.0
136.90	210.0
140.80	1082.0
141.90	172.0
142.90	1369.0
143.80	167.0
144.80	357.0
145.90	239.0
147.80	314.0
149.80	154.0
152.80	102.0
153.10	113.0
155.00	273.0
156.90	168.0
160.70	201.0
166.40	105.0
170.70	229.0
171.80	1044.0
172.90	974.0
173.90	83864.0

Instrument :
MSVOA_V
ClientSampleId :
BFB273

174.90	6421.0
175.90	80496.0
176.90	4900.0
178.00	195.0

Instrument :
MSVOA_V
ClientSampleId :
BFB273