

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091124\
 Data File : VV037250.D
 Acq On : 11 Sep 2024 10:42
 Operator : SY/MD
 Sample : VV0911WBL01
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK240

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR091024WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV037250.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.275	66	73	90	rVV	138013	152474	12.58%	1.521%
2	1.529	144	152	163	rBV	148261	171867	14.18%	1.714%
3	2.053	305	315	329	rBV	273923	398172	32.86%	3.971%
4	2.442	424	436	446	rBV2	9820	18275	1.51%	0.182%
5	3.847	859	873	914	rBV2	73274	435544	35.95%	4.344%
6	4.243	981	996	1027	rVB	196168	520004	42.92%	5.186%
7	4.950	1200	1216	1246	rBV2	466673	1198168	98.89%	11.950%
8	5.529	1386	1396	1423	rBV	349207	767771	63.36%	7.658%
9	5.986	1524	1538	1569	rBV2	264292	589418	48.65%	5.879%
10	6.915	1815	1827	1849	rBV2	95566	210626	17.38%	2.101%
11	7.239	1915	1928	1963	rBV	514645	987437	81.49%	9.849%
12	7.558	2016	2027	2051	rBV2	51738	123247	10.17%	1.229%
13	8.030	2163	2174	2220	rBV	486452	1211667	100.00%	12.085%
14	8.780	2396	2407	2438	rBV	559925	997408	82.32%	9.948%
15	10.149	2822	2833	2853	rBV	209643	352472	29.09%	3.516%
16	11.181	3144	3154	3176	rBV	578621	962045	79.40%	9.595%
17	11.554	3259	3270	3294	rBV	526982	893542	73.74%	8.912%
18	13.207	3776	3784	3798	rBV	6747	14426	1.19%	0.144%
19	13.455	3853	3861	3872	rBV	9870	21569	1.78%	0.215%




Sum of corrected areas: 10026132

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091124\
Data File : VV037250.D
Acq On : 11 Sep 2024 10:42
Operator : SY/MD
Sample : VV0911WBL01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK240

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR091024WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

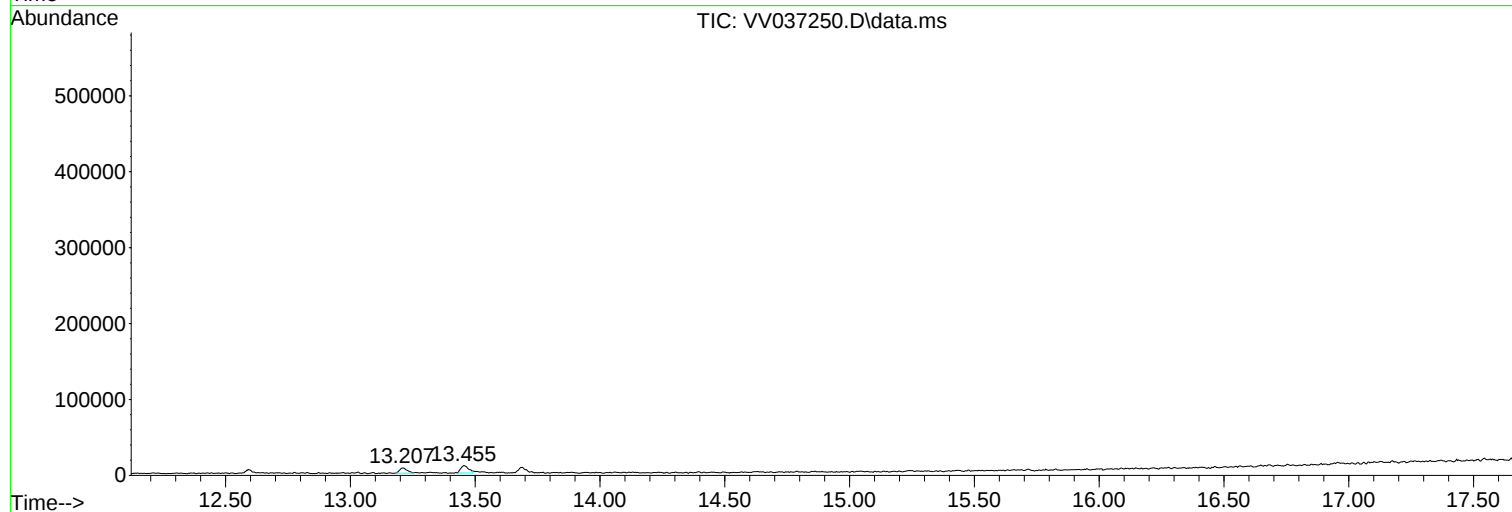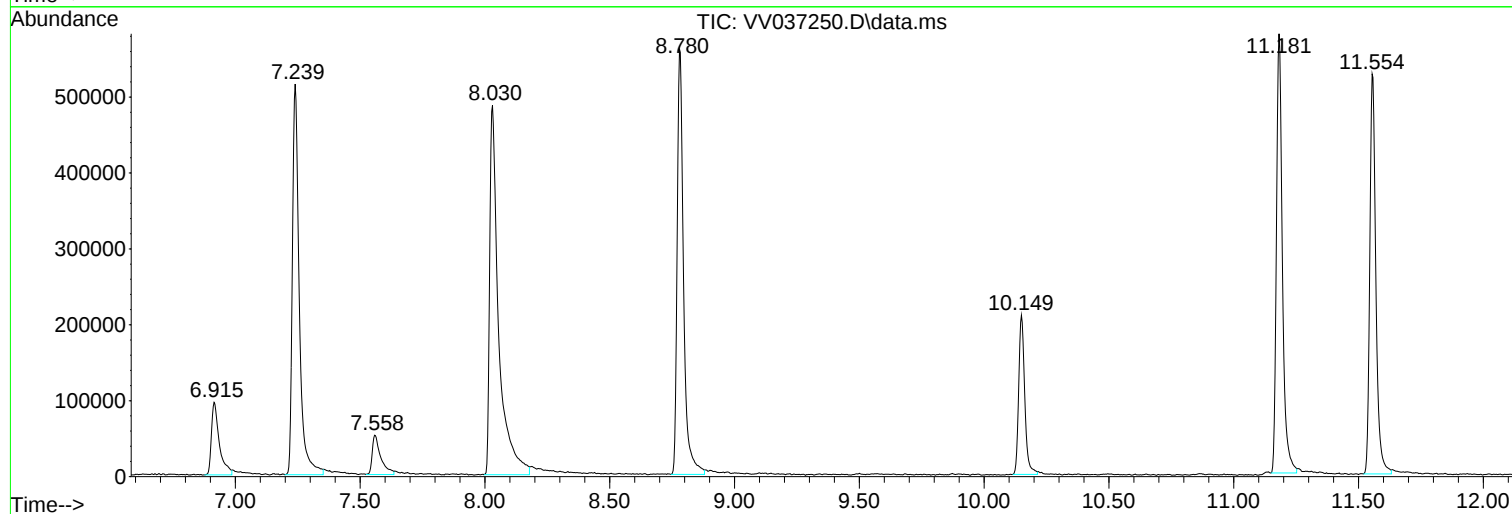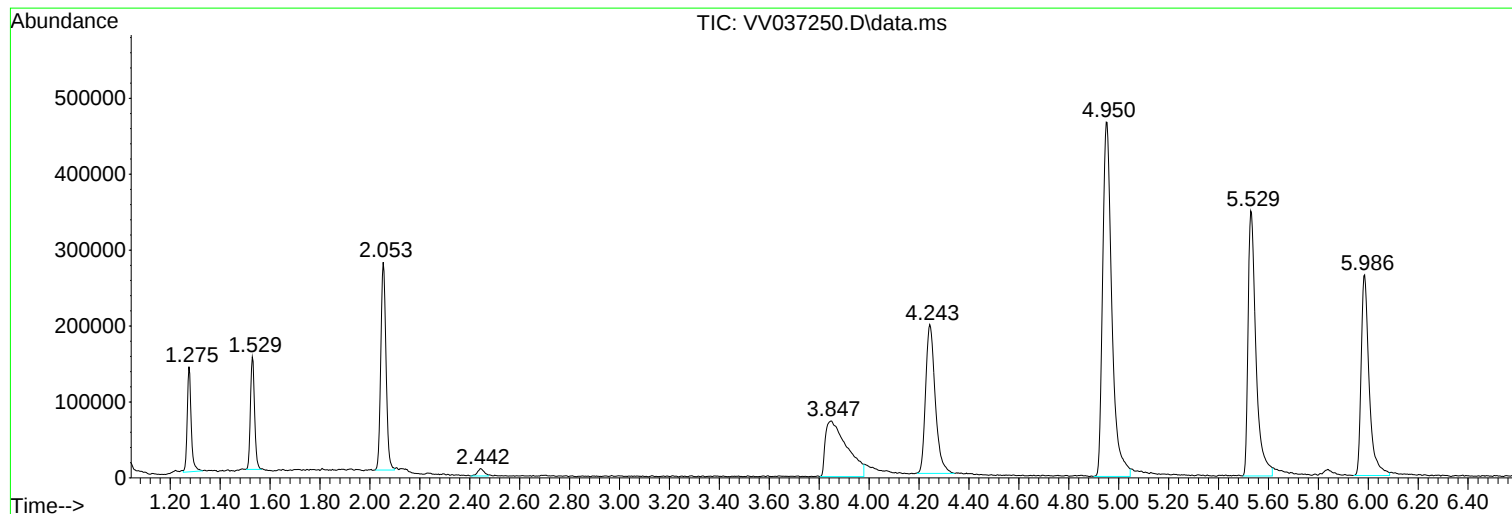

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091124\
Data File : VV037250.D
Acq On : 11 Sep 2024 10:42
Operator : SY/MD
Sample : VV0911WBL01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK240

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR091024WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091124\
Data File : VV037250.D
Acq On : 11 Sep 2024 10:42
Operator : SY/MD
Sample : VV0911WBL01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK240

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR091024WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc