
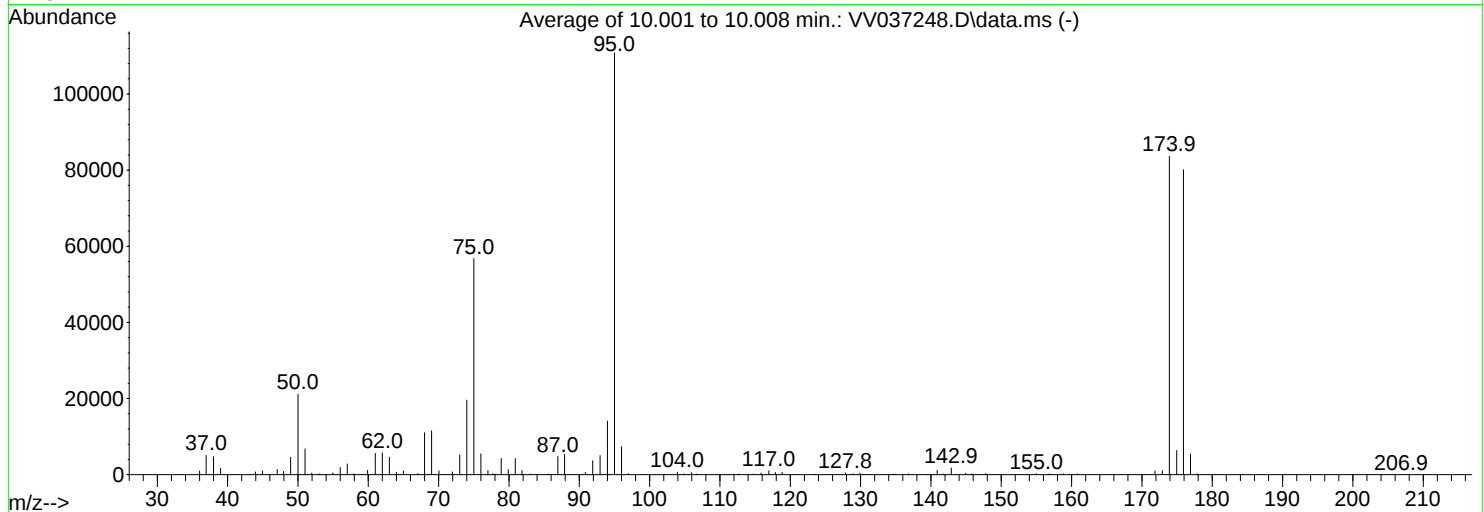


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091124\
Data File : VV037248.D
Acq On : 11 Sep 2024 07:59
Operator : SY/MD
Sample : BFB274
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB274

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR091024WMA.M
Title : TRACE VOA SFAM1.0
Last Update : Thu Sep 12 01:56:15 2024

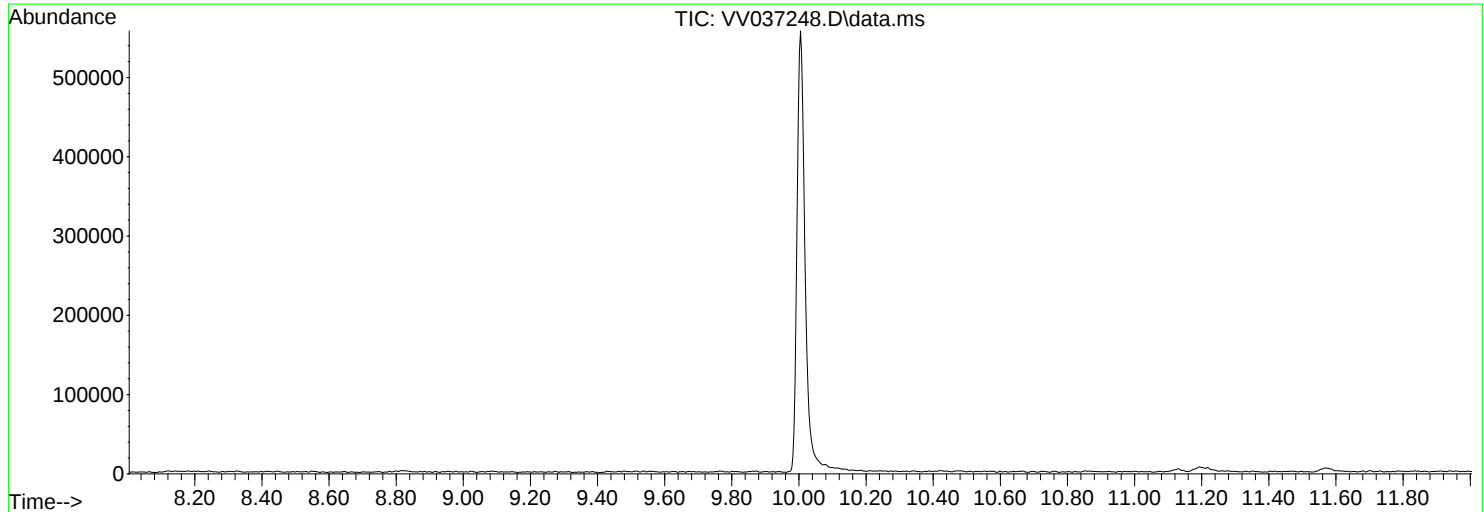

AutoFind: Scans 2787, 2788, 2789; Background Corrected with Scan 2775

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.1	21138	PASS
75	95	30	80	51.2	56763	PASS
95	95	100	100	100.0	110819	PASS
96	95	5	9	6.6	7355	PASS
173	174	0.00	2	1.2	1044	PASS
174	95	50	120	75.5	83635	PASS
175	174	5	9	7.6	6335	PASS
176	174	95	105	95.8	80131	PASS
177	176	5	10	6.7	5401	PASS

m/z	Abundance
36.90	110.0
39.00	205.0
39.90	309.0
42.20	155.0
43.90	657.0
50.00	102.0
60.20	129.0
67.40	119.0
73.10	105.0

Instrument :
MSVOA_V
ClientSampleId :
BFB274

m/z	Abundance
36.00	947.0
37.00	5329.0
38.00	4657.0
39.00	1894.0
40.00	328.0
40.80	148.0
43.10	129.0
44.00	1339.0
45.00	979.0
45.80	147.0
47.10	1591.0
48.00	809.0
49.00	4572.0
50.00	21752.0
51.00	6889.0
51.90	419.0
53.00	237.0
54.90	501.0
56.00	1712.0
57.00	2955.0
57.90	180.0
59.90	1032.0
61.00	5550.0
62.00	5837.0
63.00	4751.0
64.00	645.0
65.00	955.0
67.00	285.0
68.00	11093.0
69.00	11232.0
70.00	978.0
70.90	151.0
72.00	798.0
73.00	5179.0
74.00	19904.0
75.00	55488.0
76.00	5326.0
77.00	991.0
77.70	408.0
78.90	4392.0
79.90	1211.0
80.90	4223.0
81.90	1119.0
83.00	183.0
85.60	148.0
86.90	4800.0
87.90	5101.0
90.90	664.0
91.90	3621.0
92.90	4960.0
94.00	14181.0
95.00	108720.0
96.00	7600.0
97.00	291.0
104.00	619.0
104.90	271.0
106.00	497.0
106.70	160.0
109.80	141.0
112.00	108.0
112.70	158.0
114.80	155.0
115.90	398.0
117.00	1020.0
117.90	470.0
118.80	561.0
127.90	469.0
129.00	245.0
130.00	387.0
130.80	132.0
134.60	135.0
135.00	164.0
136.90	202.0
139.50	105.0
140.90	1179.0
141.70	166.0
142.90	1732.0
144.90	336.0
145.80	155.0
147.80	291.0
155.00	235.0
156.70	187.0
158.90	225.0
160.80	212.0
171.90	870.0
172.90	983.0
173.90	80336.0
175.00	6370.0
175.90	77896.0
176.90	5223.0
177.80	200.0

Instrument :
MSVOA_V
ClientSampleId :
BFB274

m/z	Abundance
36.00	983.0
37.00	5307.0
38.00	4837.0
39.00	1927.0
39.90	340.0
40.80	108.0
44.00	1372.0
45.00	944.0
45.90	161.0
47.10	1426.0
48.00	902.0
48.90	4735.0
50.00	21928.0
51.00	7044.0
51.90	436.0
53.00	223.0
55.00	434.0
56.00	1923.0
57.00	2891.0
57.90	241.0
59.00	107.0
59.90	1173.0
61.00	5787.0
62.00	5955.0
63.00	4737.0
64.00	612.0
65.00	967.0
67.00	309.0
68.00	11412.0
69.00	11976.0
70.00	992.0
70.90	125.0
72.00	736.0
73.00	5477.0
74.00	20216.0
75.00	58736.0
76.00	5649.0
77.00	1081.0
77.70	358.0
78.10	360.0
78.90	4357.0
79.90	1365.0
80.90	4389.0
81.90	1161.0
83.00	198.0
85.70	182.0
87.00	4891.0
87.90	5584.0
90.90	595.0
91.90	3773.0
93.00	5152.0
94.00	14557.0
95.00	114392.0
96.00	7533.0
97.00	286.0
103.90	645.0
104.90	230.0
106.00	572.0
106.70	163.0
109.90	122.0
111.90	176.0
112.70	184.0
114.80	158.0
115.80	442.0
117.00	1053.0
117.90	609.0
118.90	651.0
123.60	111.0
127.80	462.0
128.90	241.0
129.90	407.0
134.80	191.0
136.80	210.0
140.90	1111.0
141.80	147.0
142.90	1787.0
144.90	319.0
145.80	212.0
147.80	313.0
155.00	275.0
156.70	182.0
157.00	187.0
158.90	256.0
160.80	206.0
170.50	111.0
171.80	1000.0
172.90	1062.0
173.90	86392.0
175.00	6493.0
175.90	82728.0
176.90	5638.0
177.90	228.0

Instrument :
MSVOA_V
ClientSampleId :
BFB274

m/z	Abundance
36.00	949.0
37.00	4887.0
38.00	4643.0
39.00	1795.0
39.90	365.0
43.10	120.0
44.00	1468.0
44.90	892.0
47.00	1212.0
47.90	832.0
48.90	4362.0
50.00	20040.0
51.00	6381.0
52.00	446.0
53.00	207.0
53.90	107.0
54.90	425.0
56.00	1926.0
57.00	2601.0
58.00	259.0
59.00	108.0
59.90	1237.0
61.00	5464.0
62.00	5424.0
63.00	4252.0
64.00	578.0
65.00	967.0
67.10	288.0
68.00	10612.0
69.00	11322.0
70.10	993.0
71.90	588.0
73.00	5209.0
74.00	18712.0
75.00	56064.0
76.00	5416.0
77.00	1090.0
78.90	4001.0
79.90	1302.0
80.90	4058.0
81.80	1014.0
83.00	176.0
85.70	217.0
86.90	4531.0
87.90	5279.0
90.80	505.0
91.90	3618.0
93.00	4893.0
94.00	13469.0
95.00	109344.0
96.00	6933.0
97.00	211.0
103.90	595.0
104.90	170.0
105.90	552.0
106.70	141.0
109.90	127.0
111.90	225.0
112.70	176.0
114.80	154.0
115.80	462.0
116.90	960.0
117.90	569.0
118.90	664.0
123.50	103.0
127.80	494.0
128.90	226.0
129.80	422.0
134.70	253.0
136.70	249.0
140.90	1073.0
141.90	170.0
142.90	1690.0
145.00	318.0
145.80	269.0
147.80	294.0
149.60	126.0
152.90	118.0
153.70	107.0
155.00	278.0
157.00	176.0
158.80	218.0
160.80	200.0
170.40	125.0
171.80	1024.0
172.90	1086.0
173.90	84176.0
174.90	6141.0
175.90	79768.0
176.90	5342.0
177.90	221.0
206.90	114.0

Instrument :
MSVOA_V
ClientSampleId :
BFB274