

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091224\
 Data File : VV037263.D
 Acq On : 12 Sep 2024 12:51
 Operator : SY/MD
 Sample : VIBLK
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :

Quant Time: Sep 13 00:46:08 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082624WMA.M
 Quant Title : VOC Analysis
 QLast Update : Fri Sep 13 00:43:12 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.529	114	683226	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.780	117	656652	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.178	152	321680	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.278	65	216739	34.679	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	69.360%
7) Chloroethane-d5	1.532	69	192268	39.805	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	79.600%
11) 1,1-Dichloroethene-d2	2.060	65	98339	37.436	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	74.880%
21) 2-Butanone-d5	3.793	46	221636	91.575	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	91.580%
24) Chloroform-d	4.243	84	449899	45.994	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	91.980%
26) 1,2-Dichloroethane-d4	4.937	65	305294	49.561	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	99.120%
32) Benzene-d6	4.953	84	892482	44.999	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	90.000%
36) 1,2-Dichloropropane-d6	5.985	67	290863	46.822	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	93.640%
41) Toluene-d8	7.239	98	776248	43.366	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	86.740%
43) trans-1,3-Dichloroprop...	7.551	79	133594	46.484	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	92.960%
47) 2-Hexanone-d5	8.024	63	157612	92.965	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	92.960%
56) 1,1,2,2-Tetrachloroeth...	10.146	84	340197	45.154	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	90.300%
66) 1,2-Dichlorobenzene-d4	11.554	152	297107	46.116	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	92.240%
Target Compounds						
39) cis-1,3-Dichloropropene	6.908	75	8413	1.049	ug/L	Qvalue # 62


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091224\
Data File : VV037263.D
Acq On : 12 Sep 2024 12:51
Operator : SY/MD
Sample : VIBLK
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :

Quant Time: Sep 13 00:46:08 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082624WMA.M
Quant Title : VOC Analysis
QLast Update : Fri Sep 13 00:43:12 2024
Response via : Initial Calibration

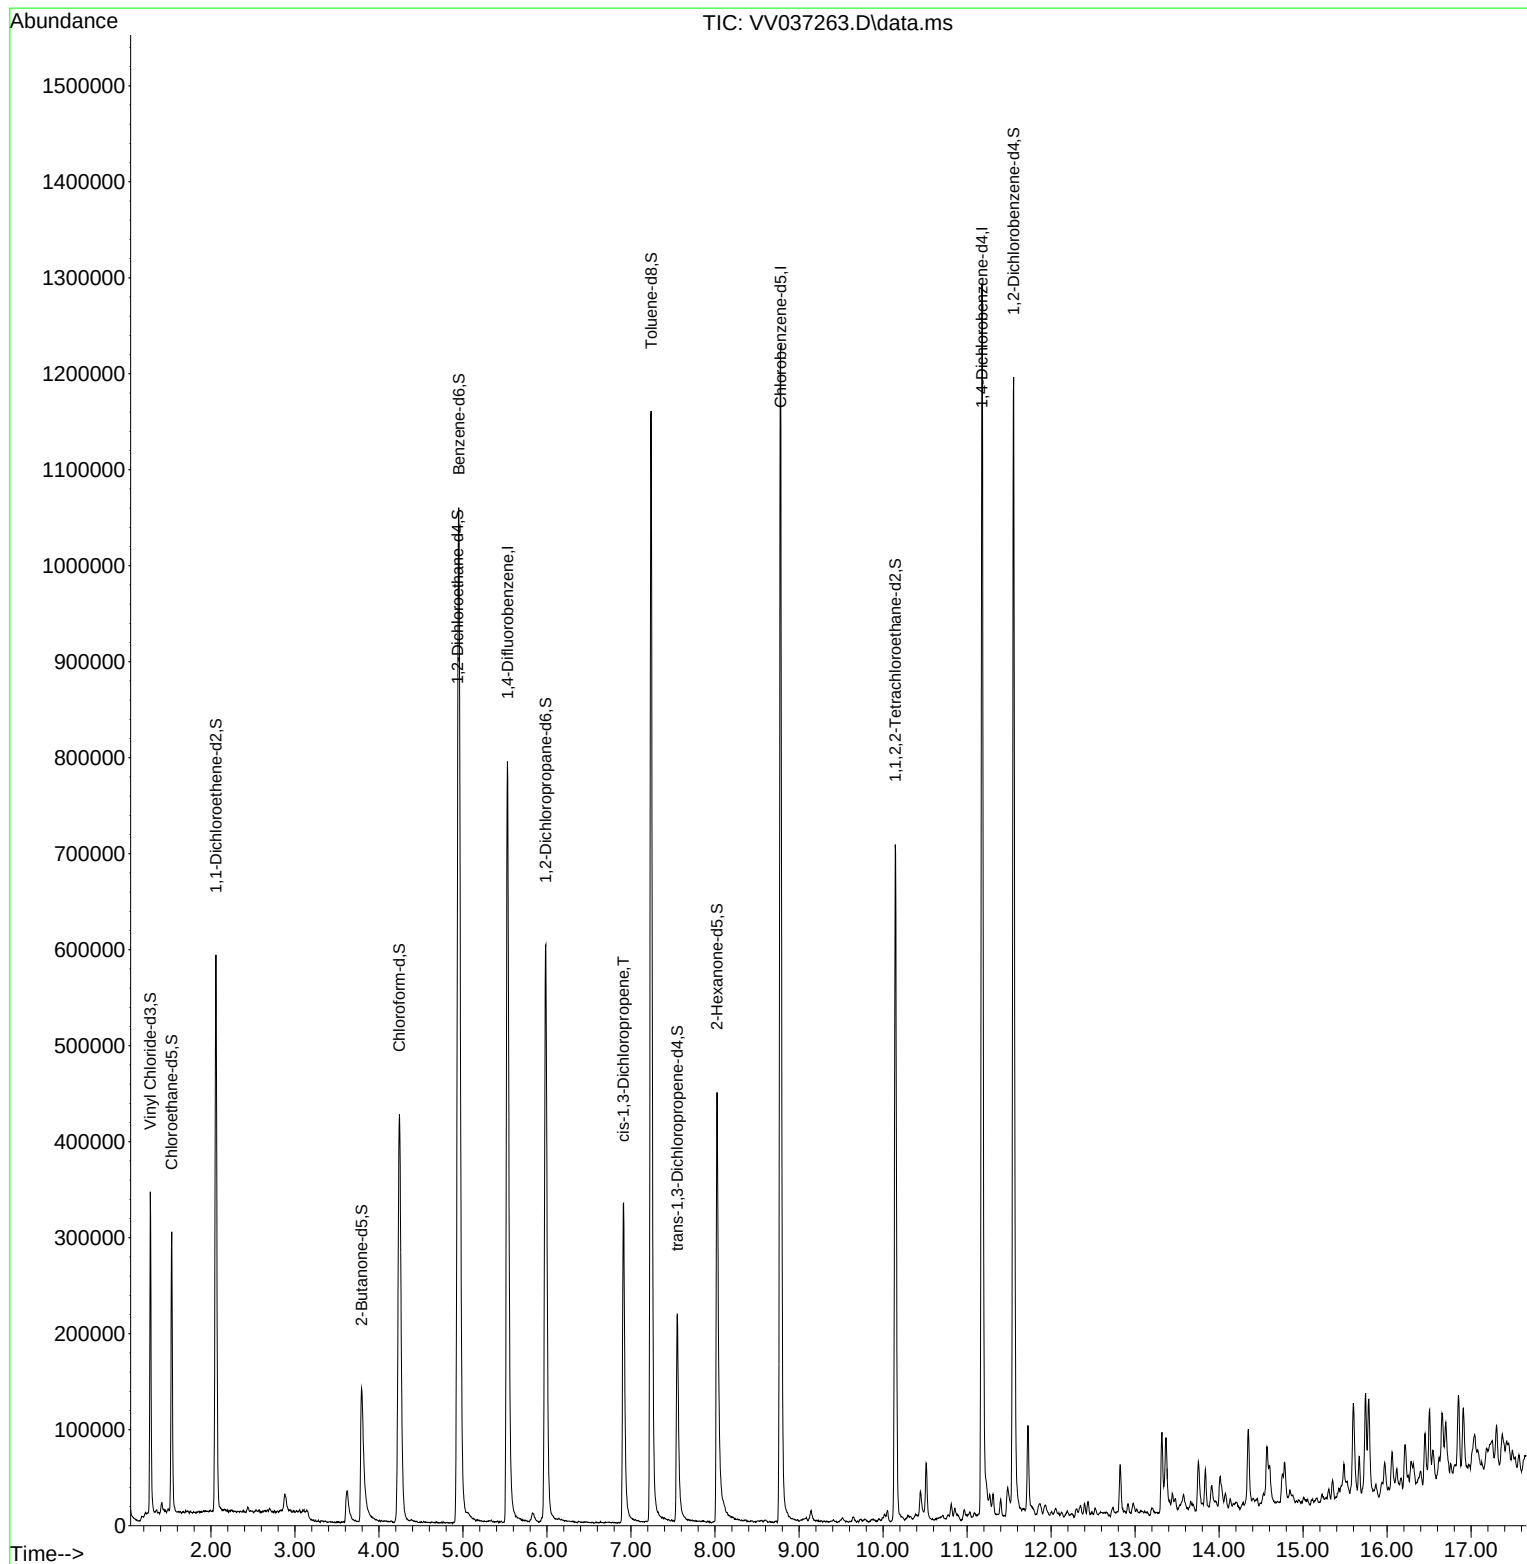

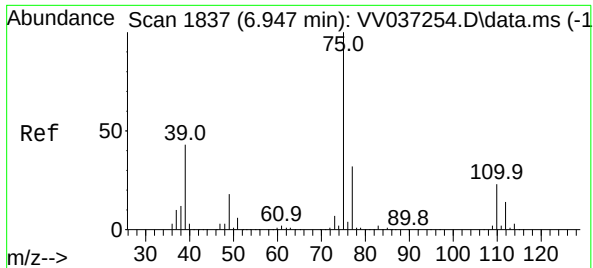

#39
 cis-1,3-Dichloropropene
 Concen: 1.049 ug/L
 RT: 6.908 min Scan# 11
 Delta R.T. -0.039 min
 Lab File: VV037263.D
 Acq: 12 Sep 2024 12:51

Instrument :
 MSVOA_V
 ClientSampleId :

Tgt Ion: 75 Resp: 8413
 Ion Ratio Lower Upper
 75 100
 77 51.9 21.7 40.3#

