

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091224\
 Data File : VV037267.D
 Acq On : 12 Sep 2024 14:48
 Operator : SY/MD
 Sample : P3934-04
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :

Quant Time: Sep 13 00:47:05 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082624WMA.M
 Quant Title : VOC Analysis
 QLast Update : Fri Sep 13 00:43:12 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.526	114	769318	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.776	117	713048	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.178	152	350605	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.278	65	321596	45.698	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	91.400%
7) Chloroethane-d5	1.532	69	253074	46.530	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	93.060%
11) 1,1-Dichloroethene-d2	2.057	65	139845	47.279	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	94.560%
21) 2-Butanone-d5	3.786	46	243106	89.206	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	89.210%
24) Chloroform-d	4.236	84	534900	48.565	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	97.120%
26) 1,2-Dichloroethane-d4	4.934	65	340163	49.042	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	98.080%
32) Benzene-d6	4.947	84	1084242	50.344	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	100.680%
36) 1,2-Dichloropropane-d6	5.979	67	336102	49.825	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	99.660%
41) Toluene-d8	7.233	98	963495	49.570	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	99.140%
43) trans-1,3-Dichloroprop...	7.545	79	158963	50.936	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	101.880%
47) 2-Hexanone-d5	8.021	63	174612	94.846	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	94.850%
56) 1,1,2,2-Tetrachloroeth...	10.146	84	365706	44.701	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	89.400%
66) 1,2-Dichlorobenzene-d4	11.555	152	347996	49.559	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	99.120%
Target Compounds						Qvalue
10) 1,1,2-Trichloro-1,2,2-...	2.060	101	4211	0.790	ug/L	# 25


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091224\
Data File : VV037267.D
Acq On : 12 Sep 2024 14:48
Operator : SY/MD
Sample : P3934-04
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :


Quant Time: Sep 13 00:47:05 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082624WMA.M
Quant Title : VOC Analysis
QLast Update : Fri Sep 13 00:43:12 2024
Response via : Initial Calibration

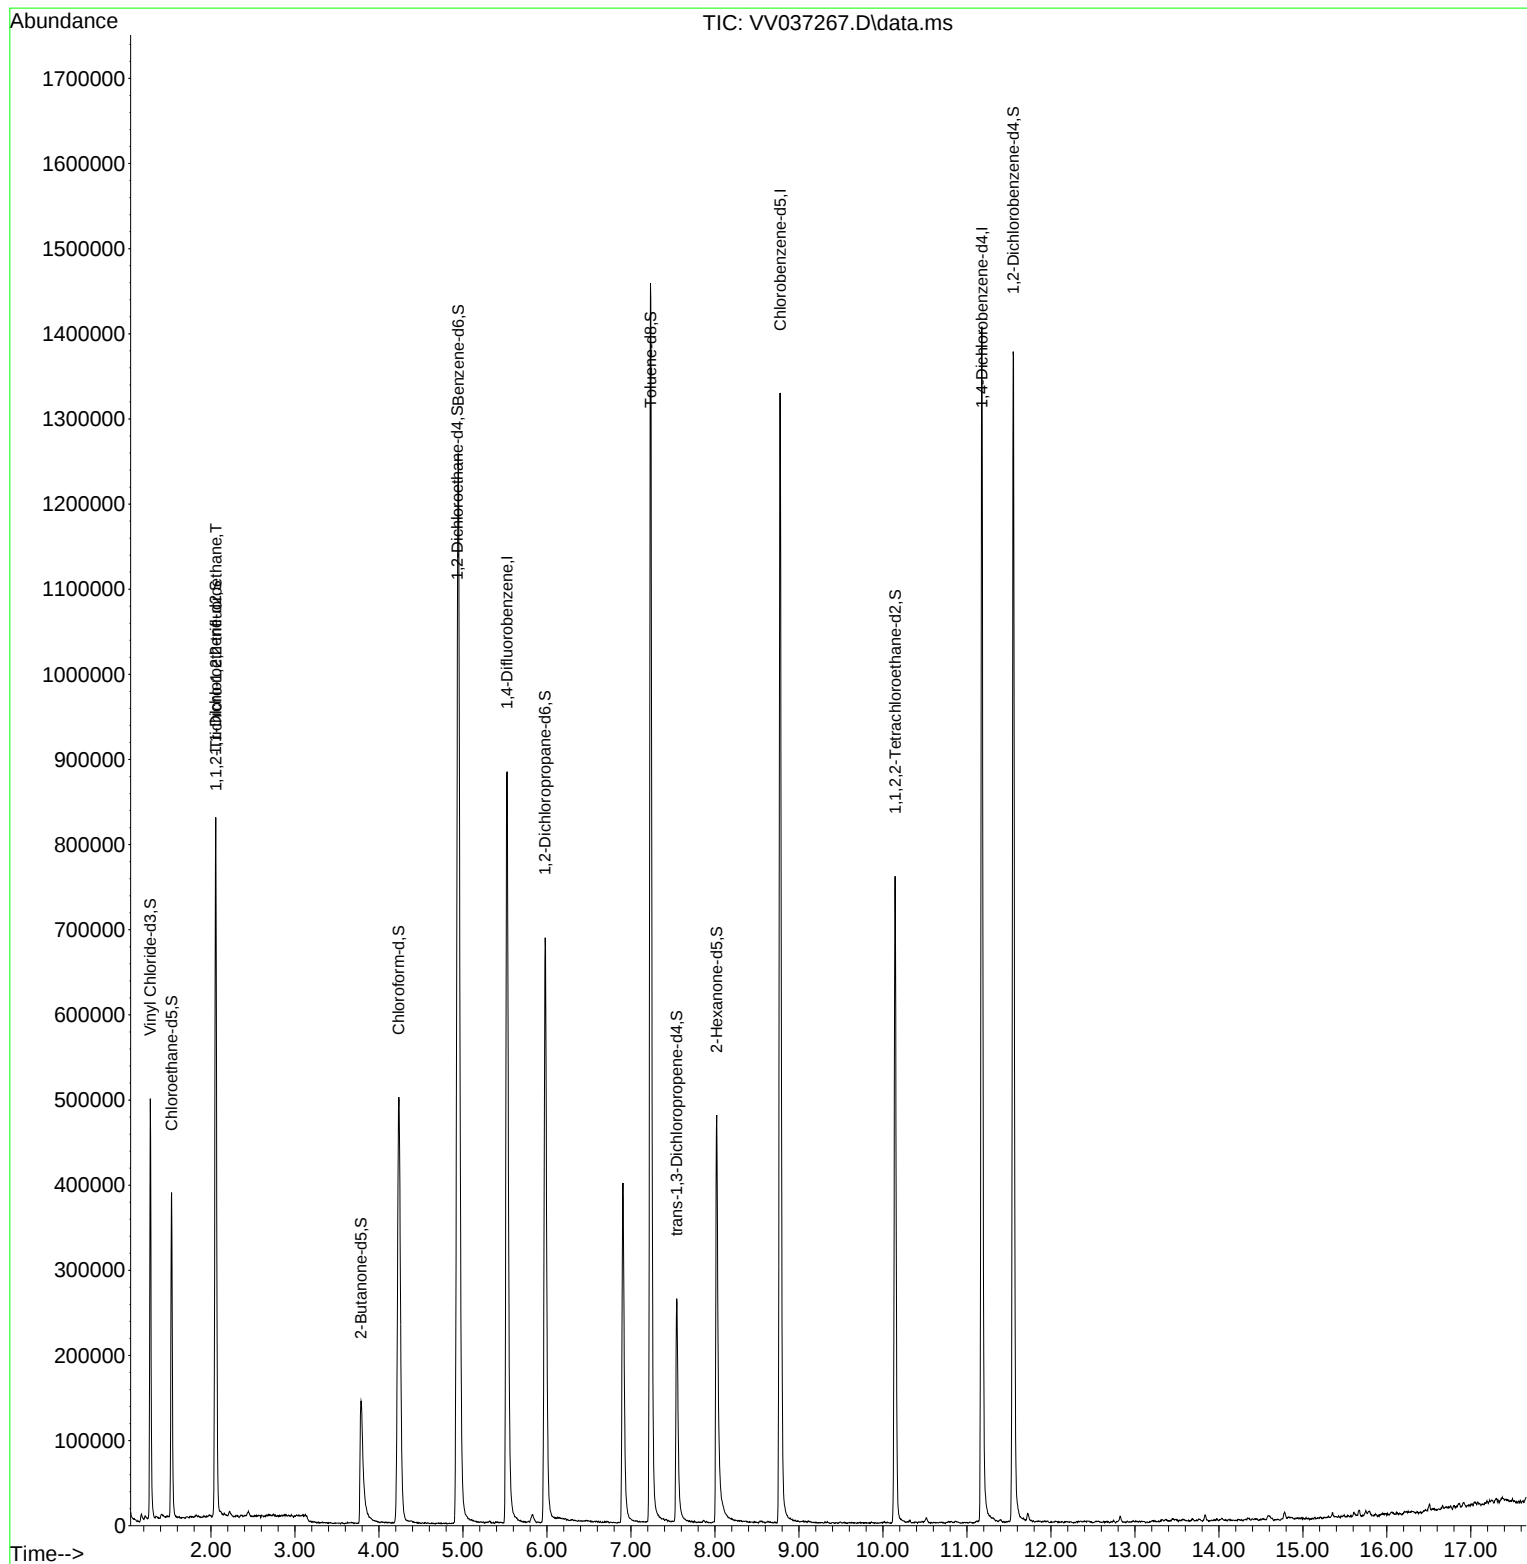

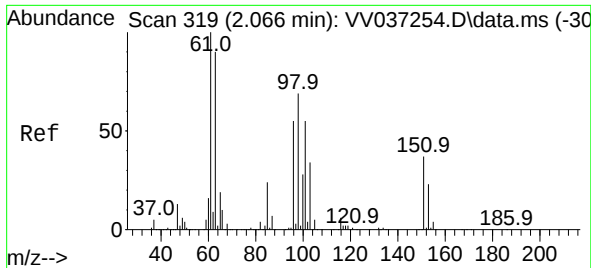

#10
 1,1,2-Trichloro-1,2,2-trifluoroethane
 Concen: 0.790 ug/L
 RT: 2.060 min Scan# 31
 Delta R.T. -0.006 min
 Lab File: VV037267.D
 Acq: 12 Sep 2024 14:48

Instrument :
 MSVOA_V
 ClientSampleId :

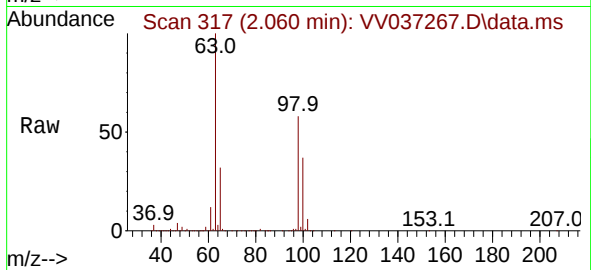

Tgt Ion:101 Resp: 4211
 Ion Ratio Lower Upper
 101 100
 85 5.5 35.6 53.4#
 151 0.0 55.0 82.4#

