

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091224\
 Data File : VV037261.D
 Acq On : 12 Sep 2024 12:08
 Operator : SY/MD
 Sample : VIBLK380
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK380

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082624WMA.M
 Title : VOC Analysis

Signal : TIC: VV037261.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.179	36	43	47	rBV2	5995	9109	0.33%	0.045%
2	1.217	51	55	59	rBV6	4547	4479	0.16%	0.022%
3	1.278	67	74	90	rBV	336052	353328	12.94%	1.759%
4	1.532	145	153	167	rBV	298406	352190	12.90%	1.754%
5	2.060	307	317	331	rBV	595178	856975	31.38%	4.267%
6	3.243	683	685	688	rVB2	1854	1086	0.04%	0.005%
7	3.265	688	692	696	rBV7	1397	1018	0.04%	0.005%
8	3.317	705	708	713	rBV5	1309	1096	0.04%	0.005%
9	3.564	782	785	790	rVB4	1188	876	0.03%	0.004%
10	3.635	800	807	810	rBV4	3660	4294	0.16%	0.021%
11	3.793	848	856	881	rBV	130566	347120	12.71%	1.728%
12	4.056	936	938	943	rVB6	1820	1207	0.04%	0.006%
13	4.243	976	996	1030	rBV	436289	1119050	40.98%	5.572%
14	4.375	1035	1037	1041	rBV5	1187	874	0.03%	0.004%
15	4.458	1061	1063	1068	rBV5	941	794	0.03%	0.004%
16	4.522	1078	1083	1084	rBV5	1491	1195	0.04%	0.006%
17	4.584	1097	1102	1108	rBV7	1484	1667	0.06%	0.008%
18	4.629	1113	1116	1120	rVB4	939	875	0.03%	0.004%
19	4.651	1120	1123	1126	rBV6	1256	783	0.03%	0.004%
20	4.667	1126	1128	1133	rVB3	1168	834	0.03%	0.004%
21	4.821	1172	1176	1179	rVB4	1021	734	0.03%	0.004%
22	4.873	1188	1192	1194	rVB4	1452	993	0.04%	0.005%
23	4.950	1194	1216	1251	rBV2	1071258	2730884	100.00%	13.597%
24	5.262	1310	1313	1315	rBV3	1391	861	0.03%	0.004%
25	5.371	1343	1347	1350	rBV4	1045	755	0.03%	0.004%
26	5.529	1383	1396	1428	rVV	784490	1614916	59.14%	8.041%
27	5.754	1463	1466	1468	rBV3	1404	816	0.03%	0.004%
28	5.828	1480	1489	1491	rBV5	12868	16786	0.61%	0.084%
29	5.985	1524	1538	1566	rBV	602972	1250563	45.79%	6.227%
30	6.445	1678	1681	1686	rVV6	1148	796	0.03%	0.004%
31	6.545	1709	1712	1715	rBV4	1164	817	0.03%	0.004%
32	6.606	1728	1731	1733	rVV3	1312	719	0.03%	0.004%
33	6.696	1755	1759	1761	rBV4	1278	778	0.03%	0.004%
34	6.728	1765	1769	1771	rBV4	1019	810	0.03%	0.004%
35	6.760	1777	1779	1786	rVB6	1236	1070	0.04%	0.005%
36	6.908	1813	1825	1856	rBV	331199	649073	23.77%	3.232%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091224\
Data File : VV037261.D
Acq On : 12 Sep 2024 12:08
Operator : SY/MD
Sample : VIBLK380
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK380

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082624WMA.M
Title : VOC Analysis

37	7.104	1883	1886	1888	rBV4	1290	802	0.03%	0.004%
38	7.239	1916	1928	1952	rBV	1170226	2081258	76.21%	10.363%
39	7.481	2000	2003	2007	rVB5	1704	1428	0.05%	0.007%
40	7.551	2015	2025	2052	rBV	216674	410028	15.01%	2.042%
41	7.908	2131	2136	2137	rBV5	1616	1179	0.04%	0.006%
42	7.982	2155	2159	2163	rVB7	1034	968	0.04%	0.005%
43	8.024	2163	2172	2219	rBV	418876	873083	31.97%	4.347%
44	8.426	2295	2297	2301	rBV6	1143	988	0.04%	0.005%
45	8.551	2331	2336	2340	rVV7	1879	2278	0.08%	0.011%
46	8.780	2394	2407	2440	rBV	1211753	2018407	73.91%	10.050%
47	9.185	2530	2533	2537	rVB5	1402	844	0.03%	0.004%
48	9.297	2565	2568	2569	rBV3	1480	740	0.03%	0.004%
49	9.361	2585	2588	2592	rBV5	1199	1255	0.05%	0.006%
50	9.416	2601	2605	2608	rVB6	911	788	0.03%	0.004%
51	9.480	2618	2625	2626	rBV6	2890	2687	0.10%	0.013%
52	9.519	2629	2637	2646	rVB6	4731	9162	0.34%	0.046%
53	9.635	2669	2673	2675	rBV4	1417	886	0.03%	0.004%
54	9.654	2677	2679	2683	rVV6	867	711	0.03%	0.004%
55	9.757	2707	2711	2714	rBV5	1018	993	0.04%	0.005%
56	9.776	2714	2717	2722	rBV6	839	731	0.03%	0.004%
57	9.812	2723	2728	2731	rBV7	804	885	0.03%	0.004%
58	9.869	2739	2746	2748	rBV7	1282	1291	0.05%	0.006%
59	9.889	2750	2752	2754	rVB3	1895	836	0.03%	0.004%
60	9.934	2763	2766	2770	rBV4	1627	1272	0.05%	0.006%
61	9.995	2780	2785	2787	rBV5	845	903	0.03%	0.004%
62	10.095	2813	2816	2818	rVB4	1254	703	0.03%	0.004%
63	10.146	2818	2832	2846	rBV	692790	1098837	40.24%	5.471%
64	10.291	2874	2877	2879	rBV4	1183	828	0.03%	0.004%
65	10.390	2905	2908	2914	rBV8	2414	2205	0.08%	0.011%
66	10.429	2918	2920	2921	rBV2	1526	700	0.03%	0.003%
67	10.477	2926	2935	2941	rBV7	5470	9222	0.34%	0.046%
68	10.599	2971	2973	2981	rVB8	1744	1399	0.05%	0.007%
69	10.632	2981	2983	2986	rBV3	1596	1079	0.04%	0.005%
70	10.812	3033	3039	3041	rVV8	1804	1802	0.07%	0.009%
71	10.853	3046	3052	3061	rVB3	10096	15173	0.56%	0.076%
72	10.924	3071	3074	3078	rVB5	1240	886	0.03%	0.004%
73	10.963	3082	3086	3092	rBV9	2685	3307	0.12%	0.016%
74	10.992	3092	3095	3098	rBV4	941	959	0.04%	0.005%
75	11.127	3127	3137	3140	rBV4	5908	6794	0.25%	0.034%
76	11.178	3142	3153	3180	rBV	1259823	2020873	74.00%	10.062%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091224\
 Data File : VV037261.D
 Acq On : 12 Sep 2024 12:08
 Operator : SY/MD
 Sample : VIBLK380
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK380

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082624WMA.M
 Title : VOC Analysis

77	11.400	3216	3222	3228	rVB10	2266	3661	0.13%	0.018%
78	11.509	3248	3256	3257	rVV7	3855	4684	0.17%	0.023%
79	11.554	3259	3270	3302	rVV	1211189	1948477	71.35%	9.701%
80	11.725	3318	3323	3335	rVB4	12861	18055	0.66%	0.090%
81	11.837	3355	3358	3360	rBV4	2111	1460	0.05%	0.007%
82	12.004	3406	3410	3414	rBV6	1719	1511	0.06%	0.008%
83	12.046	3420	3423	3427	rBV6	1978	1707	0.06%	0.008%
84	12.107	3440	3442	3446	rVB5	1257	763	0.03%	0.004%
85	12.191	3465	3468	3471	rBV5	1927	1376	0.05%	0.007%
86	12.365	3516	3522	3526	rVV9	3797	5292	0.19%	0.026%
87	12.439	3540	3545	3550	rBV7	2956	3513	0.13%	0.017%
88	12.500	3561	3564	3566	rBV4	1174	866	0.03%	0.004%
89	12.725	3630	3634	3635	rBV3	1861	1192	0.04%	0.006%
90	12.824	3659	3665	3676	rVB3	10204	14874	0.54%	0.074%
91	12.943	3698	3702	3706	rBV6	2028	2129	0.08%	0.011%
92	12.975	3706	3712	3722	rVV6	3370	6019	0.22%	0.030%
93	13.130	3757	3760	3763	rVB5	1967	1315	0.05%	0.007%
94	13.207	3773	3784	3791	rBV9	10672	19503	0.71%	0.097%
95	13.326	3816	3821	3827	rBV9	4385	5658	0.21%	0.028%
96	13.374	3828	3836	3846	rVV5	34046	53102	1.94%	0.264%
97	13.442	3850	3857	3875	rVB	26492	55034	2.02%	0.274%
98	13.577	3890	3899	3910	rBV	4461	9685	0.35%	0.048%
99	13.747	3948	3952	3953	rBV3	2654	1816	0.07%	0.009%
100	13.837	3975	3980	3991	rVB4	10317	13293	0.49%	0.066%


Sum of corrected areas: 20084376

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091224\
Data File : VV037261.D
Acq On : 12 Sep 2024 12:08
Operator : SY/MD
Sample : VIBLK380
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK380

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

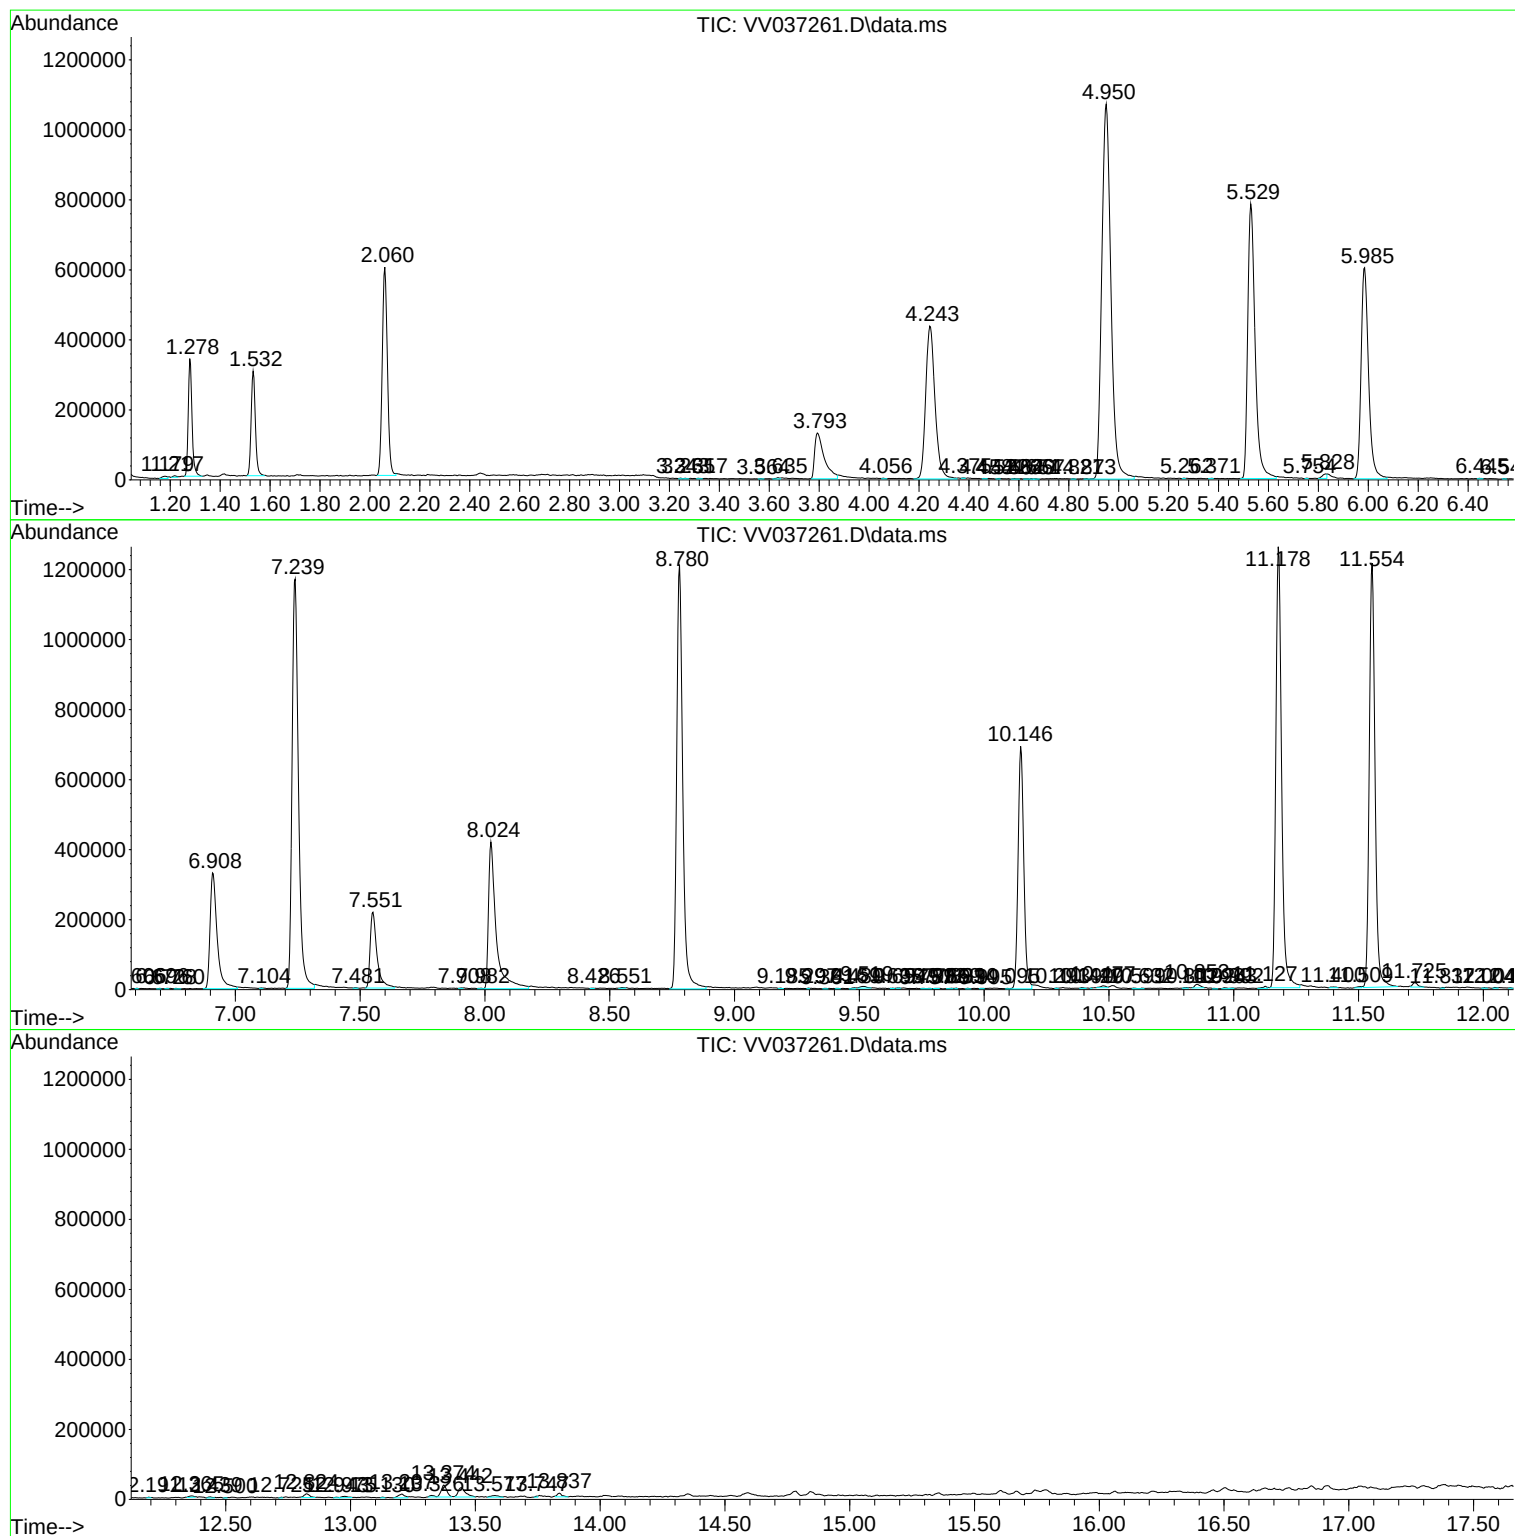

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091224\
Data File : VV037261.D
Acq On : 12 Sep 2024 12:08
Operator : SY/MD
Sample : VIBLK380
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK380

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091224\
Data File : VV037261.D
Acq On : 12 Sep 2024 12:08
Operator : SY/MD
Sample : VIBLK380
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK380

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc