

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091324\
 Data File : VV037283.D
 Acq On : 13 Sep 2024 15:49
 Operator : SY/MD
 Sample : P3967-15
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :

Quant Time: Sep 14 03:51:04 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVSIM091324.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Sat Sep 14 03:38:32 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.566	114	13382	0.500	ug/L	0.00
5) Chlorobenzene-d5	8.800	117	12838	0.500	ug/L	0.00
11) 1,4-Dichlorobenzene-d4	11.191	152	6541	0.500	ug/L	0.00
System Monitoring Compounds						
2) Vinyl Chloride-d3	1.273	65	7166	0.500	ug/L	0.00
Spiked Amount	0.500	Range	40 - 130	Recovery	=	100.000%
4) 1,2-Dichloroethane-d4	4.970	65	4265	0.523	ug/L	0.00
Spiked Amount	0.500	Range	70 - 130	Recovery	=	104.000%
7) 1,2-Dichloropropane-d6	5.996	67	5304	0.498	ug/L	0.00
Spiked Amount	0.500	Range	60 - 140	Recovery	=	100.000%
8) Toluene-d8	7.254	98	14397	0.460	ug/L	0.00
Spiked Amount	0.500	Range	70 - 130	Recovery	=	92.000%
10) 1,1,2,2-Tetrachloroeth...	10.146	84	4159	0.521	ug/L	0.00
Spiked Amount	0.500	Range	65 - 120	Recovery	=	104.000%
Target Compounds						
					Qvalue	
3) Vinyl chloride	1.379	62	345	0.027	ug/L	95
6) Trichloroethene	5.853	95	3317	0.331	ug/L	100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091324\
Data File : VV037283.D
Acq On : 13 Sep 2024 15:49
Operator : SY/MD
Sample : P3967-15
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :

Quant Time: Sep 14 03:51:04 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVSIM091324.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Sat Sep 14 03:38:32 2024
Response via : Initial Calibration

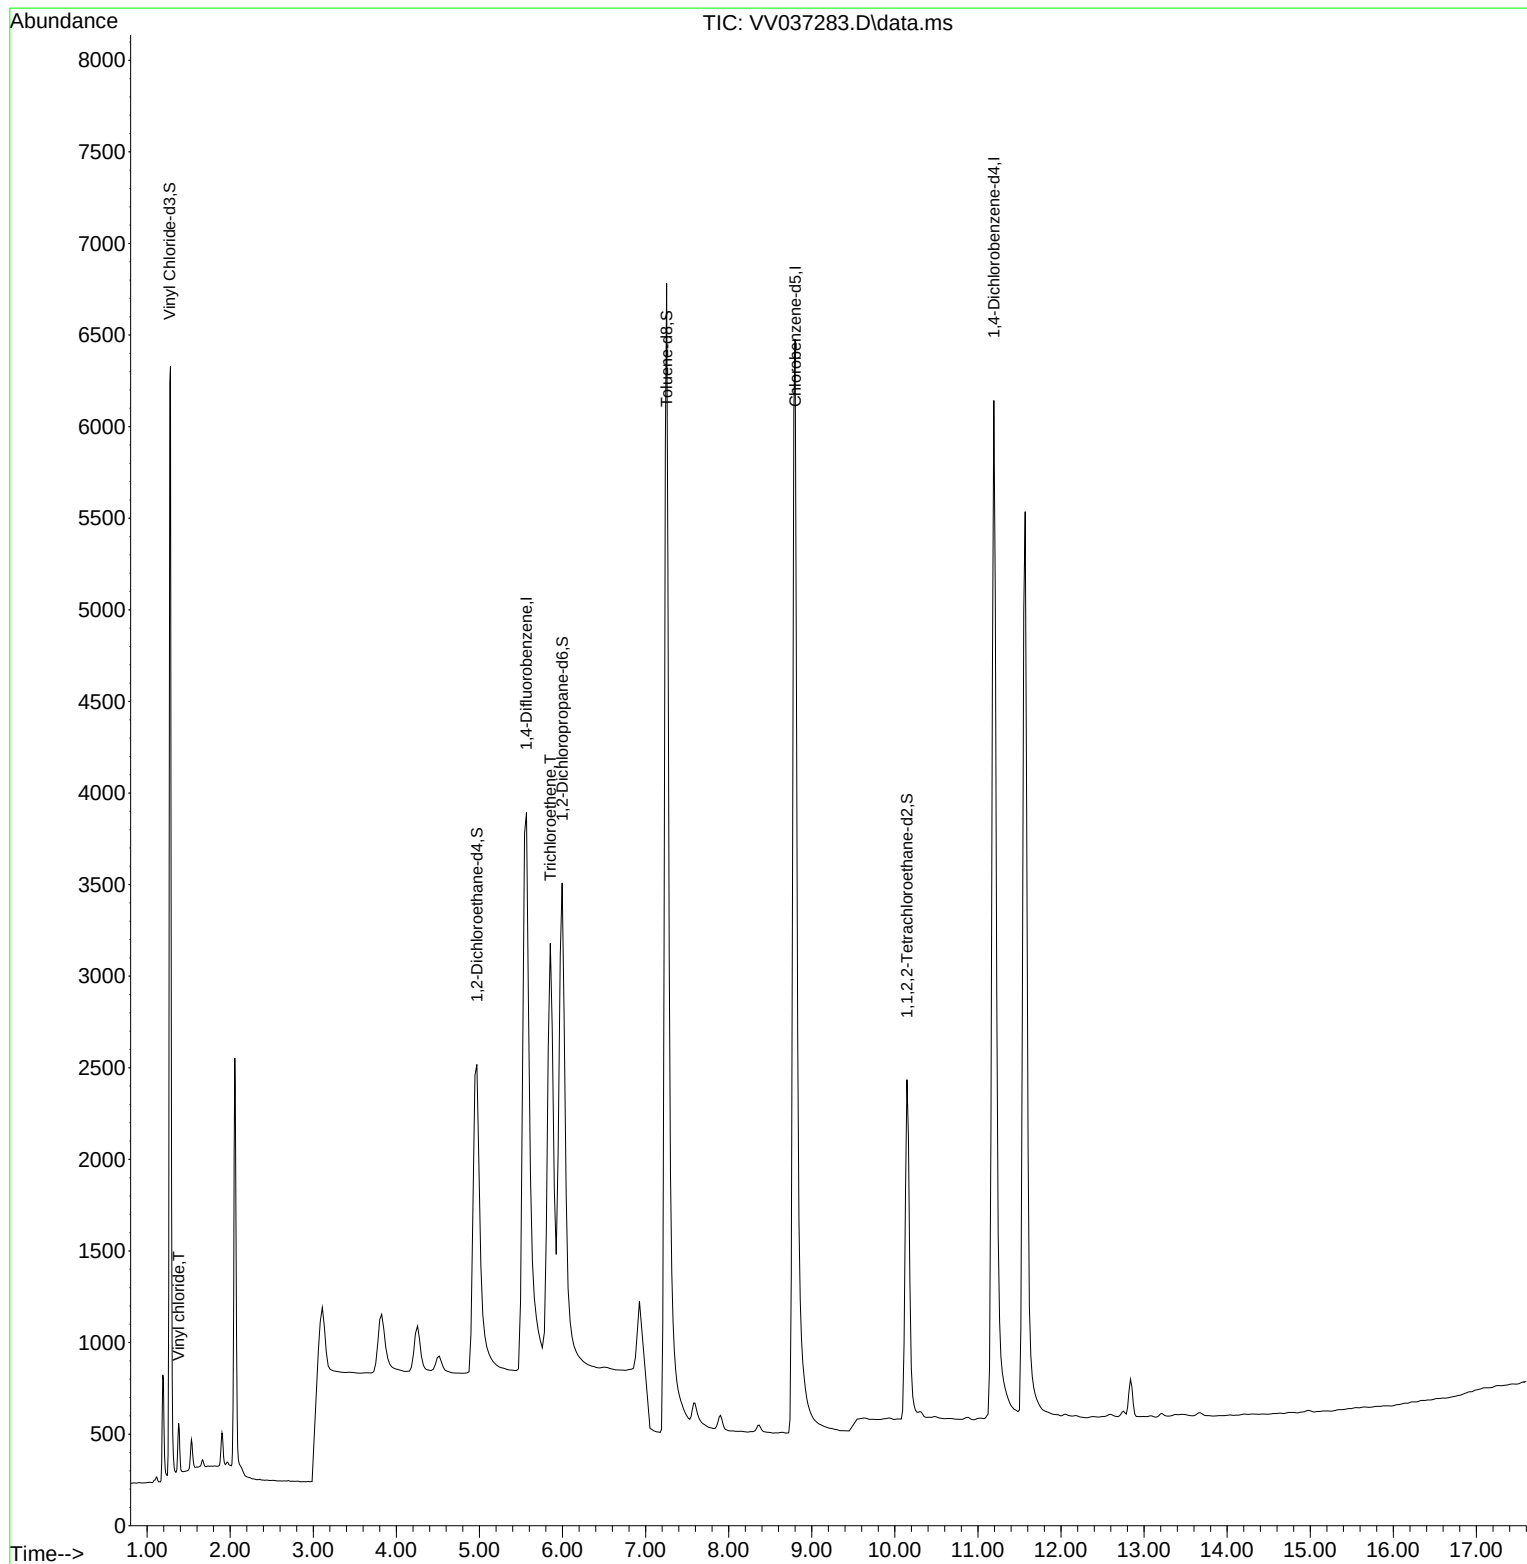

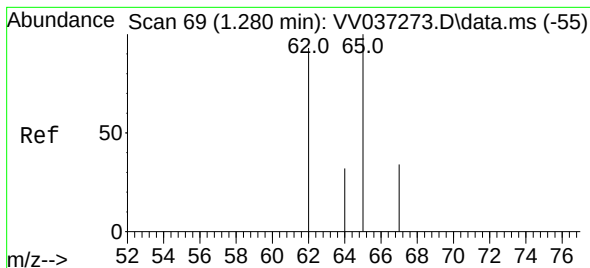

#3

Vinyl chloride

Concen: 0.027 ug/L

RT: 1.379 min Scan# 81

Delta R.T. 0.099 min

Lab File: VV037283.D

Acq: 13 Sep 2024 15:49

Instrument :

MSVOA_V





ClientSampleId :

Tgt Ion: 62 Resp: 345

Ion Ratio Lower Upper

62 100

64 38.2 24.6 45.6

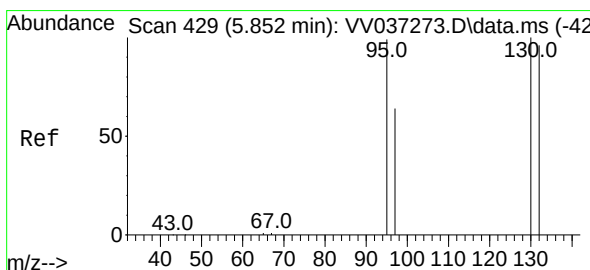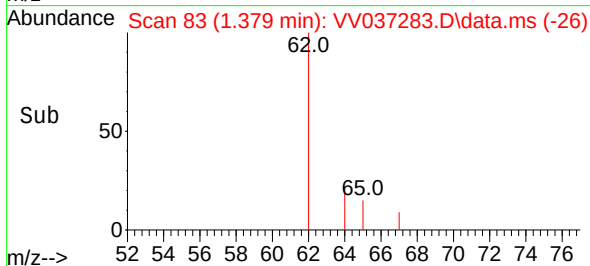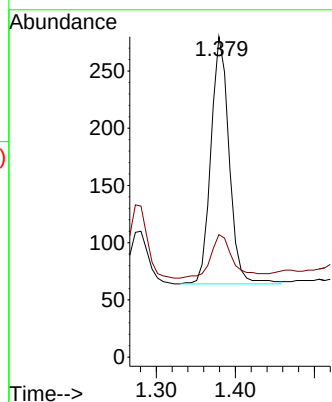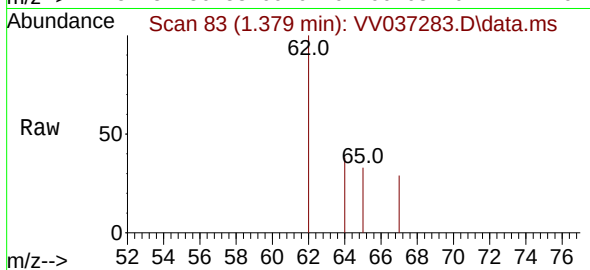

#6

Trichloroethene

Concen: 0.331 ug/L

RT: 5.853 min Scan# 429

Delta R.T. 0.000 min

Lab File: VV037283.D

Acq: 13 Sep 2024 15:49

Tgt Ion: 95 Resp: 3317

Ion Ratio Lower Upper

95 100

97 67.3 46.4 86.2

132 96.6 67.5 125.4

130 100.6 70.3 130.7

