

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091324\
 Data File : VV037282.D
 Acq On : 13 Sep 2024 15:25
 Operator : SY/MD
 Sample : P3967-14
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AN4

Quant Time: Sep 14 03:50:56 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVSIM091324.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Sat Sep 14 03:38:32 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.566	114	13107	0.500	ug/L	0.00
5) Chlorobenzene-d5	8.800	117	12849	0.500	ug/L	0.00
11) 1,4-Dichlorobenzene-d4	11.191	152	6526	0.500	ug/L	0.00
System Monitoring Compounds						
2) Vinyl Chloride-d3	1.280	65	7365	0.525	ug/L	0.00
Spiked Amount 0.500	Range 40 - 130		Recovery = 106.000%			
4) 1,2-Dichloroethane-d4	4.969	65	4434	0.555	ug/L	0.00
Spiked Amount 0.500	Range 70 - 130		Recovery = 110.000%			
7) 1,2-Dichloropropane-d6	5.995	67	5452	0.511	ug/L	0.00
Spiked Amount 0.500	Range 60 - 140		Recovery = 102.000%			
8) Toluene-d8	7.254	98	15322	0.490	ug/L	0.00
Spiked Amount 0.500	Range 70 - 130		Recovery = 98.000%			
10) 1,1,2,2-Tetrachloroeth...	10.146	84	4266	0.534	ug/L	0.00
Spiked Amount 0.500	Range 65 - 120		Recovery = 106.000%			
Target Compounds						
						Qvalue
3) Vinyl chloride	1.280	62	1361	0.107	ug/L	86
6) Trichloroethene	5.852	95	7306	0.727	ug/L	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091324\
Data File : VV037282.D
Acq On : 13 Sep 2024 15:25
Operator : SY/MD
Sample : P3967-14
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
COAN4

Quant Time: Sep 14 03:50:56 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVSIM091324.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Sat Sep 14 03:38:32 2024
Response via : Initial Calibration




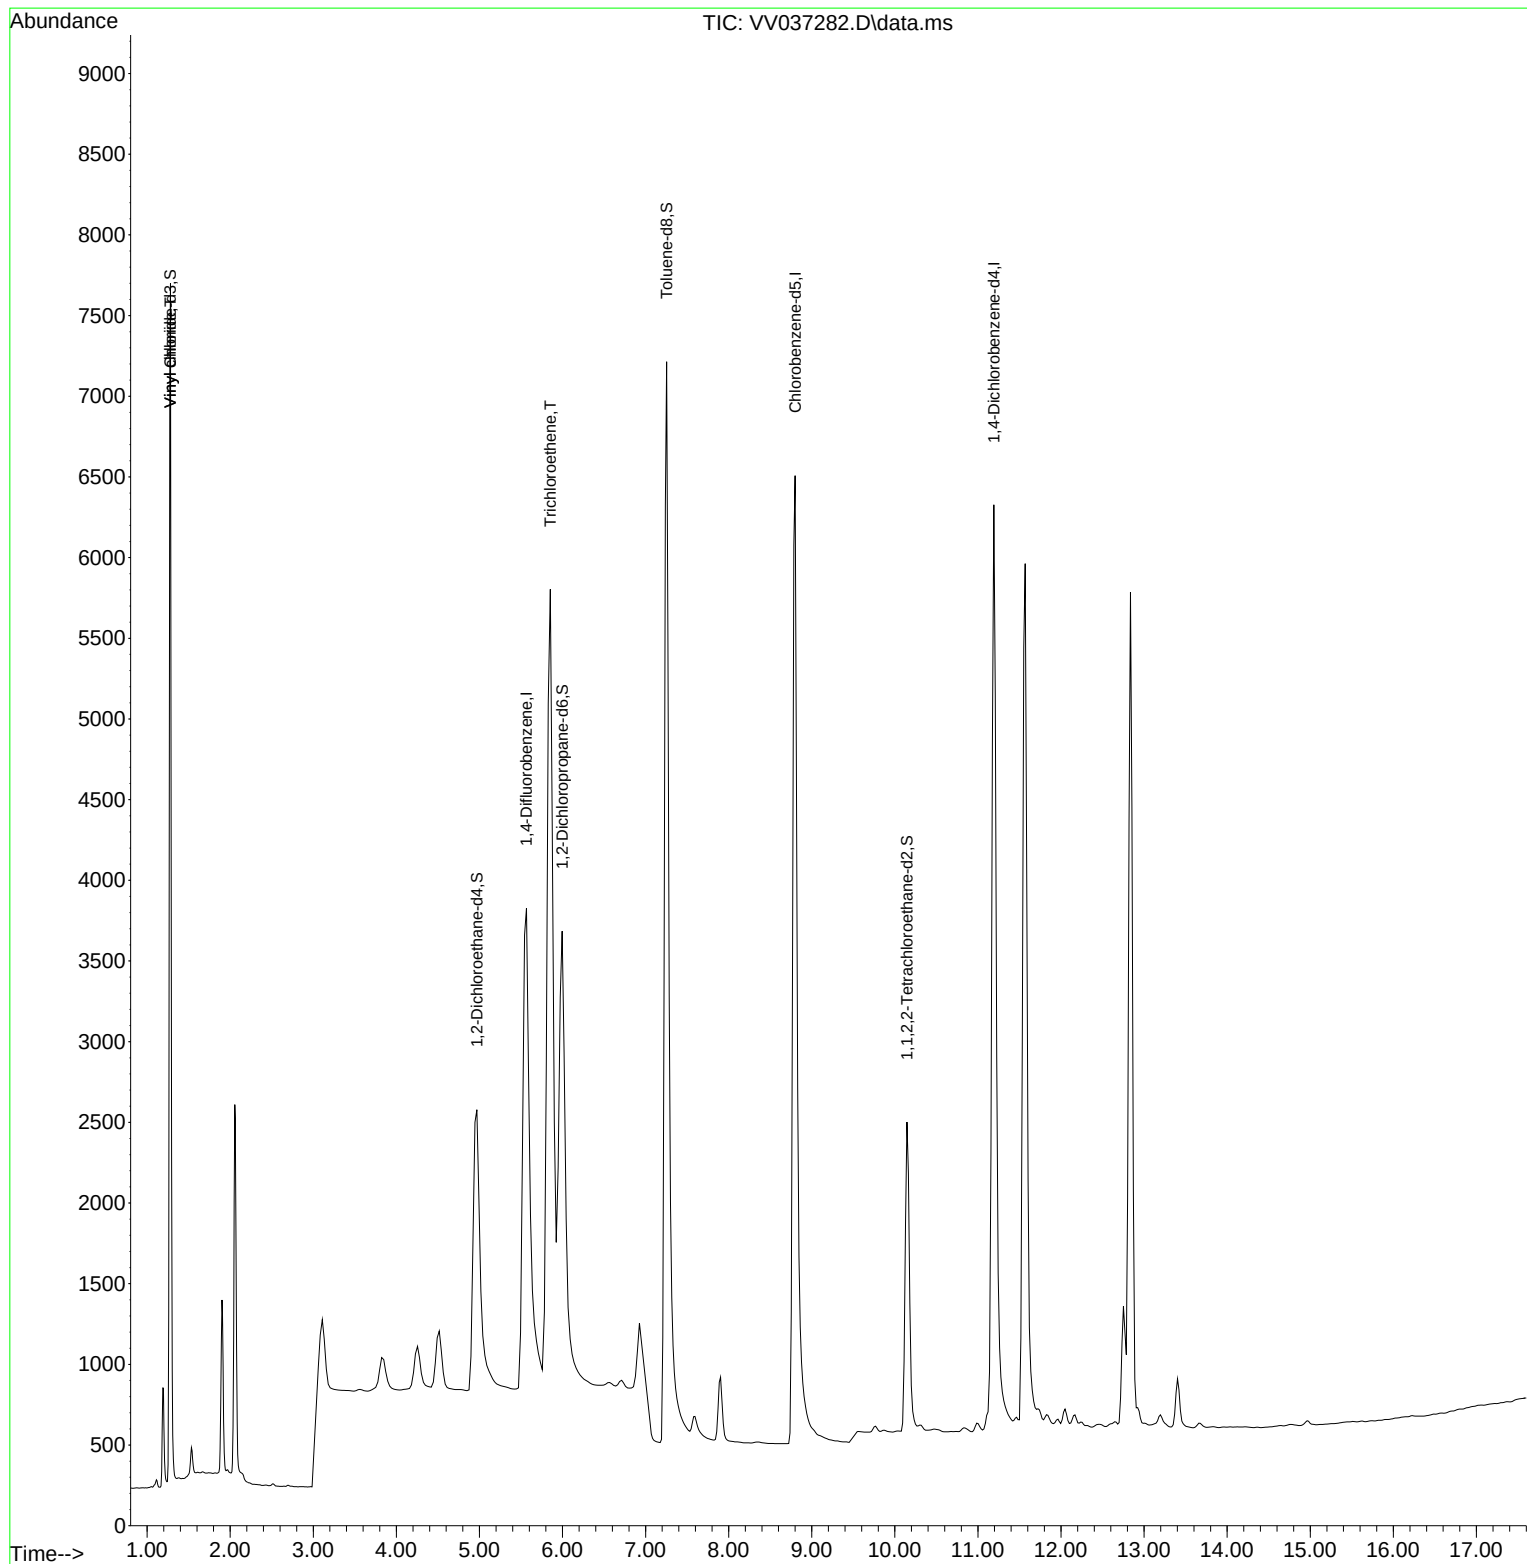


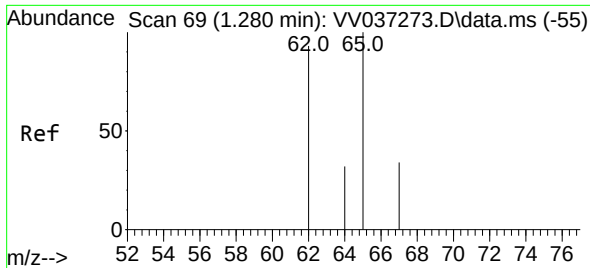

#3
 Vinyl chloride
 Concen: 0.107 ug/L
 RT: 1.280 min Scan# 69
 Delta R.T. 0.000 min
 Lab File: VV037282.D
 Acq: 13 Sep 2024 15:25

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AN4

Tgt Ion: 62 Resp: 1361
 Ion Ratio Lower Upper
 62 100
 64 43.1 24.6 45.6

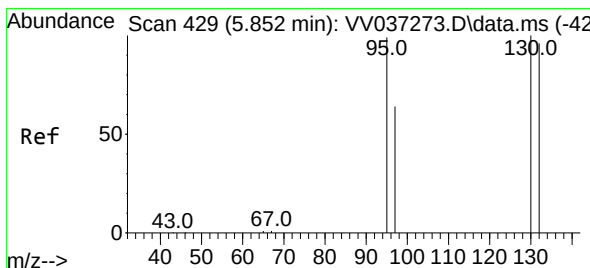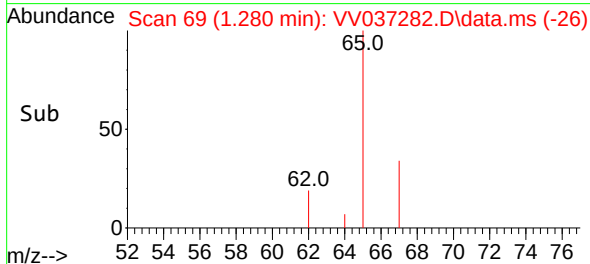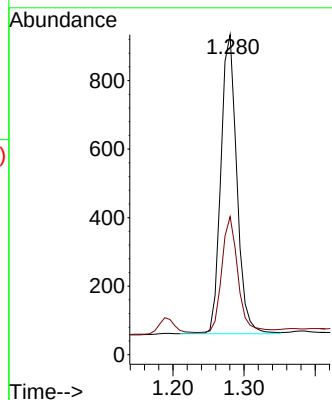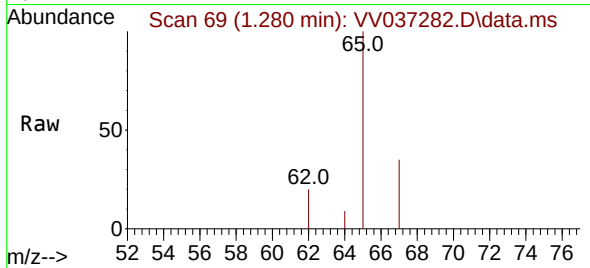

#6
 Trichloroethene
 Concen: 0.727 ug/L
 RT: 5.852 min Scan# 429
 Delta R.T. 0.000 min
 Lab File: VV037282.D
 Acq: 13 Sep 2024 15:25

Tgt Ion: 95 Resp: 7306
 Ion Ratio Lower Upper
 95 100
 97 66.1 46.4 86.2
 132 95.9 67.5 125.4
 130 99.1 70.3 130.7

