


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091324\
Data File : VV037270.D
Acq On : 13 Sep 2024 08:06
Operator : SY/MD
Sample : BFB220
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB220

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVSIM091324.M
Title : TRACE VOA SOM01.0
Last Update : Sat Sep 14 03:38:32 2024

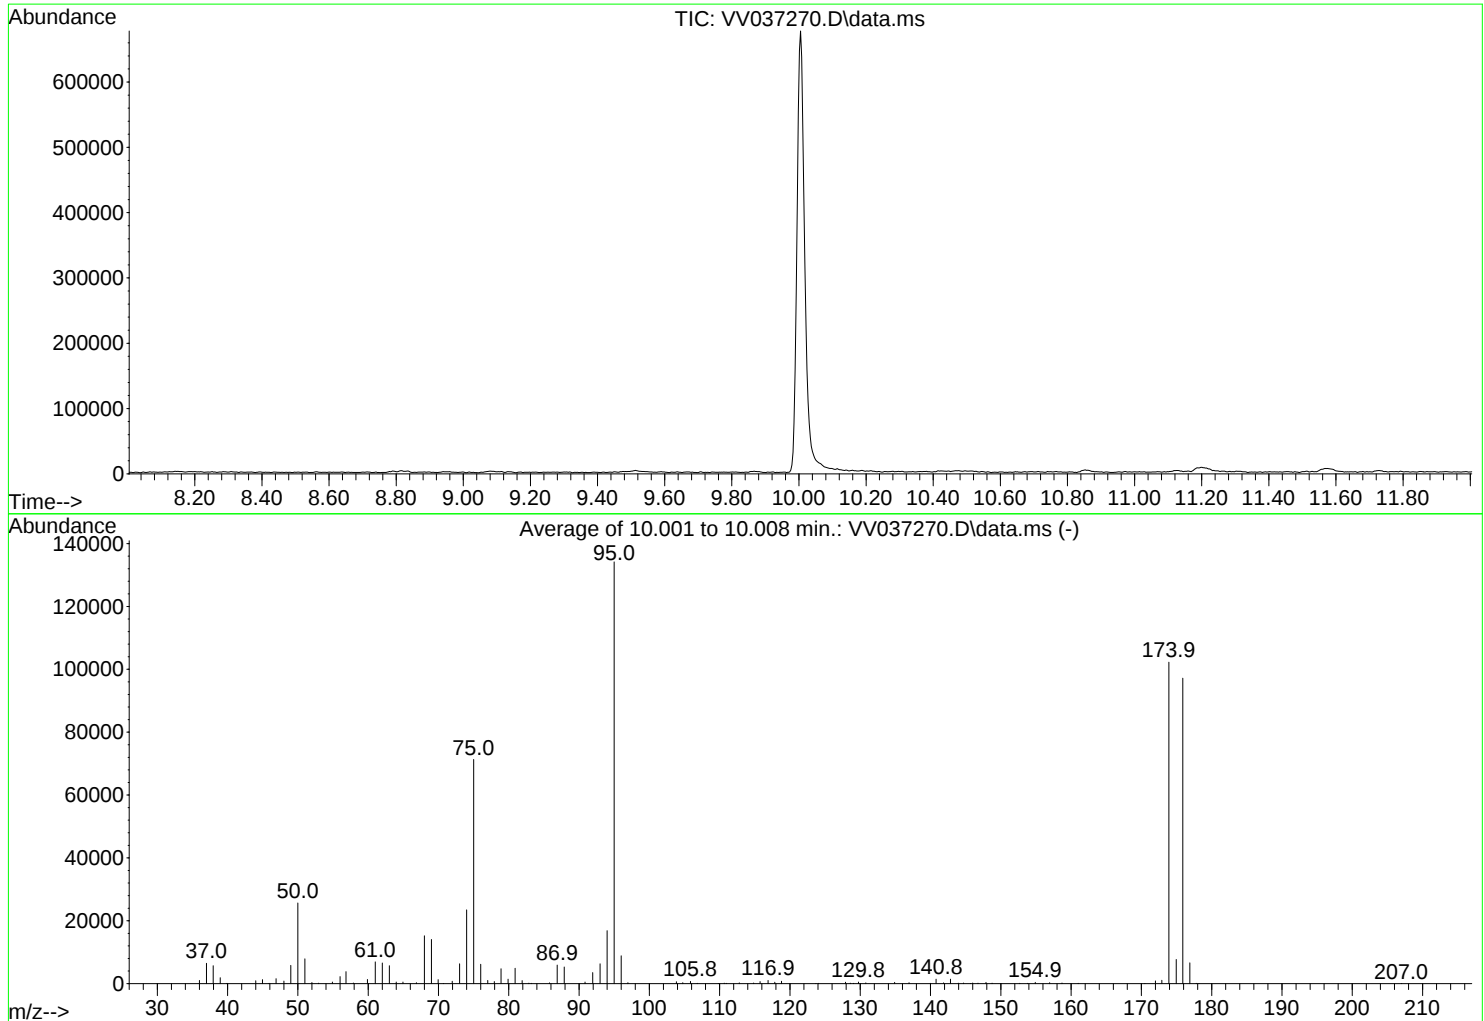

AutoFind: Scans 2787, 2788, 2789; Background Corrected with Scan 2773

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.1	25648	PASS
75	95	30	80	53.1	71299	PASS
95	95	100	100	100.0	134192	PASS
96	95	5	9	6.6	8875	PASS
173	174	0.00	2	1.0	1073	PASS
174	95	50	120	76.2	102256	PASS
175	174	5	9	7.5	7711	PASS
176	174	95	101	95.1	97197	PASS
177	176	5	9	6.8	6636	PASS

m/z	Abundance
37.80	136.0
38.80	171.0
39.30	159.0
40.00	348.0
41.10	134.0
42.00	114.0
42.90	246.0
44.00	743.0
55.20	105.0
56.70	164.0
76.90	187.0
132.80	105.0

Instrument :
MSVOA_V
ClientSampleId :
BFB220

m/z	Abundance
36.10	928.0
37.00	6447.0
38.00	6225.0
39.00	2104.0
39.90	482.0
42.10	141.0
43.00	212.0
44.00	1675.0
45.00	1240.0
46.90	1546.0
48.00	736.0
49.00	5569.0
50.00	25864.0
51.00	8140.0
52.00	331.0
53.00	149.0
54.90	511.0
56.00	2276.0
56.90	4096.0
57.90	228.0
59.90	1320.0
61.00	6762.0
62.00	6596.0
63.00	5345.0
64.00	474.0
65.00	549.0
66.90	330.0
68.00	15203.0
69.00	13847.0
69.90	1312.0
70.70	111.0
72.00	879.0
73.00	6070.0
74.00	23616.0
75.00	71720.0
76.00	6119.0
77.10	1176.0
77.90	747.0
78.90	4777.0
79.90	1327.0
80.90	4956.0
81.90	941.0
82.80	177.0
83.20	197.0
85.80	163.0
86.90	5553.0
87.90	5065.0
90.80	425.0
91.90	3559.0
93.00	6453.0
94.00	16984.0
95.00	134848.0
96.00	8817.0
97.00	359.0
103.80	628.0
104.80	280.0
105.80	747.0
106.80	164.0
110.60	137.0
111.00	167.0
112.80	249.0
114.80	152.0
115.80	649.0
116.90	950.0
117.90	437.0
118.80	767.0
123.70	113.0
127.90	490.0
128.60	170.0
129.00	176.0
129.80	496.0
130.80	242.0
132.80	103.0
134.90	378.0
136.90	237.0
140.00	102.0
140.80	1458.0
141.80	282.0
142.90	1348.0
143.90	196.0
144.70	176.0
145.70	150.0
146.10	135.0
146.80	125.0
147.90	379.0
148.80	108.0
152.70	158.0
154.90	438.0
157.00	303.0
158.70	223.0
161.00	140.0
172.00	861.0

Instrument :
MSVOA_V
ClientSampleId :
BFB220

172.90	1029.0
173.90	99224.0
174.90	7387.0
175.90	93464.0
176.90	6385.0
177.80	154.0

Instrument :
MSVOA_V
ClientSampleId :
BFB220

m/z	Abundance
36.00	1057.0
37.00	6656.0
38.00	6017.0
39.00	2145.0
39.90	438.0
42.10	117.0
43.00	246.0
44.00	1711.0
44.90	1291.0
45.90	122.0
46.90	1648.0
48.00	848.0
49.00	5962.0
50.00	26344.0
51.00	8232.0
52.00	369.0
52.90	148.0
54.90	534.0
56.00	2323.0
56.90	4164.0
57.90	227.0
59.90	1399.0
61.00	7239.0
62.00	6800.0
63.00	5963.0
64.00	507.0
64.90	546.0
66.90	322.0
68.00	15838.0
69.00	14510.0
70.00	1356.0
71.90	783.0
73.00	6543.0
74.00	24224.0
75.00	74040.0
76.00	6302.0
77.10	1292.0
78.00	730.0
78.90	4889.0
79.90	1457.0
80.90	5092.0
81.90	1019.0
82.90	185.0
83.20	182.0
85.80	274.0
86.90	6254.0
87.90	5532.0
90.80	521.0
91.90	3599.0
93.00	6528.0
94.00	17424.0
95.00	138624.0
96.00	9175.0
97.00	319.0
103.90	602.0
104.70	317.0
105.80	788.0
106.80	137.0
110.60	173.0
110.90	154.0
112.80	294.0
114.90	219.0
115.70	710.0
116.90	1110.0
117.90	501.0
118.80	798.0
124.10	110.0
127.90	461.0
128.60	169.0
129.10	147.0
129.70	503.0
130.80	256.0
134.90	446.0
137.00	312.0
140.00	119.0
140.80	1457.0
141.90	293.0
142.80	1495.0
143.90	179.0
144.70	192.0
146.00	198.0
146.70	168.0
147.90	427.0
148.70	142.0
152.70	122.0
153.80	131.0
154.90	397.0
156.90	313.0
158.70	220.0
161.00	131.0
172.00	951.0
172.90	1078.0

Instrument :
MSVOA_V
ClientSampleId :
BFB220

173.90	106016.0
175.00	8000.0
175.90	100568.0
176.90	6863.0
177.80	129.0
178.20	121.0
207.00	101.0

Instrument :
MSVOA_V
ClientSampleId :
BFB220

m/z	Abundance
35.90	1111.0
37.00	6361.0
38.00	5247.0
39.00	1983.0
39.90	435.0
41.00	121.0
43.10	261.0
44.00	1556.0
44.90	1248.0
45.90	185.0
46.90	1511.0
48.00	800.0
49.00	5853.0
50.00	24736.0
51.00	7306.0
52.00	376.0
52.90	145.0
54.90	561.0
56.00	2177.0
56.90	3691.0
57.90	221.0
59.90	1334.0
61.00	6730.0
62.00	6245.0
63.00	5735.0
64.00	558.0
64.90	480.0
66.80	289.0
68.00	14564.0
69.00	13768.0
70.00	1212.0
71.90	598.0
73.00	6401.0
74.00	22528.0
75.00	68136.0
76.00	6012.0
77.00	1147.0
77.90	583.0
78.90	4538.0
79.90	1441.0
80.90	4618.0
81.90	1025.0
82.90	154.0
85.80	333.0
86.90	5974.0
87.90	5286.0
90.90	530.0
92.00	3405.0
93.00	5967.0
94.00	16106.0
95.00	129104.0
96.00	8632.0
96.90	318.0
103.90	575.0
104.70	288.0
105.90	695.0
109.80	104.0
110.70	158.0
112.80	278.0
114.90	268.0
115.70	615.0
116.90	1077.0
117.80	482.0
118.80	769.0
124.00	130.0
127.90	407.0
128.60	149.0
129.80	480.0
130.80	211.0
134.90	412.0
137.00	350.0
140.00	121.0
140.80	1390.0
141.90	249.0
142.80	1388.0
144.00	132.0
144.70	194.0
145.90	245.0
146.70	142.0
147.90	411.0
148.70	160.0
150.00	116.0
153.80	133.0
154.90	447.0
156.90	267.0
158.70	158.0
161.00	114.0
170.50	108.0
172.00	768.0
172.90	1111.0
173.90	101528.0
175.00	7745.0

Instrument :
MSVOA_V
ClientSampleId :
BFB220

175.90

176.90

207.00

97560.0

6659.0

113.0

Instrument :

MSVOA_V

ClientSampleId :

BFB220