




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV091525\
Data File : VV039067.D
Acq On : 15 Sep 2025 09:55
Operator : SY/MD
Sample : VSTD00154
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VSTD001254

Manual IntegrationsAPPROVED

Reviewed By :Mahesh Dadoda 09/16/2025
Supervised By :Semsettin Yesilyurt 09/16/2025

Quant Time: Sep 16 01:36:39 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR091525wMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Tue Sep 16 01:35:33 2025
Response via : Initial Calibration

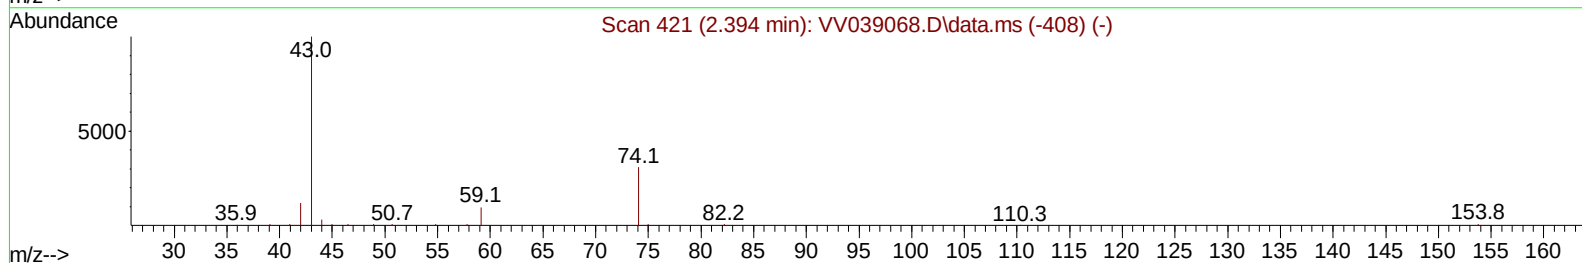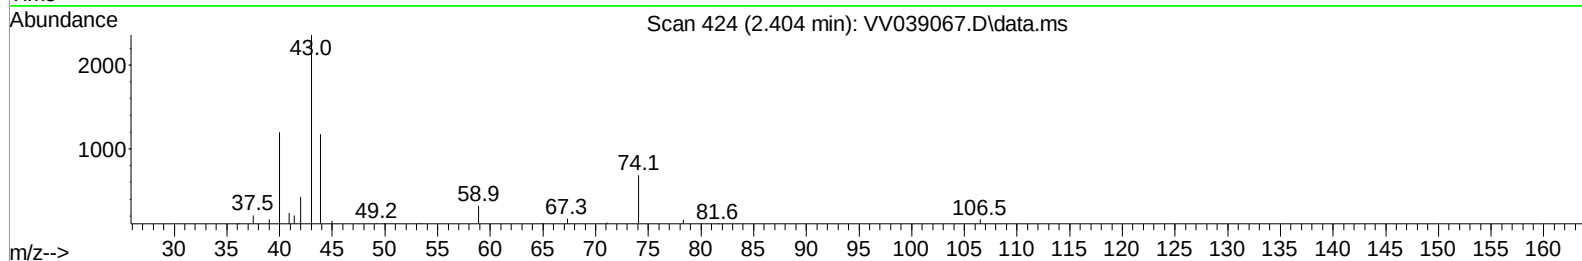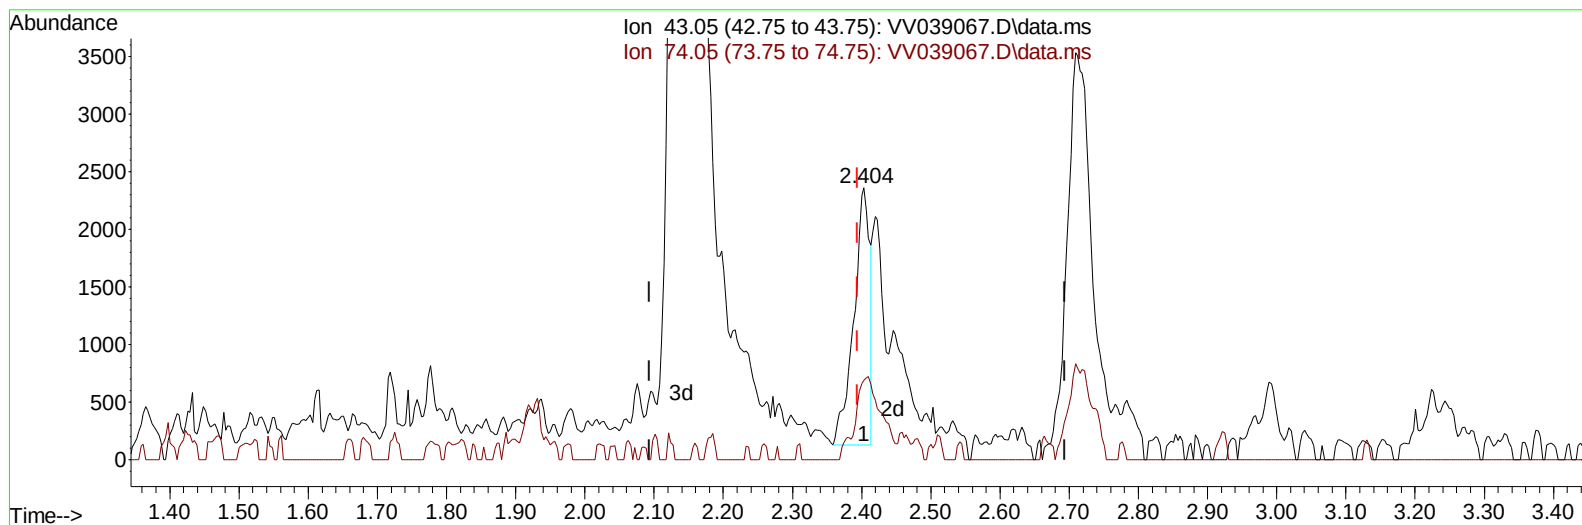

TIC: VV039067.D\data.ms

(15) Methyl Acetate (T)

2.404min (+ 0.010) 0.37 ug/L

response 3579

Ion	Exp%	Act%
43.05	100.00	100.00
74.05	23.50	53.23#
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV091525\
Data File : VV039067.D
Acq On : 15 Sep 2025 09:55
Operator : SY/MD
Sample : VSTD00154
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VSTD001254

Manual IntegrationsAPPROVED

Quant Time: Sep 16 01:36:39 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR091525wMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Tue Sep 16 01:35:33 2025
Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 09/16/2025
Supervised By :Semsettin Yesilyurt 09/16/2025

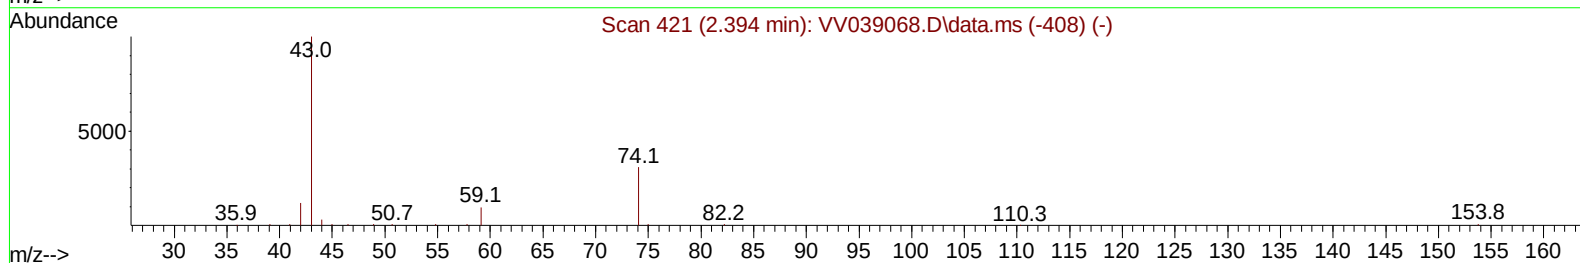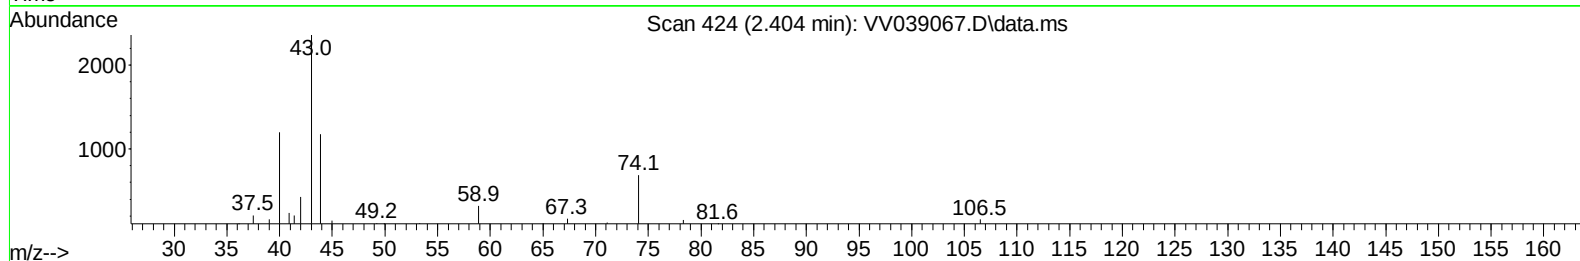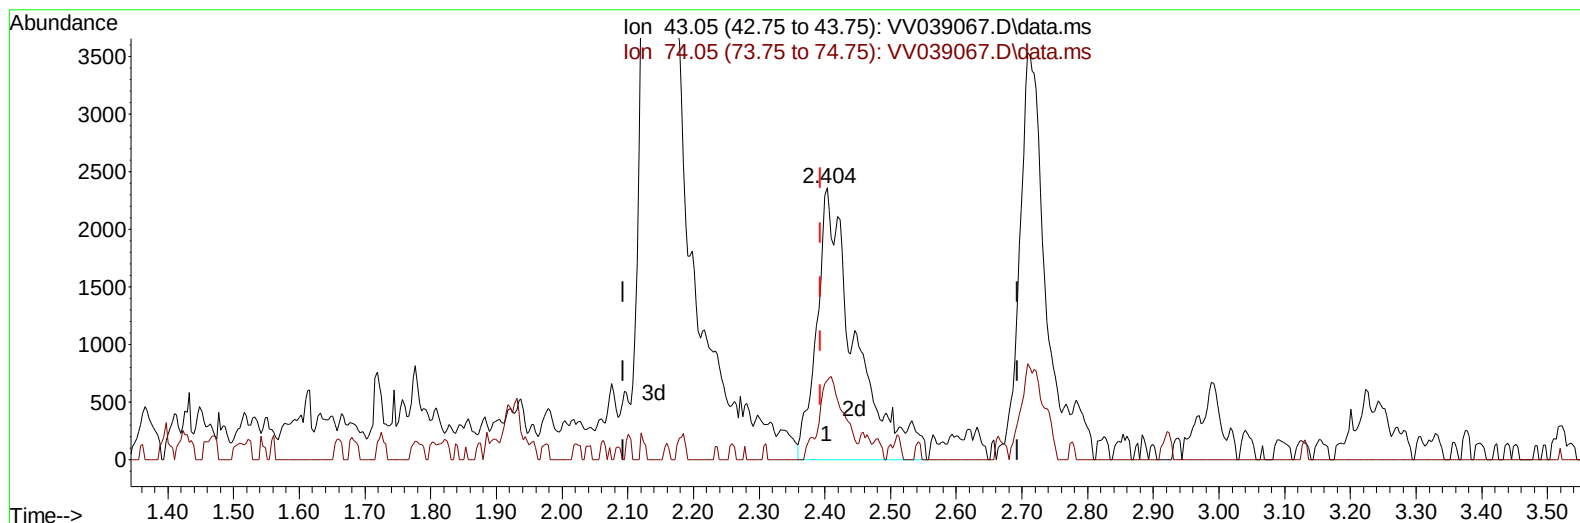

TIC: VV039067.D\data.ms

(15) Methyl Acetate (T)

2.404min (+ 0.010) 0.98 ug/L m

response 9584

Ion	Exp%	Act%
43.05	100.00	100.00
74.05	23.50	19.88
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV091525\
Data File : VV039067.D
Acq On : 15 Sep 2025 09:55
Operator : SY/MD
Sample : VSTD00154
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VSTD001254

Manual IntegrationsAPPROVED

Reviewed By :Mahesh Dadoda 09/16/2025
Supervised By :Semsettin Yesilyurt 09/16/2025

Quant Time: Sep 16 01:36:39 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR091525wMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Tue Sep 16 01:35:33 2025
Response via : Initial Calibration

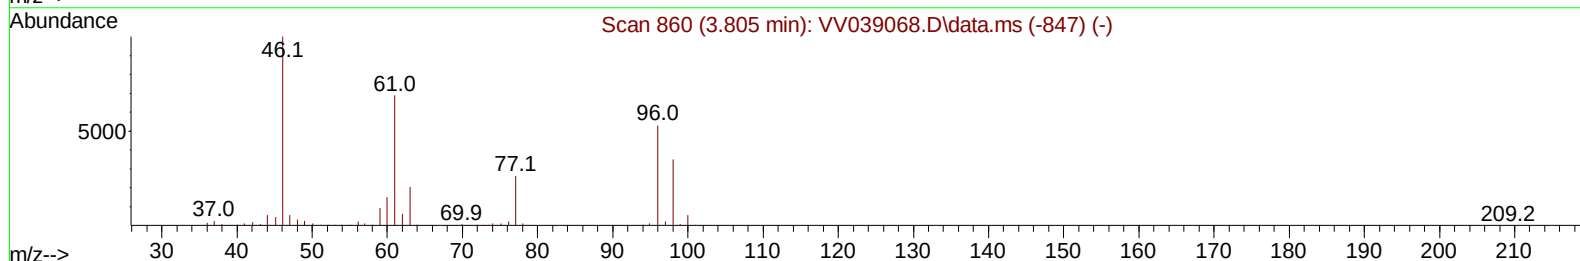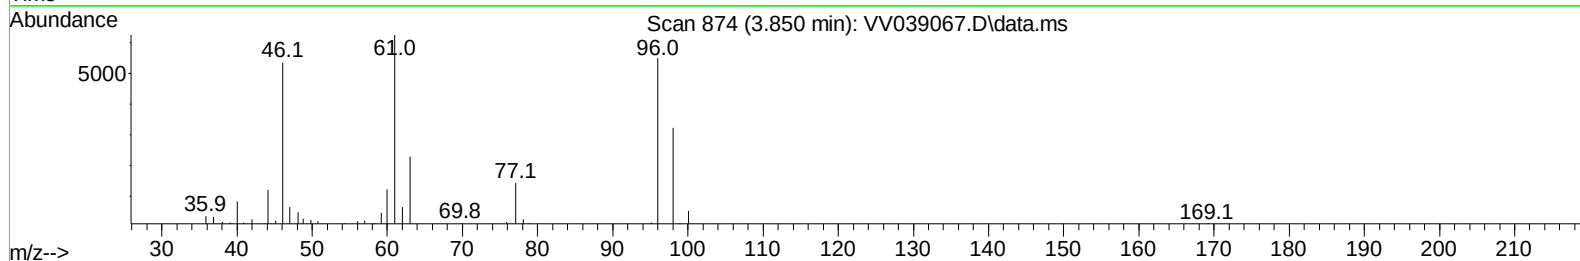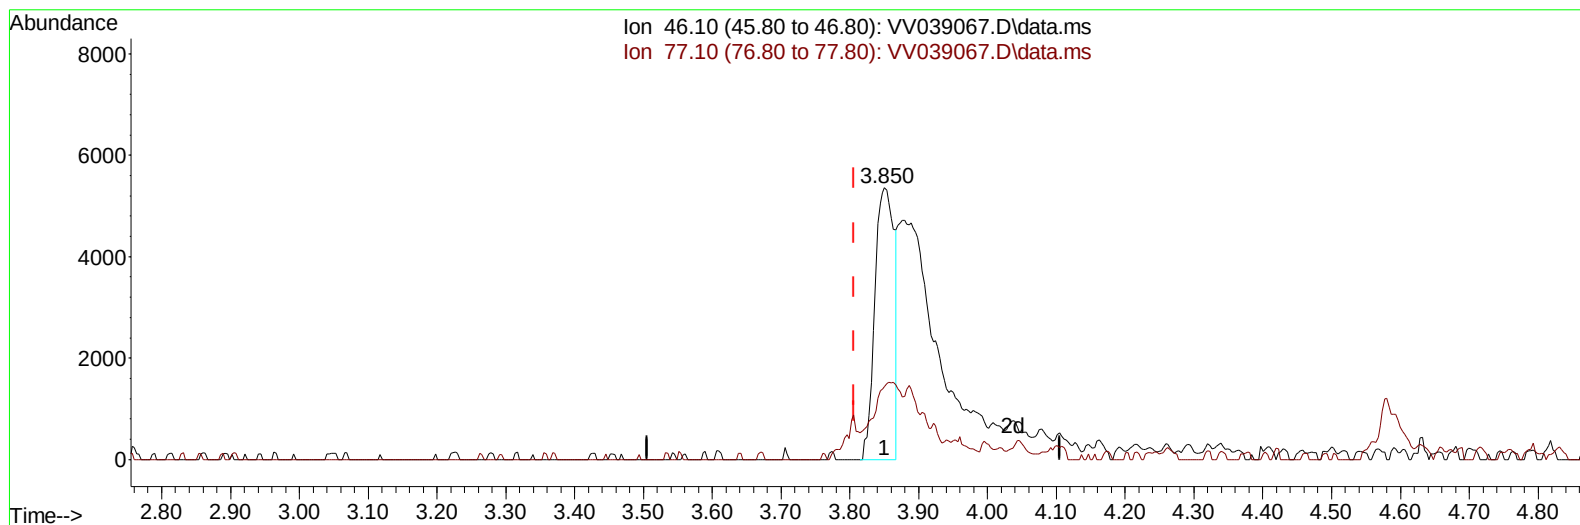

TIC: VV039067.D\data.ms

(20) 2-Butanone-d5 (S)**3.850min (+ 0.045) 2.61 ug/L****response 10426**

Ion	Exp%	Act%
46.10	100.00	100.00
77.10	24.00	28.57
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV091525\
Data File : VV039067.D
Acq On : 15 Sep 2025 09:55
Operator : SY/MD
Sample : VSTD00154
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VSTD001254

Manual IntegrationsAPPROVED

Reviewed By :Mahesh Dadoda 09/16/2025
Supervised By :Semsettin Yesilyurt 09/16/2025

Quant Time: Sep 16 01:36:39 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR091525wMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Tue Sep 16 01:35:33 2025
Response via : Initial Calibration

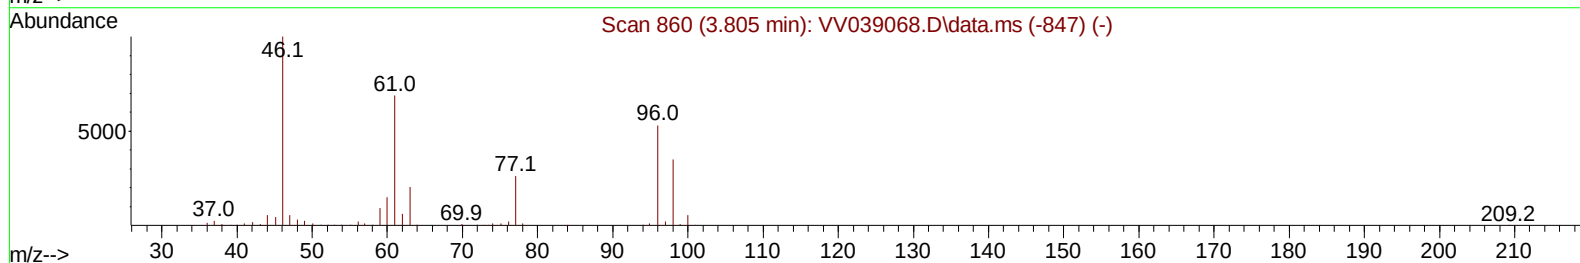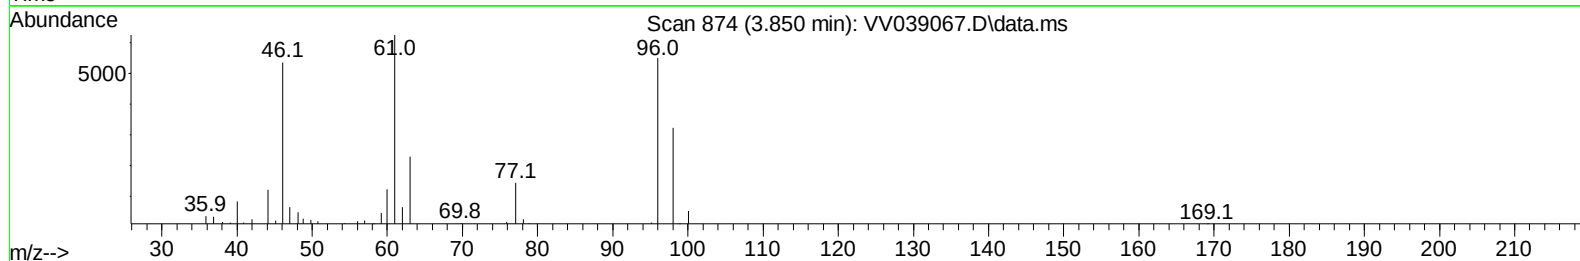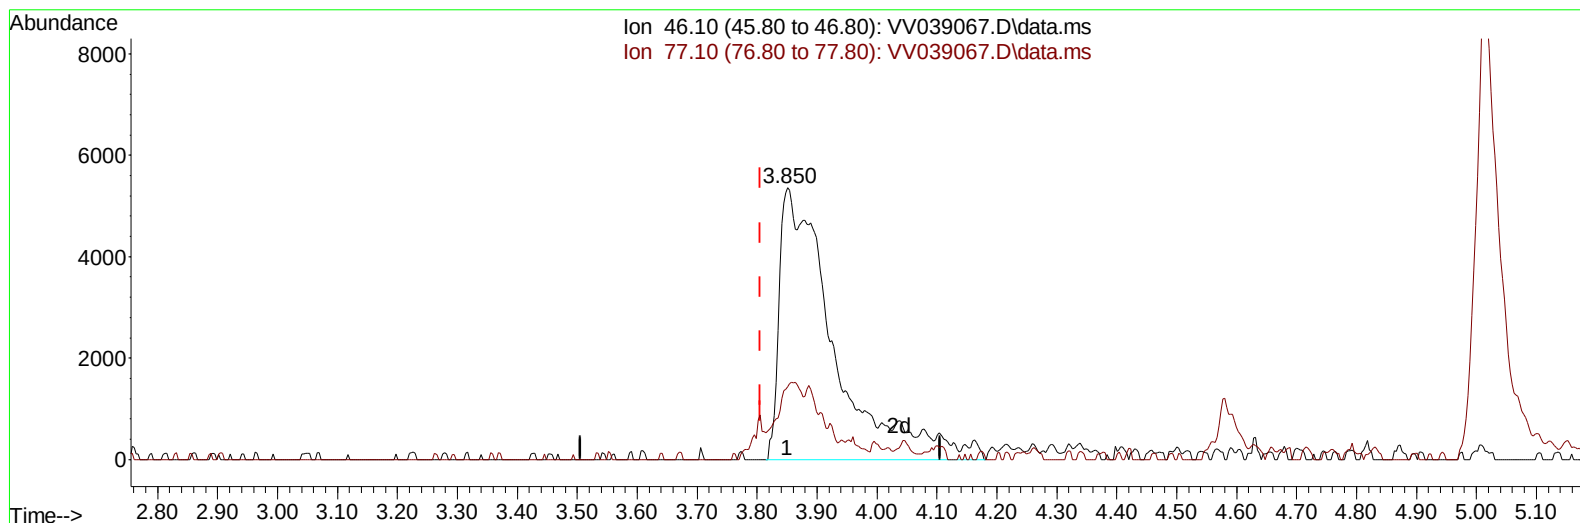

TIC: VV039067.D\data.ms

(20) 2-Butanone-d5 (S)

3.850min (+ 0.045) 8.52 ug/L m

response 34037

Ion	Exp%	Act%
46.10	100.00	100.00
77.10	24.00	8.75#
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV091525\
Data File : VV039067.D
Acq On : 15 Sep 2025 09:55
Operator : SY/MD
Sample : VSTD00154
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VSTD001254

Manual IntegrationsAPPROVED

Reviewed By :Mahesh Dadoda 09/16/2025
Supervised By :Semsettin Yesilyurt 09/16/2025

Quant Time: Sep 16 01:36:39 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR091525WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Tue Sep 16 01:35:33 2025
Response via : Initial Calibration

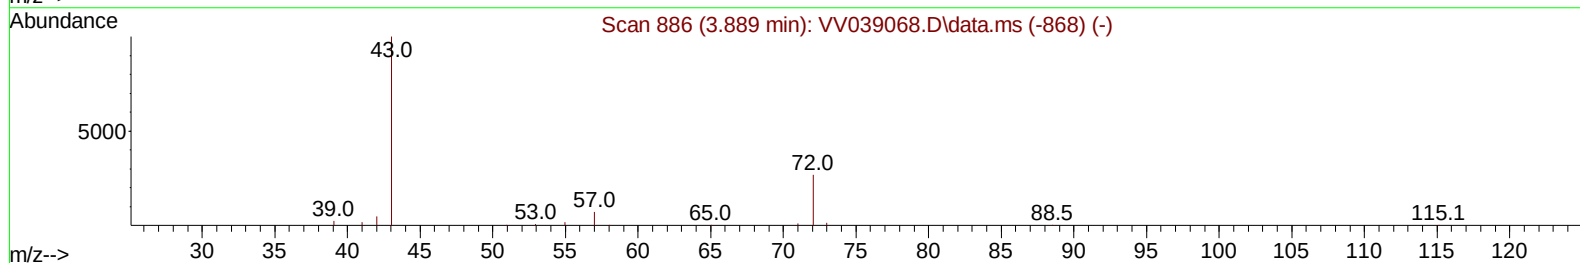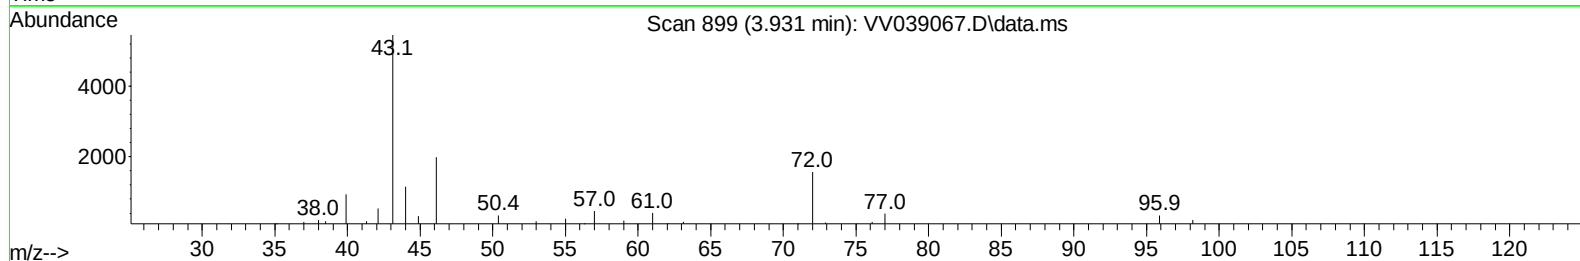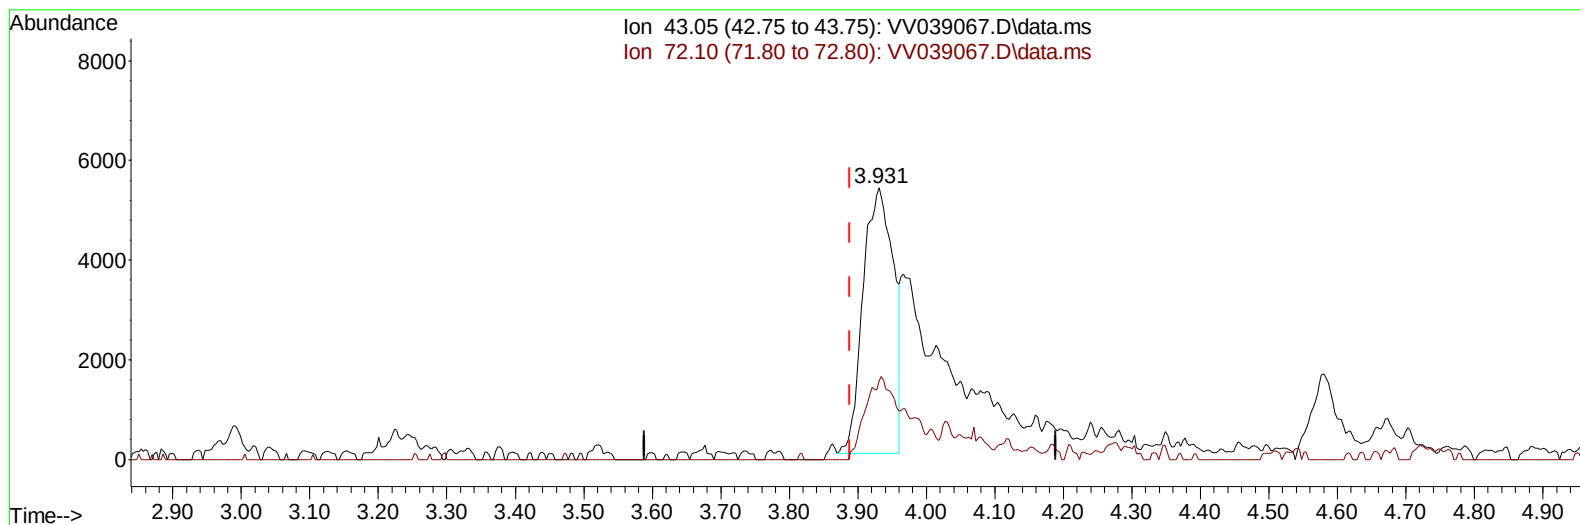

TIC: VV039067.D\data.ms

(21) 2-Butanone (T)

3.931min (+ 0.042) 3.70 ug/L

response 16259

Ion	Exp%	Act%
43.05	100.00	100.00
72.10	24.00	30.30
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV091525\
Data File : VV039067.D
Acq On : 15 Sep 2025 09:55
Operator : SY/MD
Sample : VSTD00154
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VSTD001254

Manual IntegrationsAPPROVED

Quant Time: Sep 16 01:36:39 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR091525WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Tue Sep 16 01:35:33 2025
Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 09/16/2025
Supervised By :Semsettin Yesilyurt 09/16/2025

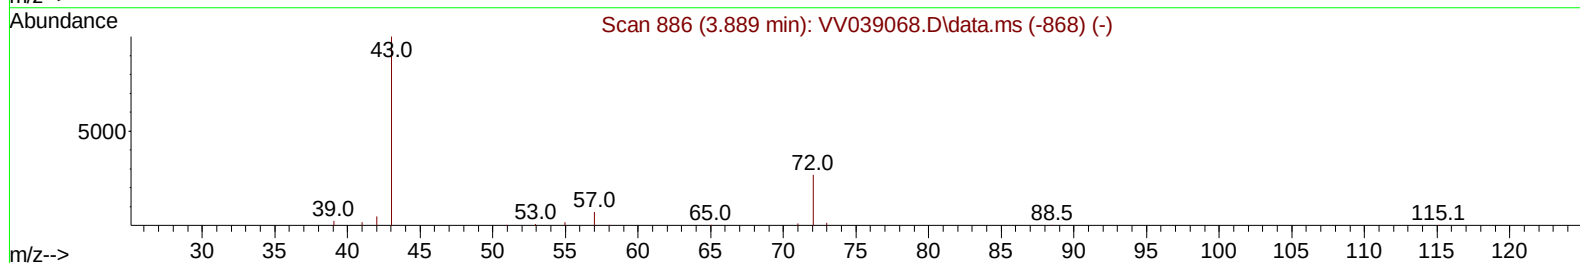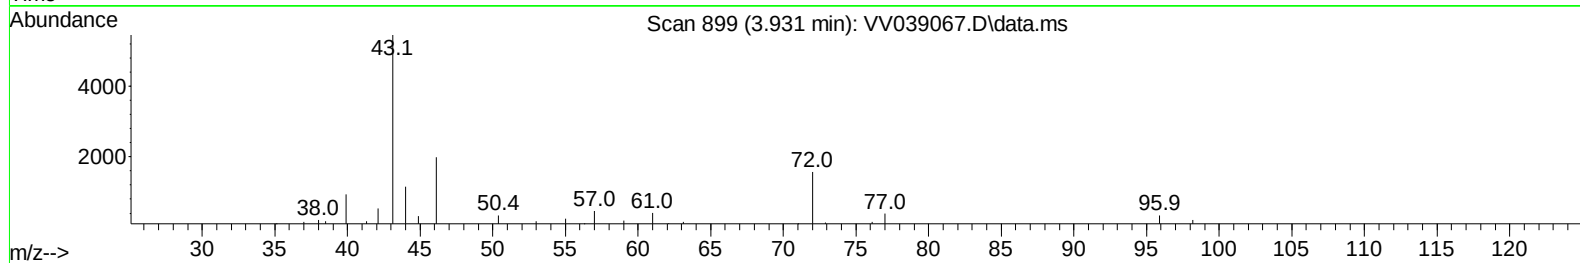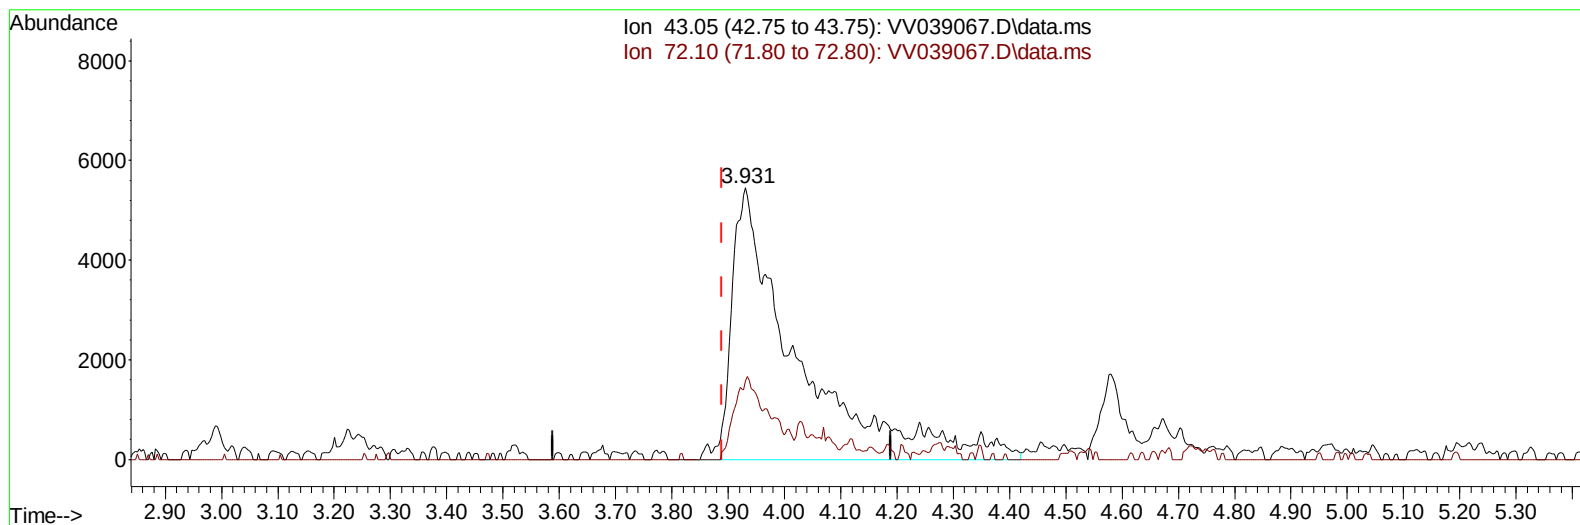

TIC: VV039067.D\data.ms

(21) 2-Butanone (T)

3.931min (+ 0.042) 9.97 ug/L m

response 43798

Ion	Exp%	Act%
43.05	100.00	100.00
72.10	24.00	11.25#
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV091525\
Data File : VV039067.D
Acq On : 15 Sep 2025 09:55
Operator : SY/MD
Sample : VSTD00154
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VSTD001254

Manual IntegrationsAPPROVED

Quant Time: Sep 16 01:36:39 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR091525WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Tue Sep 16 01:35:33 2025
Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 09/16/2025
Supervised By :Semsettin Yesilyurt 09/16/2025

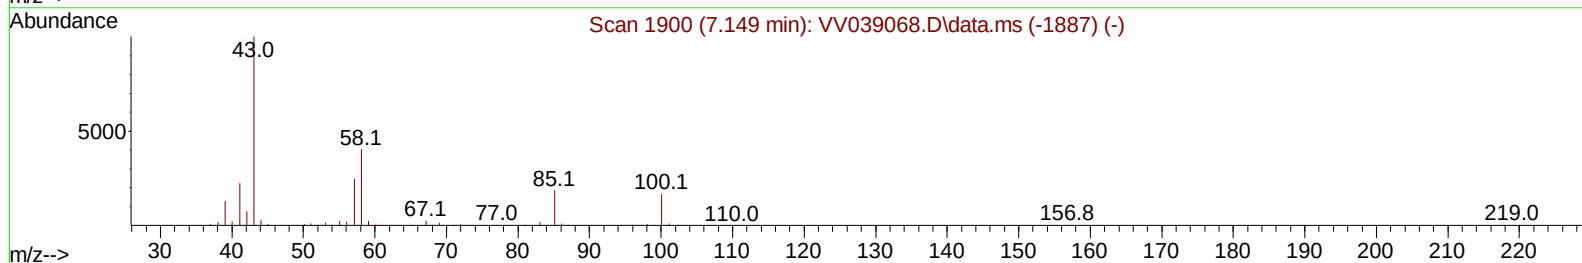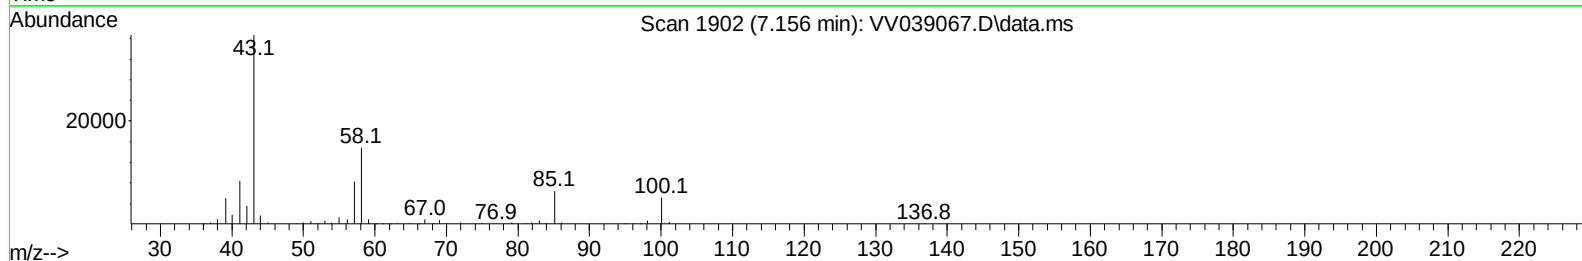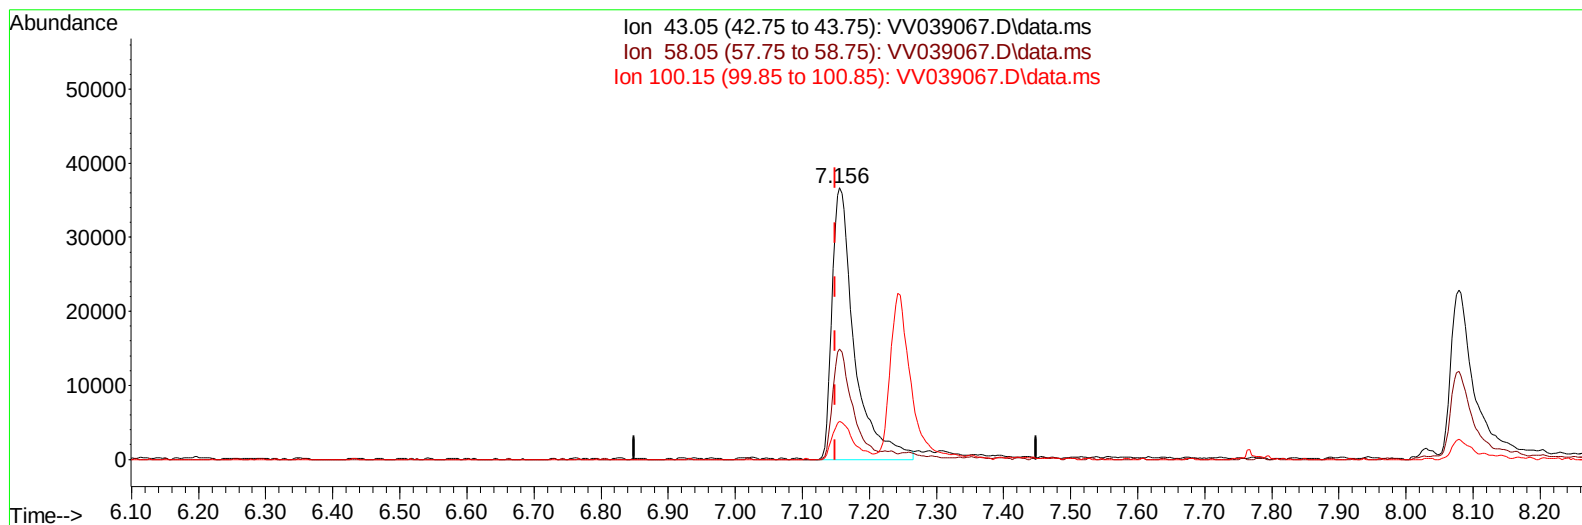

TIC: VV039067.D\data.ms

(40) 4-Methyl-2-pentanone (T)

7.156min (+ 0.006) 6.70 ug/L

response 84914

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	39.60	36.06
100.15	16.20	13.55
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV091525\
 Data File : VV039067.D
 Acq On : 15 Sep 2025 09:55
 Operator : SY/MD
 Sample : VSTD00154
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VSTD001254

Manual IntegrationsAPPROVED

Quant Time: Sep 16 01:36:39 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR091525WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Tue Sep 16 01:35:33 2025
 Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 09/16/2025
 Supervised By :Semsettin Yesilyurt 09/16/2025

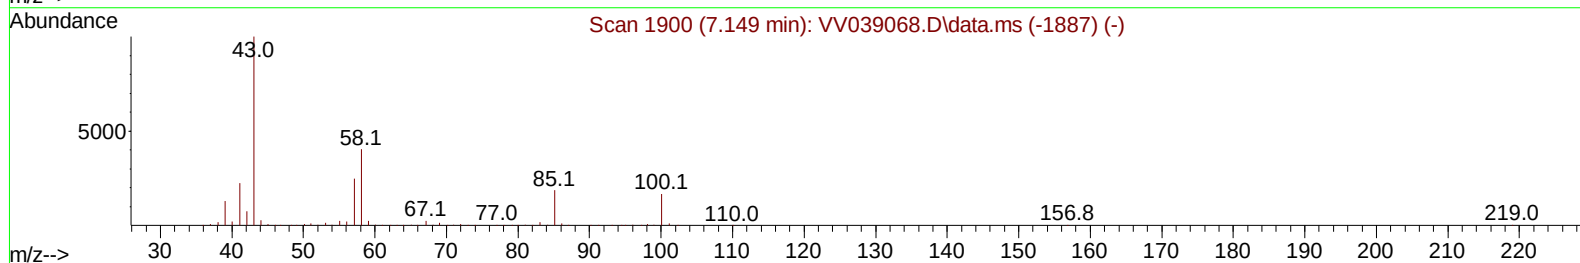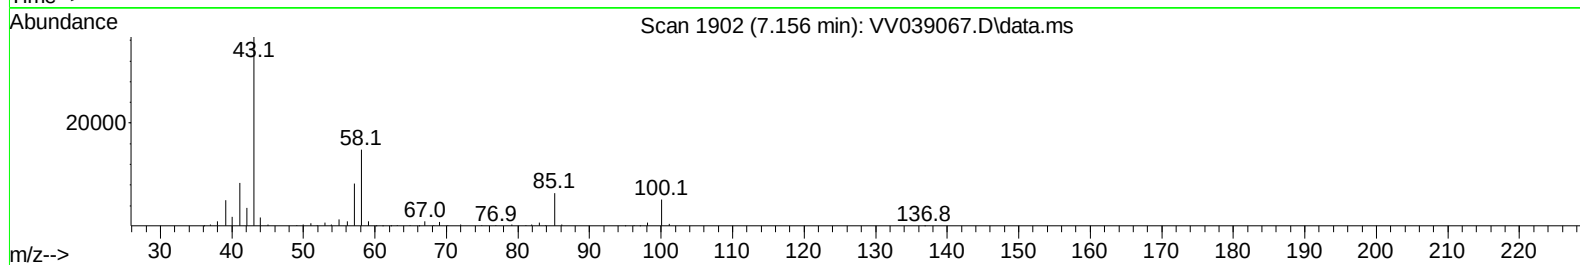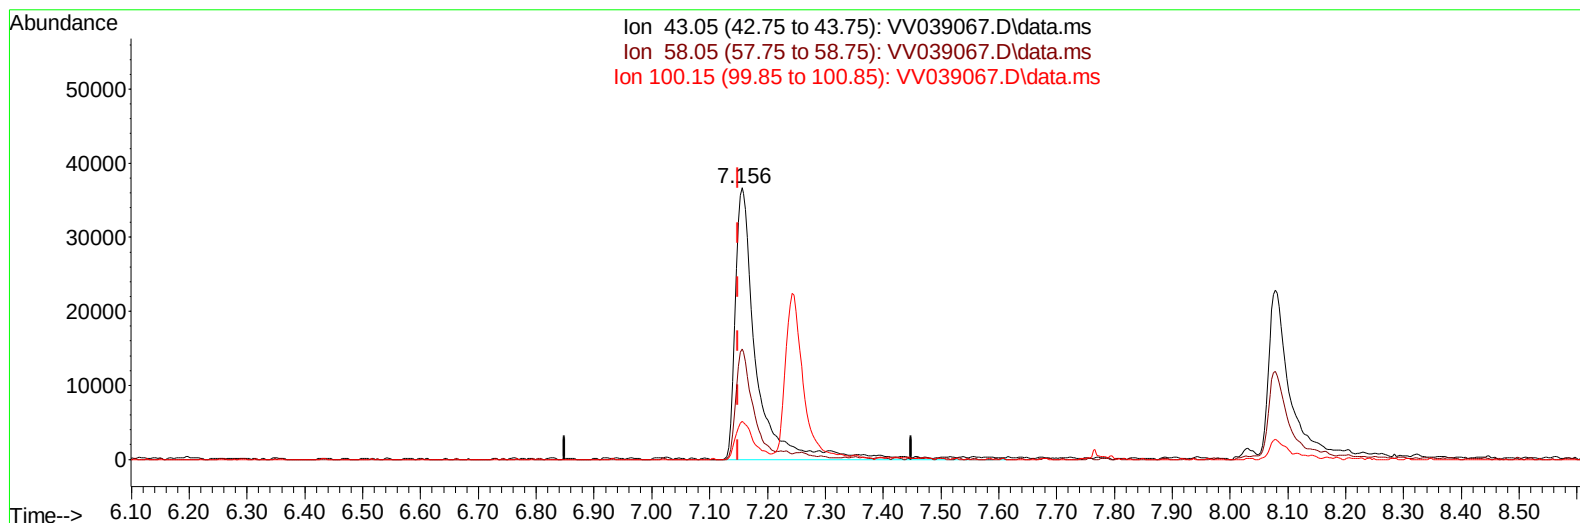

TIC: VV039067.D\data.ms

(40) 4-Methyl-2-pentanone (T)

7.156min (+ 0.006) 7.51 ug/L m

response 95150

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	39.60	32.18
100.15	16.20	12.09#
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV091525\
Data File : VV039067.D
Acq On : 15 Sep 2025 09:55
Operator : SY/MD
Sample : VSTD00154
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VSTD001254

Manual IntegrationsAPPROVED

Reviewed By :Mahesh Dadoda 09/16/2025
Supervised By :Semsettin Yesilyurt 09/16/2025

Quant Time: Sep 16 01:36:39 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR091525WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Tue Sep 16 01:35:33 2025
Response via : Initial Calibration

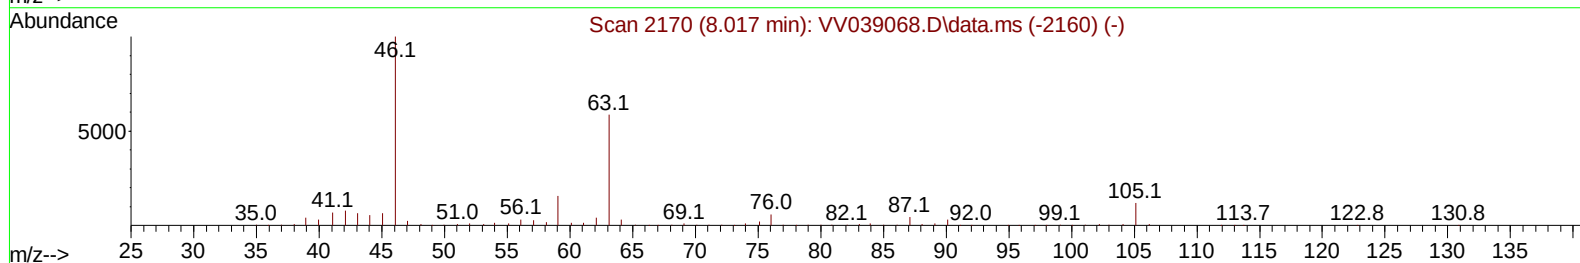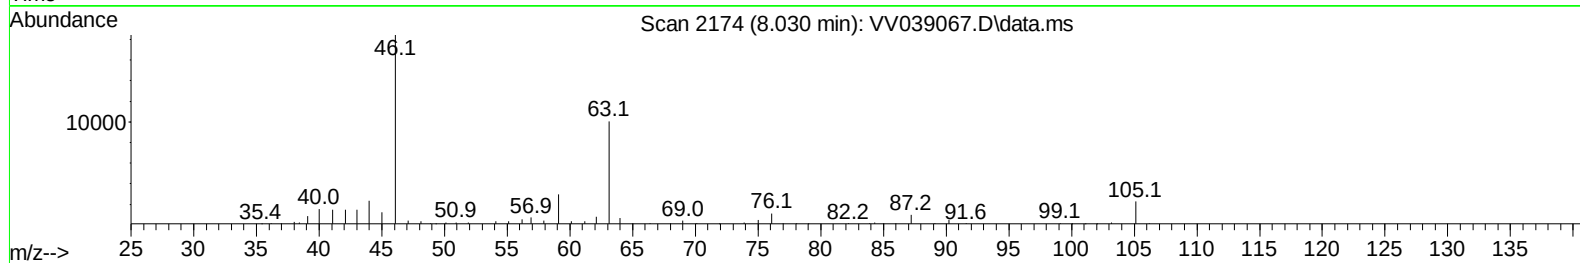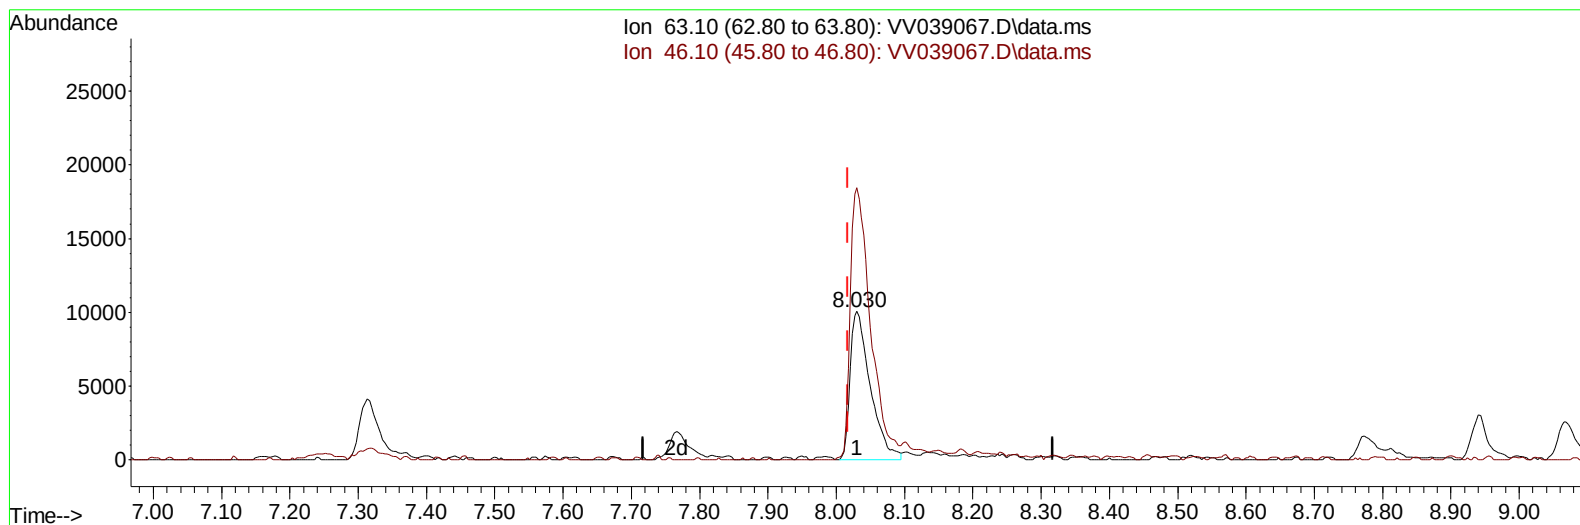

TIC: VV039067.D\data.ms

(46) 2-Hexanone-d5 (S)

8.030min (+ 0.013) 5.84 ug/L

response 20645

Ion	Exp%	Act%
63.10	100.00	100.00
46.10	175.20	185.85
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV091525\
Data File : VV039067.D
Acq On : 15 Sep 2025 09:55
Operator : SY/MD
Sample : VSTD00154
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VSTD001254

Manual IntegrationsAPPROVED

Reviewed By :Mahesh Dadoda 09/16/2025
Supervised By :Semsettin Yesilyurt 09/16/2025

Quant Time: Sep 16 01:36:39 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR091525WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Tue Sep 16 01:35:33 2025
Response via : Initial Calibration

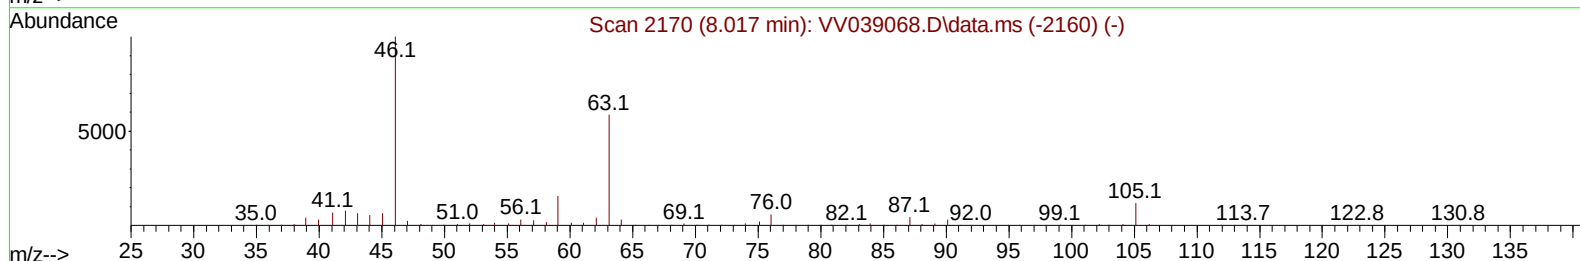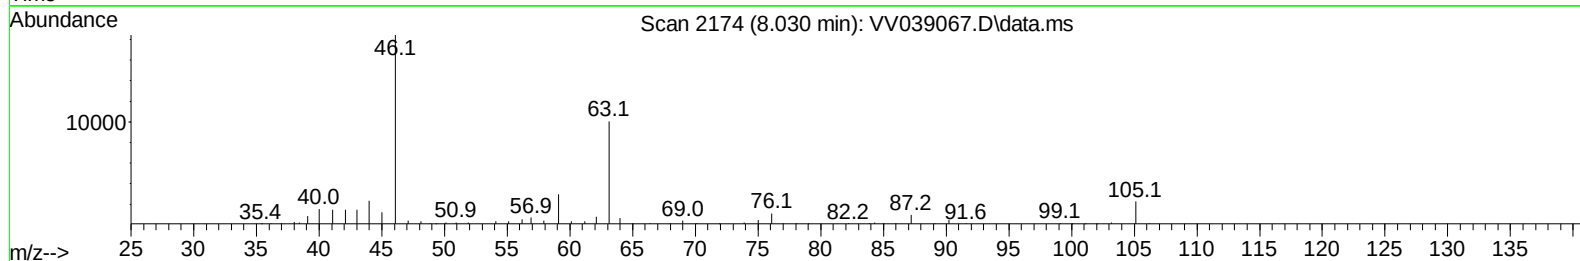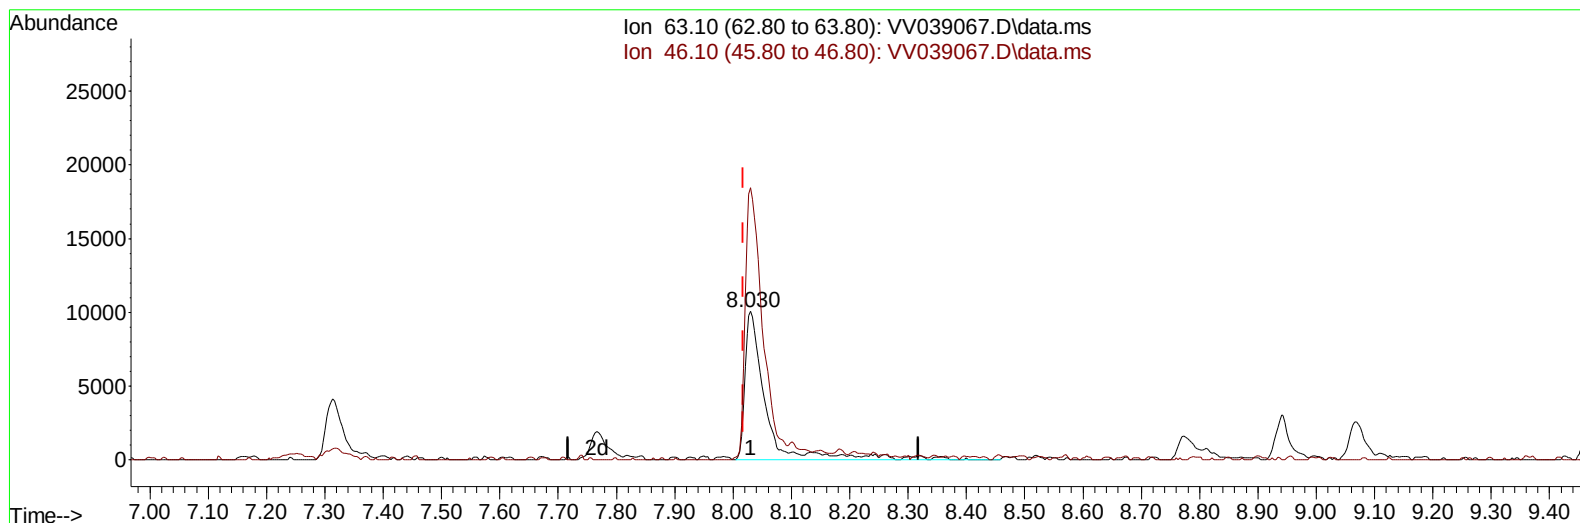

TIC: VV039067.D\data.ms

(46) 2-Hexanone-d5 (S)

8.030min (+ 0.013) 6.96 ug/L m

response 24602

Ion	Exp%	Act%
63.10	100.00	100.00
46.10	175.20	155.96
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV091525\
Data File : VV039067.D
Acq On : 15 Sep 2025 09:55
Operator : SY/MD
Sample : VSTD00154
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VSTD001254

Manual IntegrationsAPPROVED

Quant Time: Sep 16 01:36:39 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR091525WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Tue Sep 16 01:35:33 2025
Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 09/16/2025
Supervised By :Semsettin Yesilyurt 09/16/2025

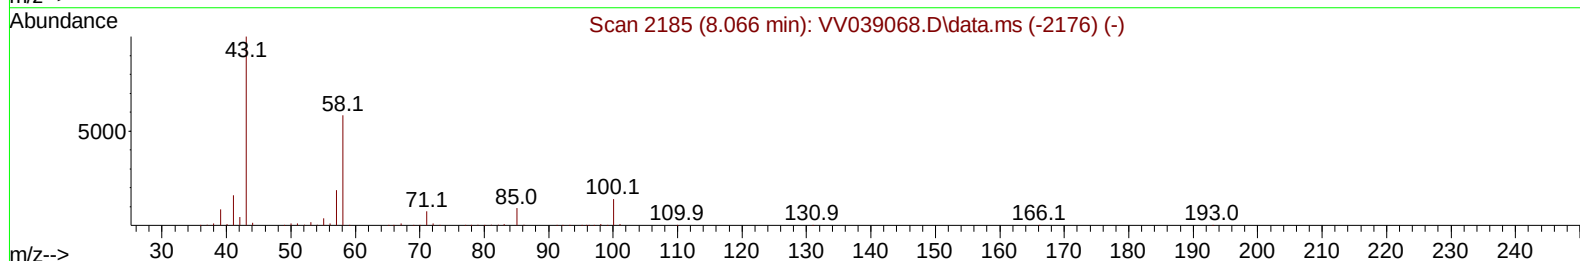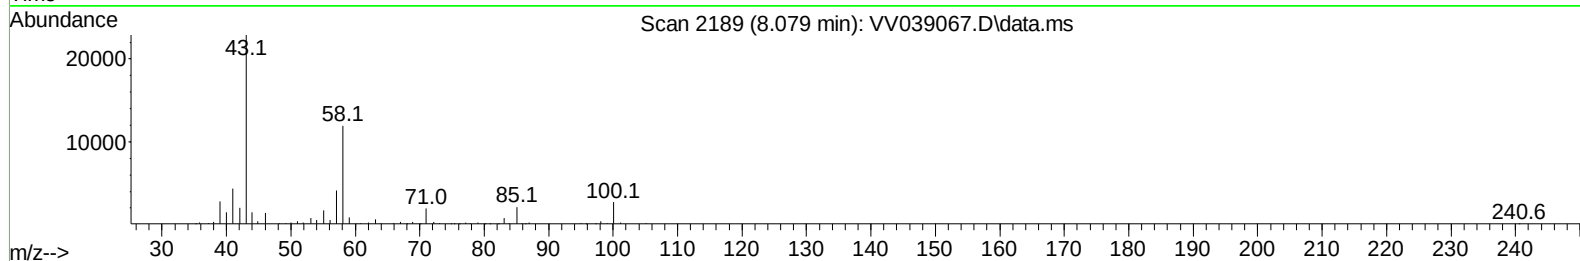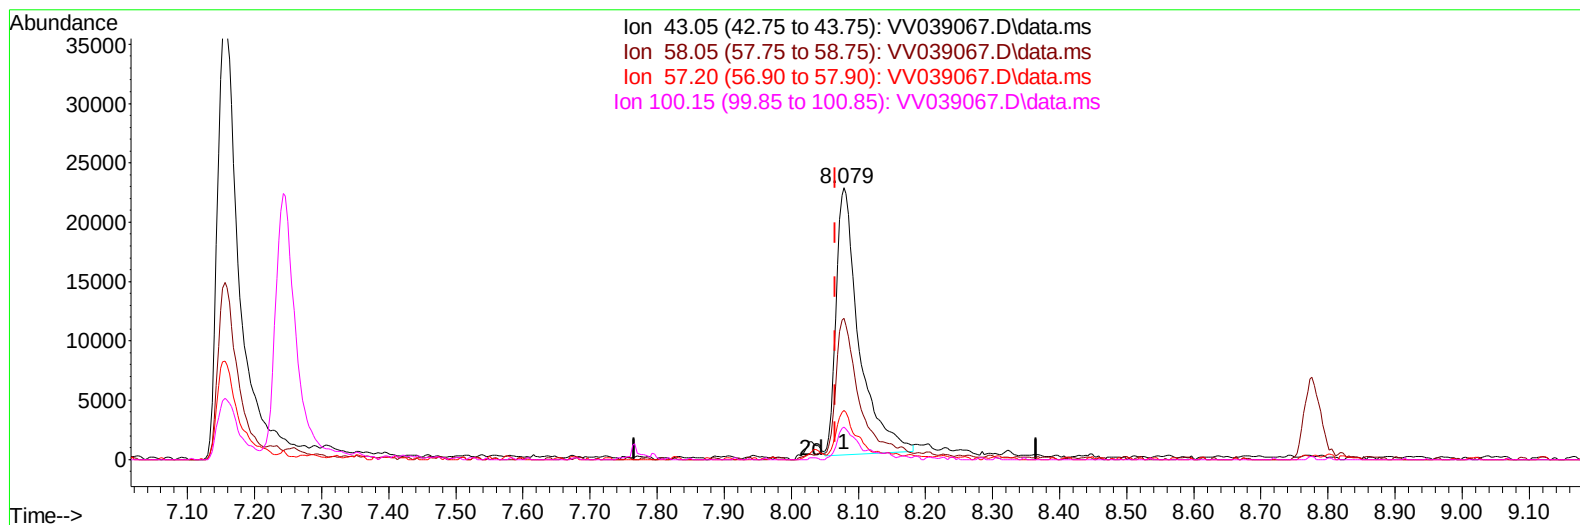

TIC: VV039067.D\data.ms

(48) 2-Hexanone (T)

8.079min (+ 0.013) 6.41 ug/L

response 53594

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	57.00	50.90
57.20	19.50	13.75#
100.15	13.10	9.84#




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV091525\
Data File : VV039067.D
Acq On : 15 Sep 2025 09:55
Operator : SY/MD
Sample : VSTD00154
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VSTD001254

Manual IntegrationsAPPROVED

Reviewed By :Mahesh Dadoda 09/16/2025
Supervised By :Semsettin Yesilyurt 09/16/2025

Quant Time: Sep 16 01:36:39 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR091525WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Tue Sep 16 01:35:33 2025
Response via : Initial Calibration

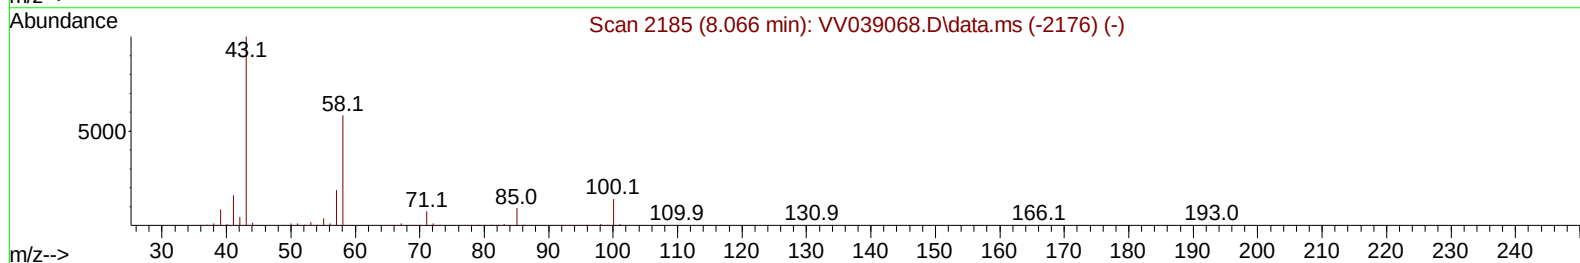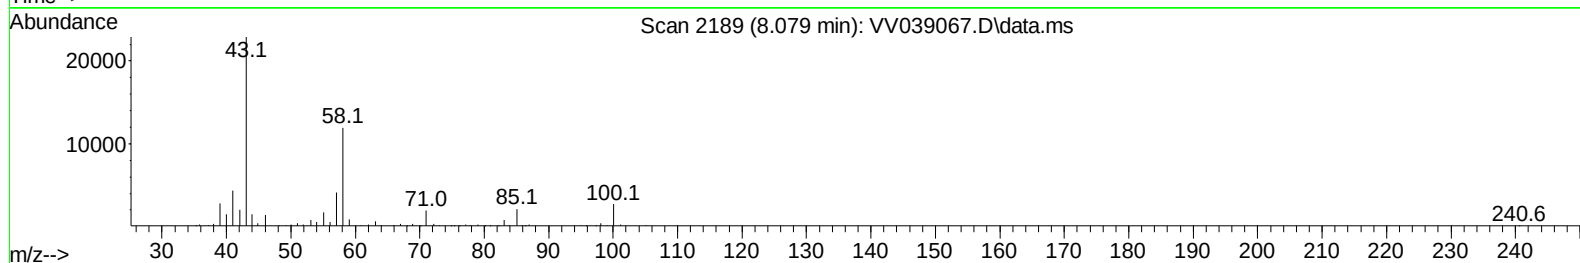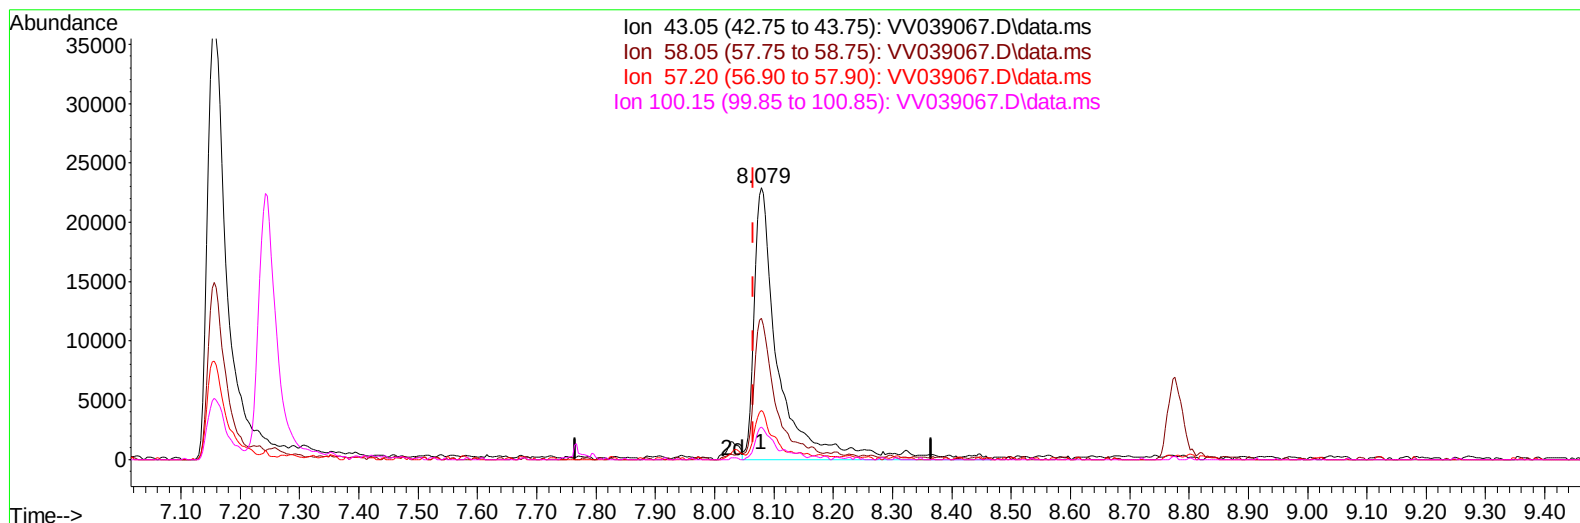

TIC: VV039067.D\data.ms

(48) 2-Hexanone (T)

8.079min (+ 0.013) 8.00 ug/L m

response 66832

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	57.00	40.82#
57.20	19.50	11.03#
100.15	13.10	7.89#




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV091525\
Data File : VV039067.D
Acq On : 15 Sep 2025 09:55
Operator : SY/MD
Sample : VSTD00154
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VSTD001254

Manual IntegrationsAPPROVED

Quant Time: Sep 16 01:36:39 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR091525WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Tue Sep 16 01:35:33 2025
Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 09/16/2025
Supervised By :Semsettin Yesilyurt 09/16/2025

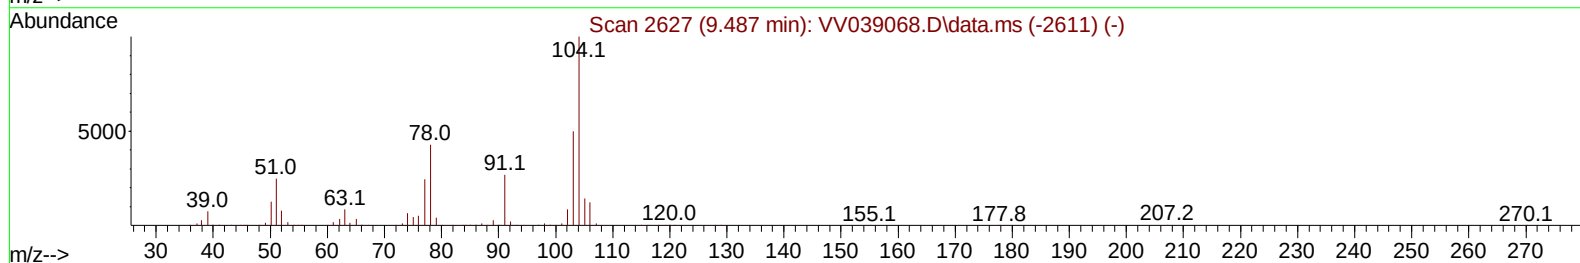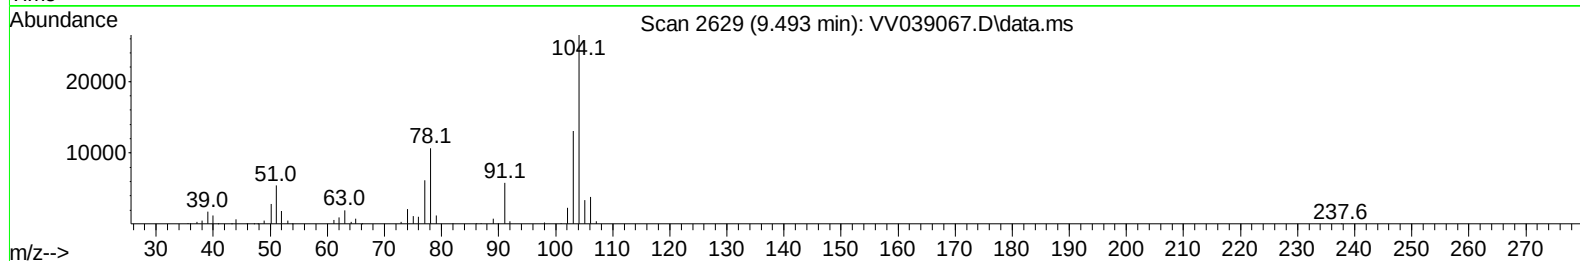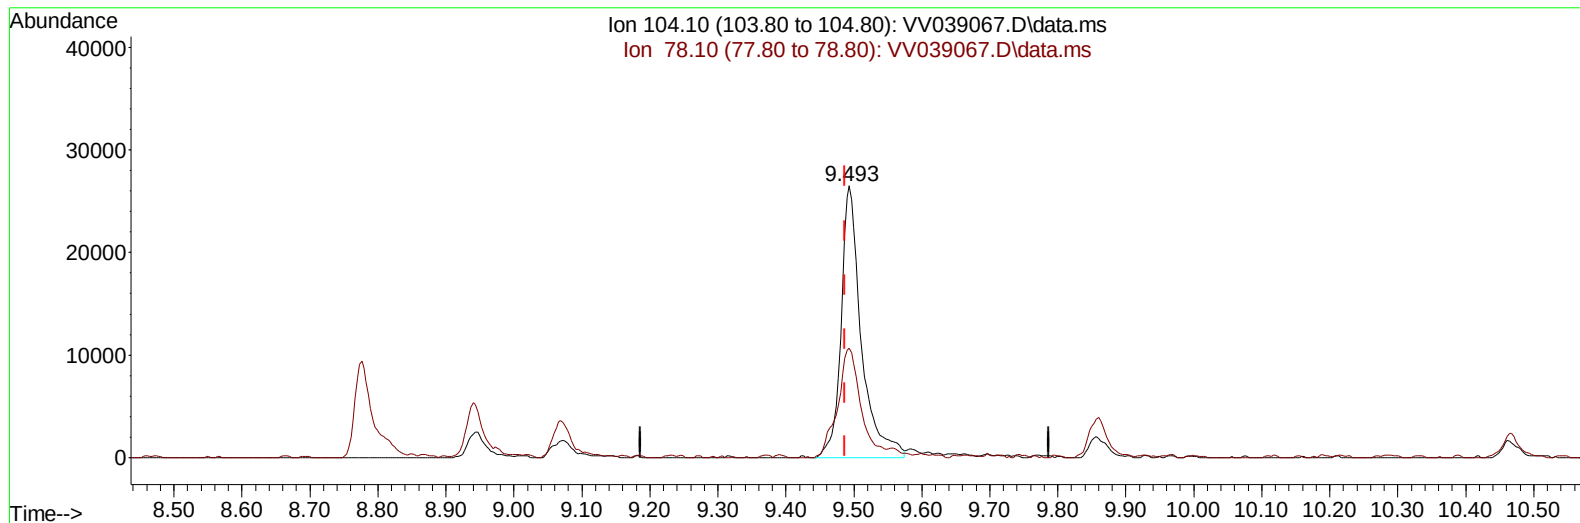

TIC: VV039067.D\data.ms

(55) Styrene (T)

9.493min (+ 0.006) 0.64 ug/L

response 54522

Ion	Exp%	Act%
104.10	100.00	100.00
78.10	42.70	40.31
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV091525\
Data File : VV039067.D
Acq On : 15 Sep 2025 09:55
Operator : SY/MD
Sample : VSTD00154
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VSTD001254

Manual IntegrationsAPPROVED

Quant Time: Sep 16 01:36:39 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR091525wMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Tue Sep 16 01:35:33 2025
Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 09/16/2025
Supervised By :Semsettin Yesilyurt 09/16/2025

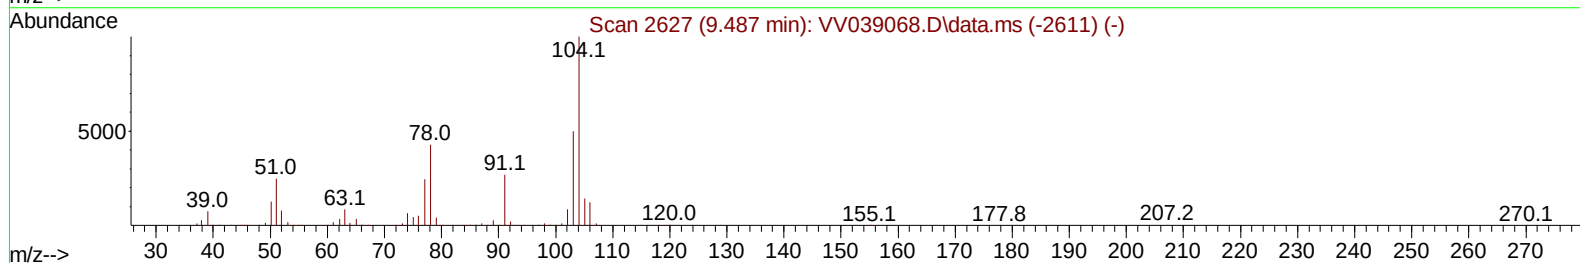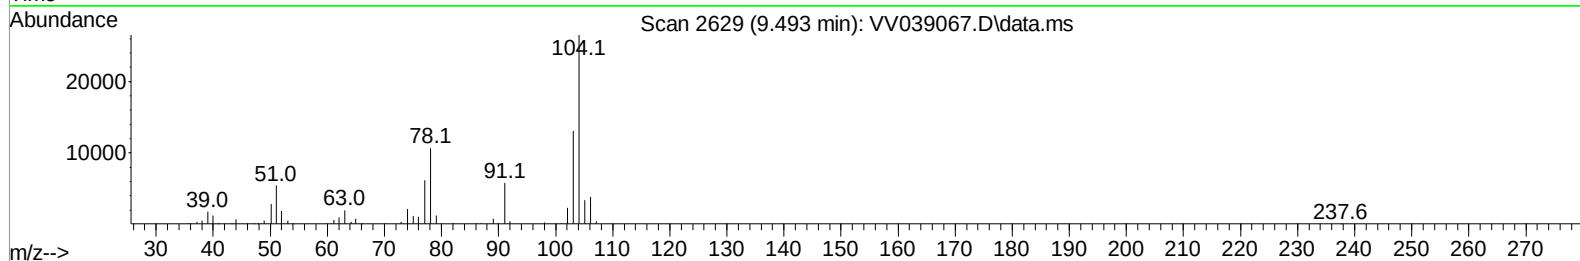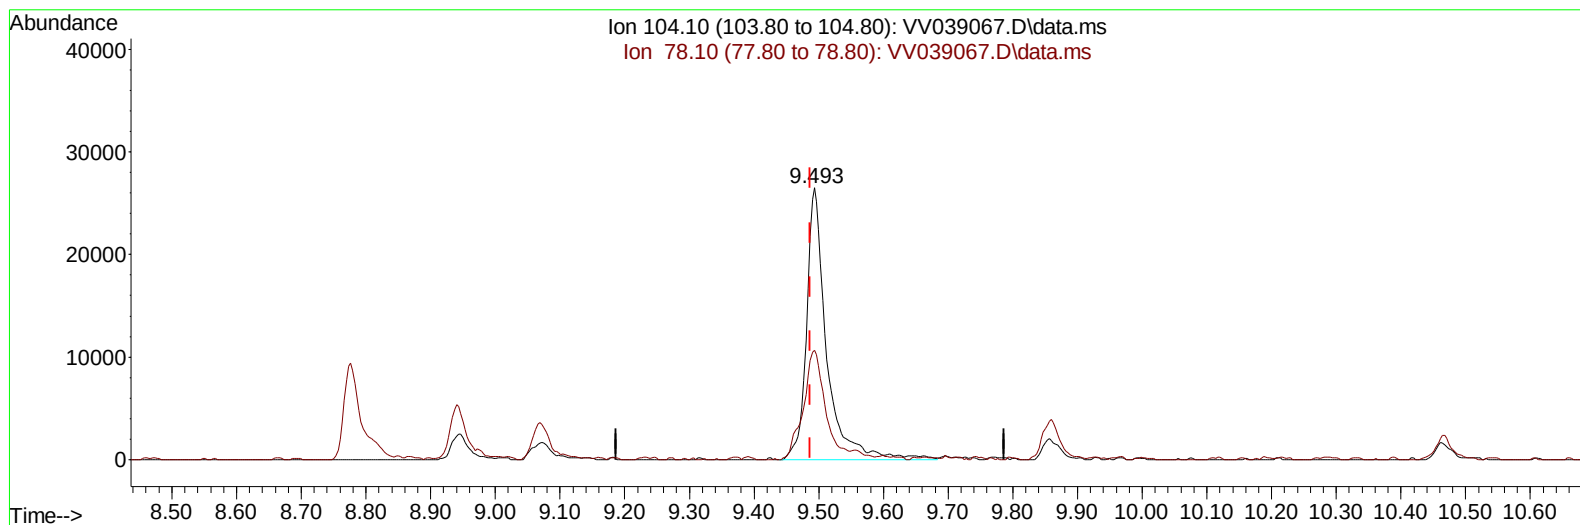

TIC: VV039067.D\data.ms

(55) Styrene (T)

9.493min (+ 0.006) 0.67 ug/L m

response 57219

Ion	Exp%	Act%
104.10	100.00	100.00
78.10	42.70	40.31
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV091525\
 Data File : VV039067.D
 Acq On : 15 Sep 2025 09:55
 Operator : SY/MD
 Sample : VSTD00154
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VSTD001254

Manual IntegrationsAPPROVED

Quant Time: Sep 16 01:36:39 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR091525WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Tue Sep 16 01:35:33 2025
 Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 09/16/2025
 Supervised By :Semsettin Yesilyurt 09/16/2025

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	5.532	114	366192	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.776	117	377065	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.175	152	160227	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.291	65	27368	0.919	ug/L	0.00
7) Chloroethane-d5	1.545	69	22750	0.875	ug/L	0.00
11) 1,1-Dichloroethene-d2	2.069	65	13120	0.949	ug/L	0.00
20) 2-Butanone-d5	3.850	46	34037m	8.520	ug/L	0.05
24) Chloroform-d	4.259	84	52627	0.932	ug/L	0.00
26) 1,2-Dichloroethane-d4	4.956	65	21506	0.925	ug/L	0.01
32) Benzene-d6	4.963	84	82965	0.784	ug/L	0.00
36) 1,2-Dichloropropane-d6	5.992	67	26491	0.868	ug/L	0.00
41) Toluene-d8	7.243	98	69781	0.736	ug/L	0.00
43) trans-1,3-Dichloroprop...	7.564	79	9025	0.796	ug/L	0.01
46) 2-Hexanone-d5	8.030	63	24602m	6.962	ug/L	0.01
56) 1,1,2,2-Tetrachloroeth...	10.146	84	18764	0.814	ug/L	0.00
66) 1,2-Dichlorobenzene-d4	11.551	152	23257	0.886	ug/L	0.00
Target Compounds						
					Qvalue	
2) Dichlorodifluoromethane	1.121	85	38397	0.938	ug/L	100
3) Chloromethane	1.227	50	39047	0.968	ug/L	100
5) Vinyl chloride	1.294	62	40770	0.954	ug/L	99
6) Bromomethane	1.500	94	21598	0.909	ug/L	97
8) Chloroethane	1.561	64	24790	0.927	ug/L	98
9) Trichlorofluoromethane	1.725	101	53164	0.910	ug/L	92
10) 1,1,2-Trichloro-1,2,2-...	2.079	101	33854	0.945	ug/L	98
12) 1,1-Dichloroethene	2.079	96	29003	0.890	ug/L	94
13) Acetone	2.140	43	34008	8.757	ug/L	94
14) Carbon disulfide	2.252	76	100868	0.946	ug/L	99
15) Methyl Acetate	2.404	43	9584m	0.979	ug/L	
16) Methylene chloride	2.458	84	34768	0.759	ug/L	98
17) Methyl tert-butyl Ether	2.712	73	45057	0.803	ug/L	98
18) trans-1,2-Dichloroethene	2.706	96	28749	0.875	ug/L	98
19) 1,1-Dichloroethane	3.117	63	55670	0.929	ug/L	98
21) 2-Butanone	3.931	43	43798m	9.972	ug/L	
22) cis-1,2-Dichloroethene	3.831	96	25182	0.796	ug/L	99
23) Bromochloromethane	4.165	128	13350	0.944	ug/L	88
25) Chloroform	4.278	83	57649	0.918	ug/L	100
27) 1,2-Dichloroethane	5.059	62	25703	0.810	ug/L	99
29) 1,1,1-Trichloroethane	4.513	97	49119	0.840	ug/L	97
30) Cyclohexane	4.583	56	35392	0.705	ug/L	94
31) Carbon tetrachloride	4.735	117	46902	0.927	ug/L	97
33) Benzene	5.018	78	100822	0.780	ug/L	100
34) Trichloroethene	5.841	95	29339	0.844	ug/L	97
35) Methylcyclohexane	6.043	83	37829	0.709	ug/L	94
37) 1,2-Dichloropropane	6.098	63	26478	0.831	ug/L #	90
38) Bromodichloromethane	6.436	83	38725	0.893	ug/L	96
39) cis-1,3-Dichloropropene	6.960	75	31434	0.729	ug/L	99
40) 4-Methyl-2-pentanone	7.156	43	95150m	7.508	ug/L	
42) Toluene	7.313	91	101035	0.747	ug/L	100

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV091525\
 Data File : VV039067.D
 Acq On : 15 Sep 2025 09:55
 Operator : SY/MD
 Sample : VSTD00154
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VSTD001254

Manual IntegrationsAPPROVED

Reviewed By :Mahesh Dadoda 09/16/2025
 Supervised By :Semsettin Yesilyurt 09/16/2025

Quant Time: Sep 16 01:36:39 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR091525WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Tue Sep 16 01:35:33 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
44) trans-1,3-Dichloropropene	7.590	75	26847	0.738	ug/L	93
45) 1,1,2-Trichloroethane	7.767	97	19958	0.874	ug/L	95
47) Tetrachloroethene	7.898	164	22667	0.844	ug/L	96
48) 2-Hexanone	8.079	43	66832m	7.995	ug/L	
49) Dibromochloromethane	8.169	129	23267	0.850	ug/L	99
50) 1,2-Dibromoethane	8.284	107	17123	0.824	ug/L	97
51) Chlorobenzene	8.805	112	71209	0.807	ug/L	97
52) Ethylbenzene	8.940	91	98366	0.701	ug/L	99
53) m,p-Xylene	9.069	106	38372	0.705	ug/L	99
54) o-Xylene	9.471	106	34811	0.707	ug/L	97
55) Styrene	9.493	104	57219m	0.667	ug/L	
57) 1,1,2,2-Tetrachloroethane	10.168	83	21508	0.816	ug/L	89
59) Bromoform	9.664	173	11449	0.937	ug/L #	96
60) Isopropylbenzene	9.857	105	89604	0.754	ug/L	98
61) 1,2,3-Trichloropropane	10.204	75	13240	0.849	ug/L	97
62) 1,3,5-Trimethylbenzene	10.467	105	69613	0.770	ug/L	97
63) 1,2,4-Trimethylbenzene	10.844	105	63778	0.727	ug/L	96
64) 1,3-Dichlorobenzene	11.111	146	48419	0.852	ug/L	96
65) 1,4-Dichlorobenzene	11.201	146	50620	0.865	ug/L	97
67) 1,2-Dichlorobenzene	11.570	146	44099	0.871	ug/L	97
68) 1,2-Dibromo-3-chloropr...	12.365	75	2808	0.850	ug/L	93
69) 1,3,5-Trichlorobenzene	12.574	180	30621	0.847	ug/L	97
70) 1,2,4-trichlorobenzene	13.191	180	22087	0.794	ug/L	90
71) Naphthalene	13.435	128	33064	0.768	ug/L	98
72) 1,2,3-Trichlorobenzene	13.670	180	19031	0.766	ug/L	95

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV091525\
 Data File : VV039067.D
 Acq On : 15 Sep 2025 09:55
 Operator : SY/MD
 Sample : VSTD00154
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VSTD001254

Manual IntegrationsAPPROVED

Quant Time: Sep 16 01:36:39 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR091525WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Tue Sep 16 01:35:33 2025
 Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 09/16/2025
 Supervised By :Semsettin Yesilyurt 09/16/2025

