
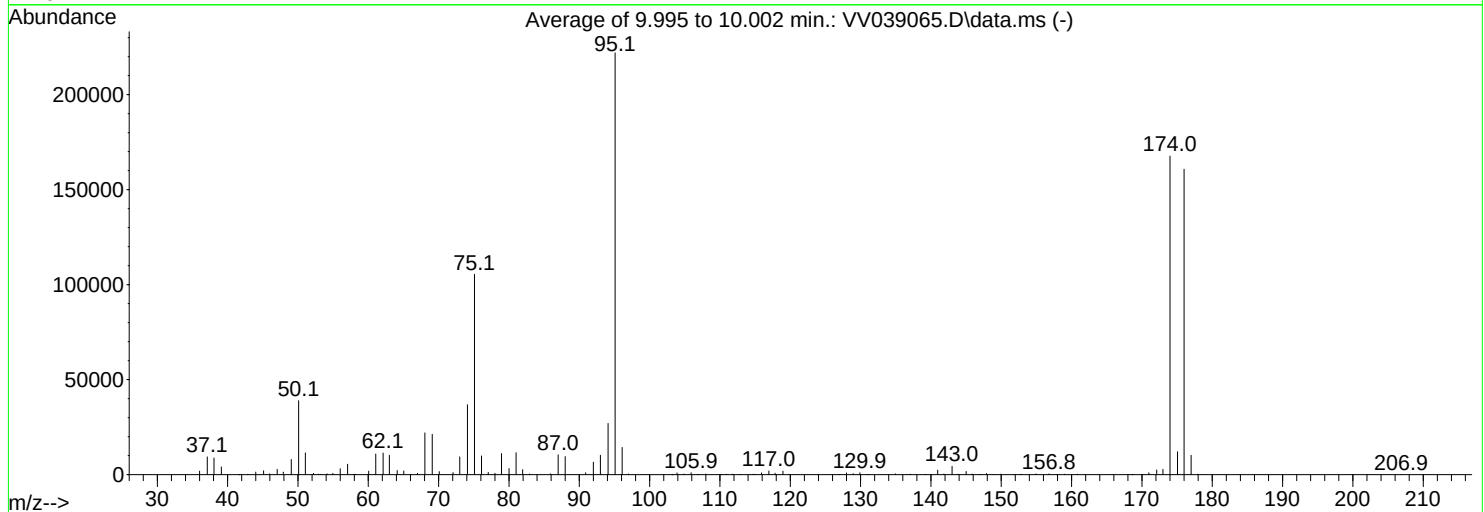


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV091525\
Data File : VV039065.D
Acq On : 15 Sep 2025 08:17
Operator : SY/MD
Sample : BFB210
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB210

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR091525WMA.M
Title : TRACE VOA SFAM1.0
Last Update : Wed Sep 17 02:19:46 2025

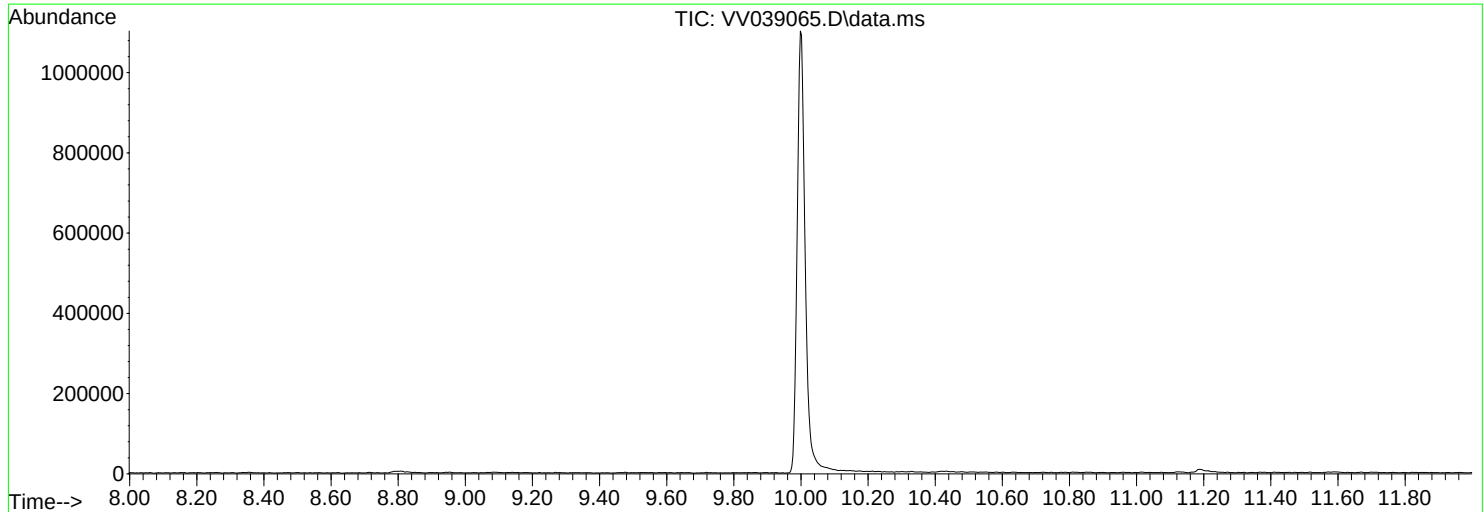

AutoFind: Scans 2785, 2786, 2787; Background Corrected with Scan 2773

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.5	38915	PASS
75	95	30	80	47.5	105424	PASS
95	95	100	100	100.0	222016	PASS
96	95	5	9	6.5	14346	PASS
173	174	0.00	2	1.7	2805	PASS
174	95	50	120	75.5	167659	PASS
175	174	5	9	7.2	12084	PASS
176	174	95	105	95.9	160811	PASS
177	176	5	10	6.4	10236	PASS

m/z	Abundance
40.00	1051.0
44.00	797.0
48.30	155.0
62.70	108.0
77.10	198.0
78.20	112.0
102.50	120.0

Instrument :
MSVOA_V
ClientSampleId :
BFB210

m/z	Abundance
36.00	1900.0
37.10	8854.0
38.10	8565.0
39.10	3801.0
40.00	1124.0
41.90	129.0
42.80	158.0
44.10	1737.0
45.10	1870.0
45.90	497.0
47.10	2738.0
47.90	1368.0
49.10	7996.0
50.10	37712.0
51.00	10694.0
52.20	632.0
52.90	169.0
53.30	152.0
54.20	421.0
55.00	601.0
56.00	3020.0
57.10	5331.0
58.20	267.0
60.00	1789.0
61.00	10001.0
62.10	10831.0
63.00	10097.0
64.10	2009.0
65.10	1827.0
66.10	242.0
67.00	652.0
68.00	21280.0
69.10	20560.0
70.10	1452.0
72.00	1033.0
73.00	8943.0
74.10	34176.0
75.10	100880.0
76.10	9012.0
77.10	1361.0
78.00	803.0
79.00	10290.0
80.00	2996.0
81.00	10543.0
81.90	2536.0
83.00	292.0
85.90	386.0
87.00	10069.0
88.00	9003.0
90.90	1033.0
92.00	6484.0
93.00	9723.0
94.10	25760.0
95.10	211392.0
96.10	13995.0
97.00	355.0
103.20	139.0
103.90	925.0
104.80	324.0
105.90	884.0
106.80	183.0
108.00	334.0
110.20	257.0
110.90	209.0
111.80	238.0
112.90	127.0
114.80	175.0
115.10	166.0
115.90	868.0
116.90	1825.0
117.80	623.0
118.90	1666.0
119.90	145.0
123.90	132.0
126.10	141.0
128.00	963.0
129.00	480.0
129.90	967.0
130.90	298.0
134.90	439.0
137.00	256.0
139.20	160.0
140.10	154.0
140.90	2195.0
141.80	289.0
143.00	4108.0
143.90	215.0
145.00	1613.0
145.80	329.0
146.90	213.0
147.90	511.0
149.00	144.0

Instrument :
MSVOA_V
ClientSampleId :
BFB210

150.00	190.0
152.80	263.0
153.90	165.0
154.90	418.0
156.80	451.0
159.00	345.0
160.80	324.0
170.00	163.0
171.00	909.0
172.10	2362.0
173.00	2558.0
174.00	152640.0
175.00	11246.0
176.00	148864.0
177.00	9638.0
177.90	286.0
206.90	181.0

Instrument :
MSVOA_V
ClientSampleId :
BFB210

m/z	Abundance
36.00	1978.0
37.10	9641.0
38.10	9141.0
39.10	4215.0
40.00	1077.0
42.00	138.0
42.90	172.0
44.00	2221.0
45.10	2012.0
45.90	390.0
47.00	2935.0
47.90	1445.0
49.10	8298.0
50.10	40480.0
51.00	11776.0
52.20	688.0
52.90	197.0
53.30	188.0
54.10	453.0
54.90	664.0
56.00	3203.0
57.10	5655.0
57.90	242.0
58.20	194.0
60.10	1905.0
61.10	11253.0
62.10	11655.0
63.00	10476.0
64.10	2234.0
65.10	2046.0
66.10	179.0
67.00	678.0
68.10	22736.0
69.10	21824.0
70.10	1645.0
72.00	1089.0
73.00	9741.0
74.10	37928.0
75.10	108792.0
76.10	10264.0
77.10	1467.0
78.00	863.0
78.90	11464.0
80.00	3345.0
81.00	11922.0
81.90	2739.0
82.90	363.0
85.90	444.0
87.00	10710.0
88.00	9922.0
90.90	1041.0
92.00	6887.0
93.00	10610.0
94.10	27960.0
95.10	229760.0
96.10	14753.0
97.00	290.0
103.90	960.0
104.90	333.0
105.90	1044.0
106.80	230.0
108.00	394.0
109.90	196.0
110.90	289.0
111.80	253.0
112.90	140.0
114.80	265.0
115.90	968.0
116.90	1939.0
117.90	818.0
118.90	1848.0
119.90	236.0
123.90	112.0
126.10	132.0
127.00	116.0
128.00	901.0
129.00	534.0
129.90	1067.0
131.10	240.0
135.00	515.0
137.10	258.0
139.20	175.0
140.10	184.0
141.00	2346.0
141.90	320.0
143.00	4505.0
143.90	236.0
145.00	1714.0
145.80	323.0
147.00	192.0
147.90	637.0
149.00	168.0

Instrument :
MSVOA_V
ClientSampleId :
BFB210

149.90	270.0
151.70	131.0
152.80	221.0
154.00	159.0
155.00	432.0
156.80	488.0
157.90	148.0
159.00	269.0
160.80	281.0
170.00	183.0
171.00	1055.0
172.10	2507.0
173.00	2945.0
174.00	173504.0
175.00	12533.0
176.00	166592.0
177.00	10563.0
177.90	303.0
206.90	106.0

Instrument :
MSVOA_V
ClientSampleId :
BFB210

m/z	Abundance
36.00	1741.0
37.10	9567.0
38.00	8540.0
39.10	4231.0
40.00	1164.0
41.60	104.0
42.00	162.0
42.90	190.0
44.00	2544.0
45.10	2098.0
46.00	317.0
47.00	2654.0
47.90	1244.0
49.00	7764.0
50.10	38552.0
51.10	11784.0
52.20	693.0
52.90	296.0
53.20	244.0
54.10	361.0
54.90	706.0
56.00	3094.0
57.00	5533.0
57.90	299.0
60.00	1873.0
61.10	11244.0
62.10	11573.0
63.00	10042.0
64.10	2230.0
65.00	2044.0
66.00	166.0
67.00	599.0
68.10	21952.0
69.10	21168.0
70.10	1764.0
72.10	1196.0
73.00	9253.0
74.10	38344.0
75.10	106600.0
76.10	10193.0
77.00	1325.0
78.00	839.0
78.90	11610.0
80.00	3401.0
81.00	12058.0
82.00	2670.0
82.90	321.0
85.90	441.0
87.00	10614.0
88.00	9681.0
90.90	1006.0
92.00	6305.0
93.00	10263.0
94.10	27200.0
95.10	224896.0
96.10	14290.0
97.00	267.0
103.90	933.0
105.00	315.0
105.90	1104.0
107.00	232.0
108.00	368.0
109.90	186.0
110.90	349.0
111.80	211.0
112.90	181.0
114.80	285.0
115.90	988.0
117.00	2010.0
117.90	935.0
119.00	2054.0
119.90	227.0
124.00	142.0
126.00	104.0
127.00	107.0
128.00	813.0
128.90	531.0
129.90	942.0
131.10	262.0
135.00	431.0
136.60	188.0
137.10	345.0
139.20	149.0
140.10	214.0
141.00	2440.0
141.90	315.0
143.00	4633.0
143.90	243.0
145.00	1748.0
145.90	306.0
147.00	169.0
147.90	748.0

Instrument :
MSVOA_V
ClientSampleId :
BFB210

148.90	182.0
149.90	309.0
151.80	168.0
152.80	180.0
153.90	125.0
155.00	465.0
156.80	442.0
157.90	161.0
158.90	200.0
160.90	235.0
168.60	125.0
170.00	148.0
171.00	1028.0
172.10	2431.0
173.00	2911.0
174.00	176832.0
175.10	12472.0
176.00	166976.0
177.00	10506.0
178.00	293.0

Instrument :
MSVOA_V
ClientSampleId :
BFB210