

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091624\
 Data File : VV037297.D
 Acq On : 16 Sep 2024 11:03
 Operator : SY/MD
 Sample : P3934-01 10X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :

Quant Time: Sep 17 05:06:40 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082624WMA.M
 Quant Title : VOC Analysis
 QLast Update : Tue Sep 17 05:05:17 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.526	114	640674	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.776	117	624658	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.178	152	293446	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.278	65	283138	48.312	ug/L	0.00
Spiked Amount 50.000	Range 60 - 135		Recovery = 96.620%			
7) Chloroethane-d5	1.532	69	229837	50.743	ug/L	0.00
Spiked Amount 50.000	Range 70 - 130		Recovery = 101.480%			
11) 1,1-Dichloroethene-d2	2.056	65	118537	48.122	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery = 96.240%			
21) 2-Butanone-d5	3.790	46	181717	80.068	ug/L	0.00
Spiked Amount 100.000	Range 40 - 130		Recovery = 80.070%			
24) Chloroform-d	4.236	84	461584	50.323	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery = 100.640%			
26) 1,2-Dichloroethane-d4	4.931	65	286211	49.549	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery = 99.100%			
32) Benzene-d6	4.947	84	962051	50.991	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery = 101.980%			
36) 1,2-Dichloropropane-d6	5.979	67	308522	52.208	ug/L	0.00
Spiked Amount 50.000	Range 70 - 120		Recovery = 104.420%			
41) Toluene-d8	7.233	98	849101	49.866	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery = 99.740%			
43) trans-1,3-Dichloroprop...	7.545	79	127293	46.560	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery = 93.120%			
47) 2-Hexanone-d5	8.021	63	112694	69.875	ug/L	0.00
Spiked Amount 100.000	Range 45 - 130		Recovery = 69.880%			
56) 1,1,2,2-Tetrachloroeth...	10.146	84	309130	43.132	ug/L	0.00
Spiked Amount 50.000	Range 65 - 120		Recovery = 86.260%			
66) 1,2-Dichlorobenzene-d4	11.554	152	302664	51.499	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery = 103.000%			
Target Compounds						Qvalue
10) 1,1,2-Trichloro-1,2,2-...	2.060	101	3408	0.768	ug/L #	25


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091624\
Data File : VV037297.D
Acq On : 16 Sep 2024 11:03
Operator : SY/MD
Sample : P3934-01 10X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :


Quant Time: Sep 17 05:06:40 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082624WMA.M
Quant Title : VOC Analysis
QLast Update : Tue Sep 17 05:05:17 2024
Response via : Initial Calibration

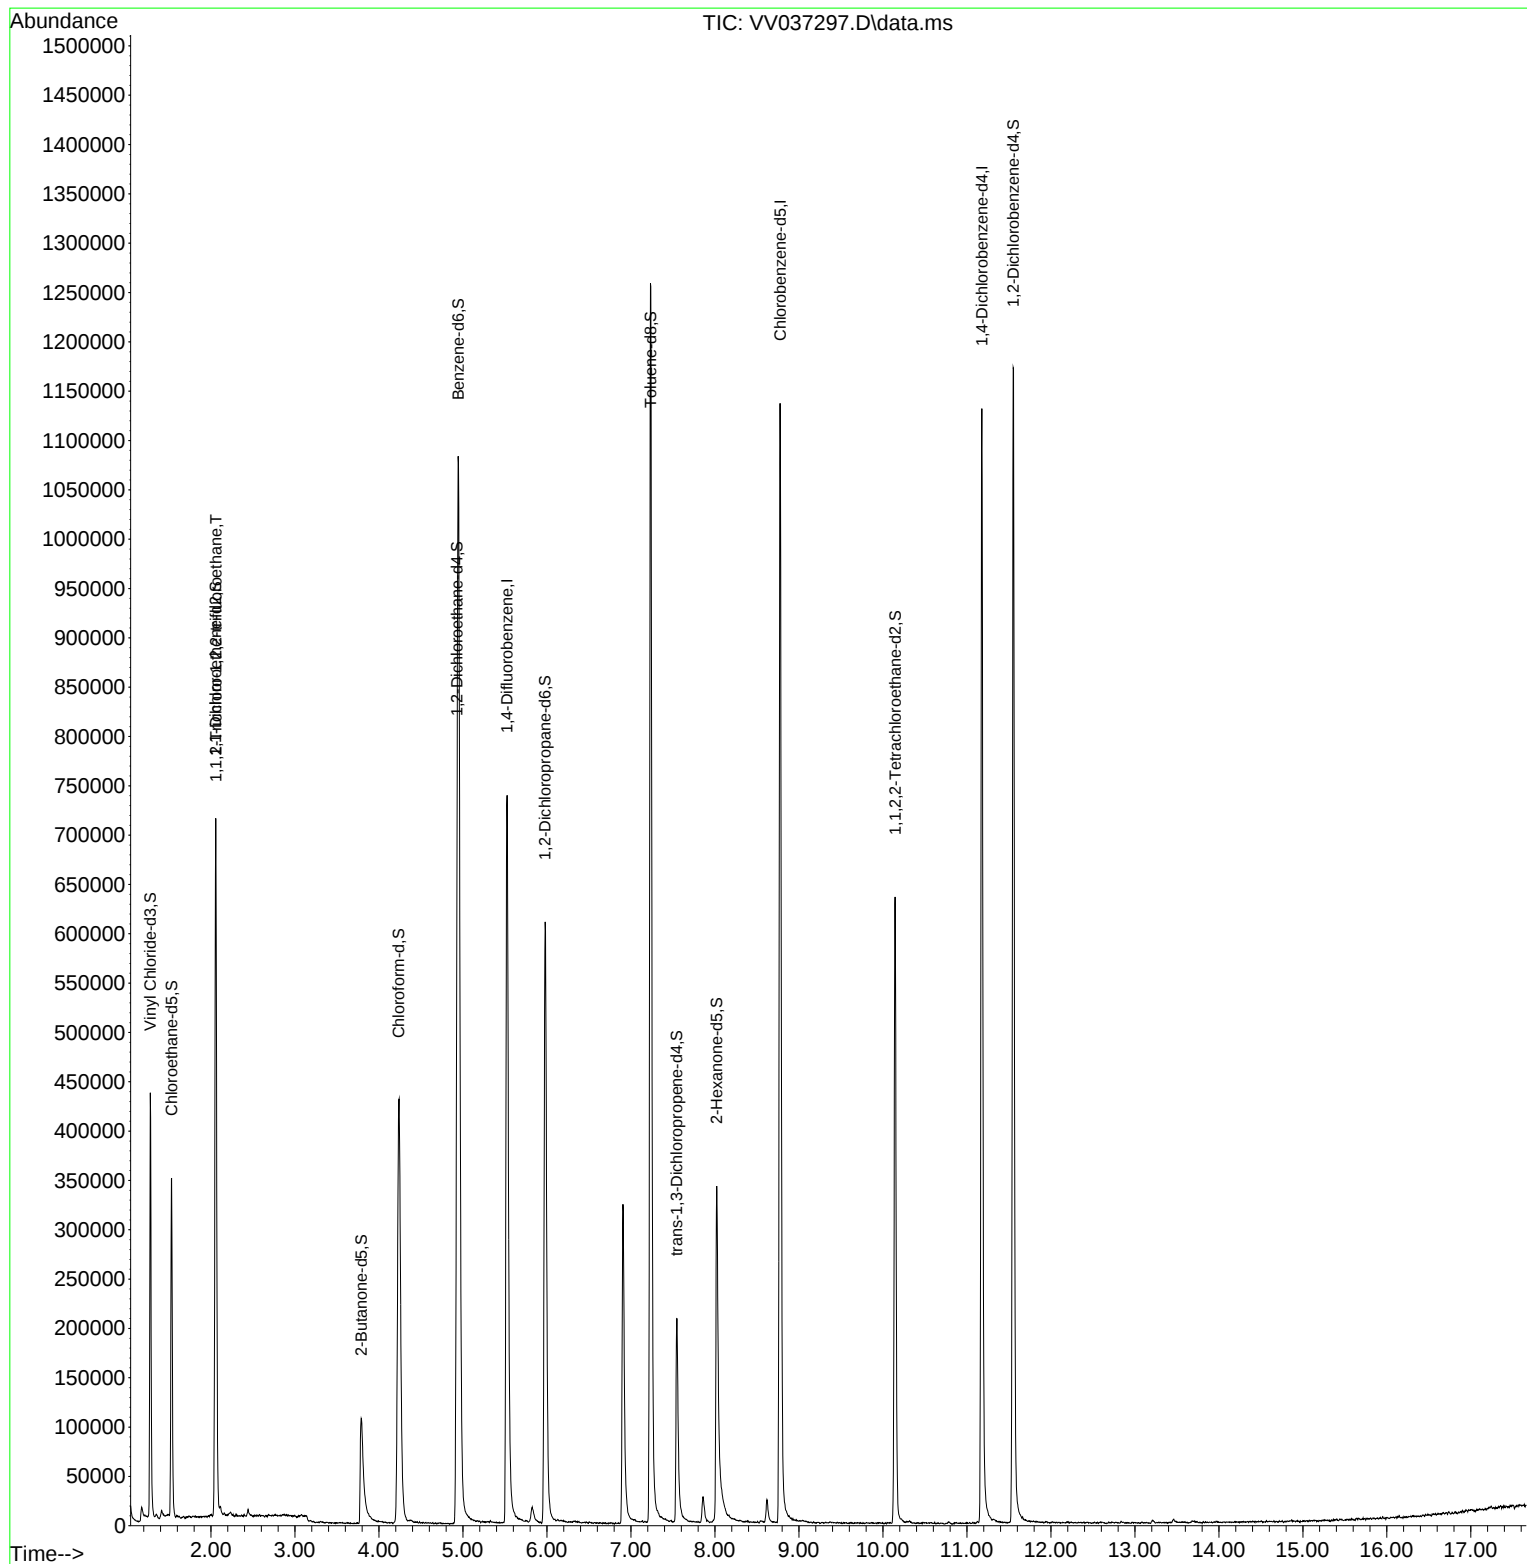

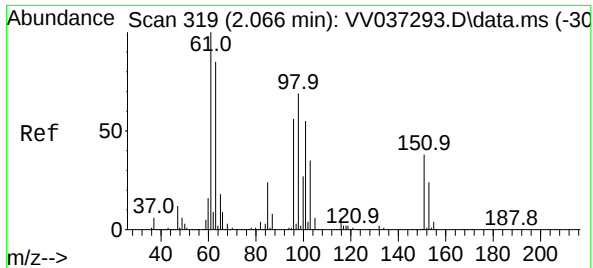

#10
 1,1,2-Trichloro-1,2,2-trifluoroethane
 Concen: 0.768 ug/L
 RT: 2.060 min Scan# 31
 Delta R.T. -0.006 min
 Lab File: VV037297.D
 Acq: 16 Sep 2024 11:03

Instrument :
 MSVOA_V
 ClientSampleId :

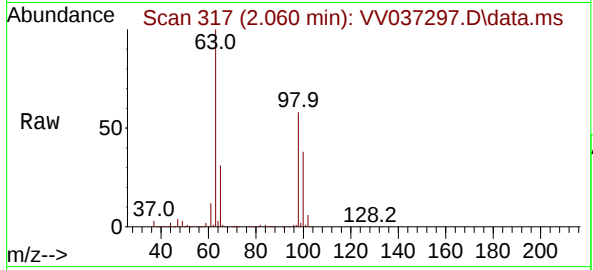

Tgt Ion:	101	Resp:	3408
Ion	Ratio	Lower	Upper
101	100		
85	3.0	35.6	53.4#
151	1.5	55.0	82.4#

