

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV091624\
 Data File : VV037295.D
 Acq On : 16 Sep 2024 09:43
 Operator : SY/MD
 Sample : VV0916WBL01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK207

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082624WMA.M

Title : VOC Analysis

Signal : TIC: VV037295.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.175	36	42	50	rBV	13373	22262	0.80%	0.115%
2	1.281	67	75	92	rVB	432172	458219	16.42%	2.358%
3	1.532	145	153	167	rVB	341944	401526	14.39%	2.067%
4	2.059	307	317	340	rVB	713685	1026569	36.78%	5.284%
5	3.333	707	713	721	rVB	1589	2566	0.09%	0.013%
6	3.407	732	736	741	rVB8	1085	1054	0.04%	0.005%
7	3.696	820	826	829	rBV5	969	1205	0.04%	0.006%
8	3.796	848	857	887	rBV	112620	320038	11.47%	1.647%
9	4.146	962	966	969	rVB5	942	734	0.03%	0.004%
10	4.243	979	996	1030	rBV	428219	1105282	39.60%	5.689%
11	4.561	1093	1095	1099	rBV5	1111	800	0.03%	0.004%
12	4.677	1128	1131	1136	rBV6	876	704	0.03%	0.004%
13	4.709	1139	1141	1145	rVB5	1383	959	0.03%	0.005%
14	4.844	1179	1183	1184	rBV3	1479	793	0.03%	0.004%
15	4.883	1192	1195	1199	rVB4	1461	1206	0.04%	0.006%
16	4.950	1199	1216	1254	rBV2	1092671	2791064	100.00%	14.365%
17	5.320	1324	1331	1332	rBV7	1966	2021	0.07%	0.010%
18	5.471	1374	1378	1381	rBV6	1051	725	0.03%	0.004%
19	5.529	1384	1396	1426	rBV	690496	1434163	51.38%	7.381%
20	5.828	1481	1489	1508	rVB6	17795	41785	1.50%	0.215%
21	5.931	1519	1521	1524	rVB3	1662	734	0.03%	0.004%
22	5.985	1524	1538	1564	rBV	610975	1260134	45.15%	6.486%
23	6.294	1632	1634	1638	rVB4	1483	818	0.03%	0.004%
24	6.345	1647	1650	1651	rBV2	1468	645	0.02%	0.003%
25	6.436	1674	1678	1682	rVB6	784	619	0.02%	0.003%
26	6.654	1743	1746	1748	rBV3	1248	696	0.02%	0.004%
27	6.670	1748	1751	1756	rBV6	1313	905	0.03%	0.005%
28	6.773	1778	1783	1785	rBV5	682	649	0.02%	0.003%
29	6.812	1793	1795	1800	rVB5	1260	927	0.03%	0.005%
30	6.908	1815	1825	1851	rBV	323304	611317	21.90%	3.146%
31	7.165	1899	1905	1907	rBV5	1753	1376	0.05%	0.007%
32	7.236	1916	1927	1957	rBV	1259152	2218317	79.48%	11.417%
33	7.551	2016	2025	2050	rBV	205192	379960	13.61%	1.956%
34	7.860	2118	2121	2124	rBV5	1521	1097	0.04%	0.006%
35	7.898	2130	2133	2135	rBV3	1258	875	0.03%	0.005%
36	8.024	2164	2172	2224	rBV2	335887	785565	28.15%	4.043%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV091624\
 Data File : VV037295.D
 Acq On : 16 Sep 2024 09:43
 Operator : SY/MD
 Sample : VV0916WBL01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK207

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082624WMA.M
 Title : VOC Analysis

37	8.442	2296	2302	2305	rBV6	1227	1093	0.04%	0.006%
38	8.497	2317	2319	2322	rBV3	1252	685	0.02%	0.004%
39	8.651	2362	2367	2369	rBV5	1061	829	0.03%	0.004%
40	8.670	2369	2373	2379	rVB8	1836	1789	0.06%	0.009%
41	8.779	2395	2407	2434	rBV	1082940	1784117	63.92%	9.183%
42	9.172	2526	2529	2531	rVV3	1095	712	0.03%	0.004%
43	9.201	2535	2538	2542	rVV4	993	876	0.03%	0.005%
44	9.223	2542	2545	2547	rVB3	1341	734	0.03%	0.004%
45	9.326	2574	2577	2580	rBV5	1401	999	0.04%	0.005%
46	9.358	2582	2587	2589	rVV5	826	789	0.03%	0.004%
47	9.500	2628	2631	2635	rVB5	988	669	0.02%	0.003%
48	9.532	2637	2641	2644	rBV5	1978	1399	0.05%	0.007%
49	9.619	2665	2668	2672	rVB5	1111	625	0.02%	0.003%
50	9.779	2716	2718	2723	rVV7	1152	706	0.03%	0.004%
51	9.808	2723	2727	2731	rVB4	923	867	0.03%	0.004%
52	9.853	2736	2741	2744	rBV6	1501	1207	0.04%	0.006%
53	9.873	2744	2747	2748	rBV2	1471	879	0.03%	0.005%
54	9.937	2765	2767	2771	rVB4	1105	664	0.02%	0.003%
55	9.979	2777	2780	2784	rBV5	989	884	0.03%	0.005%
56	10.098	2814	2817	2819	rBV3	1322	876	0.03%	0.005%
57	10.146	2820	2832	2857	rBV	634617	1028056	36.83%	5.291%
58	10.313	2881	2884	2891	rVB8	1554	1686	0.06%	0.009%
59	10.422	2914	2918	2920	rBV3	1105	762	0.03%	0.004%
60	10.435	2920	2922	2927	rVB5	1144	880	0.03%	0.005%
61	10.458	2927	2929	2931	rBV2	1173	733	0.03%	0.004%
62	10.487	2935	2938	2942	rVB4	1033	691	0.02%	0.004%
63	10.554	2954	2959	2960	rBV3	847	681	0.02%	0.004%
64	10.609	2973	2976	2983	rVV6	1554	1360	0.05%	0.007%
65	10.722	3009	3011	3015	rVB4	1252	687	0.02%	0.004%
66	10.750	3015	3020	3024	rVB6	1646	1284	0.05%	0.007%
67	10.779	3024	3029	3031	rBV4	1271	1161	0.04%	0.006%
68	10.812	3033	3039	3040	rBV5	910	816	0.03%	0.004%
69	11.024	3102	3105	3108	rVB4	926	626	0.02%	0.003%
70	11.127	3129	3137	3142	rBV10	4040	5043	0.18%	0.026%
71	11.178	3142	3153	3182	rBV	1069048	1711035	61.30%	8.806%
72	11.554	3257	3270	3298	rBV	1168695	1917617	68.71%	9.870%
73	11.892	3372	3375	3379	rBV4	1784	1548	0.06%	0.008%
74	12.020	3411	3415	3418	rBV4	1154	799	0.03%	0.004%
75	12.455	3546	3550	3551	rBV2	1764	1154	0.04%	0.006%
76	12.496	3560	3563	3567	rVB4	1251	694	0.02%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV091624\
 Data File : VV037295.D
 Acq On : 16 Sep 2024 09:43
 Operator : SY/MD
 Sample : VV0916WBL01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK207

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082624WMA.M
 Title : VOC Analysis

77	12.551	3575	3580	3582	rBV5	1327	1081	0.04%	0.006%
78	12.583	3586	3590	3592	rBV5	1461	926	0.03%	0.005%
79	12.686	3616	3622	3627	rBV7	1186	1617	0.06%	0.008%
80	12.731	3630	3636	3643	rBV6	1568	1973	0.07%	0.010%
81	13.082	3742	3745	3750	rVB6	1544	1081	0.04%	0.006%
82	13.207	3775	3784	3795	rBV6	5201	9425	0.34%	0.049%
83	13.252	3795	3798	3804	rVB5	935	805	0.03%	0.004%
84	13.364	3830	3833	3839	rVB5	1515	1416	0.05%	0.007%
85	13.400	3839	3844	3845	rBV4	1702	1470	0.05%	0.008%
86	13.448	3849	3859	3875	rVV2	13221	28346	1.02%	0.146%
87	13.580	3898	3900	3904	rVB3	1463	1073	0.04%	0.006%
88	13.680	3922	3931	3940	rBV3	5246	9827	0.35%	0.051%
89	13.901	3997	4000	4002	rBV3	1000	699	0.03%	0.004%
90	13.972	4017	4022	4024	rBV4	1325	1433	0.05%	0.007%
91	14.017	4033	4036	4038	rBV3	837	624	0.02%	0.003%
92	14.127	4067	4070	4074	rVB5	1059	845	0.03%	0.004%
93	14.355	4139	4141	4144	rVB4	1340	727	0.03%	0.004%
94	14.413	4156	4159	4161	rBV3	1379	732	0.03%	0.004%
95	14.535	4194	4197	4198	rBV3	1253	812	0.03%	0.004%
96	14.680	4234	4242	4246	rBV8	1592	2583	0.09%	0.013%
97	14.776	4267	4272	4275	rBV6	1519	1674	0.06%	0.009%
98	15.107	4371	4375	4376	rBV3	1344	1152	0.04%	0.006%
99	15.188	4396	4400	4402	rBV5	1523	1139	0.04%	0.006%
100	15.834	4599	4601	4604	rBV4	1991	900	0.03%	0.005%


Sum of corrected areas: 19429381

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV091624\
Data File : VV037295.D
Acq On : 16 Sep 2024 09:43
Operator : SY/MD
Sample : VV0916WBL01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK207

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

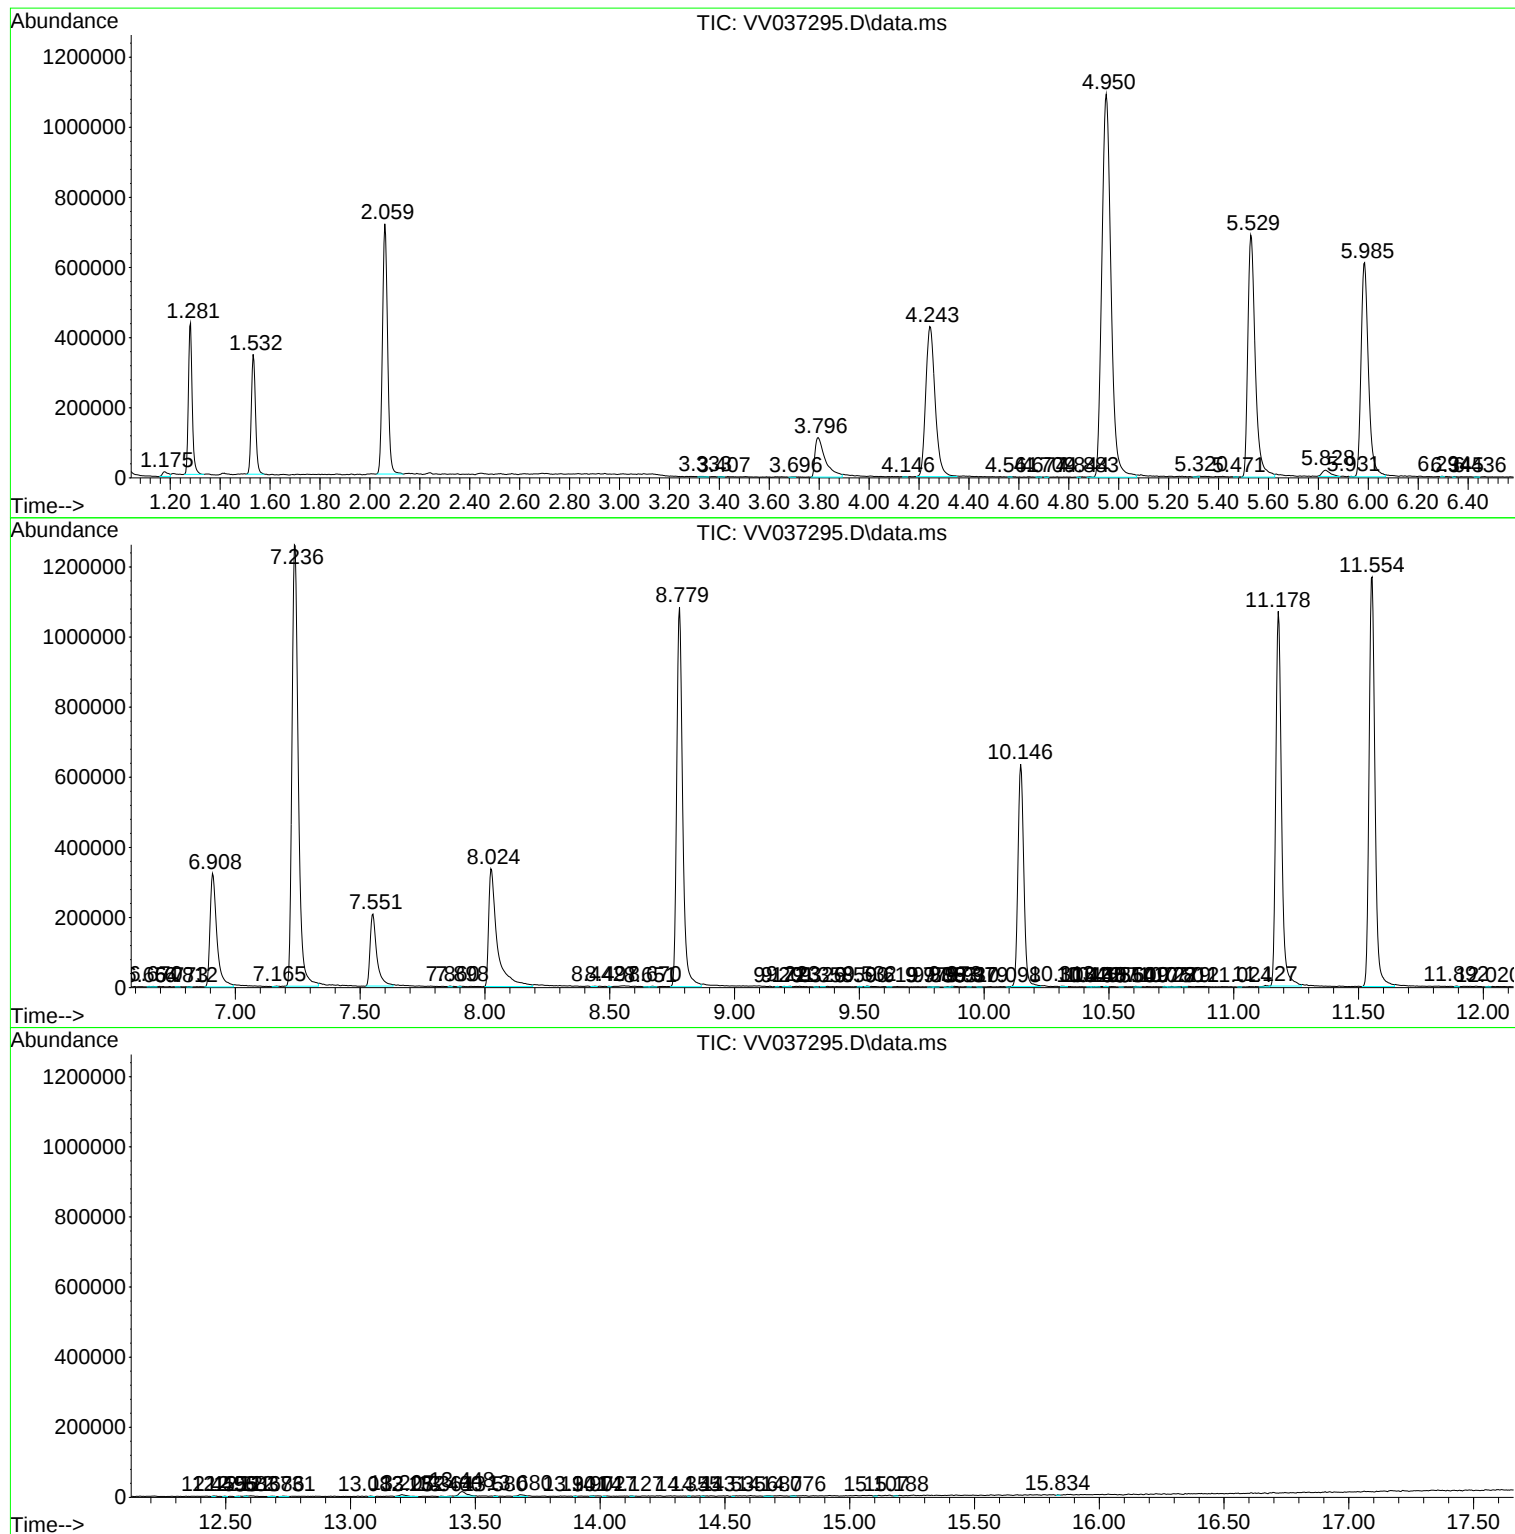

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV091624\
Data File : VV037295.D
Acq On : 16 Sep 2024 09:43
Operator : SY/MD
Sample : VV0916WBL01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK207

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV091624\
Data File : VV037295.D
Acq On : 16 Sep 2024 09:43
Operator : SY/MD
Sample : VV0916WBL01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK207

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc