

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV091624\
 Data File : VV037300.D
 Acq On : 16 Sep 2024 12:08
 Operator : SY/MD
 Sample : P3993-10
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK002

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082624WMA.M
 Title : VOC Analysis

Signal : TIC: VV037300.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.179	36	43	50	rBV2	11335	19214	0.72%	0.099%
2	1.278	68	74	89	rVB	405340	437441	16.28%	2.258%
3	1.532	145	153	172	rVB	331016	391471	14.57%	2.021%
4	2.060	307	317	331	rBV	683927	990742	36.87%	5.115%
5	3.236	680	683	687	rVB4	1736	1281	0.05%	0.007%
6	3.291	697	700	702	rBV4	1041	633	0.02%	0.003%
7	3.336	710	714	716	rBV3	1039	767	0.03%	0.004%
8	3.420	737	740	745	rVB6	1271	1056	0.04%	0.005%
9	3.458	750	752	754	rBV3	965	611	0.02%	0.003%
10	3.494	760	763	767	rBV4	735	627	0.02%	0.003%
11	3.526	769	773	776	rVV4	890	883	0.03%	0.005%
12	3.667	811	817	818	rBV5	916	838	0.03%	0.004%
13	3.796	847	857	894	rBV	111520	322111	11.99%	1.663%
14	4.246	980	997	1025	rVV	424982	1094098	40.71%	5.648%
15	4.590	1102	1104	1107	rVB3	1629	846	0.03%	0.004%
16	4.629	1114	1116	1119	rVV5	1436	881	0.03%	0.005%
17	4.658	1122	1125	1128	rVV3	1119	868	0.03%	0.004%
18	4.677	1128	1131	1133	rVV3	999	689	0.03%	0.004%
19	4.690	1133	1135	1140	rVV5	1250	1113	0.04%	0.006%
20	4.722	1143	1145	1148	rVV3	1288	836	0.03%	0.004%
21	4.744	1148	1152	1154	rVB3	1271	968	0.04%	0.005%
22	4.777	1158	1162	1166	rVB7	773	760	0.03%	0.004%
23	4.851	1181	1185	1188	rBV4	1264	882	0.03%	0.005%
24	4.873	1188	1192	1195	rBV3	660	622	0.02%	0.003%
25	4.950	1200	1216	1242	rBV2	1058859	2687266	100.00%	13.873%
26	5.288	1318	1321	1323	rBV4	878	654	0.02%	0.003%
27	5.423	1359	1363	1367	rVV4	1454	1090	0.04%	0.006%
28	5.452	1370	1372	1375	rBV3	873	630	0.02%	0.003%
29	5.529	1382	1396	1430	rBV	743299	1548938	57.64%	7.996%
30	5.831	1481	1490	1503	rVB7	12345	26068	0.97%	0.135%
31	5.986	1522	1538	1572	rBV	593244	1240527	46.16%	6.404%
32	6.223	1608	1612	1616	rVB5	1672	1427	0.05%	0.007%
33	6.256	1618	1622	1624	rBV4	976	803	0.03%	0.004%
34	6.314	1635	1640	1641	rBV5	1252	1041	0.04%	0.005%
35	6.416	1668	1672	1673	rBV5	1150	795	0.03%	0.004%
36	6.532	1706	1708	1711	rVB4	1518	803	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV091624\
Data File : VV037300.D
Acq On : 16 Sep 2024 12:08
Operator : SY/MD
Sample : P3993-10
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK002

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082624WMA.M
Title : VOC Analysis

37	6.593	1724	1727	1730	rBV4	1061	714	0.03%	0.004%
38	6.651	1741	1745	1746	rBV5	1170	661	0.02%	0.003%
39	6.757	1776	1778	1780	rVB2	1313	643	0.02%	0.003%
40	6.783	1784	1786	1790	rVB3	1493	983	0.04%	0.005%
41	6.809	1790	1794	1796	rBV5	1190	895	0.03%	0.005%
42	6.908	1812	1825	1856	rBV	310499	600871	22.36%	3.102%
43	7.240	1916	1928	1955	rBV	1212816	2167050	80.64%	11.187%
44	7.548	2016	2024	2050	rBV	202853	370618	13.79%	1.913%
45	7.876	2122	2126	2133	rVB7	1532	1783	0.07%	0.009%
46	7.973	2152	2156	2159	rBV5	852	657	0.02%	0.003%
47	8.024	2163	2172	2215	rBV2	340815	772462	28.75%	3.988%
48	8.452	2300	2305	2307	rBV4	867	704	0.03%	0.004%
49	8.510	2319	2323	2326	rBV5	1434	1088	0.04%	0.006%
50	8.654	2365	2368	2372	rBV6	1609	1345	0.05%	0.007%
51	8.683	2375	2377	2381	rVB5	974	833	0.03%	0.004%
52	8.780	2395	2407	2440	rBV	1154459	1927447	71.73%	9.950%
53	9.198	2535	2537	2540	rVB3	1477	615	0.02%	0.003%
54	9.243	2545	2551	2554	rBV7	891	1150	0.04%	0.006%
55	9.346	2580	2583	2588	rVB4	1894	1561	0.06%	0.008%
56	9.468	2618	2621	2623	rVB5	1185	609	0.02%	0.003%
57	9.506	2628	2633	2635	rBV5	1088	950	0.04%	0.005%
58	9.593	2658	2660	2663	rVV3	1198	832	0.03%	0.004%
59	9.799	2722	2724	2726	rBV4	1296	667	0.02%	0.003%
60	9.889	2748	2752	2754	rBV4	1421	1027	0.04%	0.005%
61	10.146	2819	2832	2851	rBV	647737	1006235	37.44%	5.195%
62	10.429	2913	2920	2921	rBV5	803	777	0.03%	0.004%
63	10.458	2926	2929	2933	rBV3	1543	1024	0.04%	0.005%
64	10.477	2933	2935	2938	rBV5	1000	600	0.02%	0.003%
65	10.548	2953	2957	2960	rBV5	991	798	0.03%	0.004%
66	10.690	2998	3001	3005	rVB5	741	654	0.02%	0.003%
67	10.780	3023	3029	3031	rBV4	1606	1526	0.06%	0.008%
68	10.863	3048	3055	3056	rBV4	1408	1363	0.05%	0.007%
69	10.902	3063	3067	3071	rVB5	1487	1118	0.04%	0.006%
70	10.934	3071	3077	3078	rBV5	789	852	0.03%	0.004%
71	10.960	3082	3085	3087	rBV5	1158	826	0.03%	0.004%
72	11.014	3100	3102	3110	rVB6	1121	898	0.03%	0.005%
73	11.066	3115	3118	3121	rVB5	933	629	0.02%	0.003%
74	11.120	3133	3135	3138	rBV4	1361	921	0.03%	0.005%
75	11.178	3142	3153	3184	rBV	1136611	1819162	67.70%	9.391%
76	11.554	3257	3270	3299	rBV	1152078	1874104	69.74%	9.675%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV091624\
 Data File : VV037300.D
 Acq On : 16 Sep 2024 12:08
 Operator : SY/MD
 Sample : P3993-10
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK002

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082624WMA.M
 Title : VOC Analysis

77	11.853	3360	3363	3365	rBV4	994	686	0.03%	0.004%
78	11.940	3386	3390	3392	rBV5	940	758	0.03%	0.004%
79	12.053	3422	3425	3428	rBV4	1486	974	0.04%	0.005%
80	12.194	3466	3469	3472	rBV4	1038	622	0.02%	0.003%
81	12.310	3503	3505	3508	rBV4	1192	699	0.03%	0.004%
82	12.419	3535	3539	3544	rBV5	1690	1819	0.07%	0.009%
83	12.516	3565	3569	3574	rBV6	1246	1369	0.05%	0.007%
84	12.558	3579	3582	3584	rVB4	987	595	0.02%	0.003%
85	12.587	3589	3591	3594	rBV3	1039	753	0.03%	0.004%
86	12.683	3618	3621	3625	rBV4	1391	1090	0.04%	0.006%
87	12.747	3638	3641	3644	rBV4	928	702	0.03%	0.004%
88	12.773	3647	3649	3656	rVV7	1193	1141	0.04%	0.006%
89	12.876	3676	3681	3684	rBV6	1312	1089	0.04%	0.006%
90	13.027	3724	3728	3730	rBV3	1343	1009	0.04%	0.005%
91	13.082	3742	3745	3746	rBV3	1221	606	0.02%	0.003%
92	13.127	3753	3759	3764	rBV7	1777	2233	0.08%	0.012%
93	13.570	3895	3897	3900	rVB2	1629	716	0.03%	0.004%
94	13.673	3921	3929	3931	rBV9	1061	1321	0.05%	0.007%
95	13.689	3931	3934	3936	rBV4	1103	617	0.02%	0.003%
96	13.770	3956	3959	3961	rBV4	1159	681	0.03%	0.004%
97	13.783	3961	3963	3968	rBV5	1215	1086	0.04%	0.006%
98	14.104	4060	4063	4068	rVB6	1133	998	0.04%	0.005%
99	14.300	4121	4124	4125	rBV2	1098	595	0.02%	0.003%
100	15.567	4516	4518	4520	rBV3	1523	986	0.04%	0.005%




Sum of corrected areas: 19371077

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV091624\
Data File : VV037300.D
Acq On : 16 Sep 2024 12:08
Operator : SY/MD
Sample : P3993-10
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK002

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

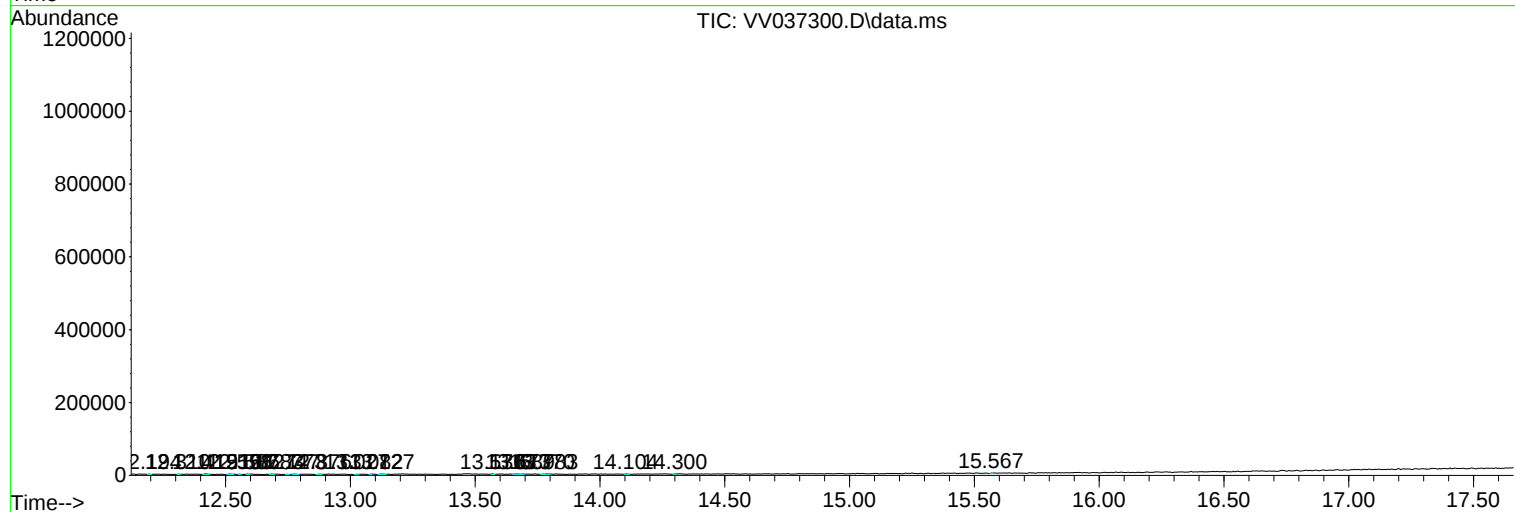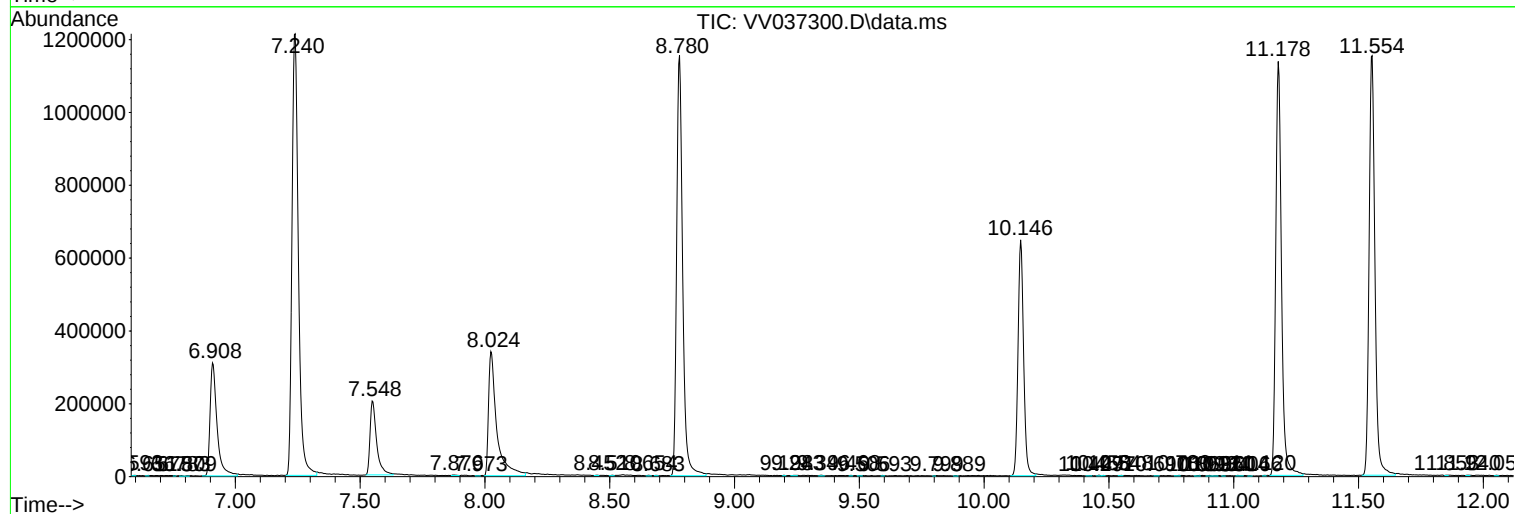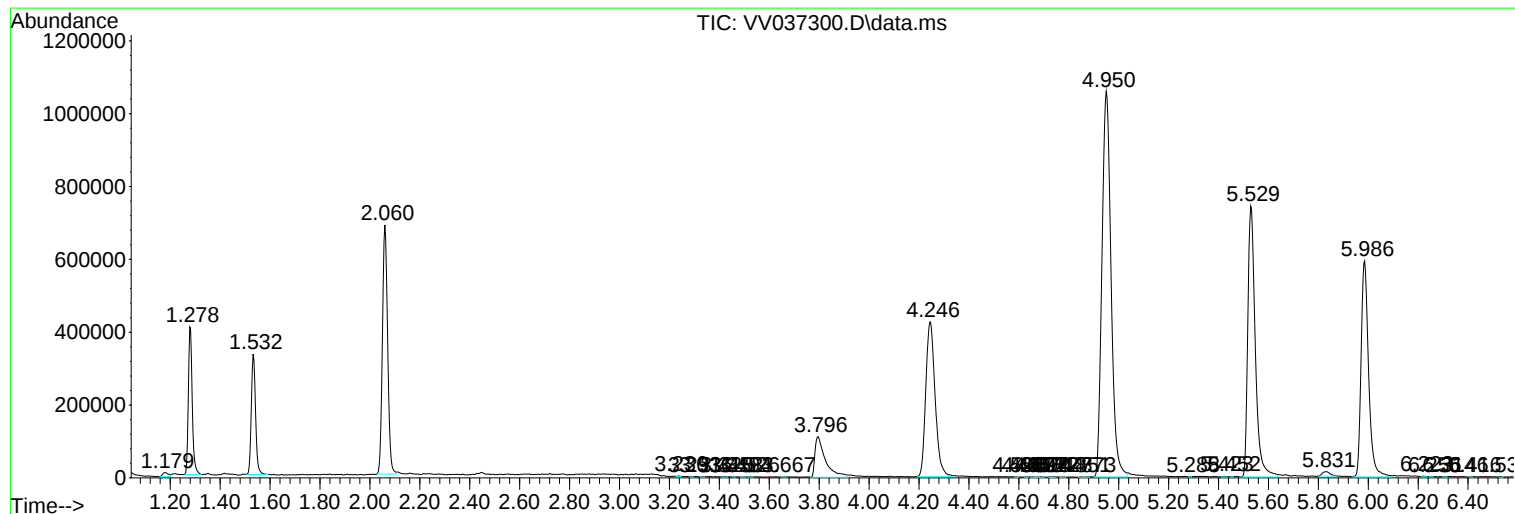

Library Search Compound Report

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV091624\
Data File : VV037300.D
Acq On : 16 Sep 2024 12:08
Operator : SY/MD
Sample : P3993-10
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK002

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV091624\
Data File : VV037300.D
Acq On : 16 Sep 2024 12:08
Operator : SY/MD
Sample : P3993-10
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK002

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc