
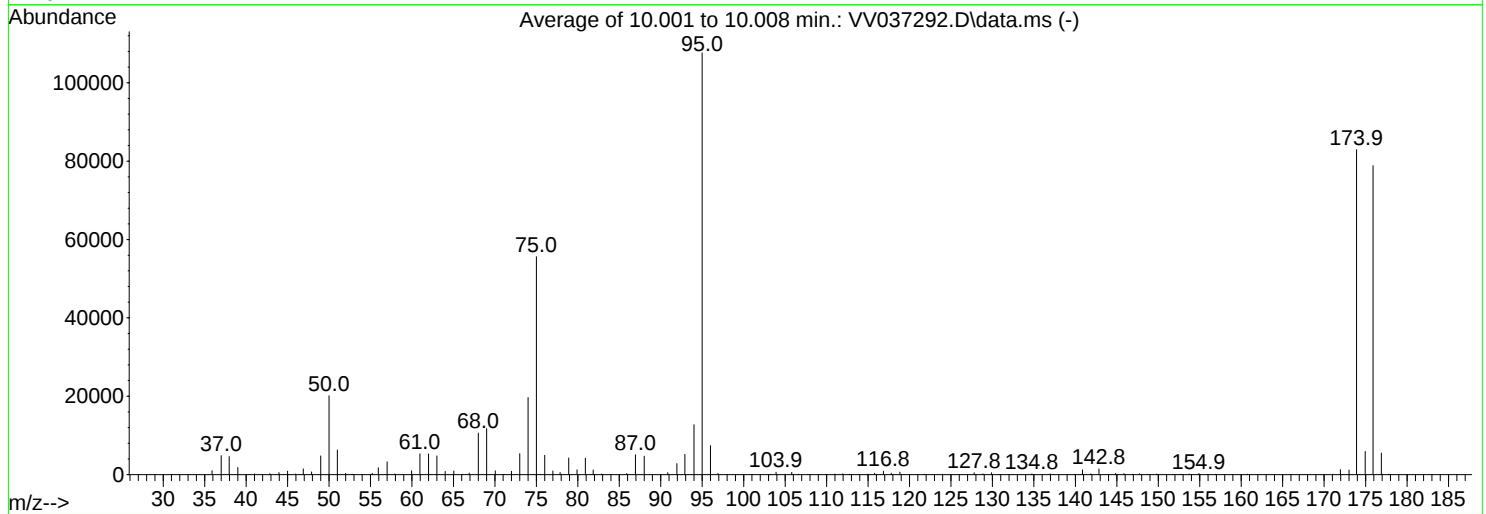


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV091624\
Data File : VV037292.D
Acq On : 16 Sep 2024 08:13
Operator : SY/MD
Sample : BFB378
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB378

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082624WMA.M
Title : VOC Analysis
Last Update : Tue Sep 17 05:05:17 2024

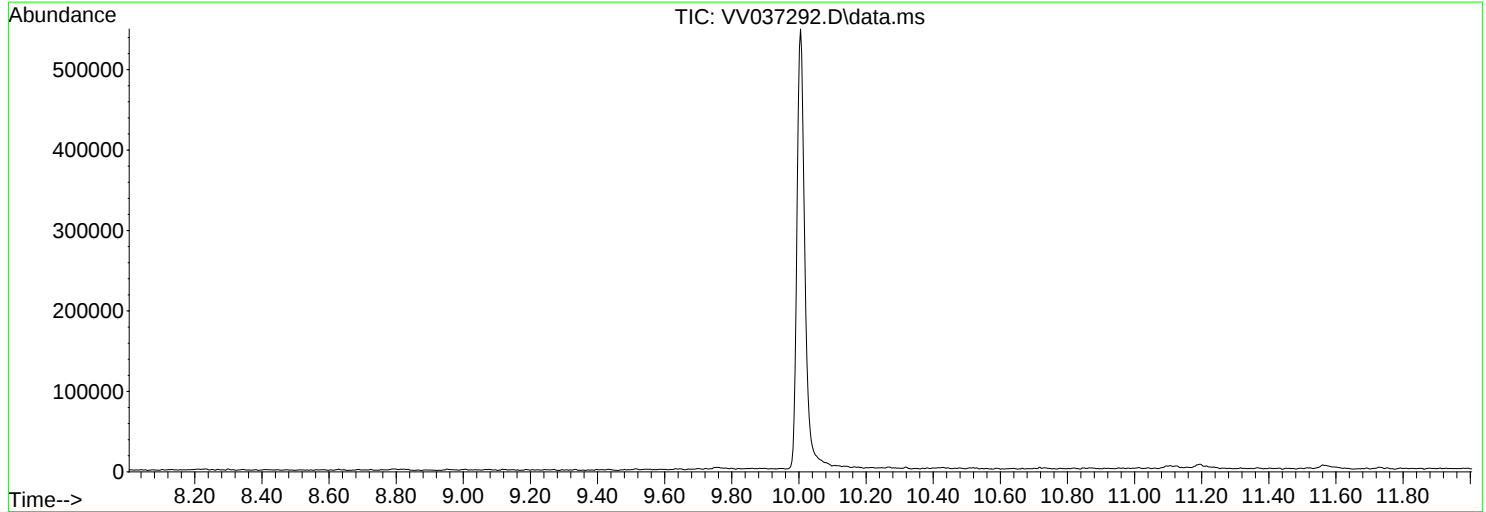

AutoFind: Scans 2787, 2788, 2789; Background Corrected with Scan 2776

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.7	20131	PASS
75	95	30	80	51.7	55619	PASS
95	95	100	100	100.0	107640	PASS
96	95	5	9	6.8	7373	PASS
173	174	0.00	2	1.4	1192	PASS
174	95	50	120	77.0	82925	PASS
175	174	5	9	7.1	5925	PASS
176	174	95	105	95.1	78851	PASS
177	176	5	10	7.0	5526	PASS

m/z	Abundance
35.90	1163.0
37.90	358.0
39.00	169.0
40.00	397.0
42.00	160.0
42.60	101.0
43.10	156.0
44.00	754.0
45.00	173.0
53.90	132.0
54.70	127.0
56.70	148.0

Instrument :
MSVOA_V
ClientSampleId :
BFB378

m/z	Abundance
36.00	2158.0
37.00	4973.0
38.00	5015.0
39.00	1942.0
40.10	467.0
41.00	208.0
42.20	120.0
42.80	224.0
43.90	1247.0
45.00	1003.0
46.00	155.0
46.90	1432.0
47.90	792.0
49.00	4980.0
50.00	20096.0
51.00	5841.0
52.00	358.0
52.90	158.0
53.90	141.0
55.20	341.0
55.90	1848.0
57.00	3270.0
58.00	182.0
59.90	925.0
61.00	5291.0
62.00	5335.0
63.00	4726.0
63.90	829.0
65.00	824.0
66.00	107.0
66.90	412.0
68.00	10844.0
69.00	11812.0
70.00	949.0
72.00	780.0
73.00	5484.0
74.00	19296.0
75.00	56312.0
76.00	4977.0
77.00	1005.0
77.90	542.0
78.90	4076.0
79.90	1155.0
80.90	4235.0
81.90	1233.0
82.90	141.0
86.00	318.0
87.00	4920.0
88.00	4568.0
90.80	637.0
91.90	2747.0
92.90	4949.0
94.00	12428.0
95.00	108368.0
96.00	7403.0
96.90	346.0
103.90	615.0
105.00	155.0
105.80	516.0
106.70	108.0
107.80	103.0
111.00	140.0
112.00	180.0
112.80	113.0
114.90	150.0
115.80	368.0
116.90	871.0
117.90	362.0
118.80	755.0
121.80	130.0
124.00	119.0
127.80	480.0
128.90	279.0
129.90	472.0
130.80	168.0
134.70	236.0
136.90	171.0
139.90	102.0
140.90	1134.0
141.90	153.0
142.90	1458.0
144.90	303.0
145.80	275.0
146.90	155.0
147.70	180.0
149.80	159.0
151.70	133.0
152.80	150.0
153.70	110.0
155.00	247.0
157.00	155.0
158.90	114.0

Instrument :
MSVOA_V
ClientSampleId :
BFB378

160.80	134.0
171.90	1197.0
173.00	1099.0
173.90	80552.0
175.00	5752.0
175.90	76672.0
176.90	5346.0
177.80	103.0

Instrument :
MSVOA_V
ClientSampleId :
BFB378

m/z	Abundance
35.90	2212.0
37.00	4939.0
38.00	5107.0
39.00	2060.0
40.10	499.0
41.10	200.0
42.20	150.0
42.90	255.0
43.90	1326.0
45.00	1108.0
46.00	152.0
46.90	1564.0
47.90	679.0
49.00	4932.0
50.00	20752.0
51.00	6516.0
52.00	354.0
52.80	140.0
53.90	200.0
55.20	348.0
56.00	1798.0
57.00	3438.0
58.00	205.0
59.90	973.0
61.00	5555.0
62.00	5406.0
63.00	4962.0
64.00	859.0
65.10	1006.0
66.00	125.0
66.90	452.0
68.00	10939.0
69.00	12275.0
70.00	1006.0
72.00	937.0
73.00	5589.0
74.00	20456.0
75.00	57416.0
76.00	5174.0
77.00	955.0
77.80	578.0
78.90	4400.0
79.90	1280.0
80.90	4235.0
81.80	1233.0
82.80	171.0
85.90	296.0
86.90	5161.0
88.00	4864.0
90.80	556.0
92.00	2916.0
92.90	5396.0
94.00	13182.0
95.00	110936.0
96.00	7801.0
96.90	351.0
103.20	125.0
103.90	637.0
105.00	150.0
105.80	601.0
106.60	143.0
107.70	102.0
109.90	140.0
111.00	189.0
112.00	205.0
112.80	105.0
115.00	138.0
115.80	399.0
116.90	901.0
117.80	349.0
118.80	660.0
121.70	121.0
124.00	119.0
127.80	481.0
128.80	213.0
129.90	497.0
134.70	220.0
137.00	209.0
140.80	1245.0
141.90	250.0
142.90	1519.0
144.80	346.0
145.90	301.0
146.90	115.0
147.80	245.0
148.70	125.0
149.80	157.0
151.80	132.0
152.80	139.0
153.70	189.0
154.90	252.0
155.90	121.0

Instrument :
MSVOA_V
ClientSampleId :
BFB378

157.00	138.0
159.00	103.0
160.80	127.0
171.10	193.0
171.90	1280.0
173.00	1283.0
173.90	85848.0
174.90	6035.0
175.90	81464.0
176.90	5712.0
177.80	131.0

Instrument :
MSVOA_V
ClientSampleId :
BFB378

m/z	Abundance
35.90	2202.0
37.00	4614.0
38.00	4801.0
39.00	2058.0
40.00	527.0
41.10	215.0
42.20	192.0
42.90	239.0
44.00	1352.0
45.00	1087.0
45.90	165.0
46.90	1403.0
47.90	590.0
49.00	4428.0
50.00	19544.0
51.00	6509.0
52.00	273.0
52.70	132.0
54.00	170.0
54.80	321.0
55.20	323.0
56.00	1576.0
57.00	3124.0
57.90	219.0
60.00	1004.0
60.90	5100.0
62.00	5025.0
63.00	4646.0
64.10	764.0
65.10	1043.0
66.10	136.0
66.90	418.0
68.00	10053.0
69.00	11245.0
70.10	981.0
71.10	105.0
72.00	855.0
73.00	4978.0
74.00	19240.0
75.00	53128.0
76.00	4641.0
77.00	832.0
77.80	462.0
78.90	4320.0
79.90	1257.0
80.90	4100.0
81.80	1137.0
82.80	159.0
85.80	266.0
86.90	5134.0
88.00	4703.0
90.90	454.0
92.00	2843.0
92.90	5259.0
94.00	12614.0
95.00	103616.0
96.00	6914.0
96.90	313.0
103.20	134.0
103.90	550.0
105.00	131.0
105.80	613.0
106.60	167.0
109.90	158.0
111.00	175.0
111.90	210.0
112.70	109.0
115.00	123.0
115.80	382.0
116.80	860.0
117.70	382.0
118.90	596.0
124.00	122.0
127.80	504.0
128.80	141.0
129.90	451.0
134.80	156.0
137.00	246.0
140.80	1279.0
141.80	274.0
142.80	1397.0
144.90	346.0
145.90	297.0
147.80	299.0
148.70	158.0
149.80	138.0
152.70	130.0
153.70	194.0
154.80	315.0
156.90	122.0
160.70	133.0
170.90	179.0

Instrument :
MSVOA_V
ClientSampleId :
BFB378

172.00	1313.0
173.00	1195.0
173.90	82376.0
174.90	5988.0
175.90	78416.0
176.90	5519.0
177.80	122.0

Instrument :
MSVOA_V
ClientSampleId :
BFB378