

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV091719\
 Data File : VV012877.D
 Acq On : 17 Sep 2019 21:33
 Operator : SY/MD
 Sample : K4892-06
 Misc : 25.0mL/MSVOA V/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0MR5

Quant Time: Sep 18 02:55:11 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR091719WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Wed Sep 18 01:09:35 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.66	114	382136	5.00	ug/L	0.00
28) Chlorobenzene-d5	8.89	117	375180	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.29	152	137986	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	192146	5.08	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	101.60%
7) Chloroethane-d5	1.58	69	156243	5.24	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	104.80%
11) 1,1-Dichloroethene-d2	2.13	63	238383	4.27	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	85.40%
20) 2-Butanone-d5	3.98	46	422367	53.33	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	106.66%
24) Chloroform-d	4.40	84	318029	5.15	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	103.00%
26) 1,2-Dichloroethane-d4	5.08	65	166692	5.53	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	110.60%
32) Benzene-d6	5.09	84	654167	5.26	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	105.20%
36) 1,2-Dichloropropane-d6	6.12	67	204817	5.41	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	108.20%
41) Toluene-d8	7.36	98	527011	4.77	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	95.40%
43) trans-1,3-Dichloropropene-	7.66	79	66868	4.91	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	98.20%
46) 2-Hexanone-d5	8.14	63	304230	53.18	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	106.36%
57) 1,1,2,2-Tetrachloroethane-	10.26	84	148899	5.08	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	101.60%
64) 1,2-Dichlorobenzene-d4	11.67	152	175024	5.87	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	117.40%


Target Compounds					Ovalue
34) Trichloroethene	5.96	95	11463	0.457 ug/L	93


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV091719\
Data File : VV012877.D
Acq On : 17 Sep 2019 21:33
Operator : SY/MD
Sample : K4892-06
Misc : 25.0mL/MSVOA V/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0MR5


Quant Time: Sep 18 02:55:11 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR091719WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Wed Sep 18 01:09:35 2019
Response via : Initial Calibration

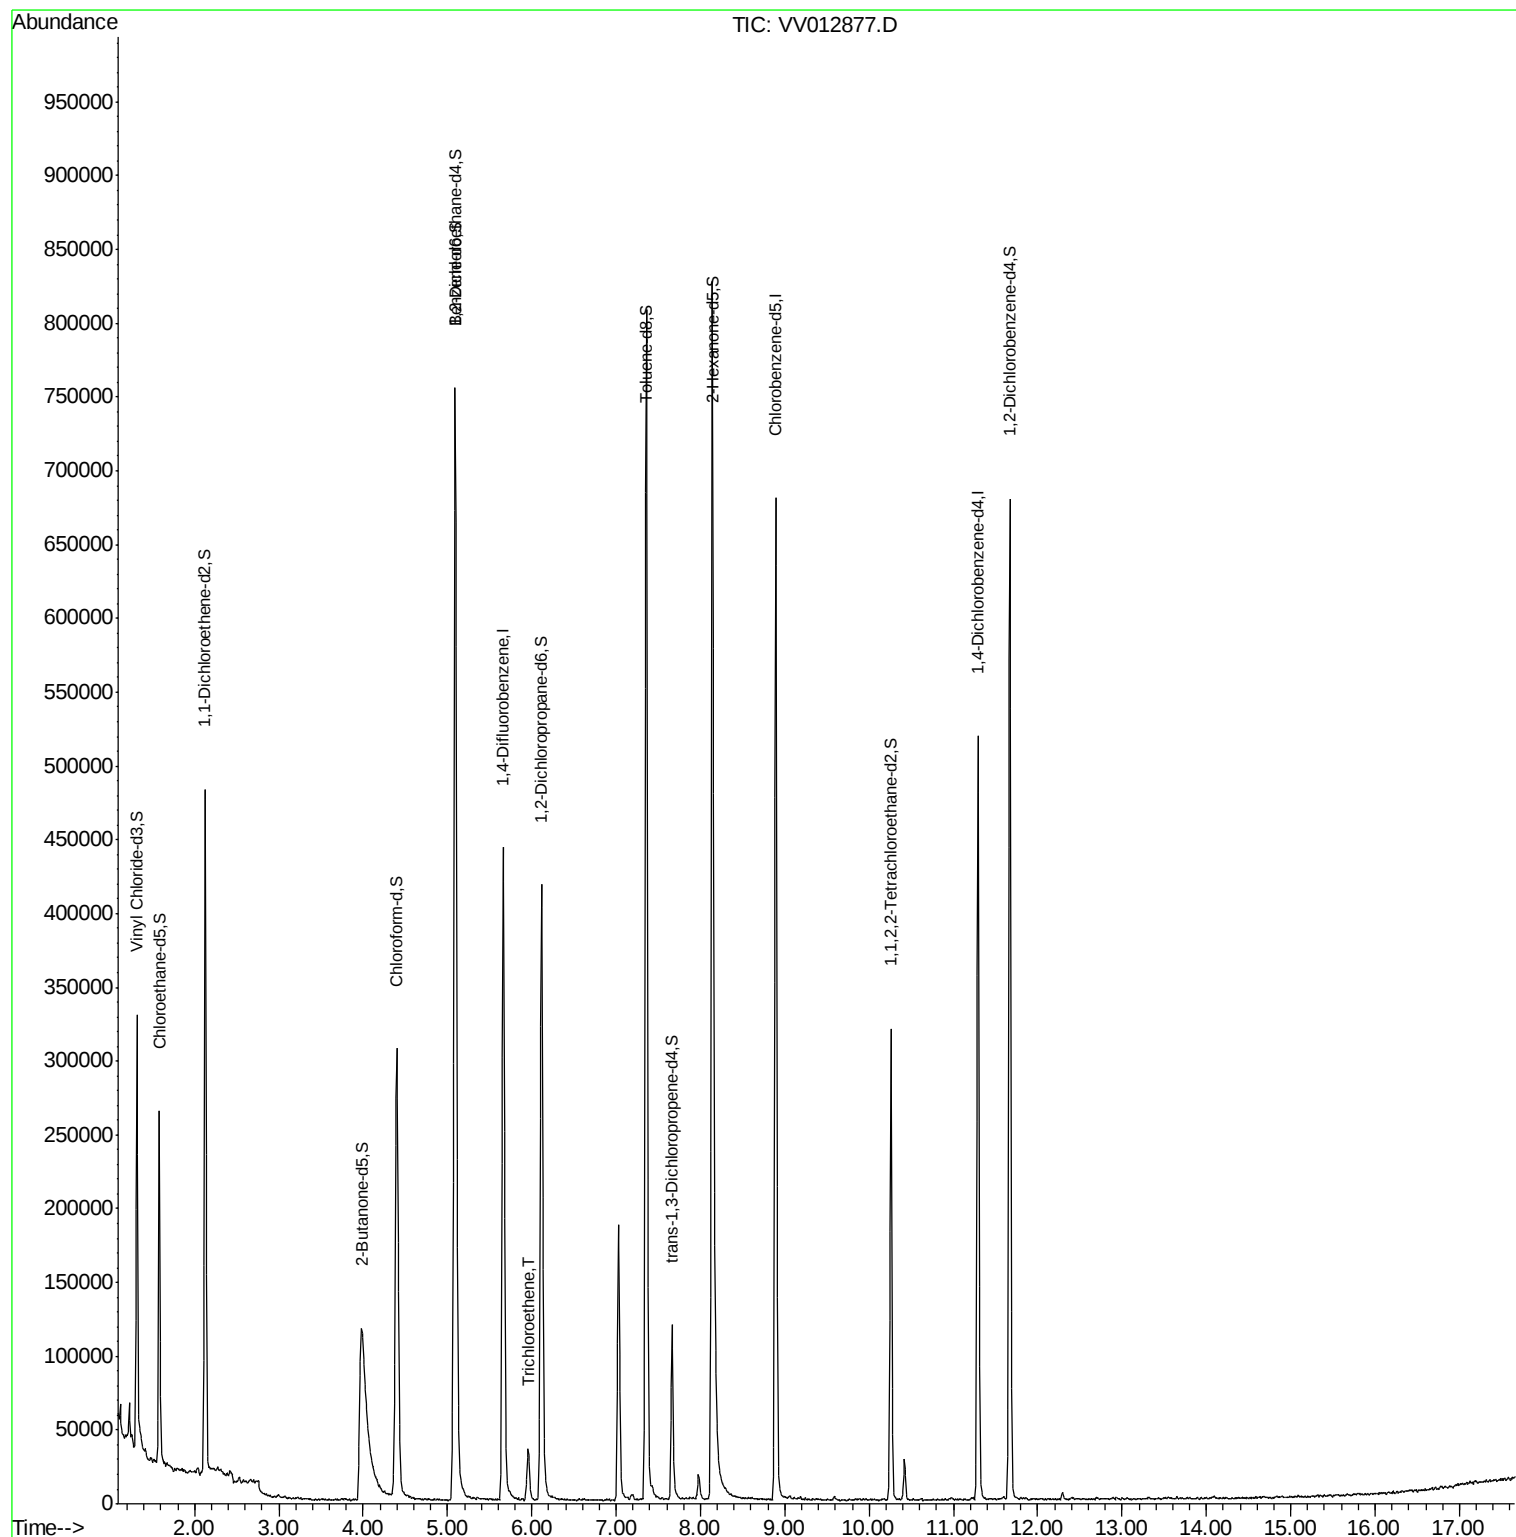

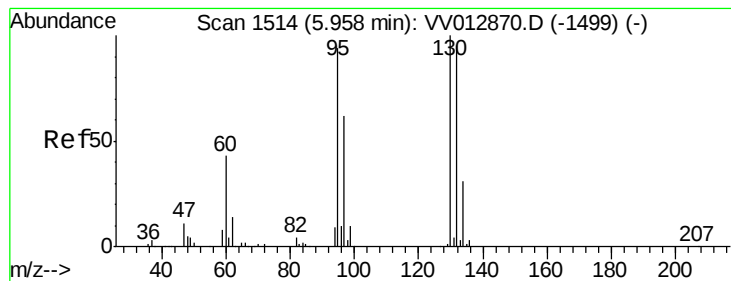

#34
 Trichloroethene
 Concen: 0.457 ug/L
 RT: 5.96 min Scan# 1514
 Delta R.T. 0.00 min
 Lab File: VV012877.D
 Acq: 17 Sep 2019 21:33

Instrument :
 MSVOA_V
 ClientSampleId :
 C0MR5

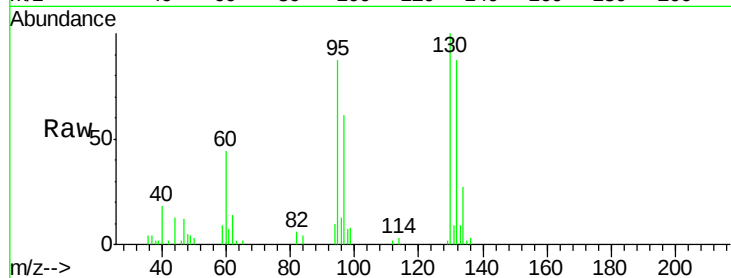

Tot Ion:	95	Resp:	11463
Ion	Ratio	Lower	Upper
95	100		
97	70.0	45.3	84.1
132	100.0	70.6	131.0
130	115.4	71.8	133.4

