

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV091719\
 Data File : VV012881.D
 Acq On : 17 Sep 2019 23:18
 Operator : SY/MD
 Sample : K4834-05
 Misc : 25.0mL/MSVOA V/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 COMEO

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.1
 Stop Thrs : 0
 Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR091719WMA.M
 Title : TRACE VOA SOM01.0

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.225	39	42	61	rVB	26563	29619	2.73%	0.348%
2	1.319	63	71	85	rVB	174311	190077	17.51%	2.236%
3	1.582	146	153	165	rBV	140124	158694	14.62%	1.867%
4	2.129	314	323	336	rBV	277153	387738	35.72%	4.561%
5	3.229	657	665	676	rVB	5861	11858	1.09%	0.139%
6	3.971	879	896	900	rBV2	57430	143578	13.23%	1.689%
7	4.399	1014	1029	1050	rBV2	179430	440693	40.60%	5.184%
8	5.093	1228	1245	1270	rBV2	422501	1020053	93.98%	12.000%
9	5.663	1407	1422	1448	rBV	428027	871190	80.27%	10.248%
10	6.116	1549	1563	1588	rBV	239706	491270	45.26%	5.779%
11	7.029	1834	1847	1867	rBV2	98725	185204	17.06%	2.179%
12	7.357	1935	1949	1969	rBV	428230	756900	69.74%	8.904%
13	7.663	2030	2044	2063	rBV	59202	111524	10.28%	1.312%
14	7.981	2133	2143	2154	rBV2	10303	17337	1.60%	0.204%
15	8.142	2180	2193	2232	rBV3	319497	894482	82.41%	10.522%
16	8.894	2415	2427	2454	rBV	663788	1085368	100.00%	12.768%
17	10.260	2839	2852	2876	rBV	176528	295842	27.26%	3.480%
18	10.421	2891	2902	2912	rBV	14301	24782	2.28%	0.292%
19	11.293	3158	3173	3192	rBV	494593	784318	72.26%	9.227%
20	11.669	3277	3290	3308	rBV	369725	600161	55.30%	7.060%


Sum of corrected areas: 8500688

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV091719\
Data File : VV012881.D
Acq On : 17 Sep 2019 23:18
Operator : SY/MD
Sample : K4834-05
Misc : 25.0mL/MSVOA V/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
COME0

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR091719WMA.M
Quant Title : TRACE VOA SOM01.0

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

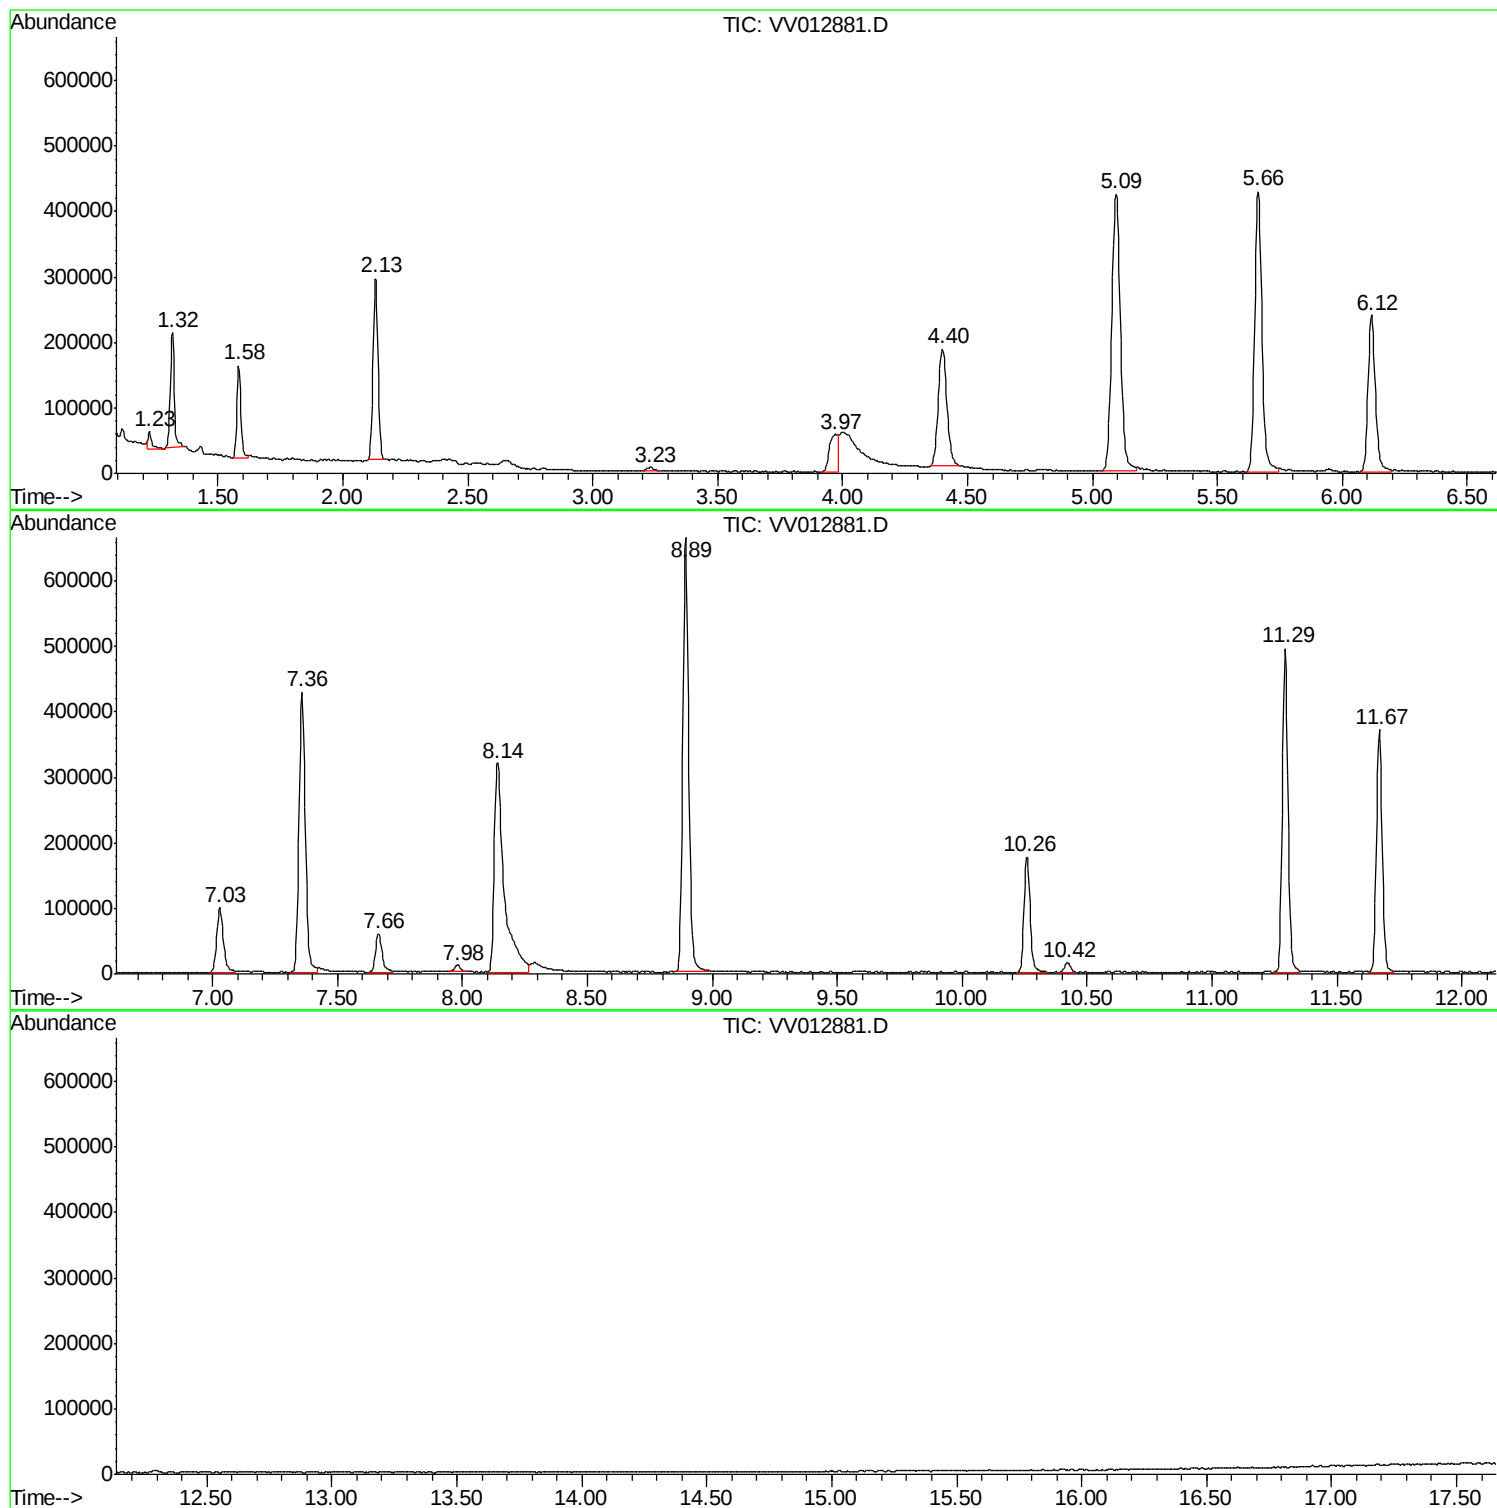

Data_Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV091719\
Data_File : VV012881.D
Acq_On : 17 Sep 2019 23:188
Operator : SY/MDD
Sample : K4834-055
Misc : 25.0mL/MSVOA_V/WATER
ALS_Vial : 21 Sample_Multiplier: 11

Instrument :
MSVOA_V
ClientSampleId :
COMEO

Quant_Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR091719WMA.MM
Quant_Title : TRACE_VOA_SOM01.00

TIC_Library : C:\DATABASE\NIST11.LL
TIC_Integration Parameters: LSCINT.PP

TIC Top Hit name	RT	EstConc	Units	Response	Internal Standard
				#	RT Resp Conc

No Library Search Compounds Detected
