


Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV091719\
Data File : VV012863.D
Acq On : 17 Sep 2019 12:37
Operator : SY/MD
Sample : BFB39
Misc : 25.0mL/MSVOA V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB39

Integration File: rteint.p

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR091719WMA.M
Title : TRACE VOA SOM01.0
Last Update : Wed Sep 18 01:09:35 2019

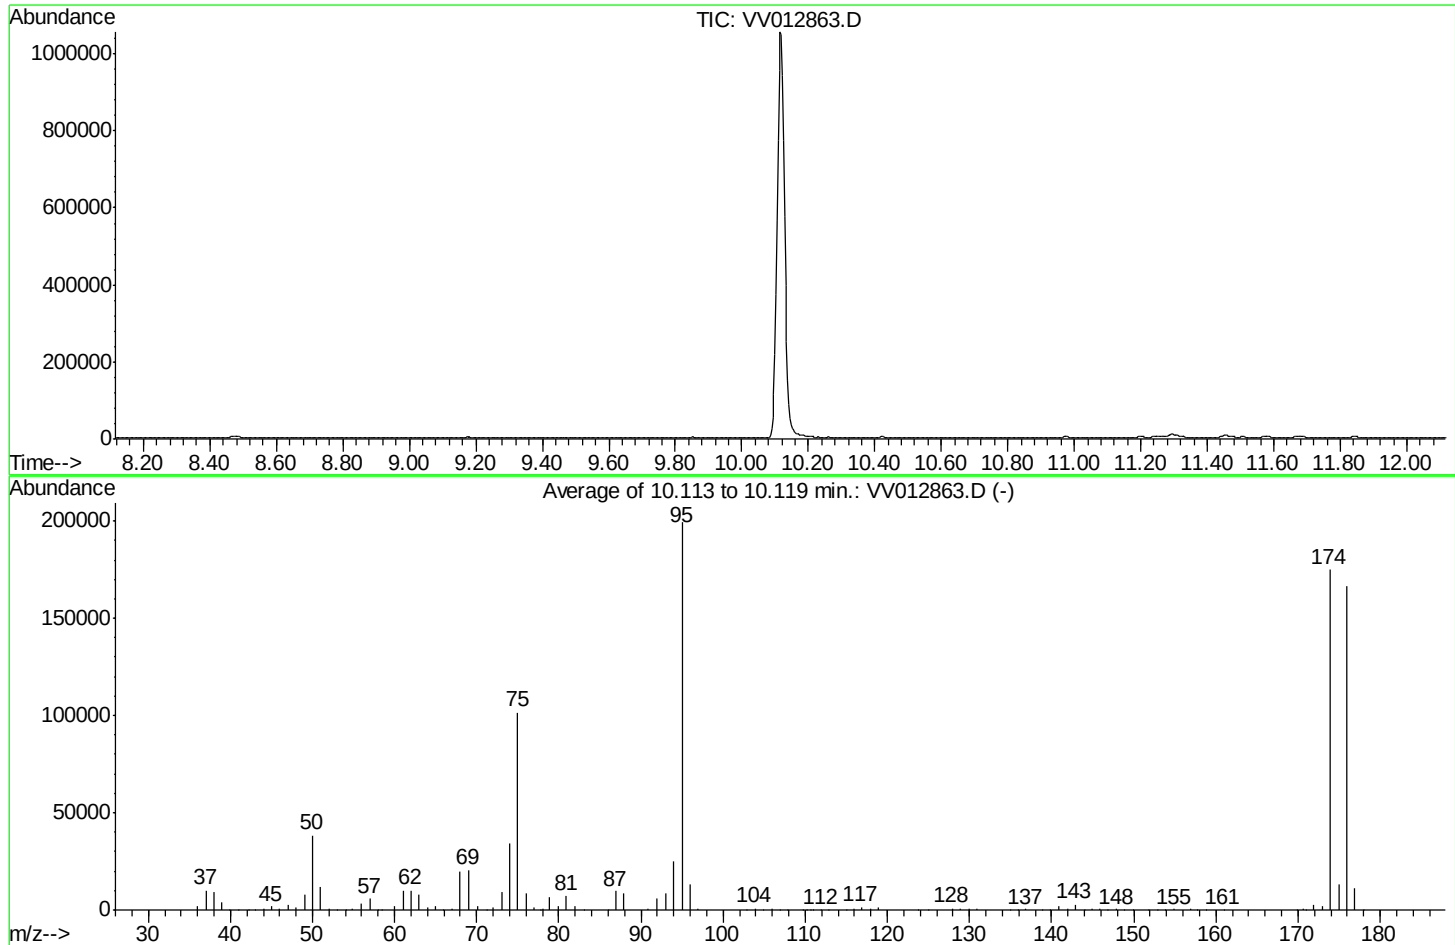

AutoFind: Scans 2806, 2807, 2808; Background Corrected with Scan 2793

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.2	38344	PASS
75	95	30	80	50.9	101408	PASS
95	95	100	100	100.0	199317	PASS
96	95	5	9	6.5	13013	PASS
173	174	0.00	2	1.3	2272	PASS
174	95	50	120	87.7	174762	PASS
175	174	5	9	7.6	13234	PASS
176	174	95	101	95.4	166784	PASS
177	176	5	9	6.9	11443	PASS

Scan 2793 (10.071 min): VV012863.D
BFB39

m/z	Abundance
36.20	163.0
40.00	1183.0
40.90	103.0
44.00	1242.0
45.00	104.0
56.60	112.0
207.00	112.0

Instrument :
MSVOA_V
ClientSampleId :
BFB39

m/z	Abundance
36.00	1980.0
37.00	9952.0
38.00	8775.0
39.00	3777.0
39.90	1445.0
40.90	213.0
42.20	157.0
43.00	281.0
44.00	2102.0
45.00	1794.0
45.90	314.0
47.00	2484.0
47.90	1349.0
49.00	7649.0
50.00	36744.0
51.00	11316.0
52.10	586.0
52.90	366.0
54.10	195.0
55.00	473.0
56.00	2894.0
57.00	5472.0
58.00	157.0
58.40	196.0
60.00	1609.0
61.00	9316.0
62.00	9650.0
63.00	7709.0
64.00	1682.0
65.00	1987.0
66.00	329.0
66.90	571.0
68.00	18776.0
69.00	19272.0
70.10	1686.0
72.00	1314.0
73.00	8581.0
74.00	32568.0
75.00	96024.0
76.00	8407.0
76.90	1023.0
77.80	839.0
78.90	6477.0
79.90	2001.0
80.90	7110.0
81.90	1664.0
83.20	143.0
85.90	325.0
86.90	9181.0
87.90	8157.0
90.90	721.0
92.00	5656.0
93.00	7864.0
94.00	23488.0
95.00	187136.0
96.00	12577.0
96.90	389.0
102.90	110.0
103.80	899.0
104.80	283.0
105.90	716.0
107.00	150.0
107.90	153.0
110.70	169.0
112.00	213.0
112.80	169.0
115.00	239.0
116.00	730.0
116.90	1527.0
117.90	650.0
118.90	1297.0
123.80	220.0
124.90	120.0
127.90	614.0
128.90	355.0
129.90	601.0
130.90	327.0
134.90	315.0
136.80	323.0
139.90	186.0
140.90	1908.0
141.90	332.0
142.90	2676.0
144.00	143.0
144.90	985.0
145.90	371.0
146.90	141.0
147.90	387.0
148.80	148.0
149.90	209.0
152.90	153.0
153.90	193.0

Instrument :
MSVOA_V
ClientSampleId :
BFB39

154.90	622.0
156.90	407.0
157.80	130.0
158.70	127.0
160.90	269.0
169.90	110.0
170.70	466.0
171.00	427.0
171.90	2438.0
173.10	2082.0
173.90	160128.0
175.00	12718.0
175.90	152128.0
176.90	11026.0
178.00	296.0

Instrument :
MSVOA_V
ClientSampleId :
BFB39

m/z	Abundance
36.00	2106.0
37.00	10604.0
38.00	9985.0
39.00	4296.0
39.90	1411.0
40.90	212.0
42.10	165.0
43.00	247.0
44.00	2183.0
45.00	2028.0
46.00	359.0
47.10	2529.0
47.90	1244.0
49.00	8418.0
50.00	39472.0
51.00	11990.0
52.00	564.0
53.00	337.0
54.10	258.0
54.90	533.0
56.00	3173.0
57.00	5976.0
57.90	215.0
58.30	209.0
60.00	1706.0
61.00	10145.0
62.00	10421.0
63.00	8355.0
64.00	1647.0
65.00	2096.0
66.00	343.0
67.00	658.0
68.00	20808.0
69.00	20984.0
70.00	1855.0
71.30	111.0
72.00	1366.0
73.00	9418.0
74.00	35272.0
75.00	104784.0
76.00	9089.0
77.00	1171.0
78.00	840.0
78.90	7137.0
79.90	2004.0
80.90	7486.0
81.90	1824.0
83.10	160.0
85.90	310.0
86.90	10270.0
87.90	9016.0
90.90	808.0
92.00	6007.0
93.00	8832.0
94.00	25944.0
95.00	206720.0
96.00	13475.0
96.90	420.0
102.90	157.0
103.90	1032.0
104.90	316.0
105.90	830.0
106.90	176.0
107.90	140.0
109.80	109.0
110.70	161.0
111.90	215.0
112.80	176.0
114.90	251.0
116.00	735.0
116.90	1534.0
117.90	786.0
118.90	1398.0
123.80	199.0
124.90	102.0
127.90	792.0
128.90	405.0
129.90	693.0
130.90	374.0
134.90	329.0
135.90	134.0
136.90	368.0
139.90	217.0
140.90	2051.0
141.90	445.0
142.90	2869.0
144.00	222.0
144.90	986.0
145.80	451.0
146.90	110.0
147.90	474.0
148.80	197.0

Instrument :
MSVOA_V
ClientSampleId :
BFB39

149.90	252.0
151.80	152.0
152.90	212.0
153.90	193.0
154.90	612.0
157.00	470.0
157.70	121.0
158.80	191.0
161.00	272.0
169.90	141.0
170.70	534.0
171.90	2687.0
173.00	2320.0
173.90	180800.0
175.00	13736.0
175.90	172480.0
176.90	11789.0
177.90	306.0

Instrument :
MSVOA_V
ClientSampleId :
BFB39

m/z	Abundance
36.00	1967.0
37.00	10055.0
38.00	9829.0
39.00	4470.0
39.90	1381.0
40.90	191.0
42.10	160.0
43.10	164.0
44.00	2254.0
45.00	2031.0
46.00	410.0
47.10	2490.0
47.90	1121.0
49.00	8454.0
50.00	38816.0
51.00	11546.0
52.00	492.0
53.00	336.0
54.10	228.0
54.80	541.0
56.00	3149.0
57.00	5709.0
57.90	252.0
60.00	1754.0
61.00	9699.0
62.00	10189.0
63.00	8180.0
64.00	1464.0
65.00	2027.0
65.90	281.0
66.90	676.0
68.00	20544.0
69.00	21016.0
70.00	1757.0
71.20	141.0
72.00	1269.0
73.00	9204.0
74.00	34408.0
75.00	103416.0
76.00	8819.0
77.00	1190.0
78.00	932.0
78.90	7175.0
80.00	1894.0
80.90	7140.0
81.90	1794.0
83.00	193.0
86.00	302.0
86.90	10148.0
87.90	8725.0
90.90	786.0
92.00	5878.0
93.00	8908.0
94.00	25432.0
95.00	204096.0
96.00	12988.0
97.00	401.0
102.80	172.0
104.00	1051.0
104.90	300.0
105.90	870.0
106.80	186.0
107.90	102.0
109.70	107.0
110.20	149.0
110.90	134.0
111.90	218.0
112.80	166.0
114.90	264.0
116.00	690.0
116.80	1473.0
117.90	799.0
118.90	1329.0
123.80	152.0
127.90	815.0
128.90	445.0
129.90	764.0
130.90	365.0
134.90	330.0
135.90	133.0
136.90	382.0
138.90	122.0
139.80	220.0
140.90	1989.0
141.90	415.0
142.90	2665.0
143.90	272.0
144.90	924.0
145.90	461.0
146.80	104.0
147.90	517.0
148.90	227.0

Instrument :
MSVOA_V
ClientSampleId :
BFB39

150.00	228.0
151.90	205.0
152.90	246.0
153.80	160.0
155.00	566.0
157.00	454.0
158.80	244.0
160.90	229.0
169.90	177.0
170.70	499.0
171.90	2736.0
173.00	2414.0
173.90	183360.0
175.00	13250.0
175.90	175744.0
176.90	11514.0
177.90	331.0

Instrument :
MSVOA_V
ClientSampleId :
BFB39