

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091722\
 Data File : VV027906.D
 Acq On : 17 Sep 2022 17:46
 Operator : SY/MD
 Sample : N4658-02
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0E77

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR091722WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV027906.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.307	75	83	102	rBV	81326	93513	17.05%	2.000%
2	1.568	156	164	179	rBV	68290	82053	14.96%	1.755%
3	2.108	321	332	345	rBV	121400	174942	31.89%	3.742%
4	2.957	586	596	606	rBV5	2930	5578	1.02%	0.119%
5	3.892	877	887	927	rBV	45573	169322	30.87%	3.622%
6	4.346	1011	1028	1061	rBV	98712	256341	46.73%	5.483%
7	5.043	1229	1245	1277	rBV3	213940	548504	100.00%	11.732%
8	5.616	1411	1423	1450	rBV	177286	368234	67.13%	7.876%
9	5.905	1503	1513	1529	rVB6	4600	10367	1.89%	0.222%
10	6.066	1550	1563	1592	rBV2	118364	252016	45.95%	5.390%
11	6.301	1626	1636	1652	rBV4	6944	16740	3.05%	0.358%
12	6.985	1836	1849	1869	rBV	58854	111513	20.33%	2.385%
13	7.313	1940	1951	1967	rBV	243069	432872	78.92%	9.258%
14	7.391	1967	1975	1989	rVB	34888	64222	11.71%	1.374%
15	7.622	2037	2047	2069	rBV	36308	66684	12.16%	1.426%
16	7.940	2133	2146	2155	rBV2	8613	15528	2.83%	0.332%
17	8.091	2182	2193	2226	rBV	191757	433407	79.02%	9.270%
18	8.249	2235	2242	2256	rVB9	8116	14380	2.62%	0.308%
19	8.850	2417	2429	2452	rBV	277440	463298	84.47%	9.909%
20	9.146	2511	2521	2534	rBV6	4433	8390	1.53%	0.179%
21	9.564	2639	2651	2673	rBV4	18133	34838	6.35%	0.745%
22	10.214	2841	2853	2869	rBV	78599	126783	23.11%	2.712%
23	10.381	2894	2905	2921	rBV2	29114	48732	8.88%	1.042%
24	11.246	3163	3174	3199	rBV	284670	456450	83.22%	9.763%
25	11.532	3252	3263	3279	rBV4	7645	13536	2.47%	0.290%
26	11.622	3279	3291	3310	rVV	255886	401372	73.18%	8.585%
27	13.509	3869	3878	3890	rBV3	3919	5803	1.06%	0.124%




Sum of corrected areas: 4675418

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091722\
Data File : VV027906.D
Acq On : 17 Sep 2022 17:46
Operator : SY/MD
Sample : N4658-02
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0E77

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR091722WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

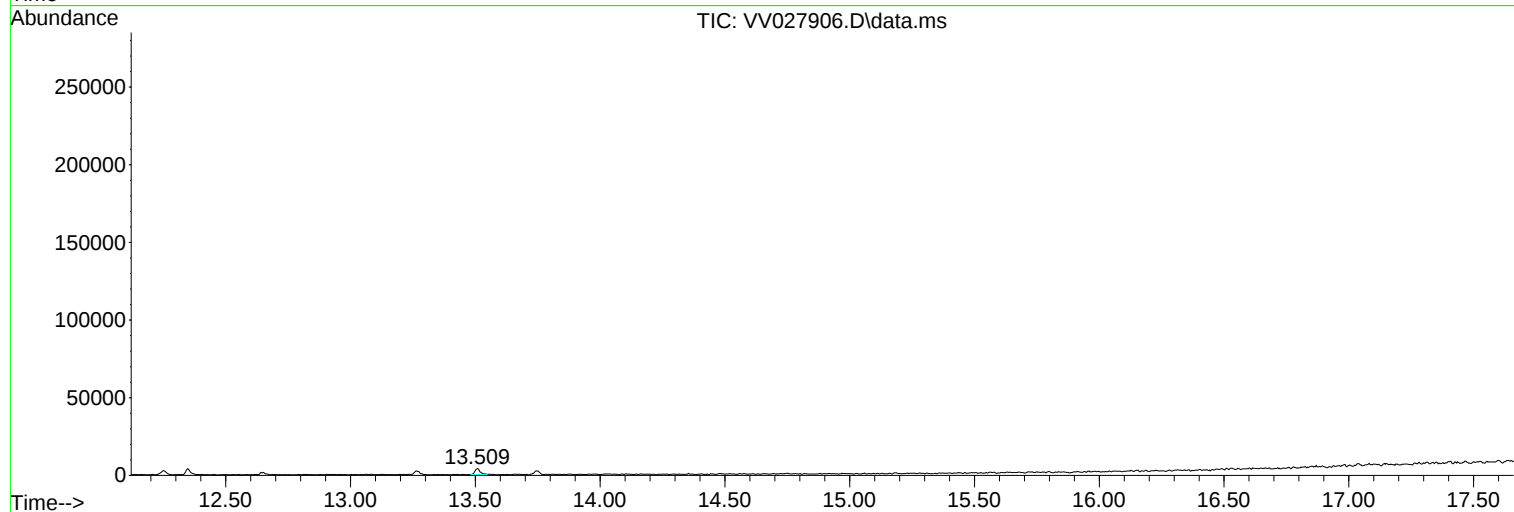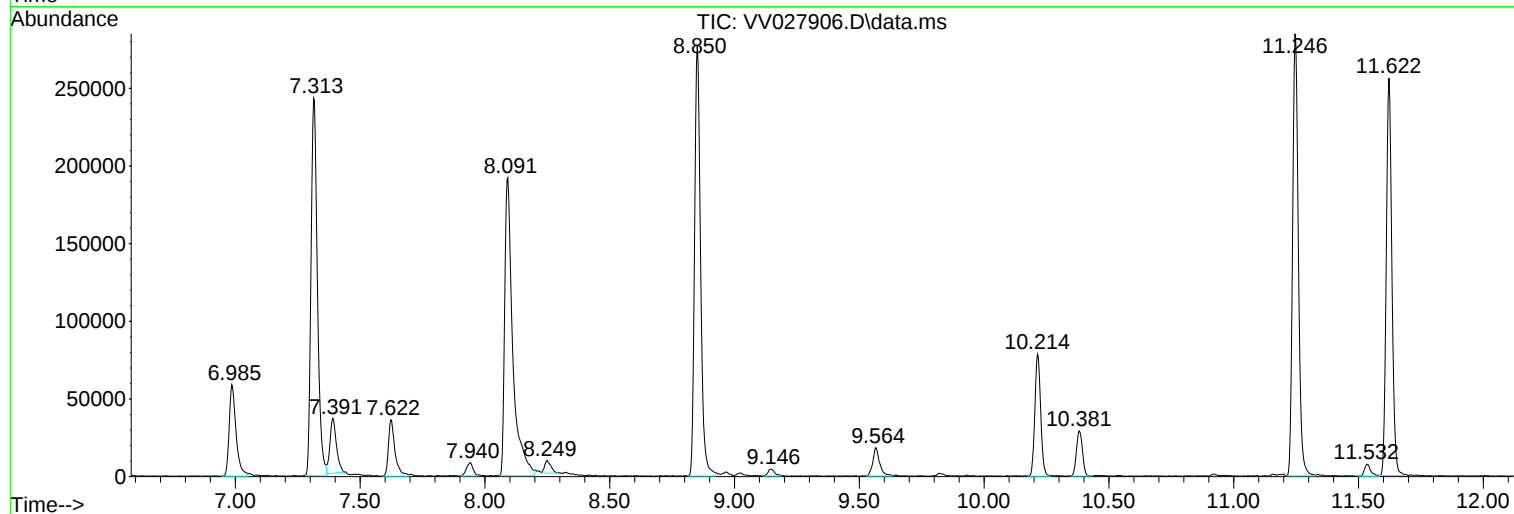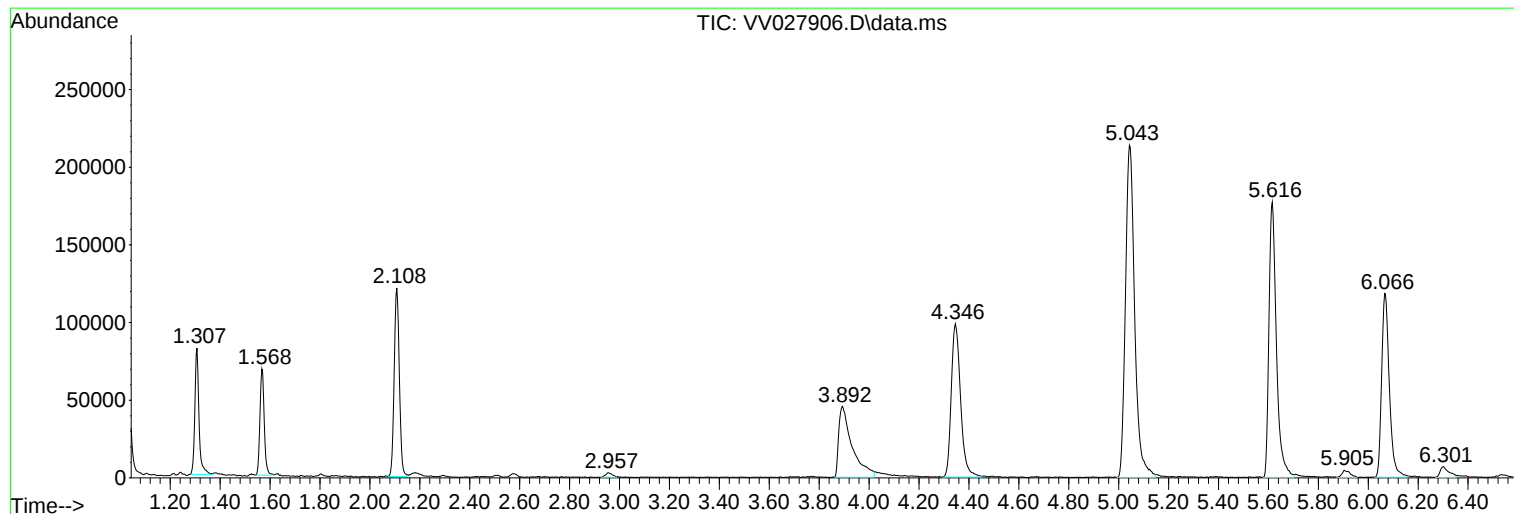

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091722\
Data File : VV027906.D
Acq On : 17 Sep 2022 17:46
Operator : SY/MD
Sample : N4658-02
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0E77

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR091722WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091722\
Data File : VV027906.D
Acq On : 17 Sep 2022 17:46
Operator : SY/MD
Sample : N4658-02
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0E77

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR091722WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
