

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091722\
 Data File : VV027907.D
 Acq On : 17 Sep 2022 18:10
 Operator : SY/MD
 Sample : N4672-05
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0EC0

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR091722WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV027907.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.307	73	83	102	rBV	81487	96618	17.41%	2.077%
2	1.568	155	164	180	rBV	70087	79963	14.41%	1.719%
3	2.108	317	332	345	rBV	122402	174900	31.51%	3.760%
4	3.892	876	887	913	rBV2	45455	152818	27.53%	3.286%
5	4.346	1012	1028	1051	rBV	101117	257377	46.37%	5.533%
6	5.043	1230	1245	1280	rBV2	216834	555006	100.00%	11.932%
7	5.616	1409	1423	1453	rBV	174159	368439	66.38%	7.921%
8	5.915	1506	1516	1531	rVB7	4977	11264	2.03%	0.242%
9	6.066	1550	1563	1593	rBV	117438	248060	44.70%	5.333%
10	6.301	1629	1636	1656	rBV5	6040	14709	2.65%	0.316%
11	6.985	1839	1849	1867	rBV	56760	108931	19.63%	2.342%
12	7.313	1939	1951	1967	rBV	245548	434628	78.31%	9.344%
13	7.391	1967	1975	1990	rVB2	33797	64577	11.64%	1.388%
14	7.622	2039	2047	2068	rBV2	34720	63842	11.50%	1.373%
15	7.937	2129	2145	2157	rBV2	10170	19518	3.52%	0.420%
16	8.088	2183	2192	2226	rBV2	190450	431354	77.72%	9.274%
17	8.249	2233	2242	2254	rBV6	7368	13054	2.35%	0.281%
18	8.850	2416	2429	2449	rBV	271498	452208	81.48%	9.722%
19	9.567	2638	2652	2667	rBV3	17707	33953	6.12%	0.730%
20	10.214	2842	2853	2871	rBV	80889	127940	23.05%	2.751%
21	10.381	2894	2905	2918	rVB2	39036	63187	11.38%	1.358%
22	11.246	3163	3174	3201	rBV	287899	452328	81.50%	9.725%
23	11.535	3253	3264	3274	rBV4	7563	12756	2.30%	0.274%
24	11.622	3280	3291	3315	rBV	251591	399940	72.06%	8.598%
25	12.249	3476	3486	3497	rVB2	5007	7920	1.43%	0.170%
26	12.345	3509	3516	3527	rBV6	4200	5995	1.08%	0.129%




Sum of corrected areas: 4651285

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091722\
Data File : VV027907.D
Acq On : 17 Sep 2022 18:10
Operator : SY/MD
Sample : N4672-05
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0EC0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR091722WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

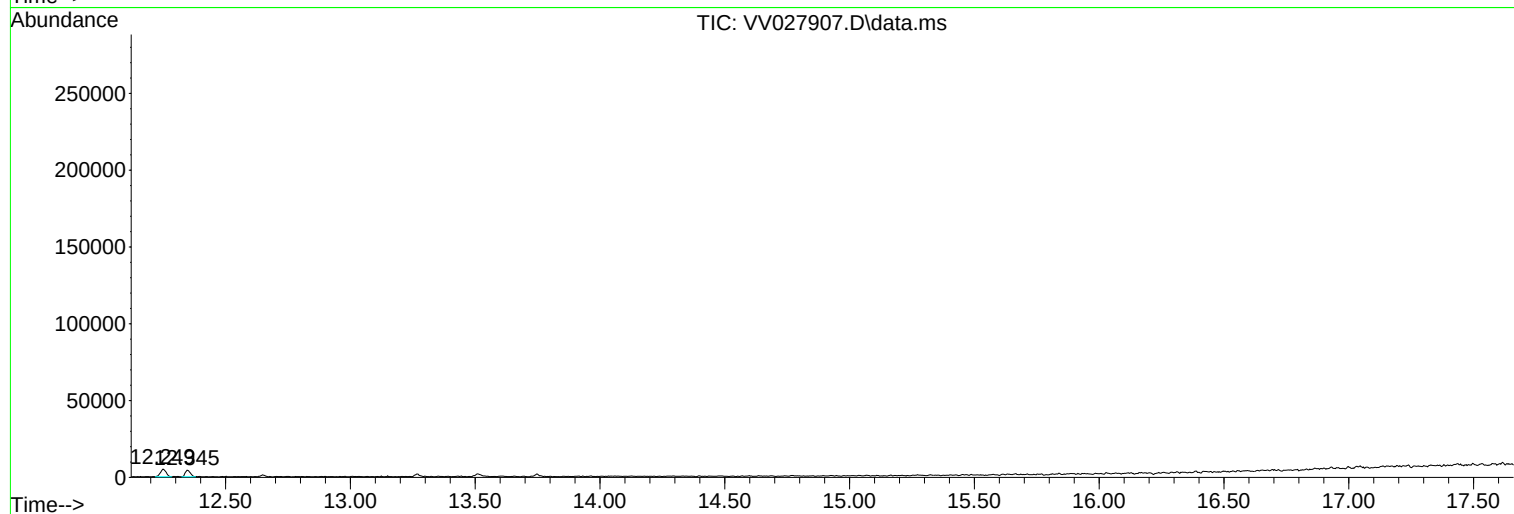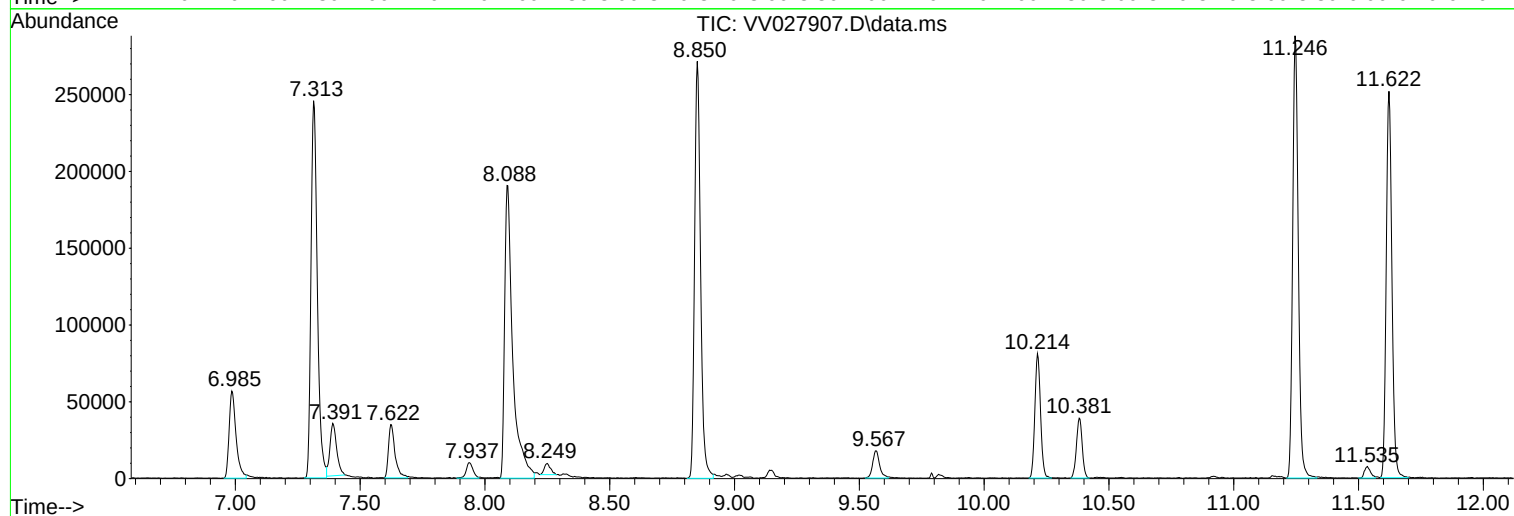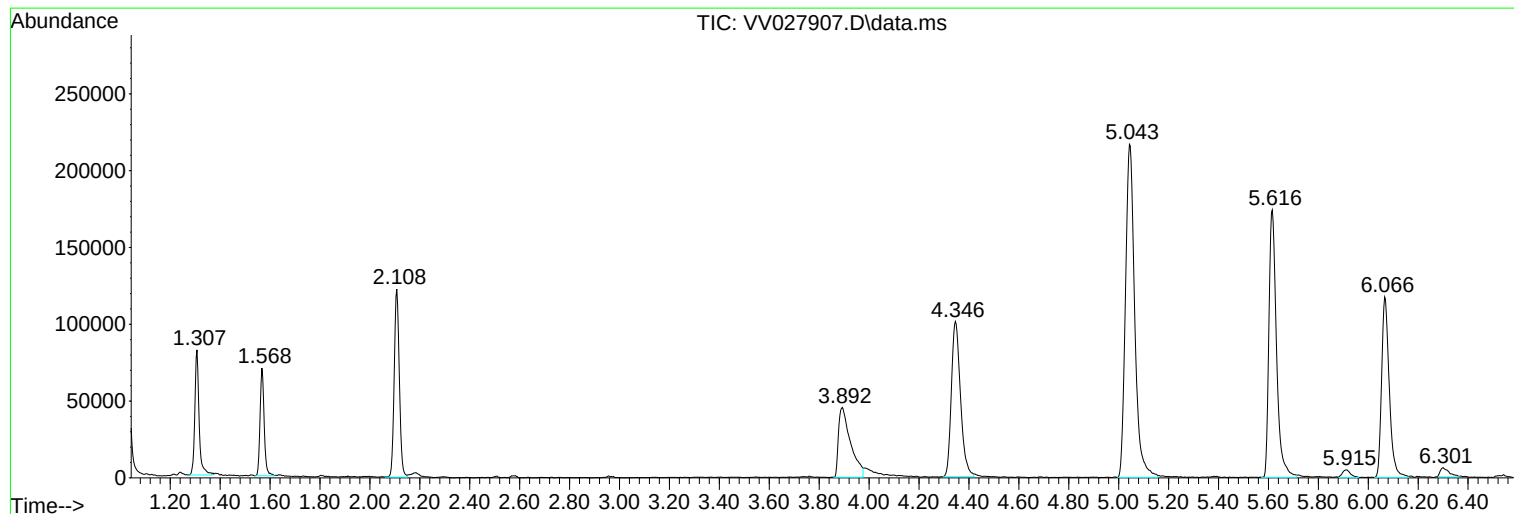

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091722\
Data File : VV027907.D
Acq On : 17 Sep 2022 18:10
Operator : SY/MD
Sample : N4672-05
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0EC0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR091722WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091722\
Data File : VV027907.D
Acq On : 17 Sep 2022 18:10
Operator : SY/MD
Sample : N4672-05
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0EC0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR091722WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc