

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091722\
 Data File : VV027908.D
 Acq On : 17 Sep 2022 18:35
 Operator : SY/MD
 Sample : N4652-01DL 40X
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EXYZ9DL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR091722WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV027908.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.307	75	83	103	rBV2	105511	127887	23.40%	2.190%
2	1.584	156	169	192	rVB2	144727	244925	44.81%	4.193%
3	2.108	321	332	347	rBV	138173	198458	36.31%	3.398%
4	2.506	446	456	469	rBV2	13558	22595	4.13%	0.387%
5	2.767	527	537	547	rBV5	3820	6575	1.20%	0.113%
6	3.188	652	668	688	rBV	159374	337905	61.82%	5.785%
7	3.905	868	891	921	rBV2	174095	544467	99.62%	9.322%
8	4.346	1013	1028	1052	rBV	98244	249452	45.64%	4.271%
9	4.606	1091	1109	1136	rBV2	111906	287245	52.55%	4.918%
10	5.043	1230	1245	1281	rBV3	211963	546571	100.00%	9.358%
11	5.612	1411	1422	1455	rBV	163405	345056	63.13%	5.908%
12	5.915	1506	1516	1529	rBV9	6463	14017	2.56%	0.240%
13	6.069	1551	1564	1580	rBV2	116121	244813	44.79%	4.192%
14	6.985	1838	1849	1872	rBV	57750	109584	20.05%	1.876%
15	7.313	1940	1951	1966	rBV	238589	427311	78.18%	7.316%
16	7.391	1967	1975	1995	rVB	35060	69496	12.71%	1.190%
17	7.625	2038	2048	2065	rBV2	33452	62618	11.46%	1.072%
18	7.940	2134	2146	2151	rBV3	7001	12448	2.28%	0.213%
19	7.976	2151	2157	2174	rVB4	11859	21321	3.90%	0.365%
20	8.088	2182	2192	2227	rBV2	191808	422482	77.30%	7.233%
21	8.850	2414	2429	2455	rBV	252342	429730	78.62%	7.358%
22	9.014	2471	2480	2495	rBV	8391	13537	2.48%	0.232%
23	9.140	2509	2519	2537	rVB	14217	24757	4.53%	0.424%
24	9.548	2634	2646	2656	rBV2	11724	19111	3.50%	0.327%
25	10.214	2840	2853	2869	rBV	80408	130999	23.97%	2.243%
26	10.384	2889	2906	2916	rBV3	16080	29113	5.33%	0.498%
27	10.452	2919	2927	2943	rVV2	6941	14503	2.65%	0.248%
28	10.542	2944	2955	2964	rVB3	3963	5861	1.07%	0.100%
29	10.738	3010	3016	3025	rBV2	6822	9864	1.80%	0.169%
30	10.915	3061	3071	3083	rBV	20139	31274	5.72%	0.535%
31	11.246	3164	3174	3193	rBV	265569	410357	75.08%	7.026%
32	11.336	3195	3202	3216	rVB2	10368	16689	3.05%	0.286%
33	11.529	3253	3262	3272	rBV6	4268	8186	1.50%	0.140%
34	11.622	3280	3291	3310	rVB	253275	401485	73.46%	6.874%

Sum of corrected areas: 5840692




Instrument :
MSVOA_V
ClientSampleId :
XYZ9DL

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091722\
Data File : VV027908.D
Acq On : 17 Sep 2022 18:35
Operator : SY/MD
Sample : N4652-01DL 40X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EXYZ9DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR091722WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

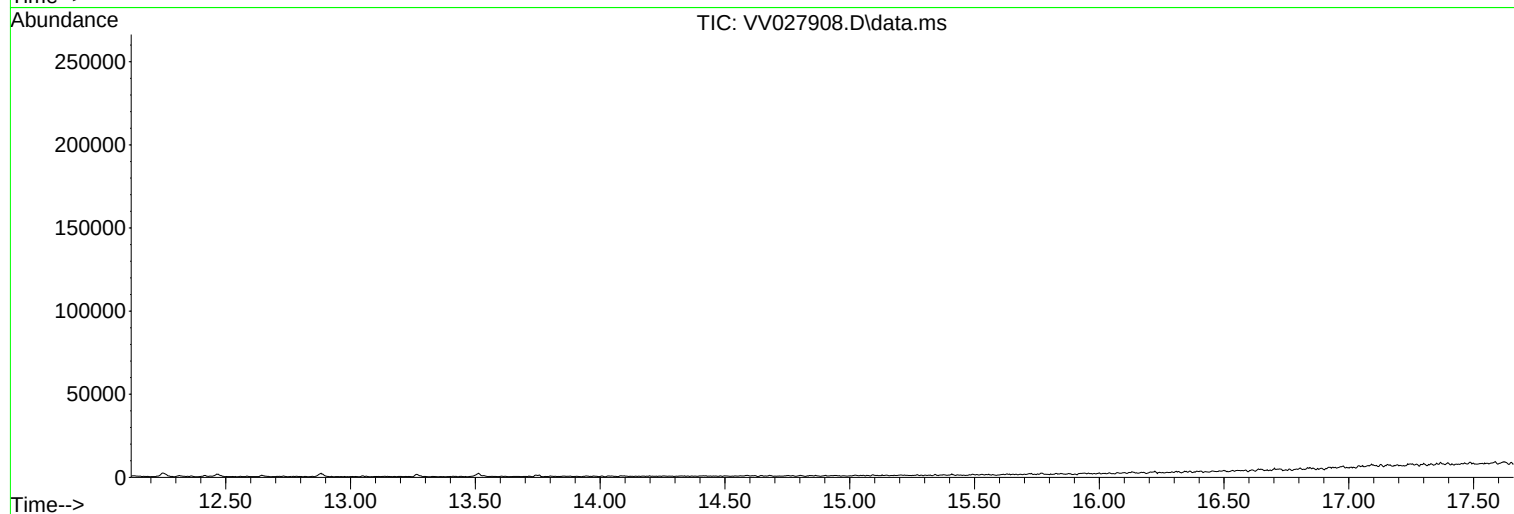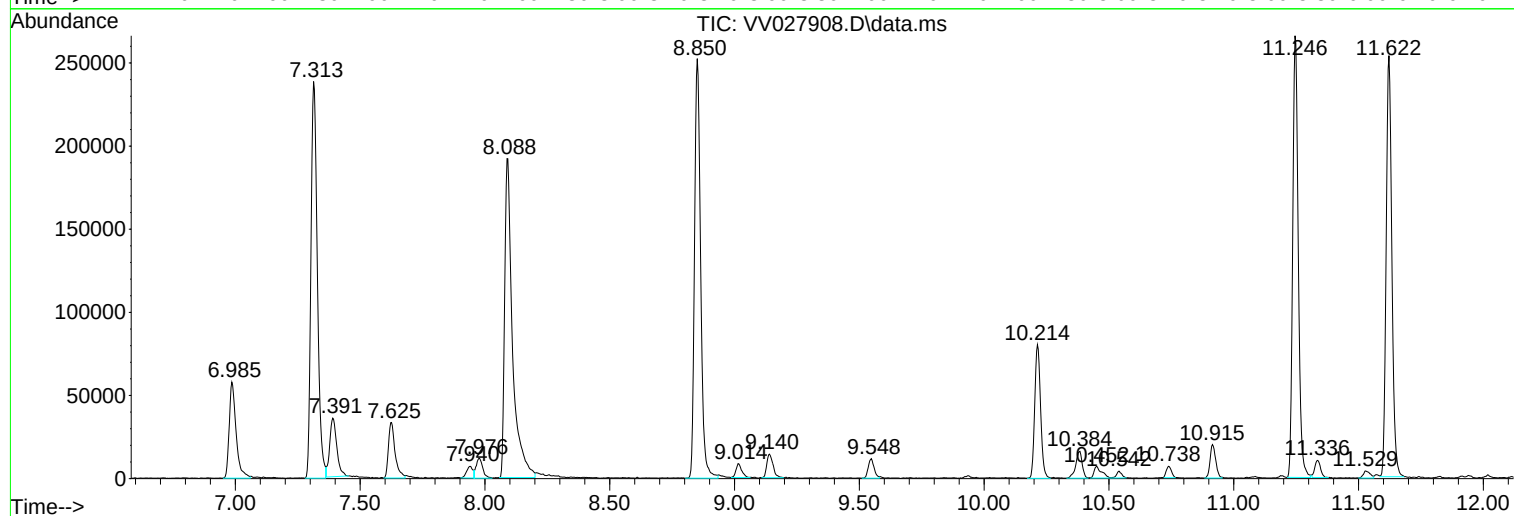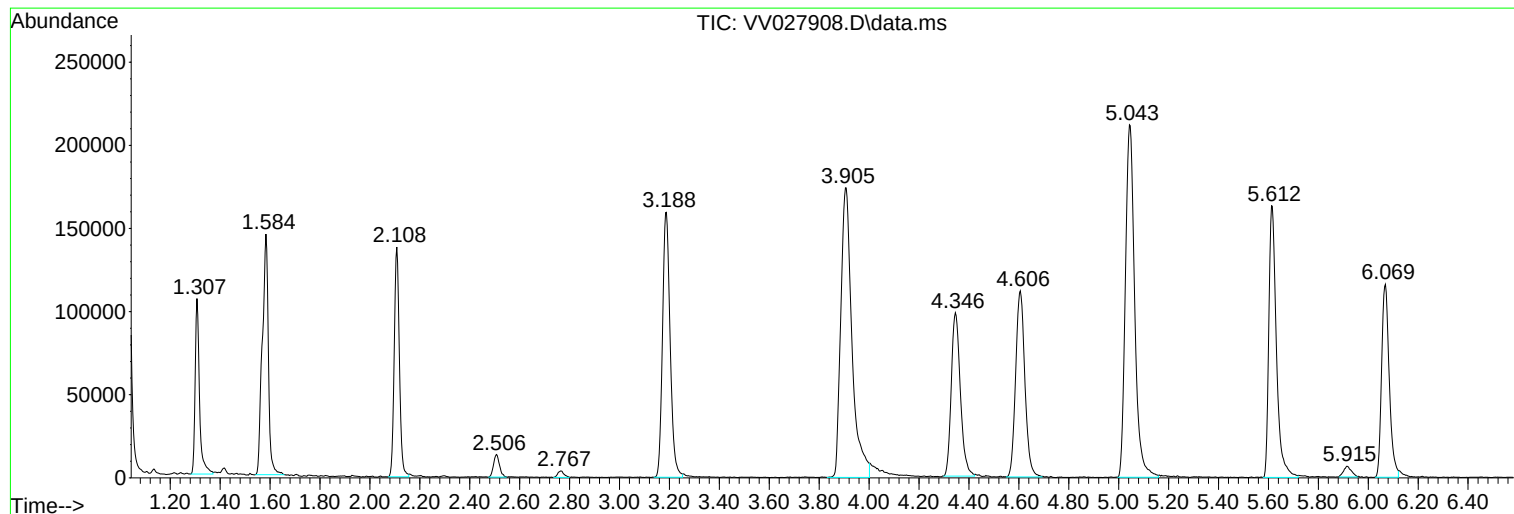

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091722\
Data File : VV027908.D
Acq On : 17 Sep 2022 18:35
Operator : SY/MD
Sample : N4652-01DL 40X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EXYZ9DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR091722WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091722\
Data File : VV027908.D
Acq On : 17 Sep 2022 18:35
Operator : SY/MD
Sample : N4652-01DL 40X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EXYZ9DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR091722WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc