

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091722\
 Data File : VV027909.D
 Acq On : 17 Sep 2022 18:59
 Operator : SY/MD
 Sample : N4672-10
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0ED7

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR091722WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV027909.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.307	76	83	92	rBV	42893	45163	9.87%	1.123%
2	1.568	156	164	175	rBV	51544	60717	13.27%	1.509%
3	2.108	322	332	346	rBV2	79833	120481	26.32%	2.995%
4	3.899	878	889	930	rBV2	48028	190545	41.63%	4.736%
5	4.349	1013	1029	1056	rBV2	88373	241083	52.67%	5.992%
6	5.043	1229	1245	1274	rBV3	176049	454691	99.34%	11.301%
7	5.616	1411	1423	1455	rBV2	138421	291353	63.66%	7.242%
8	5.911	1503	1515	1549	rBV	120844	252927	55.26%	6.287%
9	6.066	1549	1563	1584	rBV	106499	222752	48.67%	5.537%
10	6.989	1839	1850	1863	rBV2	40011	76128	16.63%	1.892%
11	7.313	1939	1951	1975	rBV	185556	332828	72.72%	8.272%
12	7.625	2039	2048	2066	rBV	25114	45409	9.92%	1.129%
13	7.940	2137	2146	2155	rBV2	3618	5750	1.26%	0.143%
14	8.088	2182	2192	2229	rBV2	204629	457703	100.00%	11.376%
15	8.850	2418	2429	2451	rBV	220046	367730	80.34%	9.140%
16	10.214	2842	2853	2870	rBV	79092	126125	27.56%	3.135%
17	10.384	2894	2906	2916	rBV2	14694	23785	5.20%	0.591%
18	11.246	3162	3174	3196	rBV	227806	365039	79.75%	9.073%
19	11.535	3256	3264	3275	rBV4	5234	9018	1.97%	0.224%
20	11.622	3280	3291	3309	rBV	206499	329523	71.99%	8.190%
21	12.249	3475	3486	3495	rBV3	2999	4580	1.00%	0.114%




Sum of corrected areas: 4023330

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091722\
Data File : VV027909.D
Acq On : 17 Sep 2022 18:59
Operator : SY/MD
Sample : N4672-10
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0ED7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR091722WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

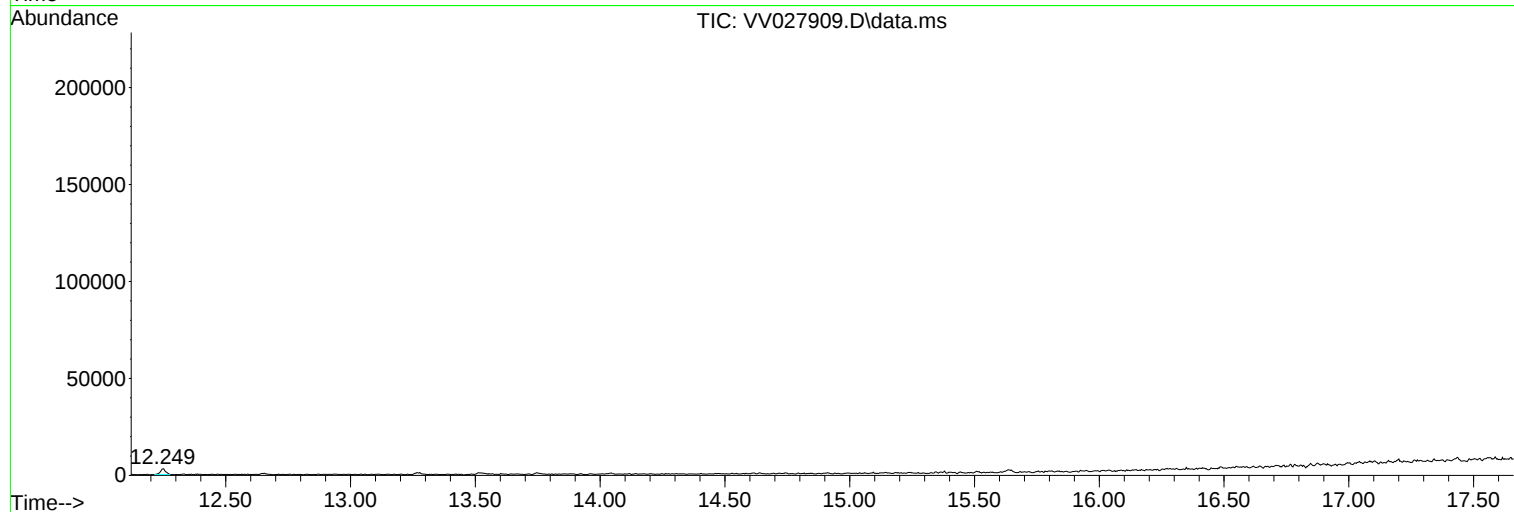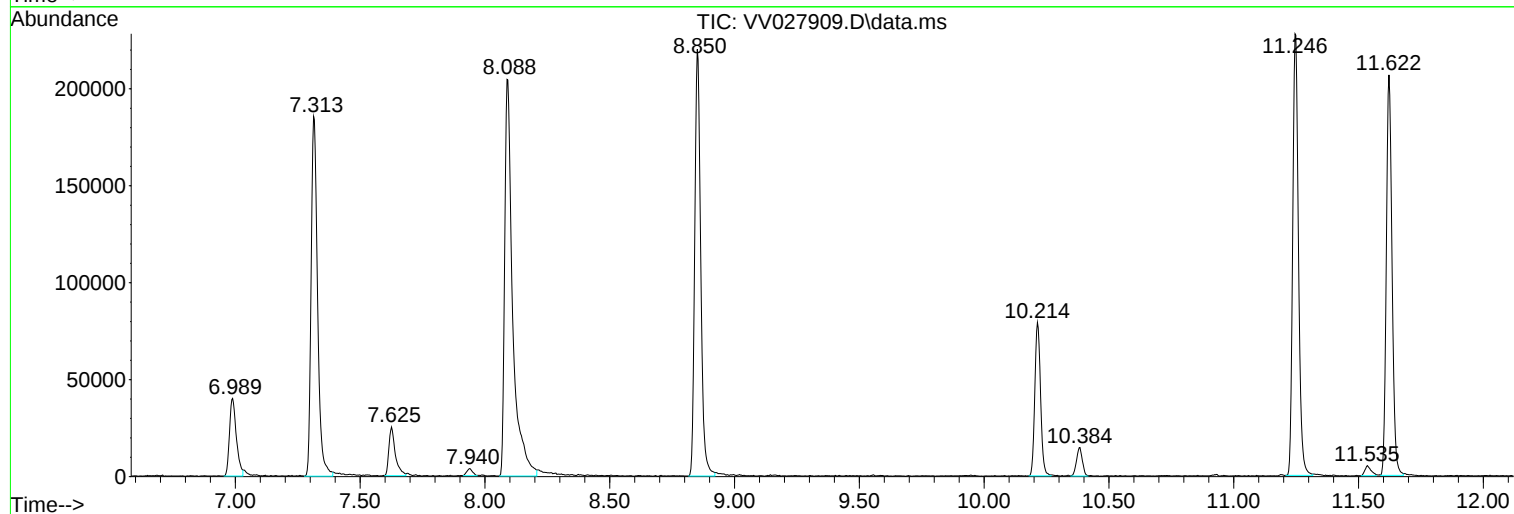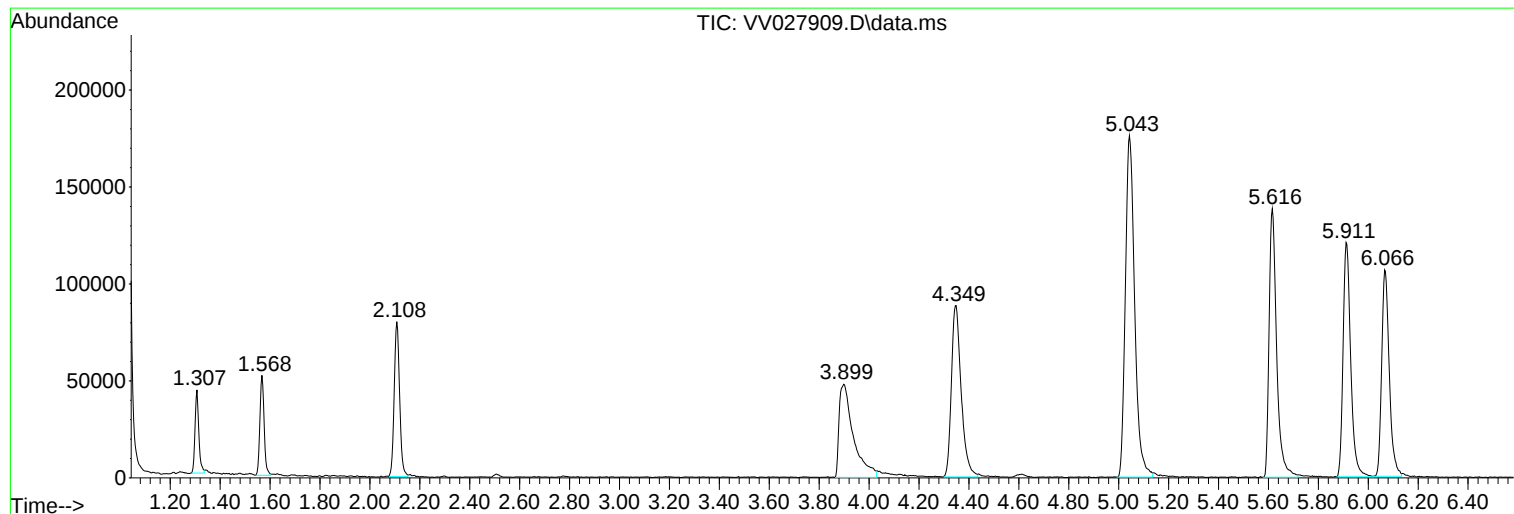

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091722\
Data File : VV027909.D
Acq On : 17 Sep 2022 18:59
Operator : SY/MD
Sample : N4672-10
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0ED7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR091722WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091722\
Data File : VV027909.D
Acq On : 17 Sep 2022 18:59
Operator : SY/MD
Sample : N4672-10
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0ED7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR091722WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc