
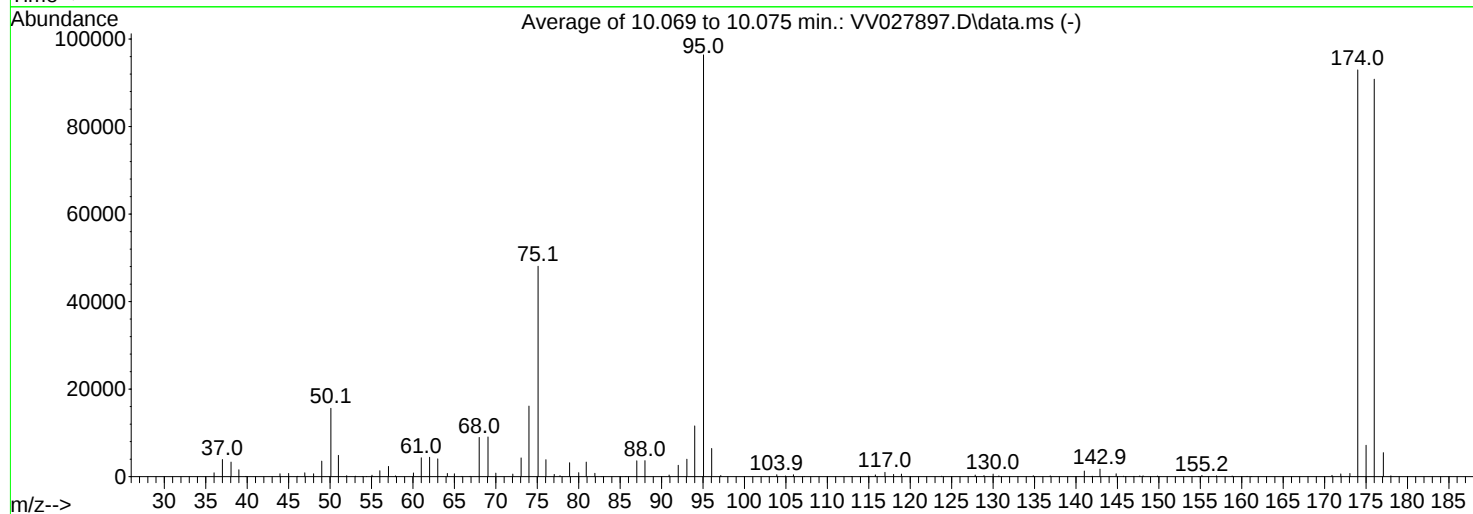


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091722\
Data File : VV027897.D
Acq On : 17 Sep 2022 10:31
Operator : SY/MD
Sample : BFB372
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB372

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR091722WMA.M
Title : TRACE VOA SFAM1.0
Last Update : Mon Sep 19 02:25:21 2022

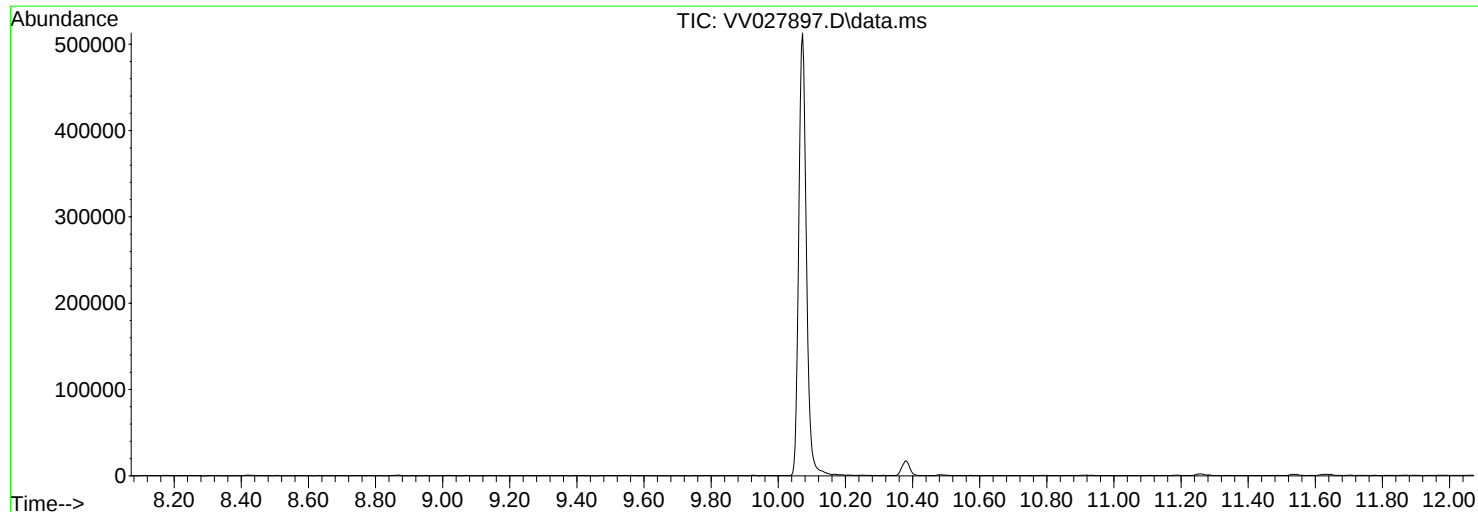

AutoFind: Scans 2808, 2809, 2810; Background Corrected with Scan 2796

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	16.2	15626	PASS
75	95	30	80	49.9	48072	PASS
95	95	100	100	100.0	96395	PASS
96	95	5	9	6.7	6427	PASS
173	174	0.00	2	0.8	725	PASS
174	95	50	120	96.4	92939	PASS
175	174	5	9	7.7	7160	PASS
176	174	95	105	97.7	90843	PASS
177	176	5	10	6.0	5474	PASS

m/z	Abundance
39.80	174.0
44.00	121.0

Instrument :
MSVOA_V
ClientSampleId :
BFB372

m/z	Abundance
36.00	943.0
37.00	3899.0
38.10	3394.0
39.00	1551.0
39.90	246.0
44.00	814.0
45.00	742.0
47.00	960.0
48.00	721.0
49.00	3611.0
50.10	16029.0
51.00	4933.0
52.00	247.0
53.00	114.0
55.10	282.0
56.00	1355.0
57.00	2358.0
57.90	174.0
60.00	871.0
61.00	4290.0
62.00	4376.0
63.00	4231.0
64.20	770.0
65.00	566.0
66.90	173.0
68.00	9083.0
69.10	9165.0
70.00	848.0
72.00	544.0
73.00	4188.0
74.00	16432.0
75.10	48224.0
76.00	3943.0
77.10	485.0
77.70	309.0
78.90	3277.0
80.00	978.0
80.90	3276.0
81.90	712.0
87.00	3693.0
88.00	3317.0
90.90	407.0
92.00	2771.0
93.00	4202.0
94.00	11745.0
95.00	97232.0
96.10	6779.0
97.20	224.0
103.90	406.0
105.00	133.0
105.90	456.0
115.10	110.0
115.80	389.0
116.90	1056.0
118.00	519.0
118.90	518.0
123.80	102.0
127.80	396.0
128.90	222.0
130.00	552.0
130.70	144.0
134.90	192.0
136.80	177.0
140.00	144.0
141.00	1264.0
142.90	1780.0
144.90	685.0
146.00	131.0
147.70	172.0
148.10	197.0
149.80	140.0
155.20	258.0
156.90	181.0
158.80	162.0
161.20	106.0
170.80	306.0
171.90	543.0
173.00	1024.0
174.00	91184.0
175.00	6992.0
176.00	90328.0
177.10	5492.0
178.00	196.0

Instrument :
MSVOA_V
ClientSampleId :
BFB372

m/z	Abundance
36.00	931.0
37.00	4015.0
38.00	3396.0
39.00	1611.0
40.00	246.0
43.90	840.0
45.00	767.0
46.10	131.0
47.00	894.0
48.00	698.0
49.00	3704.0
50.10	16186.0
51.00	5026.0
52.00	205.0
53.10	136.0
54.40	117.0
55.10	332.0
56.00	1399.0
57.00	2395.0
57.90	185.0
60.00	877.0
61.00	4447.0
62.00	4564.0
63.00	4234.0
64.20	751.0
65.00	678.0
65.90	103.0
68.00	9210.0
69.00	9305.0
70.00	824.0
72.00	610.0
73.10	4450.0
74.00	16768.0
75.10	49680.0
76.10	3953.0
77.10	558.0
78.90	3315.0
80.00	923.0
80.90	3426.0
82.00	774.0
82.80	112.0
87.00	3775.0
88.00	3851.0
90.90	380.0
92.00	2648.0
93.10	3997.0
94.00	11865.0
95.10	99824.0
96.00	6593.0
97.10	255.0
103.90	458.0
104.90	136.0
105.90	450.0
107.20	114.0
112.90	120.0
114.90	108.0
115.80	408.0
117.00	1072.0
118.00	545.0
119.00	578.0
123.80	127.0
127.90	369.0
128.90	270.0
130.00	613.0
130.70	181.0
134.80	207.0
136.90	197.0
141.00	1358.0
141.90	158.0
142.90	1782.0
144.80	686.0
145.70	182.0
147.00	109.0
147.70	188.0
148.10	198.0
149.80	164.0
155.20	302.0
157.00	203.0
158.80	164.0
160.60	121.0
170.90	310.0
171.90	664.0
173.10	1152.0
174.00	96088.0
175.00	7431.0
176.00	94016.0
177.10	5593.0
178.00	196.0

Instrument :
MSVOA_V
ClientSampleId :
BFB372

m/z	Abundance
36.00	806.0
37.00	3792.0
38.00	3217.0
39.00	1528.0
40.00	222.0
43.90	693.0
45.00	729.0
46.10	151.0
46.90	815.0
48.00	582.0
49.00	3317.0
50.10	14662.0
51.00	4669.0
52.00	196.0
53.10	121.0
53.90	114.0
55.00	332.0
56.00	1262.0
57.10	2229.0
57.90	152.0
60.10	793.0
61.00	4188.0
62.00	4361.0
63.00	3726.0
64.10	664.0
65.00	689.0
65.90	107.0
68.00	8574.0
69.00	8685.0
70.00	717.0
72.10	603.0
73.00	4163.0
74.00	15179.0
75.10	46312.0
76.10	3750.0
77.00	523.0
77.80	308.0
78.90	3018.0
80.00	799.0
80.90	3273.0
82.00	787.0
83.00	135.0
85.70	111.0
87.00	3378.0
88.00	3775.0
90.90	329.0
92.00	2410.0
93.10	3739.0
94.00	11165.0
95.10	92128.0
96.00	5909.0
97.10	253.0
103.90	447.0
104.90	132.0
105.90	395.0
114.80	120.0
115.80	381.0
117.00	859.0
118.00	499.0
119.00	635.0
123.80	102.0
127.90	383.0
128.90	287.0
130.00	552.0
130.70	206.0
134.90	236.0
137.00	190.0
141.00	1220.0
142.00	149.0
142.90	1644.0
144.00	103.0
144.80	642.0
145.80	183.0
147.00	127.0
147.70	196.0
148.10	157.0
149.90	153.0
154.80	160.0
155.20	282.0
157.00	197.0
158.90	149.0
160.70	122.0
171.00	293.0
172.00	694.0
174.00	91544.0
175.00	7057.0
176.00	88184.0
177.10	5337.0
178.00	191.0

Instrument :
MSVOA_V
ClientSampleId :
BFB372