

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV091824\
 Data File : VV037326.D
 Acq On : 18 Sep 2024 12:08
 Operator : SY/MD
 Sample : P4081-13
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AT1

Quant Time: Sep 19 01:21:38 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR091024WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Thu Sep 19 01:19:52 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.529	114	317589	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.780	117	324815	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.181	152	146941	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.275	65	66849	3.588	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	71.800%
7) Chloroethane-d5	1.529	69	75318	3.877	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	77.600%
11) 1,1-Dichloroethene-d2	2.053	65	35701	3.710	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	74.200%
20) 2-Butanone-d5	3.841	46	226060	40.598	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	81.200%
24) Chloroform-d	4.243	84	183894	4.065	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	81.400%
26) 1,2-Dichloroethane-d4	4.940	65	88558	4.181	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	83.600%
32) Benzene-d6	4.953	84	345104	3.963	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	79.200%
36) 1,2-Dichloropropane-d6	5.985	67	113978	4.208	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	84.200%
41) Toluene-d8	7.239	98	282276	3.597	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	72.000%
43) trans-1,3-Dichloroprop...	7.561	79	29422	3.303	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	66.000%
46) 2-Hexanone-d5	8.030	63	163135	37.480	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	74.960%
56) 1,1,2,2-Tetrachloroeth...	10.149	84	90633	4.106	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	82.200%
66) 1,2-Dichlorobenzene-d4	11.558	152	116554	4.462	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	89.200%
Target Compounds						Qvalue
13) Acetone	2.175	43	102306	26.387	ug/L	74


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV091824\
Data File : VV037326.D
Acq On : 18 Sep 2024 12:08
Operator : SY/MD
Sample : P4081-13
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AT1

Quant Time: Sep 19 01:21:38 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR091024WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Thu Sep 19 01:19:52 2024
Response via : Initial Calibration

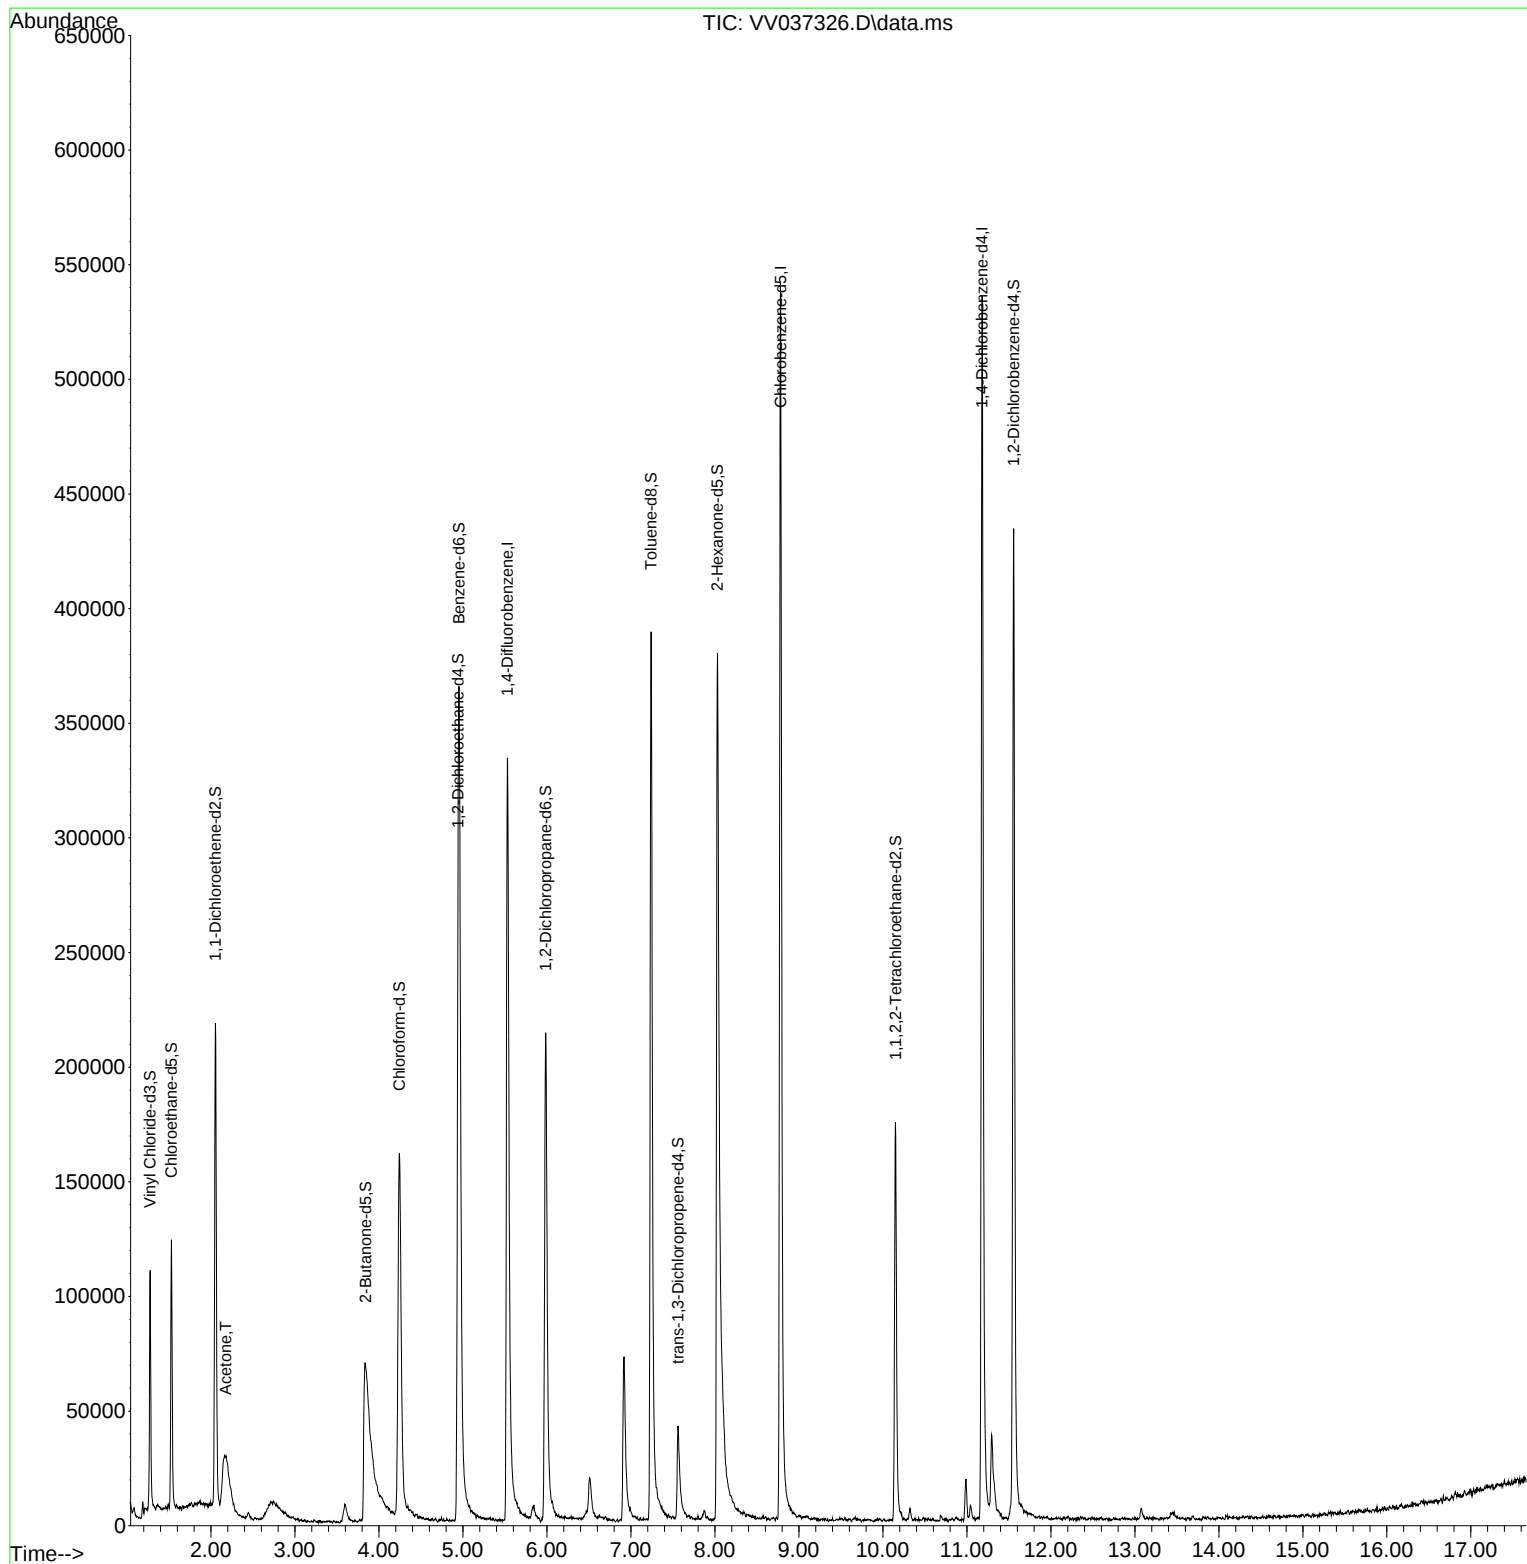

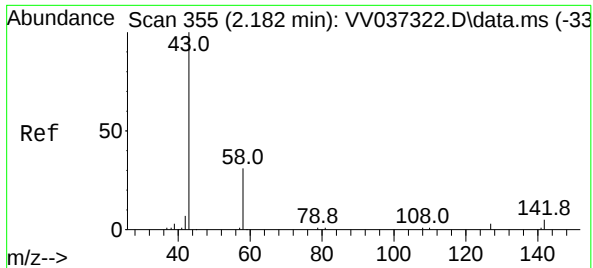

#13
 Acetone
 Concen: 26.387 ug/L
 RT: 2.175 min Scan# 353
 Delta R.T. -0.006 min
 Lab File: VV037326.D
 Acq: 18 Sep 2024 12:08

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AT1

Tgt Ion: 43 Resp: 102306
 Ion Ratio Lower Upper
 43 100
 58 19.7 0.0 69.2

