

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_V\DATA\VV091824\  
 Data File : VV037327.D  
 Acq On : 18 Sep 2024 12:32  
 Operator : SY/MD  
 Sample : P4081-14  
 Misc : 25mL/MSVOA\_V/WATER  
 ALS Vial : 1 Sample Multiplier: 1

Instrument :  
 MSVOA\_V  
 ClientSampleId :  
 C0AX1

Quant Time: Sep 19 01:21:54 2024  
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_V\Method\SFAMVTR091024WMA.M  
 Quant Title : TRACE VOA SFAM1.0  
 QLast Update : Thu Sep 19 01:19:52 2024  
 Response via : Initial Calibration


| Compound                      | R.T.   | QIon  | Response | Conc     | Units  | Dev(Min) |
|-------------------------------|--------|-------|----------|----------|--------|----------|
| -----                         |        |       |          |          |        |          |
| Internal Standards            |        |       |          |          |        |          |
| 1) 1,4-Difluorobenzene        | 5.532  | 114   | 304954   | 5.000    | ug/L   | 0.00     |
| 28) Chlorobenzene-d5          | 8.783  | 117   | 313553   | 5.000    | ug/L   | 0.00     |
| 58) 1,4-Dichlorobenzene-d4    | 11.181 | 152   | 145974   | 5.000    | ug/L   | 0.00     |
| System Monitoring Compounds   |        |       |          |          |        |          |
| 4) Vinyl Chloride-d3          | 1.275  | 65    | 67262    | 3.760    | ug/L   | 0.00     |
| Spiked Amount                 | 5.000  | Range | 40 - 130 | Recovery | =      | 75.200%  |
| 7) Chloroethane-d5            | 1.529  | 69    | 80625    | 4.322    | ug/L   | 0.00     |
| Spiked Amount                 | 5.000  | Range | 65 - 130 | Recovery | =      | 86.400%  |
| 11) 1,1-Dichloroethene-d2     | 2.056  | 65    | 36725    | 3.975    | ug/L   | 0.00     |
| Spiked Amount                 | 5.000  | Range | 60 - 125 | Recovery | =      | 79.400%  |
| 20) 2-Butanone-d5             | 3.812  | 46    | 241314   | 45.133   | ug/L   | -0.03    |
| Spiked Amount                 | 50.000 | Range | 40 - 130 | Recovery | =      | 90.260%  |
| 24) Chloroform-d              | 4.243  | 84    | 195764   | 4.507    | ug/L   | 0.00     |
| Spiked Amount                 | 5.000  | Range | 70 - 125 | Recovery | =      | 90.200%  |
| 26) 1,2-Dichloroethane-d4     | 4.940  | 65    | 94954    | 4.669    | ug/L   | 0.00     |
| Spiked Amount                 | 5.000  | Range | 70 - 130 | Recovery | =      | 93.400%  |
| 32) Benzene-d6                | 4.957  | 84    | 367146   | 4.367    | ug/L   | 0.00     |
| Spiked Amount                 | 5.000  | Range | 70 - 125 | Recovery | =      | 87.400%  |
| 36) 1,2-Dichloropropane-d6    | 5.985  | 67    | 124803   | 4.774    | ug/L   | 0.00     |
| Spiked Amount                 | 5.000  | Range | 60 - 140 | Recovery | =      | 95.400%  |
| 41) Toluene-d8                | 7.239  | 98    | 294967   | 3.894    | ug/L   | 0.00     |
| Spiked Amount                 | 5.000  | Range | 70 - 130 | Recovery | =      | 77.800%  |
| 43) trans-1,3-Dichloroprop... | 7.561  | 79    | 32144    | 3.738    | ug/L   | 0.00     |
| Spiked Amount                 | 5.000  | Range | 55 - 130 | Recovery | =      | 74.800%  |
| 46) 2-Hexanone-d5             | 8.027  | 63    | 174118   | 41.440   | ug/L   | 0.00     |
| Spiked Amount                 | 50.000 | Range | 45 - 130 | Recovery | =      | 82.880%  |
| 56) 1,1,2,2-Tetrachloroeth... | 10.149 | 84    | 96882    | 4.547    | ug/L   | 0.00     |
| Spiked Amount                 | 5.000  | Range | 65 - 120 | Recovery | =      | 91.000%  |
| 66) 1,2-Dichlorobenzene-d4    | 11.558 | 152   | 122861   | 4.734    | ug/L   | 0.00     |
| Spiked Amount                 | 5.000  | Range | 80 - 120 | Recovery | =      | 94.600%  |
| Target Compounds              |        |       |          |          |        |          |
|                               |        |       |          |          | Qvalue |          |
| 13) Acetone                   | 2.146  | 43    | 122644   | 32.943   | ug/L   | 96       |
| -----                         |        |       |          |          |        |          |


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_V\DATA\VV091824\  
Data File : VV037327.D  
Acq On : 18 Sep 2024 12:32  
Operator : SY/MD  
Sample : P4081-14  
Misc : 25mL/MSVOA\_V/WATER  
ALS Vial : 1 Sample Multiplier: 1

Instrument :  
MSVOA\_V  
ClientSampleId :  
C0AX1

Quant Time: Sep 19 01:21:54 2024  
Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_V\Method\SFAMVTR091024WMA.M  
Quant Title : TRACE VOA SFAM1.0  
QLast Update : Thu Sep 19 01:19:52 2024  
Response via : Initial Calibration

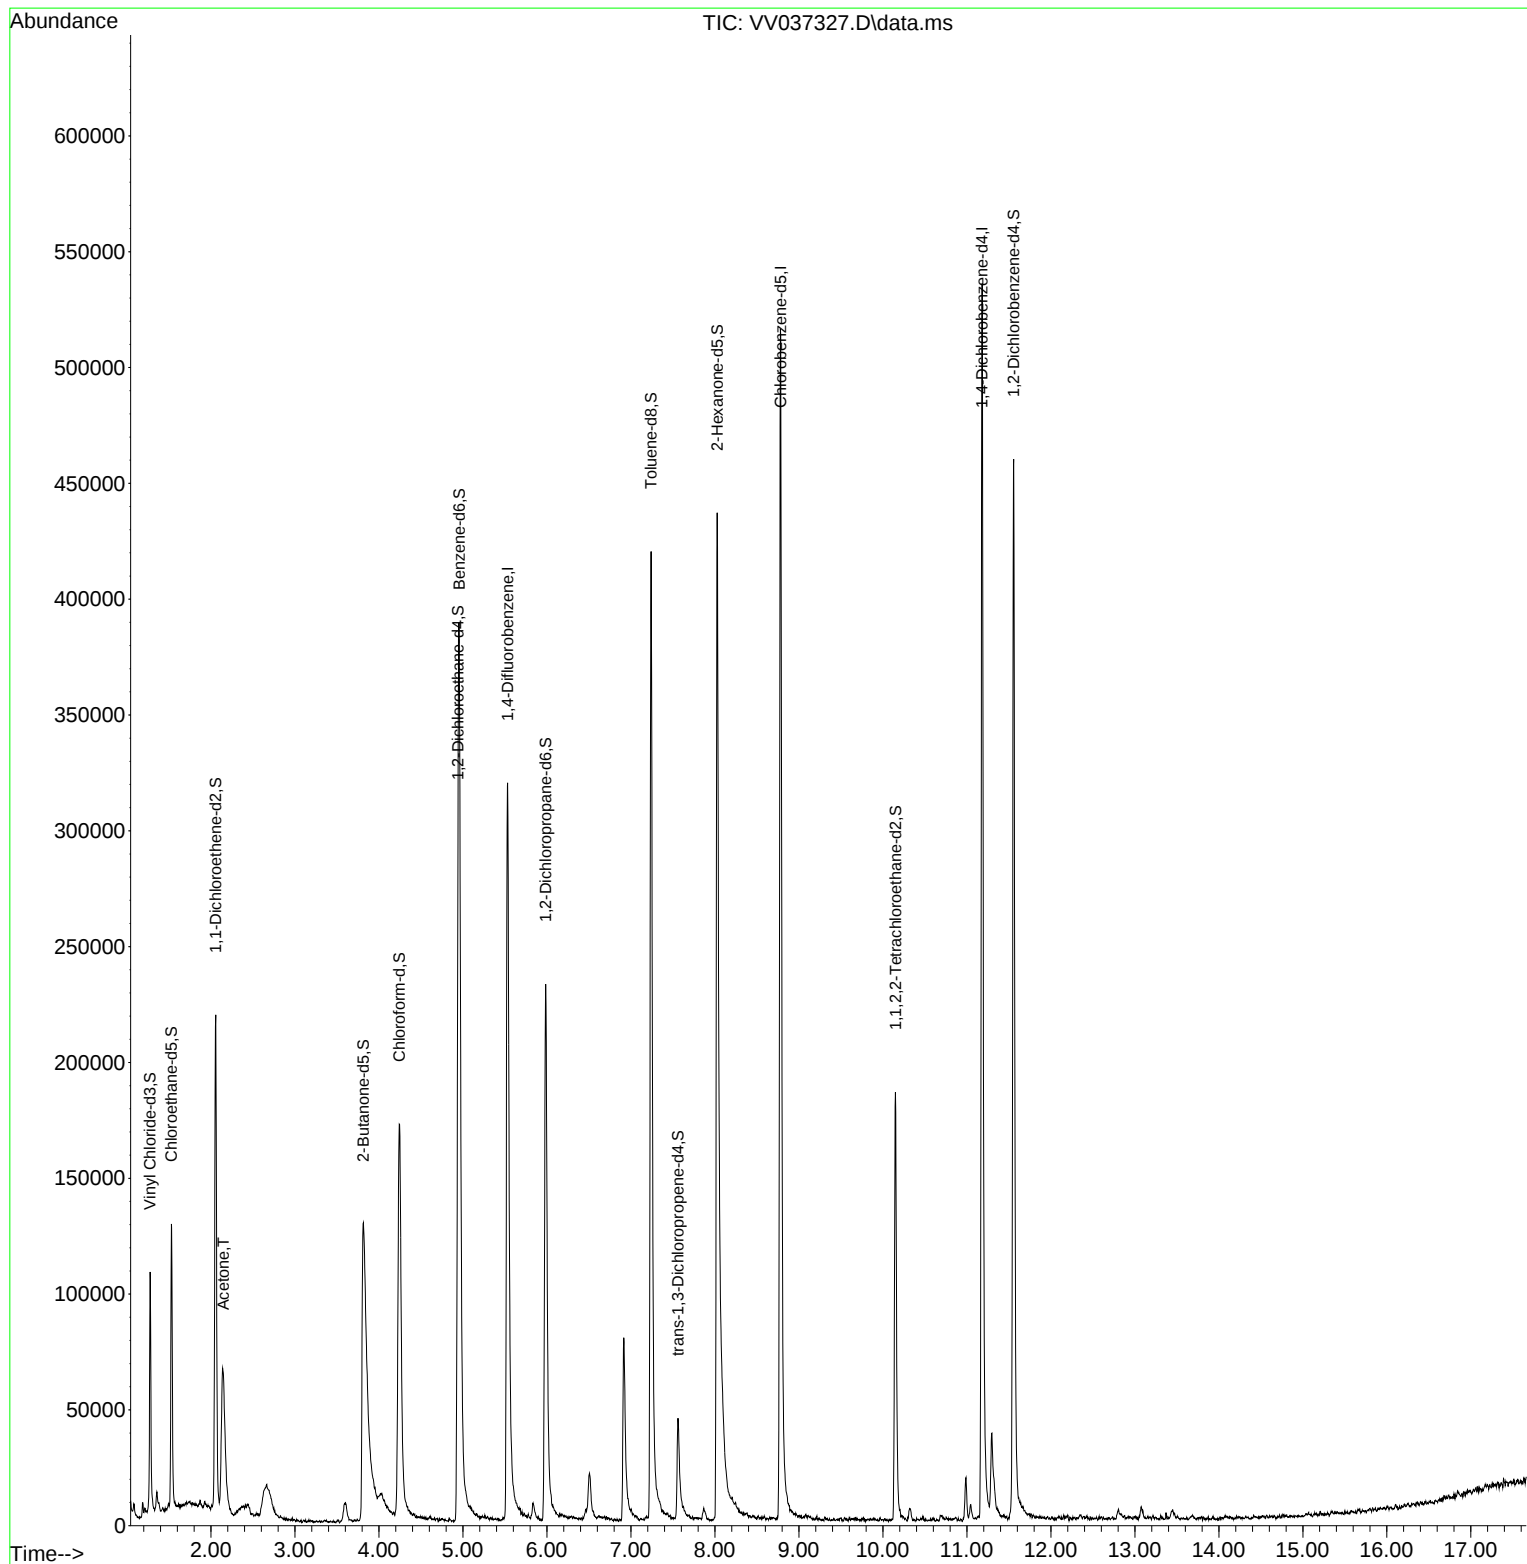

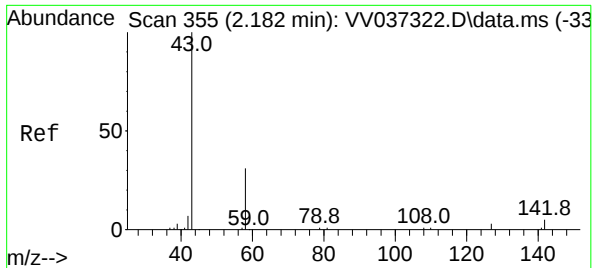

#13  
 Acetone  
 Concen: 32.943 ug/L  
 RT: 2.146 min Scan# 34  
 Delta R.T. -0.035 min  
 Lab File: VV037327.D  
 Acq: 18 Sep 2024 12:32

Instrument :  
 MSVOA\_V  
 ClientSampleId :  
 C0AX1

Tgt Ion: 43 Resp: 122644  
 Ion Ratio Lower Upper  
 43 100  
 58 32.3 0.0 69.2

