

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV091824\
 Data File : VV037329.D
 Acq On : 18 Sep 2024 13:20
 Operator : SY/MD
 Sample : P4081-16
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AX4

Quant Time: Sep 19 01:22:19 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR091024WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Thu Sep 19 01:19:52 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.532	114	307088	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.783	117	317023	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.181	152	145105	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.275	65	66634	3.699	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	74.000%
7) Chloroethane-d5	1.529	69	80673	4.295	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	85.800%
11) 1,1-Dichloroethene-d2	2.053	65	36180	3.889	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	77.800%
20) 2-Butanone-d5	3.857	46	263388	48.919	ug/L	0.01
Spiked Amount	50.000	Range	40 - 130	Recovery	=	97.840%
24) Chloroform-d	4.243	84	201114	4.598	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	92.000%
26) 1,2-Dichloroethane-d4	4.941	65	95224	4.649	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	93.000%
32) Benzene-d6	4.953	84	370137	4.355	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	87.000%
36) 1,2-Dichloropropane-d6	5.986	67	124189	4.698	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	94.000%
41) Toluene-d8	7.240	98	303158	3.958	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	79.200%
43) trans-1,3-Dichloroprop...	7.561	79	33871	3.895	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	78.000%
46) 2-Hexanone-d5	8.030	63	181591	42.746	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	85.500%
56) 1,1,2,2-Tetrachloroeth...	10.149	84	99328	4.611	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	92.200%
66) 1,2-Dichlorobenzene-d4	11.558	152	122481	4.748	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	95.000%
Target Compounds						
16) Methylene chloride	2.442	84	15351	0.620	ug/L	Qvalue 96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV091824\
Data File : VV037329.D
Acq On : 18 Sep 2024 13:20
Operator : SY/MD
Sample : P4081-16
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AX4


Quant Time: Sep 19 01:22:19 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR091024WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Thu Sep 19 01:19:52 2024
Response via : Initial Calibration

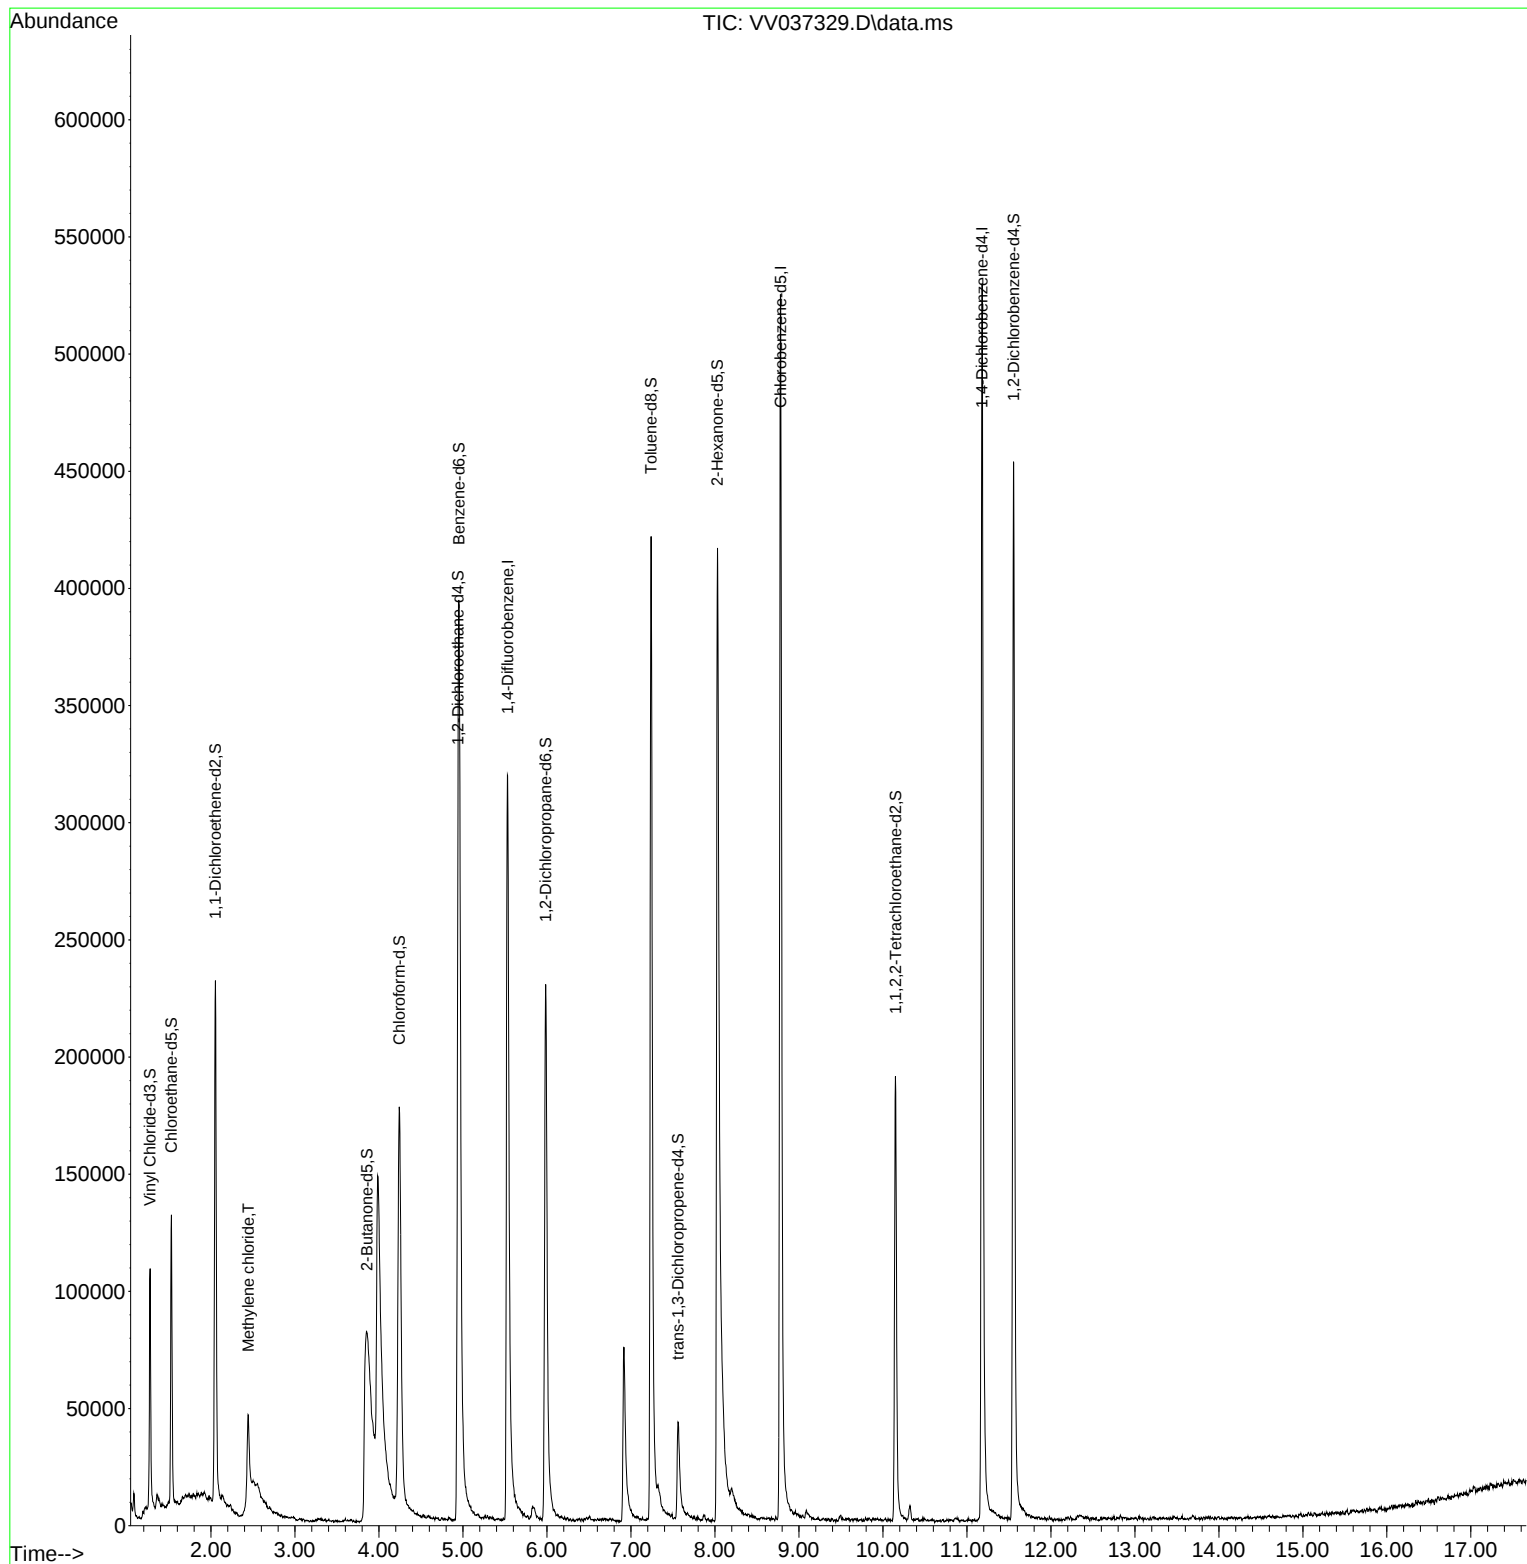

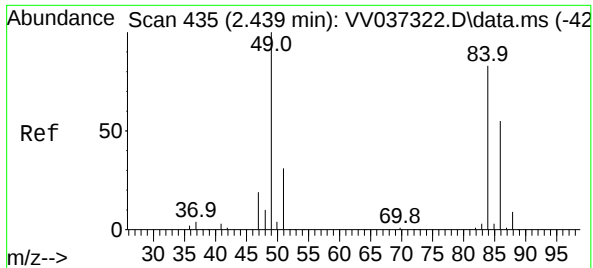

#16
Methylene chloride
Concen: 0.620 ug/L
RT: 2.442 min Scan# 41
Delta R.T. 0.003 min
Lab File: VV037329.D
Acq: 18 Sep 2024 13:20

Instrument :
MSVOA_V
ClientSampleId :
C0AX4

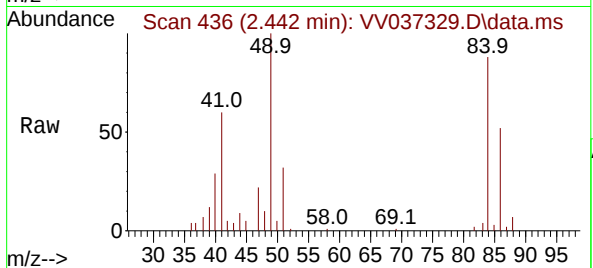

Tgt Ion:	84	Resp:	15351
Ion	Ratio	Lower	Upper
84	100		
86	58.9	44.0	81.8
49	114.1	83.0	154.1

