

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV091824\
 Data File : VV037362.D
 Acq On : 19 Sep 2024 04:39
 Operator : SY/MD
 Sample : P3986-06
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BH8M6

Quant Time: Sep 19 05:00:33 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR091024WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Thu Sep 19 02:54:38 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.529	114	314411	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.779	117	348516	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.181	152	154378	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.275	65	104468	5.663	ug/L	0.00
Spiked Amount	5.000	Range 40 - 130	Recovery	=	113.200%	
7) Chloroethane-d5	1.529	69	90231	4.692	ug/L	0.00
Spiked Amount	5.000	Range 65 - 130	Recovery	=	93.800%	
11) 1,1-Dichloroethene-d2	2.053	65	45881	4.816	ug/L	0.00
Spiked Amount	5.000	Range 60 - 125	Recovery	=	96.400%	
20) 2-Butanone-d5	3.815	46	252253	45.759	ug/L	0.01
Spiked Amount	50.000	Range 40 - 130	Recovery	=	91.520%	
24) Chloroform-d	4.239	84	206869	4.619	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	92.400%	
26) 1,2-Dichloroethane-d4	4.937	65	100121	4.775	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	95.400%	
32) Benzene-d6	4.953	84	396720	4.246	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	85.000%	
36) 1,2-Dichloropropane-d6	5.982	67	135808	4.673	ug/L	0.00
Spiked Amount	5.000	Range 60 - 140	Recovery	=	93.400%	
41) Toluene-d8	7.239	98	347566	4.128	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	82.600%	
43) trans-1,3-Dichloroprop...	7.554	79	36500	3.818	ug/L	0.00
Spiked Amount	5.000	Range 55 - 130	Recovery	=	76.400%	
46) 2-Hexanone-d5	8.024	63	234010	50.107	ug/L	0.00
Spiked Amount	50.000	Range 45 - 130	Recovery	=	100.220%	
56) 1,1,2,2-Tetrachloroeth...	10.146	84	108721	4.591	ug/L	0.00
Spiked Amount	5.000	Range 65 - 120	Recovery	=	91.800%	
66) 1,2-Dichlorobenzene-d4	11.554	152	133410	4.861	ug/L	0.00
Spiked Amount	5.000	Range 80 - 120	Recovery	=	97.200%	
Target Compounds					Qvalue	
25) Chloroform	4.268	83	50386	1.130	ug/L	94


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV091824\
Data File : VV037362.D
Acq On : 19 Sep 2024 04:39
Operator : SY/MD
Sample : P3986-06
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BH8M6

Quant Time: Sep 19 05:00:33 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR091024WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Thu Sep 19 02:54:38 2024
Response via : Initial Calibration

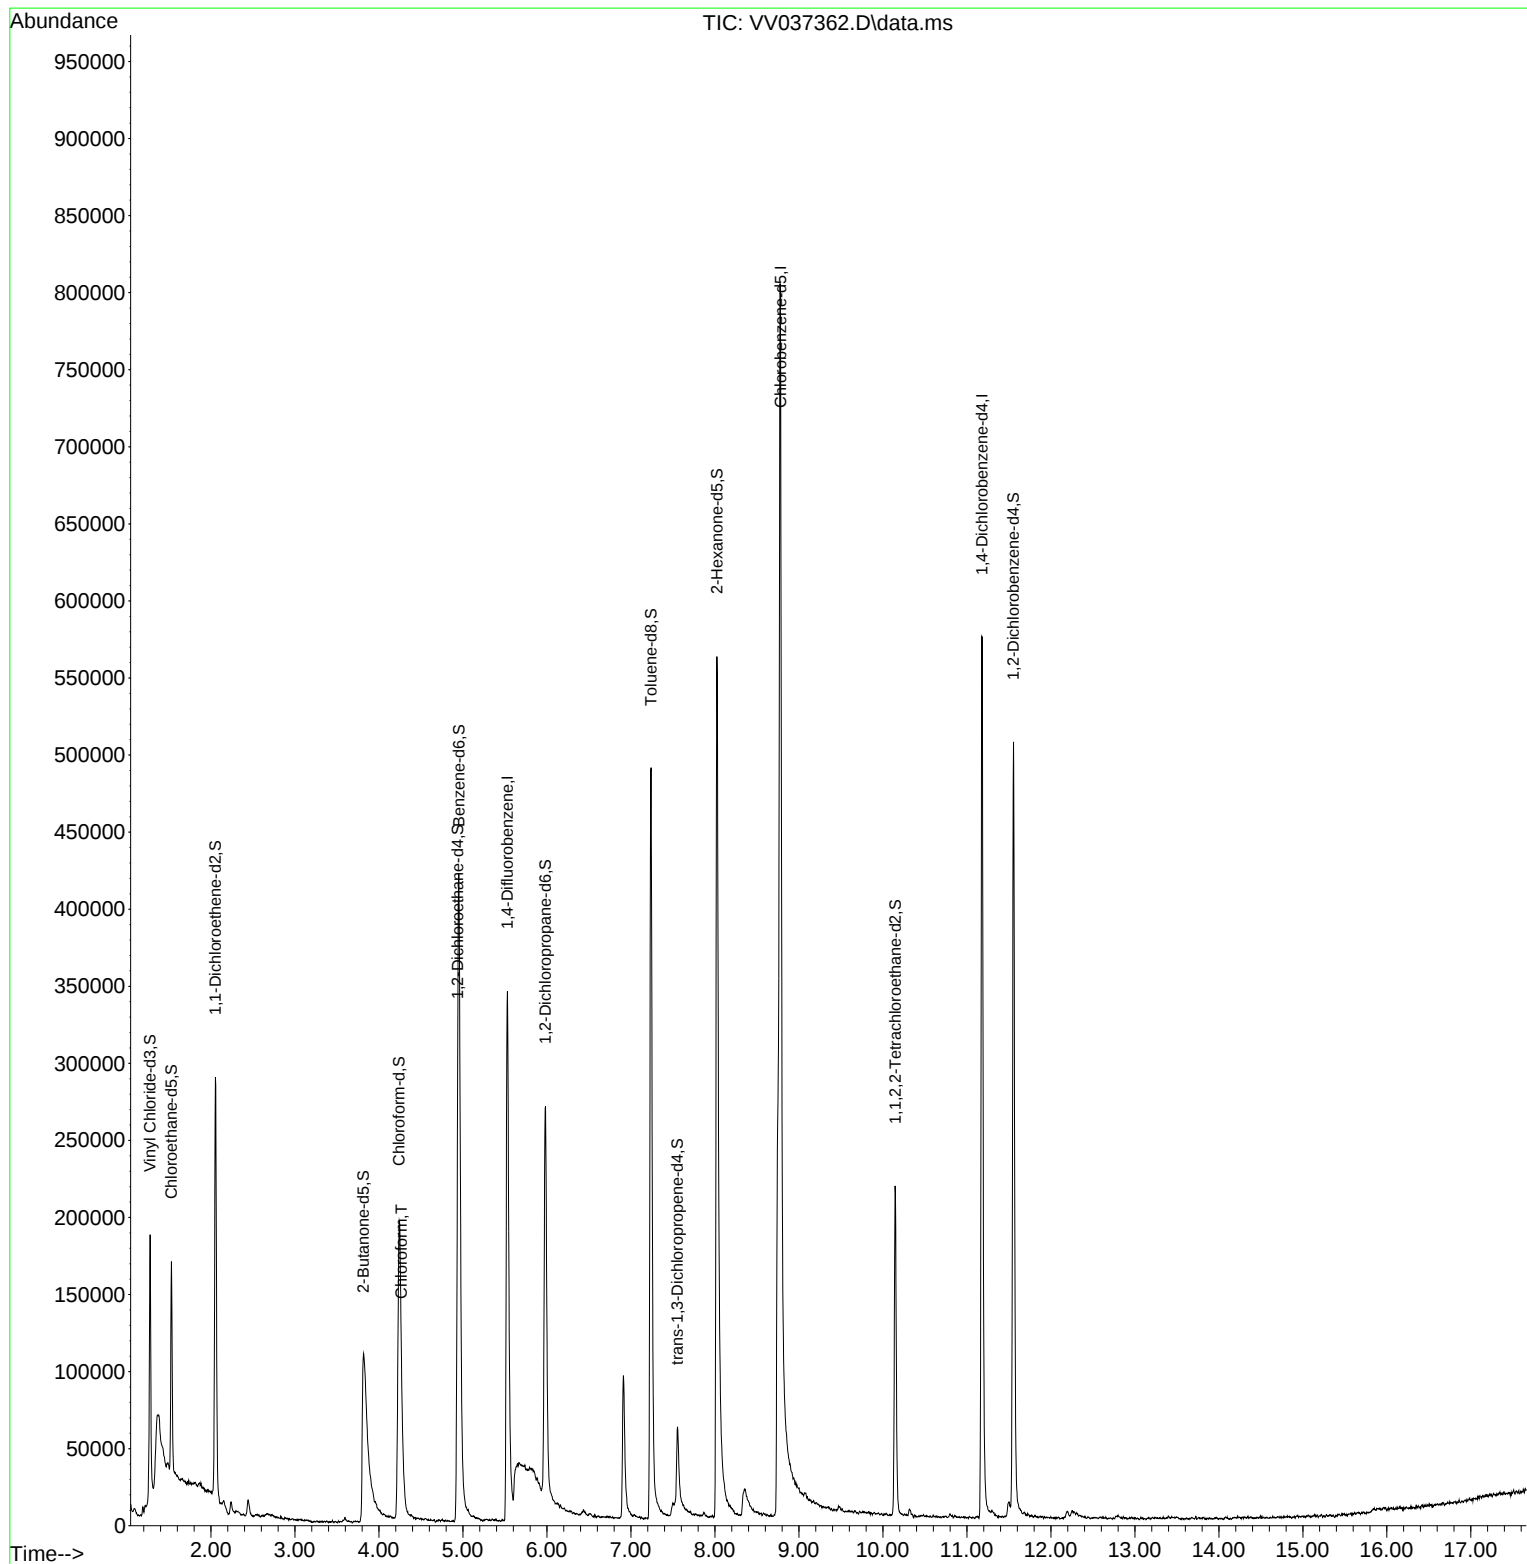

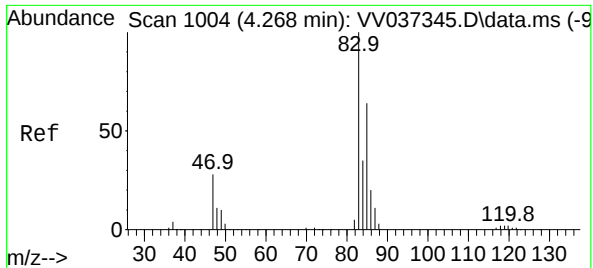

#25
 Chloroform
 Concen: 1.130 ug/L
 RT: 4.268 min Scan# 1
 Delta R.T. -0.000 min
 Lab File: VV037362.D
 Acq: 19 Sep 2024 04:39

Instrument :
 MSVOA_V
 ClientSampleId :
 BH8M6

Tgt Ion: 83 Resp: 50386
 Ion Ratio Lower Upper
 83 100
 85 67.3 43.8 81.4

