

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV091824\
 Data File : VV037363.D
 Acq On : 19 Sep 2024 05:03
 Operator : SY/MD
 Sample : P3986-07
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BH8M7

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR091024WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV037363.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.275	63	73	87	rBV2	175736	237413	14.52%	2.276%
2	1.378	91	105	115	rBV3	33656	112928	6.91%	1.083%
3	1.529	146	152	165	rVB	137678	162298	9.93%	1.556%
4	2.056	306	316	332	rVB	270628	406574	24.87%	3.898%
5	2.442	428	436	449	rVB3	9993	17758	1.09%	0.170%
6	3.815	849	863	902	rBV2	107064	455174	27.84%	4.364%
7	4.243	979	996	1034	rBV2	190160	589592	36.07%	5.653%
8	4.950	1201	1216	1245	rBV2	416471	1079010	66.01%	10.346%
9	5.529	1385	1396	1429	rBV	326997	726981	44.47%	6.971%
10	5.693	1436	1447	1448	rBV10	13427	21325	1.30%	0.204%
11	5.982	1525	1537	1562	rVB	243838	522491	31.96%	5.010%
12	6.911	1816	1826	1848	rBV	87278	181969	11.13%	1.745%
13	7.239	1915	1928	1950	rBV	478971	891220	54.52%	8.545%
14	7.558	2017	2027	2042	rBV2	51731	113825	6.96%	1.091%
15	8.024	2162	2172	2217	rBV	537349	1222552	74.79%	11.722%
16	8.779	2391	2407	2456	rBV2	675695	1634677	100.00%	15.674%
17	10.149	2820	2833	2854	rBV	205459	339352	20.76%	3.254%
18	11.181	3143	3154	3178	rBV	547875	908166	55.56%	8.708%
19	11.554	3259	3270	3291	rVV	486477	805890	49.30%	7.727%




Sum of corrected areas: 10429195

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV091824\
Data File : VV037363.D
Acq On : 19 Sep 2024 05:03
Operator : SY/MD
Sample : P3986-07
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BH8M7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR091024WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

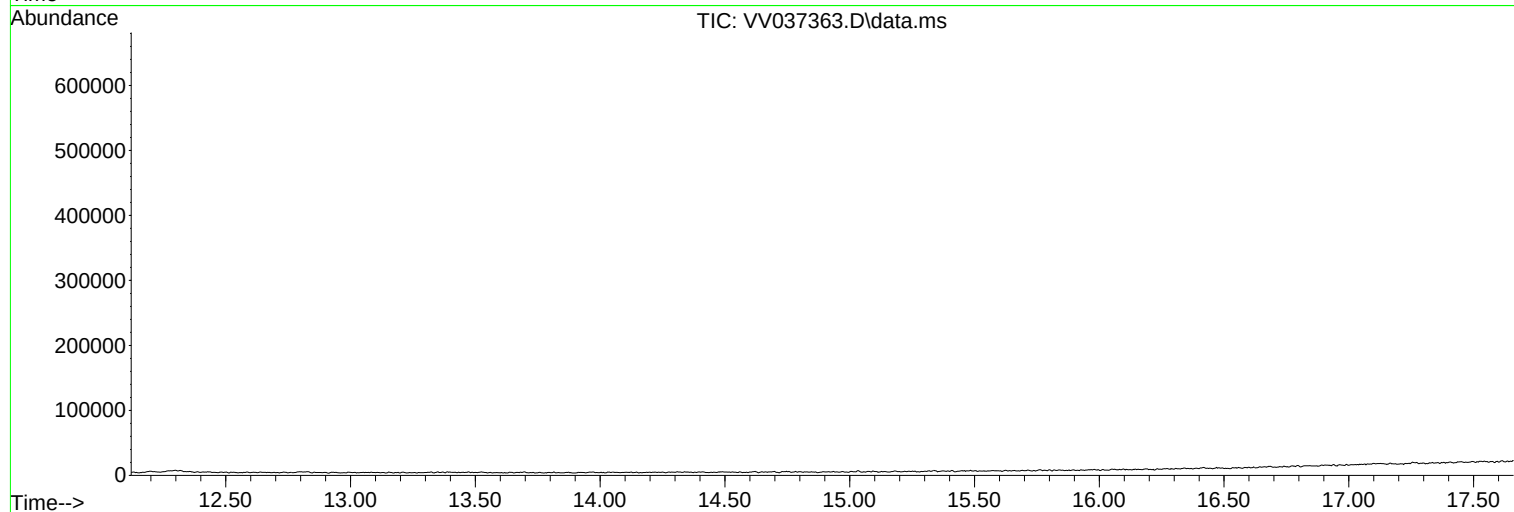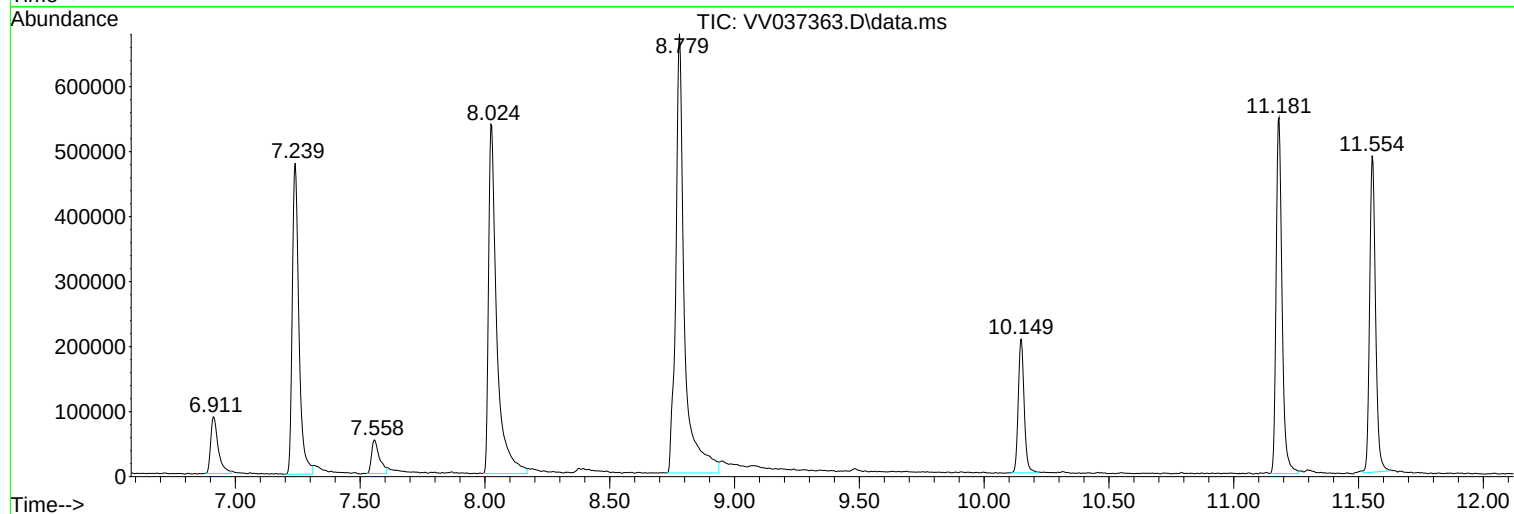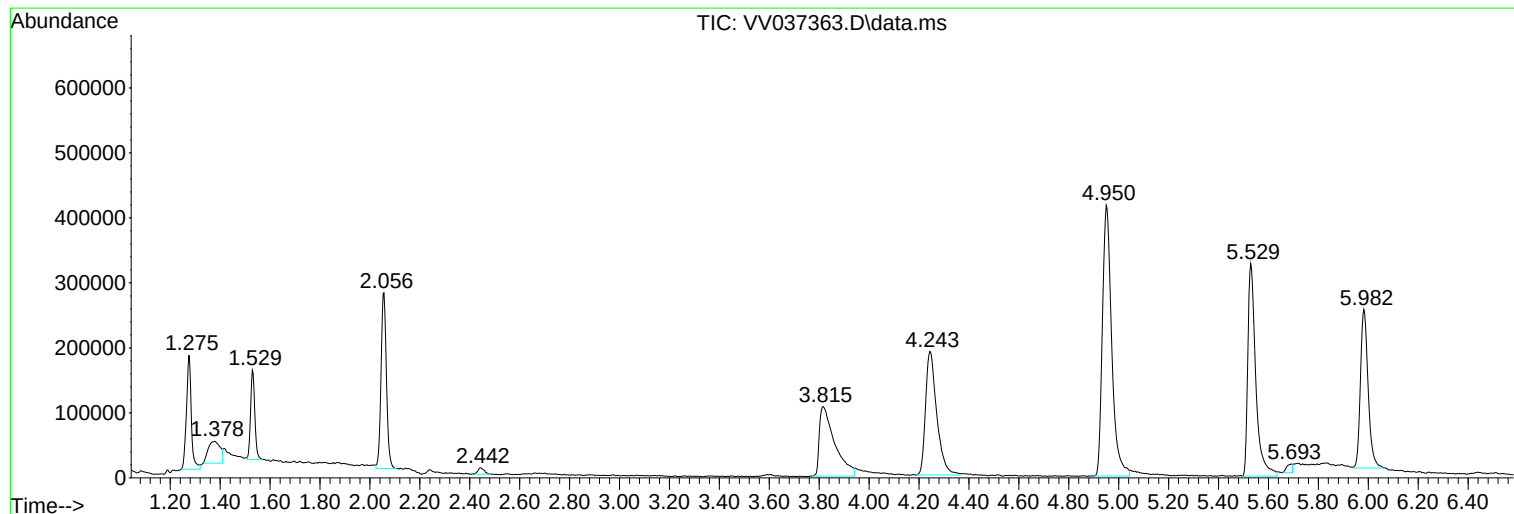

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV091824\
Data File : VV037363.D
Acq On : 19 Sep 2024 05:03
Operator : SY/MD
Sample : P3986-07
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BH8M7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR091024WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Sulfur dioxide	1.378	0.8	ug/L	112928	1	5.529	726981	5.0