




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV092024\
Data File : VV037460.D
Acq On : 21 Sep 2024 03:19
Operator : SY/MD
Sample : P4130-01
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
H0HH7

Manual IntegrationsAPPROVED

Quant Time: Sep 21 04:55:39 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR091024WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Sat Sep 21 01:15:22 2024
Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 09/23/2024
Supervised By :Semsettin Yesilyurt 09/23/2024

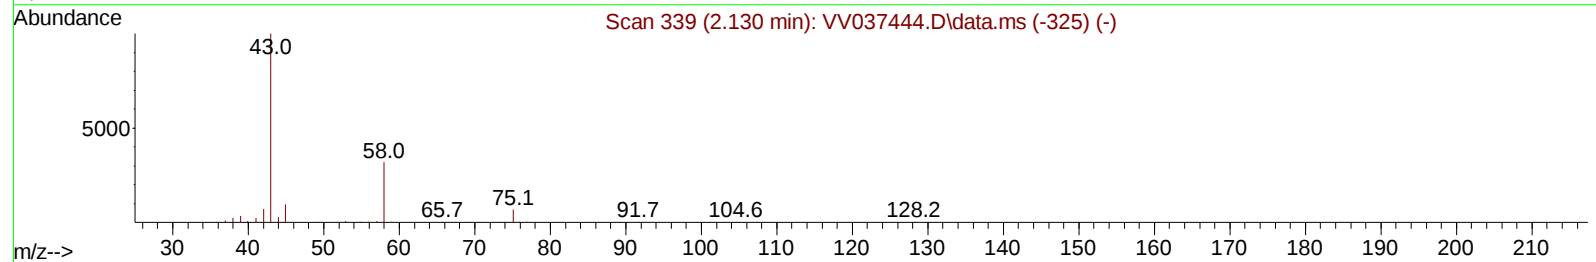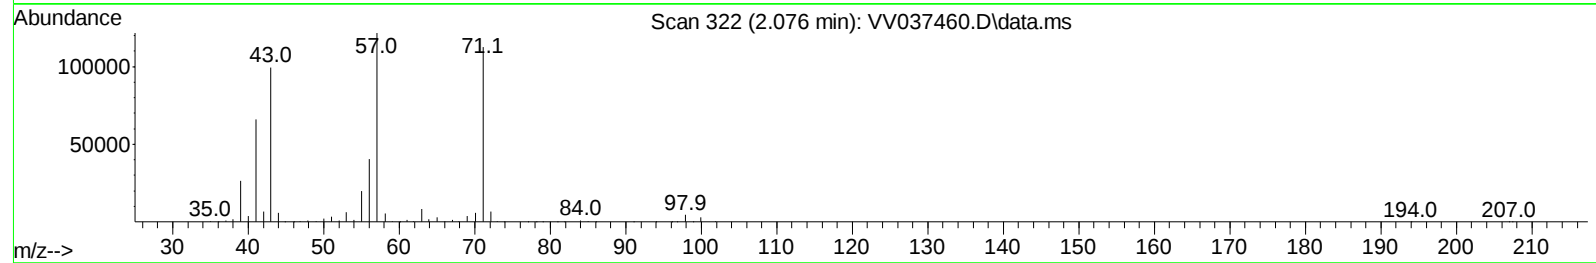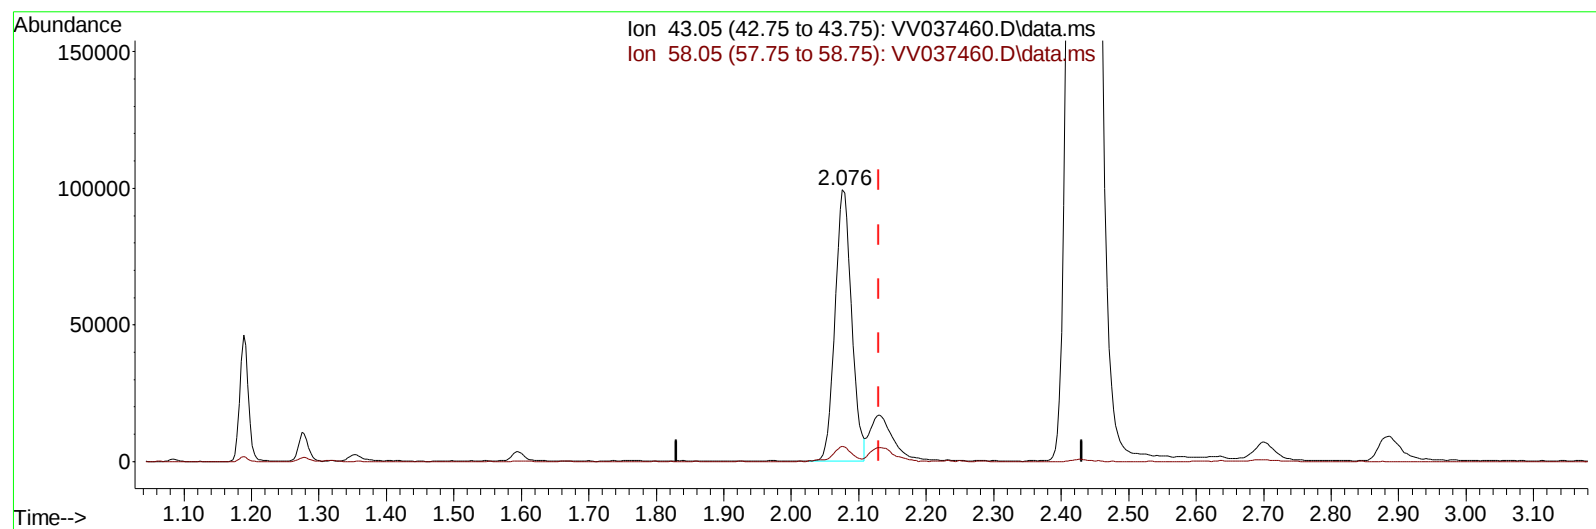

TIC: VV037460.D\data.ms

(13) Acetone (T)

2.076min (-0.055) 45.72 ug/L

response 170044

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	34.60	6.28
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV092024\
Data File : VV037460.D
Acq On : 21 Sep 2024 03:19
Operator : SY/MD
Sample : P4130-01
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
H0HH7

Manual IntegrationsAPPROVED

Quant Time: Sep 21 04:55:39 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR091024WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Sat Sep 21 01:15:22 2024
Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 09/23/2024
Supervised By :Semsettin Yesilyurt 09/23/2024

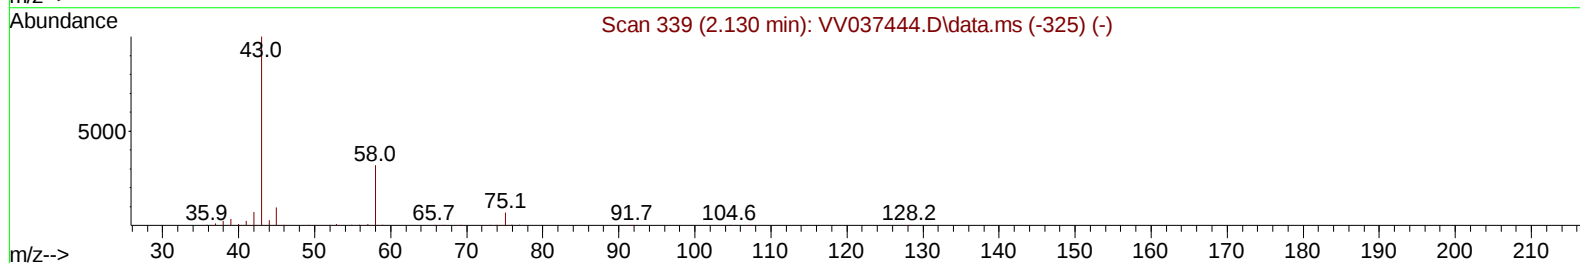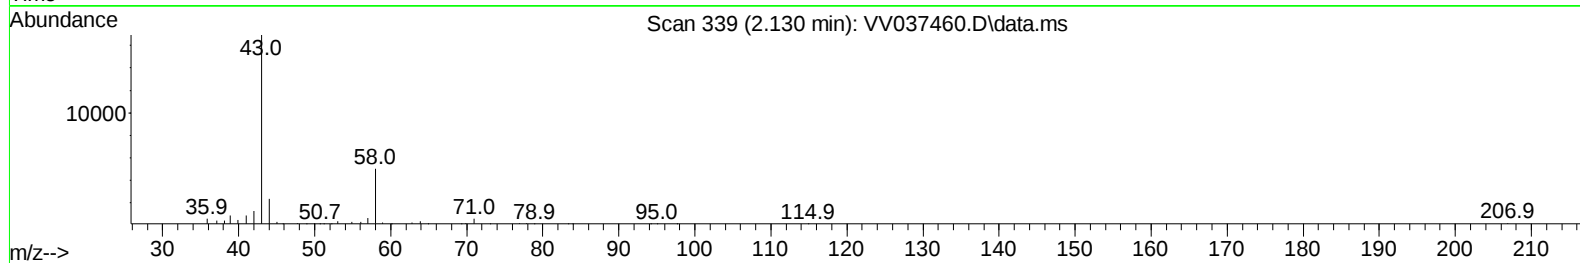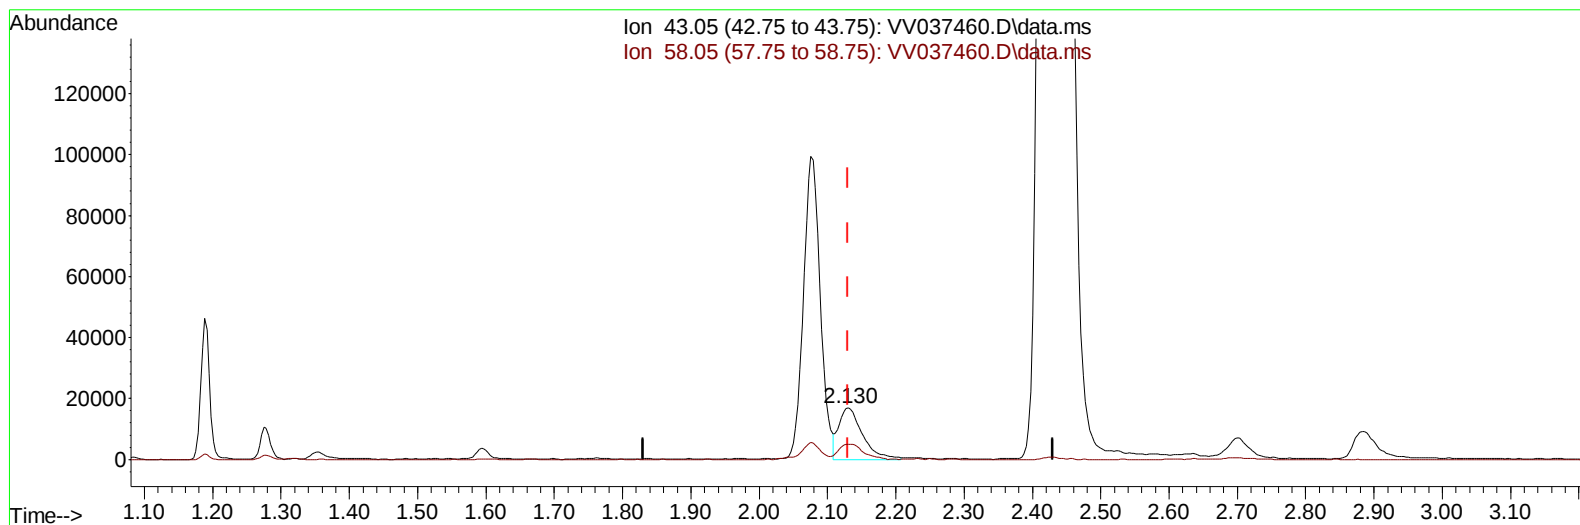

TIC: VV037460.D\data.ms

(13) Acetone (T)

2.130min (+ 0.000) 11.11 ug/L m

response 41315

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	34.60	25.86
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV092024\
Data File : VV037460.D
Acq On : 21 Sep 2024 03:19
Operator : SY/MD
Sample : P4130-01
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
H0HH7

Manual IntegrationsAPPROVED

Quant Time: Sep 21 04:55:39 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR091024WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Sat Sep 21 01:15:22 2024
Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 09/23/2024
Supervised By :Semsettin Yesilyurt 09/23/2024

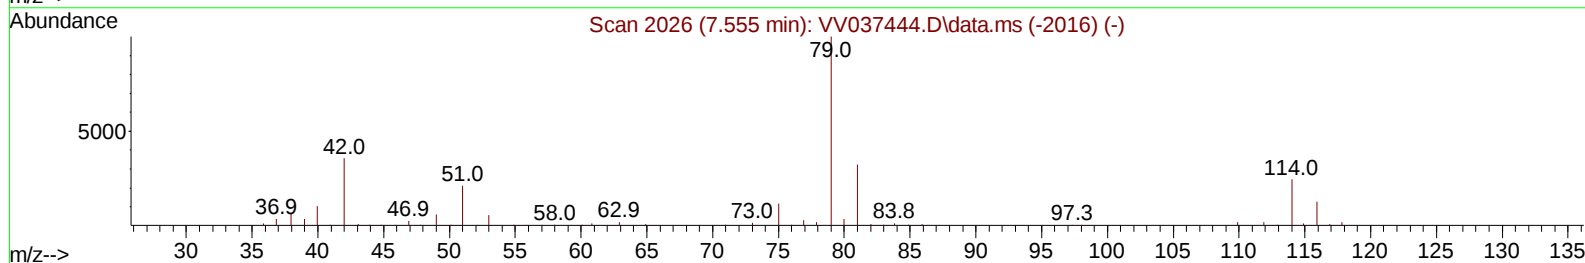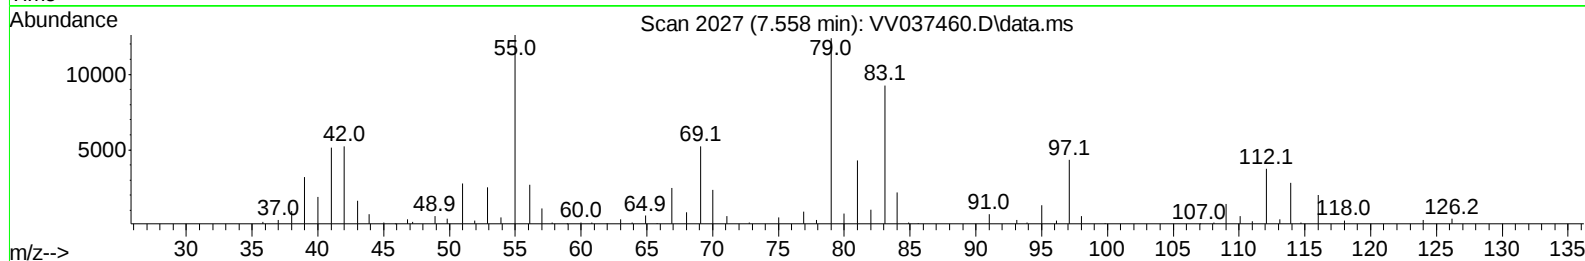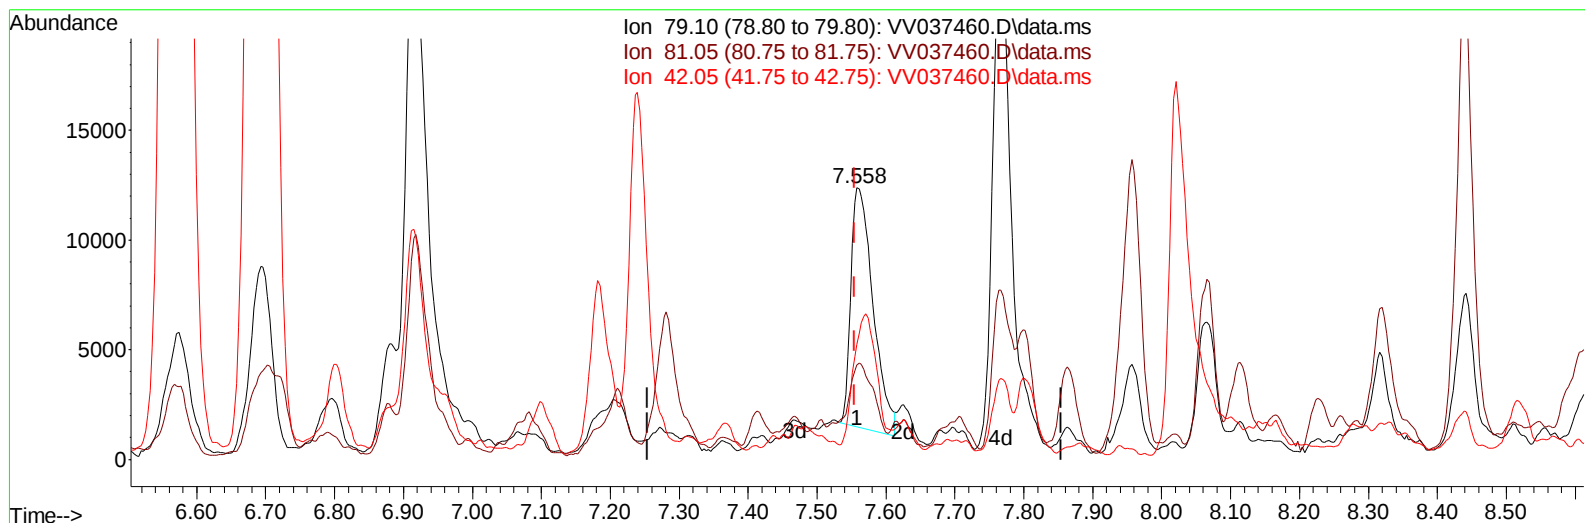

TIC: VV037460.D\data.ms

(43) trans-1,3-Dichloropropene-d4 (S)

7.558min (+ 0.003) 2.71 ug/L

response 24346

Ion	Exp%	Act%
79.10	100.00	100.00
81.05	33.90	31.93
42.05	38.70	56.49#
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV092024\
Data File : VV037460.D
Acq On : 21 Sep 2024 03:19
Operator : SY/MD
Sample : P4130-01
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
H0HH7

Manual IntegrationsAPPROVED

Quant Time: Sep 21 04:55:39 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR091024WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Sat Sep 21 01:15:22 2024
Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 09/23/2024
Supervised By :Semsettin Yesilyurt 09/23/2024

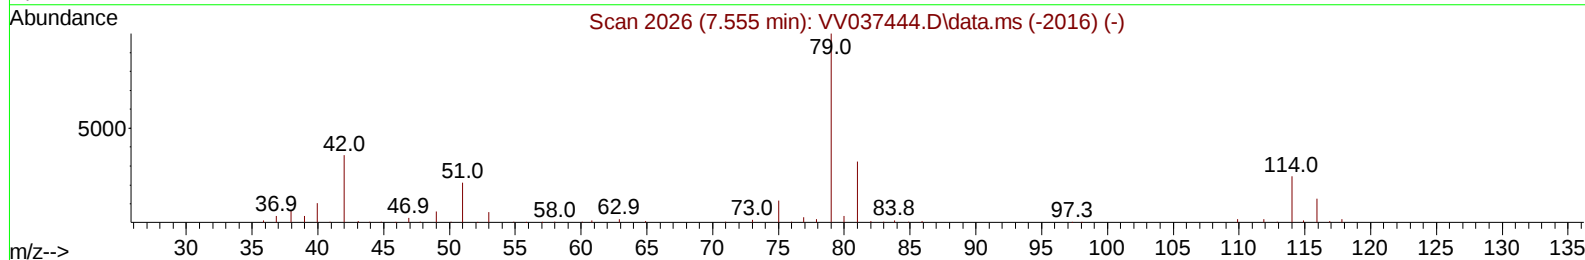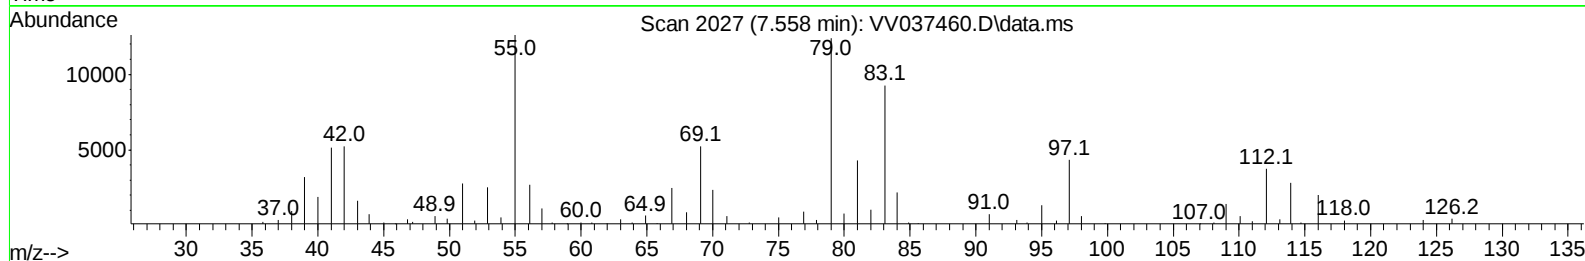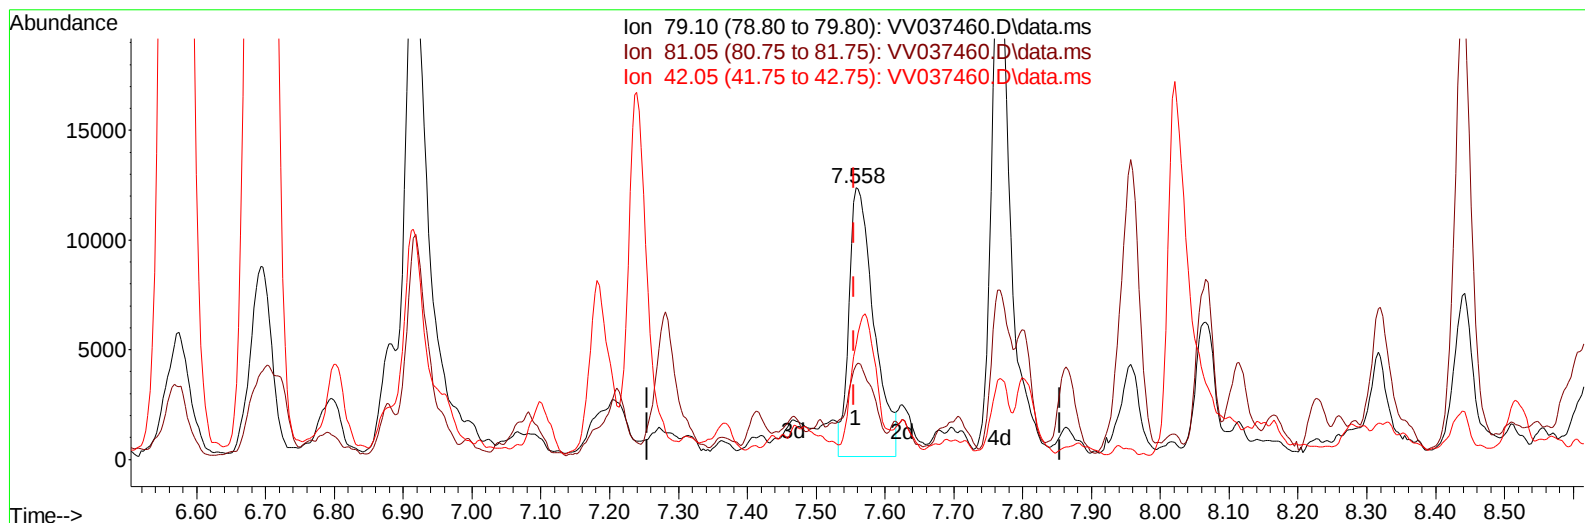

TIC: VV037460.D\data.ms

(43) trans-1,3-Dichloropropene-d4 (S)

7.558min (+ 0.003) 3.41 ug/L m

response 30635

Ion	Exp%	Act%
79.10	100.00	100.00
81.05	33.90	25.37
42.05	38.70	44.89
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV092024\
 Data File : VV037460.D
 Acq On : 21 Sep 2024 03:19
 Operator : SY/MD
 Sample : P4130-01
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 H0HH7

Manual IntegrationsAPPROVED

Quant Time: Sep 21 04:55:39 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR091024WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Sat Sep 21 01:15:22 2024
 Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 09/23/2024
 Supervised By :Semsettin Yesilyurt 09/23/2024

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Difluorobenzene	5.529	114		304679	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.780	117		327599	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.181	152		158431	5.000	ug/L	0.00
System Monitoring Compounds							
4) Vinyl Chloride-d3	1.275	65		54086	3.026	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	60.600%	
7) Chloroethane-d5	1.529	69		70700	3.794	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	75.800%	
11) 1,1-Dichloroethene-d2	2.053	65		31752	3.440	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	68.800%	
20) 2-Butanone-d5	3.799	46		269275	50.408	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	100.820%	
24) Chloroform-d	4.243	84		185348	4.271	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	85.400%	
26) 1,2-Dichloroethane-d4	4.937	65		90221	4.440	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	88.800%	
32) Benzene-d6	4.953	84		342462	3.899	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	78.000%	
36) 1,2-Dichloropropane-d6	5.982	67		125956	4.611	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	92.200%	
41) Toluene-d8	7.239	98		304601	3.849	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	77.000%	
43) trans-1,3-Dichloroprop...	7.558	79		30635m	3.410	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	68.200%	
46) 2-Hexanone-d5	8.021	63		227288	51.775	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	103.560%	
56) 1,1,2,2-Tetrachloroeth...	10.149	84		104183	4.680	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	93.600%	
66) 1,2-Dichlorobenzene-d4	11.558	152		126831	4.503	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	90.000%	
Target Compounds							
13) Acetone	2.130	43		41315m	11.108	ug/L	
17) Methyl tert-butyl Ether	2.699	73		75581	1.489	ug/L #	79
27) 1,2-Dichloroethane	5.040	62		72774	2.976	ug/L #	91

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV092024\
Data File : VV037460.D
Acq On : 21 Sep 2024 03:19
Operator : SY/MD
Sample : P4130-01
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
H0HH7

Manual IntegrationsAPPROVED

Quant Time: Sep 21 04:55:39 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR091024WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Sat Sep 21 01:15:22 2024
Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 09/23/2024
Supervised By :Semsettin Yesilyurt 09/23/2024

