

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV092024\
 Data File : VV037433.D
 Acq On : 20 Sep 2024 15:25
 Operator : SY/MD
 Sample : P3990-07
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AM9

Quant Time: Sep 20 23:36:50 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR091024WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Sep 20 23:32:27 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.532	114	284473	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.783	117	285611	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.182	152	137148	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.275	65	55528	3.327	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	66.600%
7) Chloroethane-d5	1.529	69	73444	4.221	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	84.400%
11) 1,1-Dichloroethene-d2	2.056	65	33000	3.829	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	76.600%
20) 2-Butanone-d5	3.799	46	259355	51.999	ug/L	-0.02
Spiked Amount	50.000	Range	40 - 130	Recovery	=	104.000%
24) Chloroform-d	4.243	84	197721	4.880	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	97.600%
26) 1,2-Dichloroethane-d4	4.941	65	94115	4.960	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	99.200%
32) Benzene-d6	4.953	84	350448	4.576	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	91.600%
36) 1,2-Dichloropropane-d6	5.986	67	120491	5.060	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	101.200%
41) Toluene-d8	7.240	98	288008	4.174	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	83.400%
43) trans-1,3-Dichloroprop...	7.561	79	27995	3.574	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	71.400%
46) 2-Hexanone-d5	8.024	63	202567	52.928	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	105.860%
56) 1,1,2,2-Tetrachloroeth...	10.149	84	107270	5.527	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	110.600%
66) 1,2-Dichlorobenzene-d4	11.558	152	122246	5.014	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	100.200%
Target Compounds						
13) Acetone	2.130	43	121715	35.048	ug/L	Qvalue 97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV092024\
Data File : VV037433.D
Acq On : 20 Sep 2024 15:25
Operator : SY/MD
Sample : P3990-07
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AM9

Quant Time: Sep 20 23:36:50 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR091024WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Fri Sep 20 23:32:27 2024
Response via : Initial Calibration

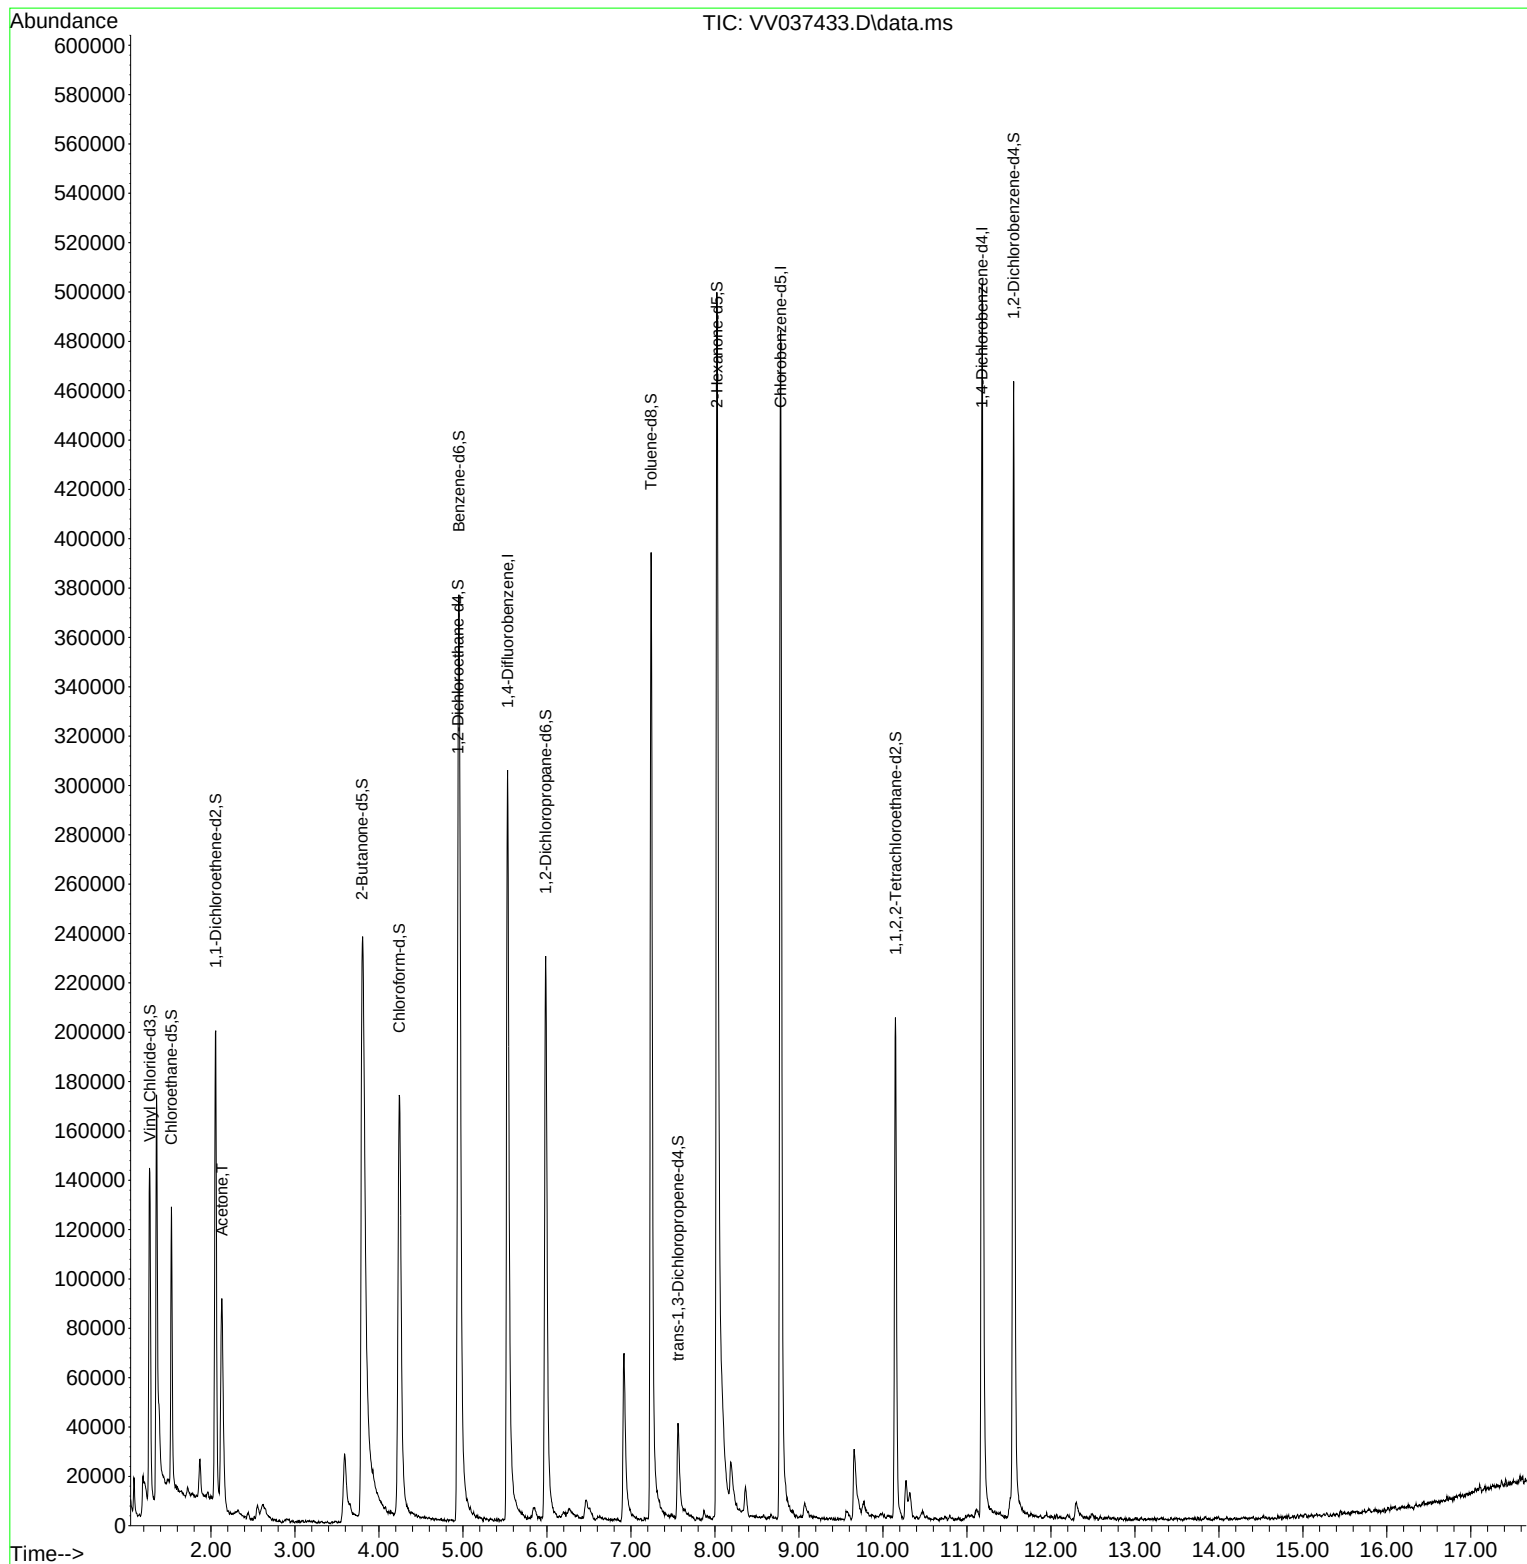

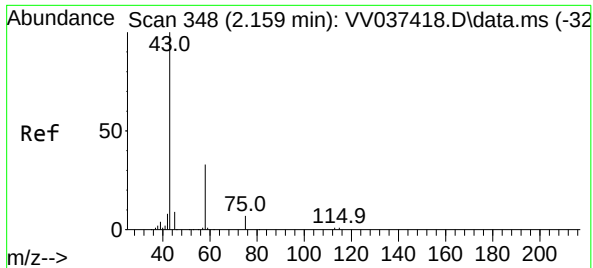

#13
Acetone
Concen: 35.048 ug/L
RT: 2.130 min Scan# 31
Delta R.T. -0.029 min
Lab File: VV037433.D
Acq: 20 Sep 2024 15:25

Instrument :
MSVOA_V
ClientSampleId :
C0AM9

Tgt Ion: 43 Resp: 121715
Ion Ratio Lower Upper
43 100
58 32.6 0.0 69.2

