

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV092024\
 Data File : VV037435.D
 Acq On : 20 Sep 2024 16:13
 Operator : SY/MD
 Sample : P3990-09
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AS1

Quant Time: Sep 20 23:37:23 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR091024WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Sep 20 23:32:27 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.532	114	287529	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.783	117	301481	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.182	152	140068	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.275	65	57006	3.379	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	67.600%
7) Chloroethane-d5	1.529	69	75208	4.276	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	85.600%
11) 1,1-Dichloroethene-d2	2.053	65	32084	3.683	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	73.600%
20) 2-Butanone-d5	3.799	46	262630	52.096	ug/L	-0.02
Spiked Amount	50.000	Range	40 - 130	Recovery	=	104.200%
24) Chloroform-d	4.246	84	196515	4.798	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	96.000%
26) 1,2-Dichloroethane-d4	4.941	65	97424	5.080	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	101.600%
32) Benzene-d6	4.957	84	350784	4.340	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	86.800%
36) 1,2-Dichloropropane-d6	5.986	67	125909	5.009	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	100.200%
41) Toluene-d8	7.243	98	286299	3.931	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	78.600%
43) trans-1,3-Dichloroprop...	7.561	79	28619	3.461	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	69.200%
46) 2-Hexanone-d5	8.024	63	208959	51.724	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	103.440%
56) 1,1,2,2-Tetrachloroeth...	10.149	84	106589	5.203	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	104.000%
66) 1,2-Dichlorobenzene-d4	11.558	152	124322	4.992	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	99.800%
Target Compounds						
13) Acetone	2.127	43	126443	36.022	ug/L	Qvalue 97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV092024\
Data File : VV037435.D
Acq On : 20 Sep 2024 16:13
Operator : SY/MD
Sample : P3990-09
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AS1

Quant Time: Sep 20 23:37:23 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR091024WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Fri Sep 20 23:32:27 2024
Response via : Initial Calibration

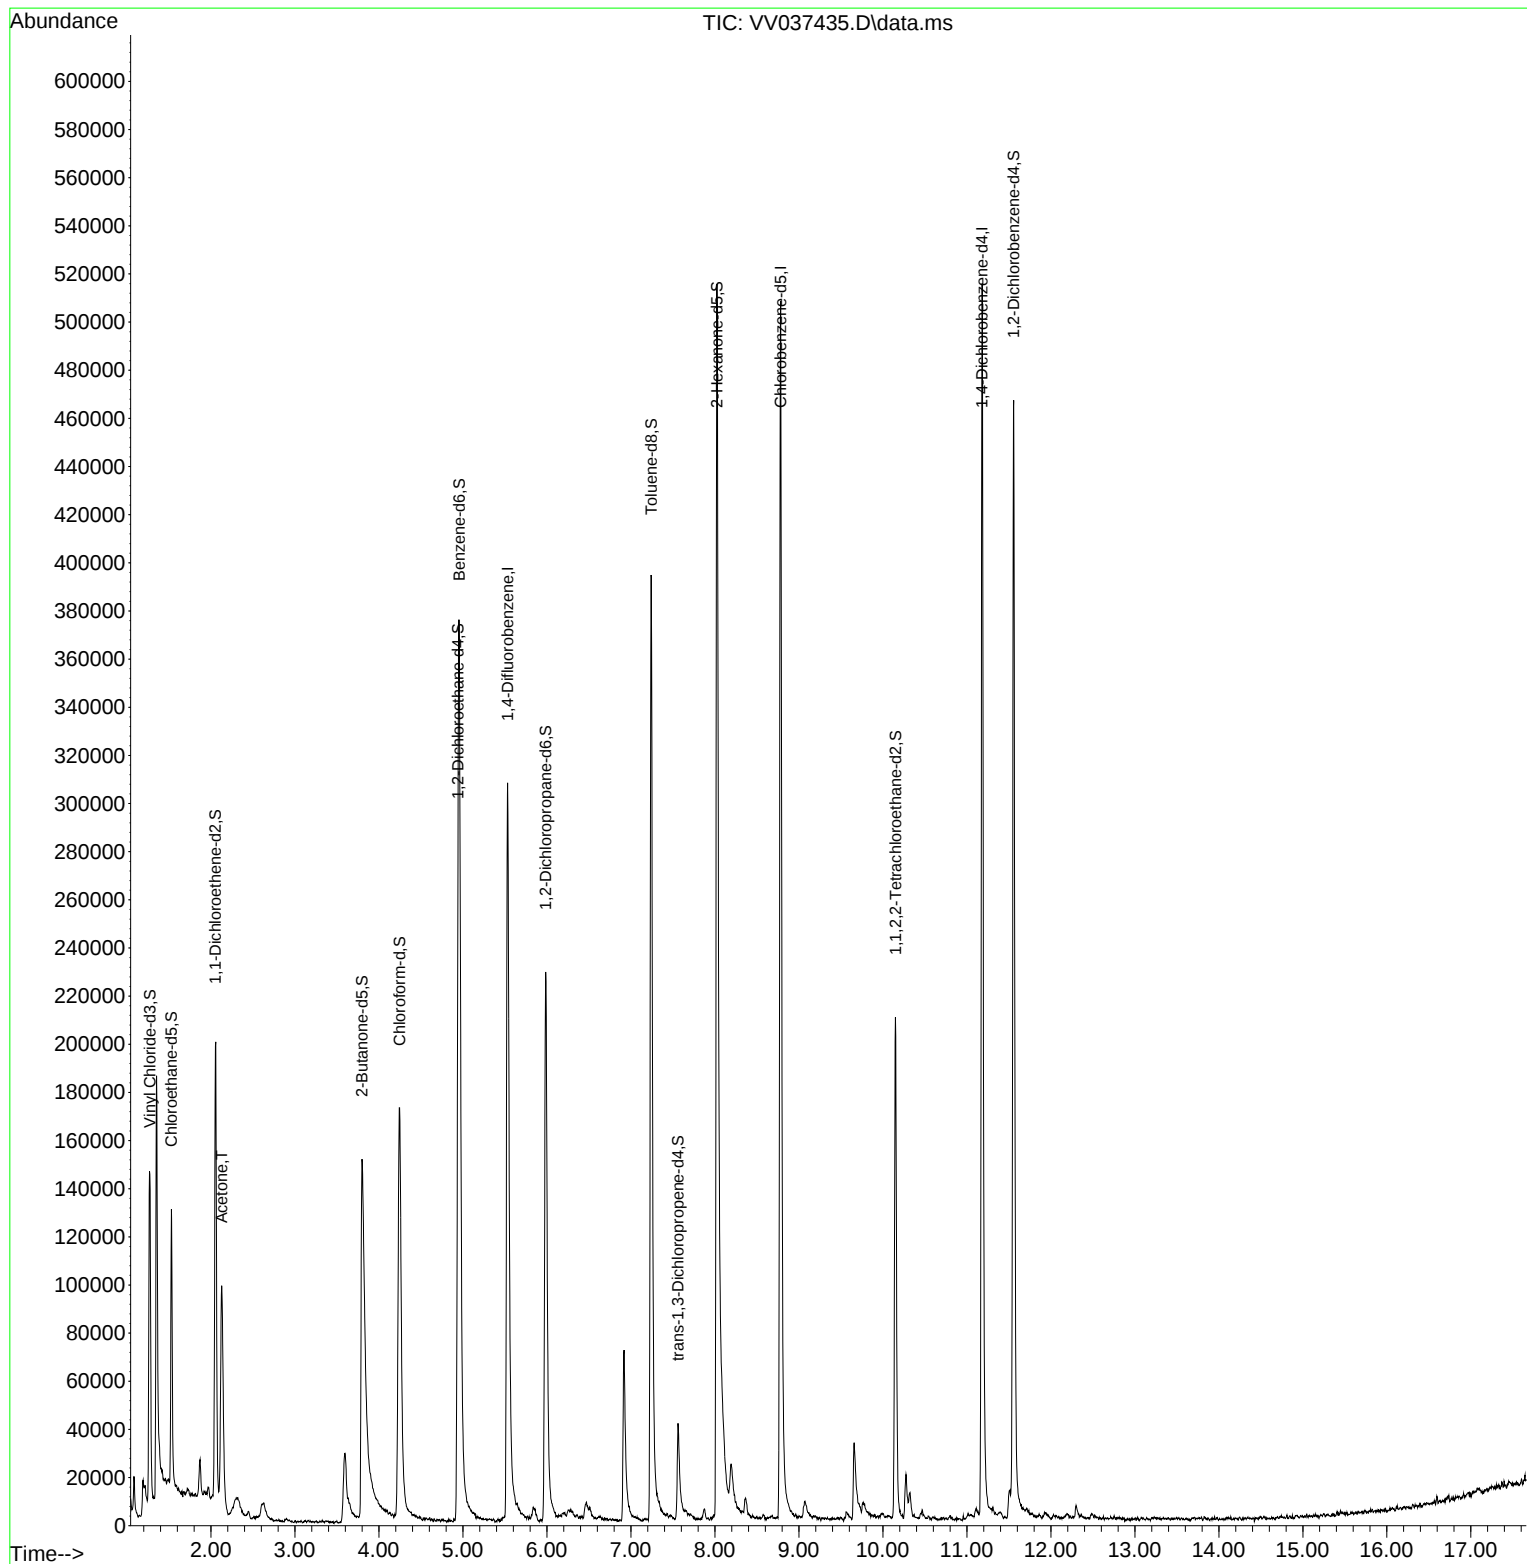

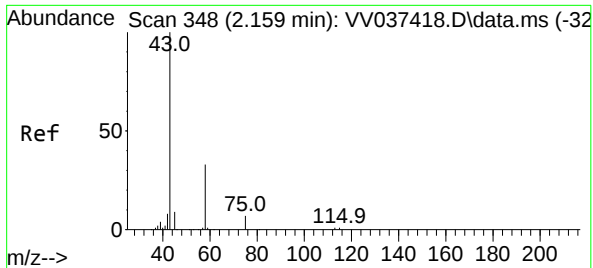

#13
 Acetone
 Concen: 36.022 ug/L
 RT: 2.127 min Scan# 31
 Delta R.T. -0.032 min
 Lab File: VV037435.D
 Acq: 20 Sep 2024 16:13

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AS1

Tgt Ion: 43 Resp: 126443
 Ion Ratio Lower Upper
 43 100
 58 33.0 0.0 69.2

