

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV092024\
 Data File : VV037436.D
 Acq On : 20 Sep 2024 16:38
 Operator : SY/MD
 Sample : P4081-01
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 COAN9

Quant Time: Sep 20 23:37:37 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR091024WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Sep 20 23:32:27 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.532	114	300317	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.783	117	308510	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.182	152	142151	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.275	65	57841	3.283	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	65.600%
7) Chloroethane-d5	1.529	69	75657	4.119	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	82.400%
11) 1,1-Dichloroethene-d2	2.053	65	34414	3.782	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	75.600%
20) 2-Butanone-d5	3.799	46	269746	51.229	ug/L	-0.02
Spiked Amount	50.000	Range	40 - 130	Recovery	=	102.460%
24) Chloroform-d	4.243	84	204557	4.782	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	95.600%
26) 1,2-Dichloroethane-d4	4.941	65	99103	4.948	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	99.000%
32) Benzene-d6	4.957	84	365600	4.420	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	88.400%
36) 1,2-Dichloropropane-d6	5.986	67	125491	4.878	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	97.600%
41) Toluene-d8	7.243	98	295240	3.961	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	79.200%
43) trans-1,3-Dichloroprop...	7.561	79	31447	3.716	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	74.400%
46) 2-Hexanone-d5	8.024	63	214998	52.006	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	104.020%
56) 1,1,2,2-Tetrachloroeth...	10.149	84	109603	5.228	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	104.600%
66) 1,2-Dichlorobenzene-d4	11.558	152	128492	5.084	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	101.600%
Target Compounds						
13) Acetone	2.130	43	31120	8.488	ug/L	Qvalue 100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV092024\
Data File : VV037436.D
Acq On : 20 Sep 2024 16:38
Operator : SY/MD
Sample : P4081-01
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
COAN9

Quant Time: Sep 20 23:37:37 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR091024WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Fri Sep 20 23:32:27 2024
Response via : Initial Calibration

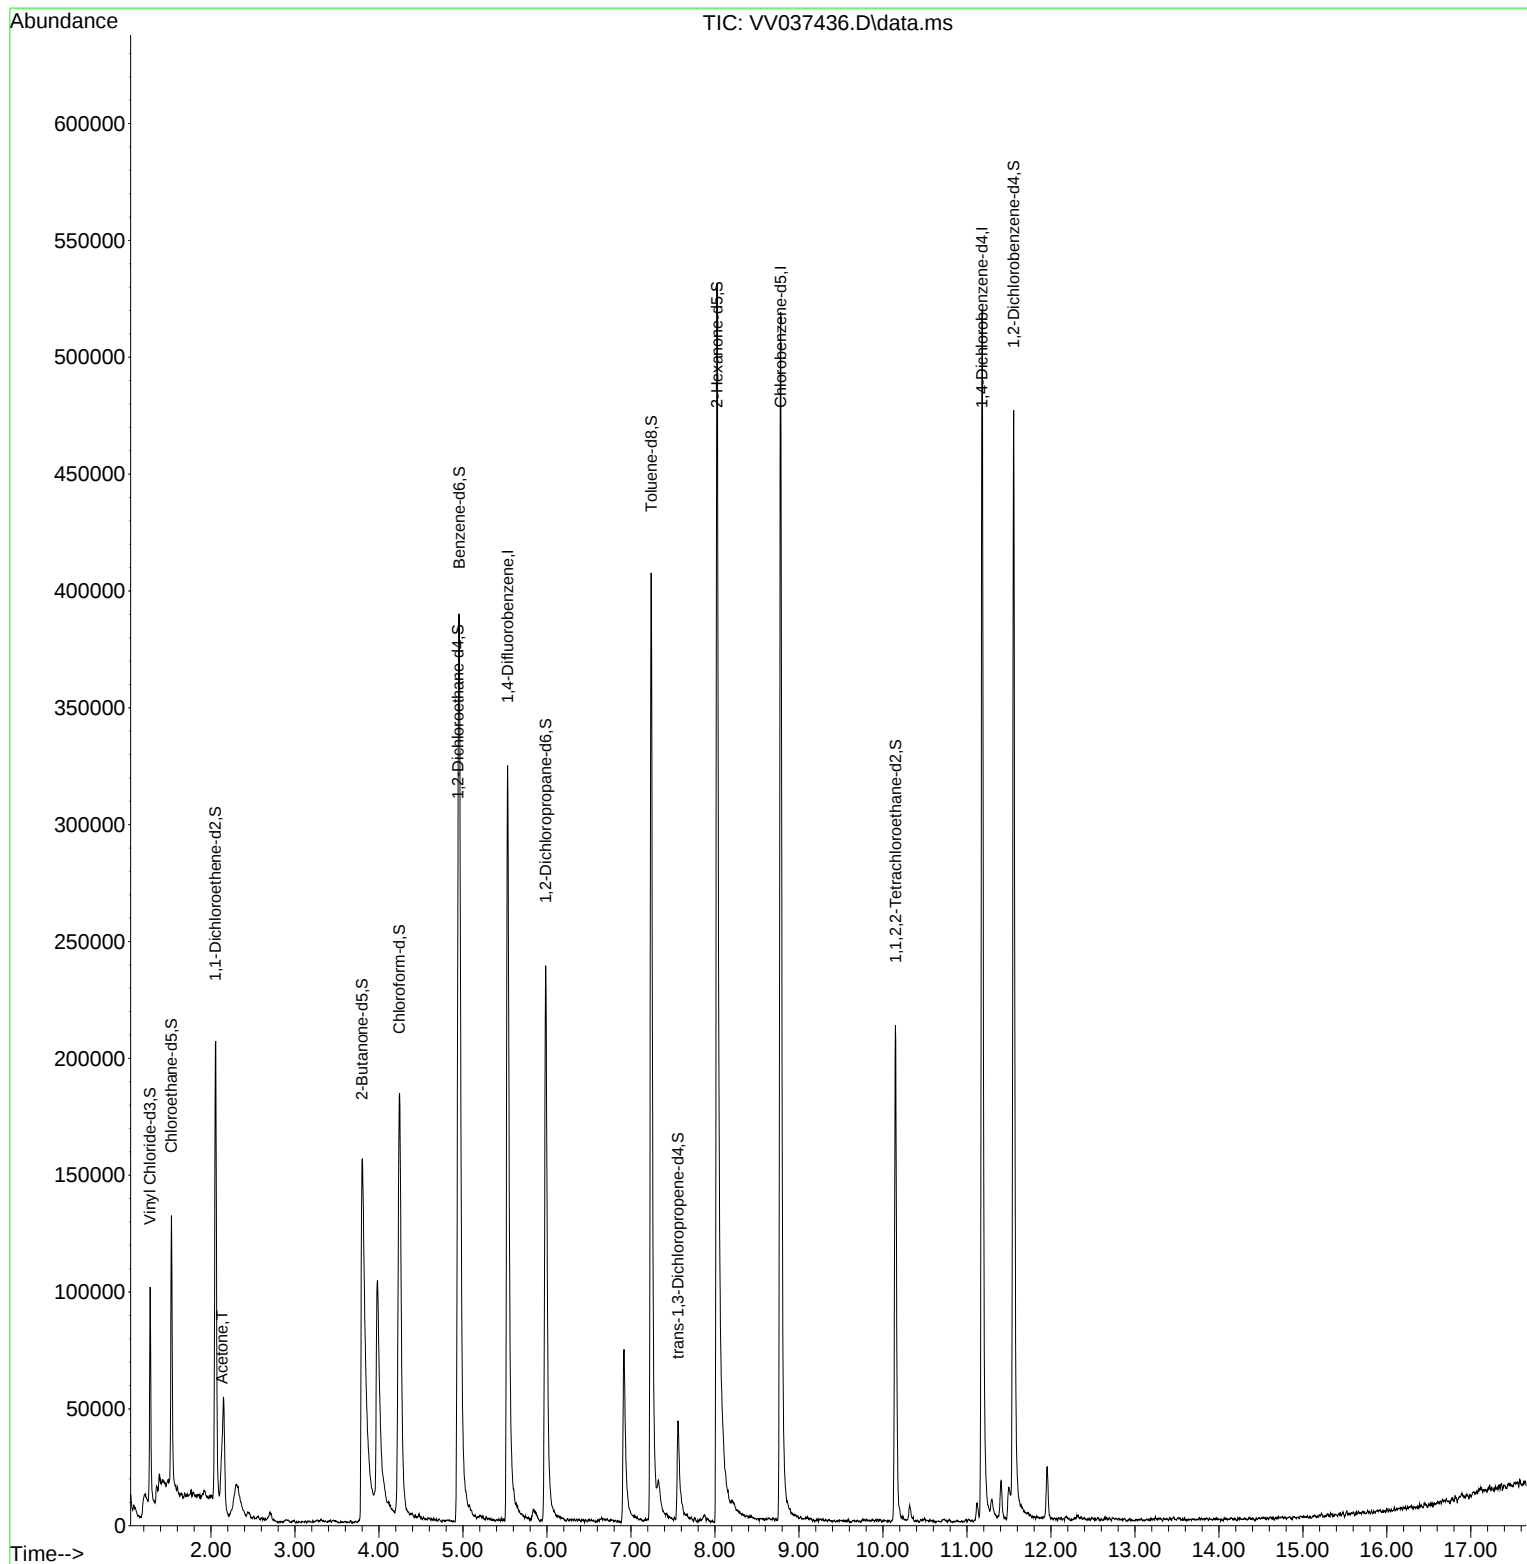

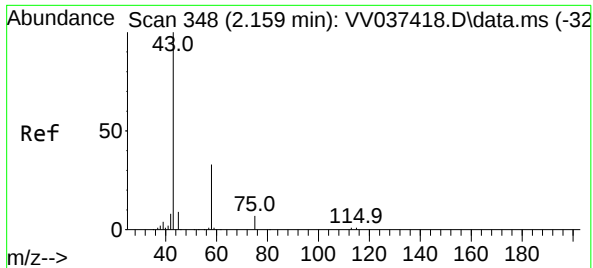

#13
 Acetone
 Concen: 8.488 ug/L
 RT: 2.130 min Scan# 31
 Delta R.T. -0.029 min
 Lab File: VV037436.D
 Acq: 20 Sep 2024 16:38

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AN9

Tgt Ion: 43 Resp: 31120
 Ion Ratio Lower Upper
 43 100
 58 34.4 0.0 69.2

