

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV092024\
 Data File : VV037441.D
 Acq On : 20 Sep 2024 18:39
 Operator : SY/MD
 Sample : P4081-08
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AP9

Quant Time: Sep 20 23:39:23 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR091024WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Sep 20 23:32:27 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.532	114	303329	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.783	117	305268	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.182	152	140077	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.275	65	55505	3.119	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	62.400%
7) Chloroethane-d5	1.529	69	71956	3.878	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	77.600%
11) 1,1-Dichloroethene-d2	2.053	65	32273	3.512	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	70.200%
20) 2-Butanone-d5	3.796	46	265876	49.993	ug/L	-0.03
Spiked Amount	50.000	Range	40 - 130	Recovery	=	99.980%
24) Chloroform-d	4.243	84	193993	4.490	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	89.800%
26) 1,2-Dichloroethane-d4	4.941	65	97507	4.820	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	96.400%
32) Benzene-d6	4.953	84	363077	4.436	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	88.800%
36) 1,2-Dichloropropane-d6	5.986	67	124856	4.905	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	98.200%
41) Toluene-d8	7.240	98	293015	3.973	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	79.400%
43) trans-1,3-Dichloroprop...	7.561	79	28283	3.378	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	67.600%
46) 2-Hexanone-d5	8.024	63	210620	51.488	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	102.980%
56) 1,1,2,2-Tetrachloroeth...	10.149	84	105668	5.094	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	101.800%
66) 1,2-Dichlorobenzene-d4	11.558	152	124706	5.007	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	100.200%
Target Compounds						
13) Acetone	2.127	43	22519	6.081	ug/L	Qvalue 95


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV092024\
Data File : VV037441.D
Acq On : 20 Sep 2024 18:39
Operator : SY/MD
Sample : P4081-08
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AP9

Quant Time: Sep 20 23:39:23 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR091024WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Fri Sep 20 23:32:27 2024
Response via : Initial Calibration

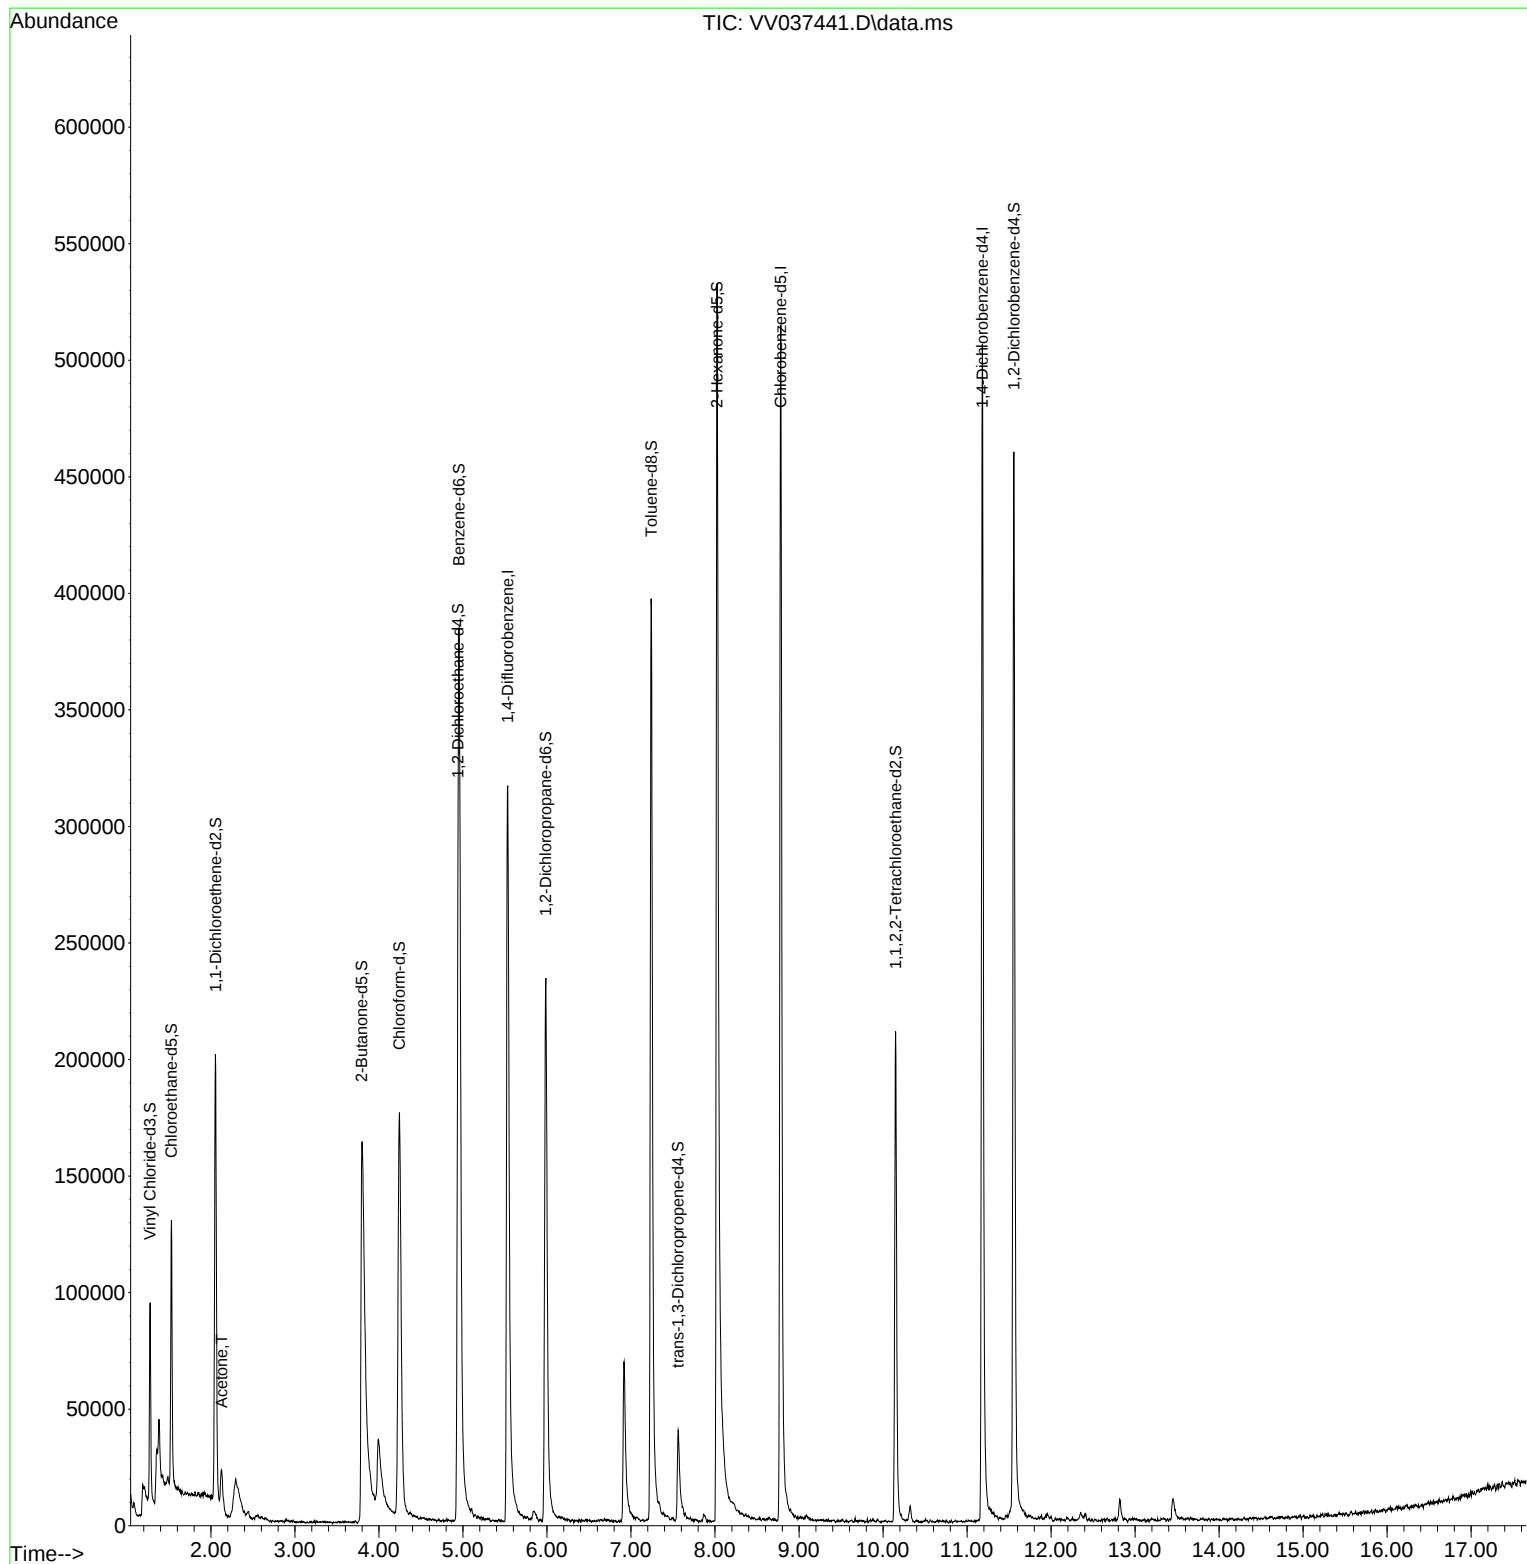

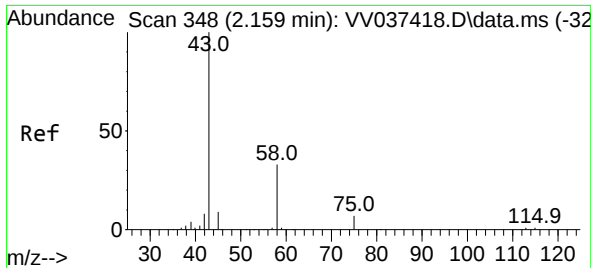

#13

Acetone

Concen: 6.081 ug/L

RT: 2.127 min Scan# 31

Delta R.T. -0.032 min

Lab File: VV037441.D

Acq: 20 Sep 2024 18:39

Instrument :

MSVOA_V

ClientSampleId :

C0AP9

Tgt Ion: 43 Resp: 22519

Ion Ratio Lower Upper

43 100

58 37.7 0.0 69.2

