

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV092024\
 Data File : VV037419.D
 Acq On : 20 Sep 2024 09:39
 Operator : SY/MD
 Sample : VV0920WBL01
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK245

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR091024WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV037419.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.275	63	73	89	rBV	138336	155587	14.16%	1.720%
2	1.529	145	152	161	rVB	120551	138951	12.64%	1.536%
3	2.053	305	315	331	rVB	249719	365392	33.24%	4.040%
4	2.445	426	437	446	rBV4	6760	11961	1.09%	0.132%
5	3.825	854	866	907	rBV2	98427	456996	41.58%	5.053%
6	4.243	980	996	1028	rBV2	168657	449793	40.92%	4.973%
7	4.950	1201	1216	1245	rBV3	392118	1026147	93.36%	11.346%
8	5.529	1385	1396	1430	rBV	329745	743044	67.60%	8.216%
9	5.847	1481	1495	1511	rBV	12251	30695	2.79%	0.339%
10	5.985	1526	1538	1568	rBV	225617	504118	45.86%	5.574%
11	6.915	1817	1827	1858	rBV	81941	183866	16.73%	2.033%
12	7.239	1918	1928	1961	rBV	448695	848860	77.23%	9.386%
13	7.561	2020	2028	2054	rBV	44232	99151	9.02%	1.096%
14	8.027	2164	2173	2210	rBV	463788	1099154	100.00%	12.154%
15	8.779	2394	2407	2438	rBV	530926	953810	86.78%	10.547%
16	10.149	2823	2833	2856	rBV	186515	318776	29.00%	3.525%
17	11.181	3143	3154	3177	rBV	523212	880201	80.08%	9.733%
18	11.557	3259	3271	3299	rBV	451392	764057	69.51%	8.448%
19	13.455	3849	3861	3869	rBV2	7429	13267	1.21%	0.147%




Sum of corrected areas: 9043826

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV092024\
Data File : VV037419.D
Acq On : 20 Sep 2024 09:39
Operator : SY/MD
Sample : VV0920WBL01
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK245

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR091024WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

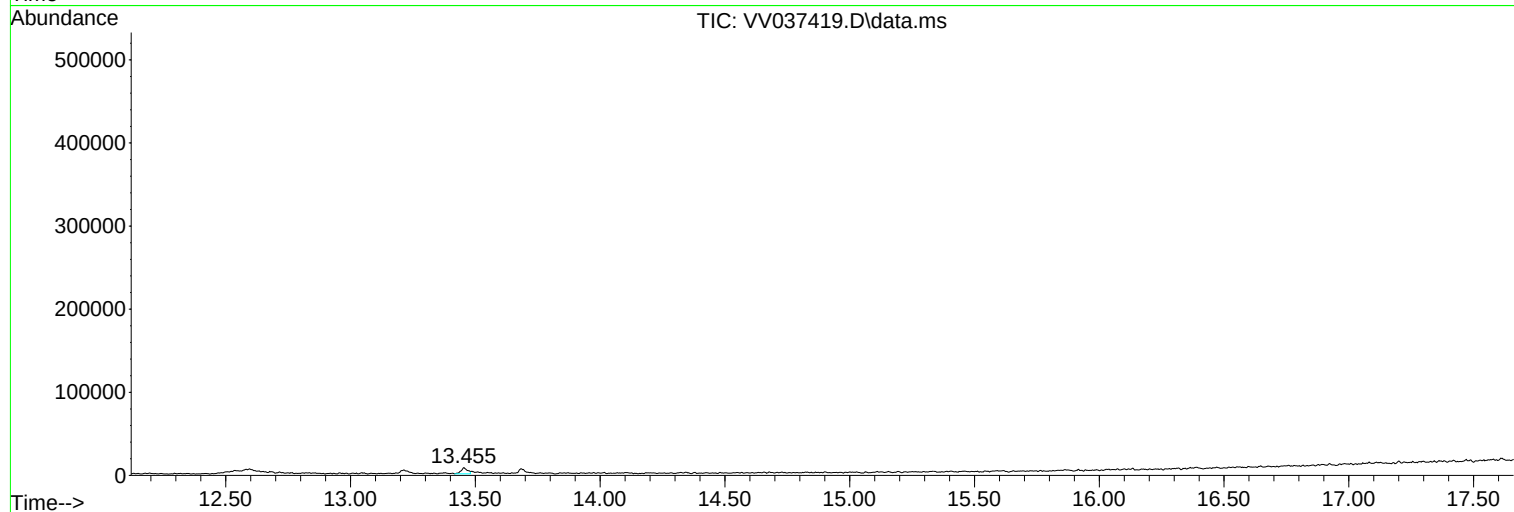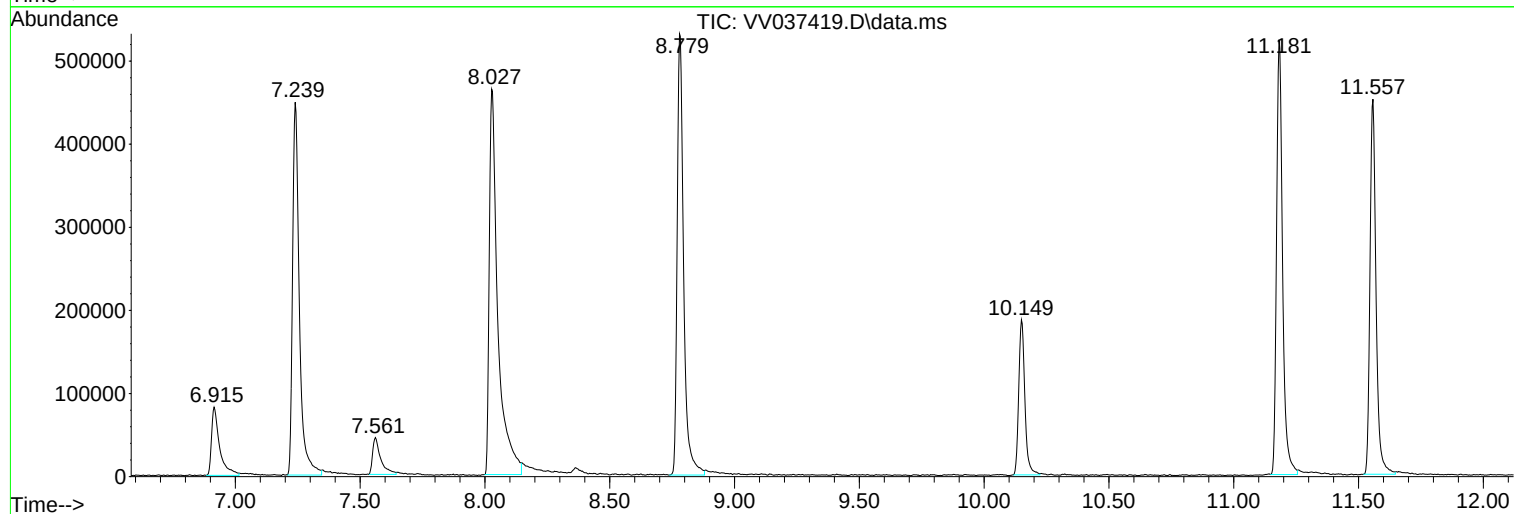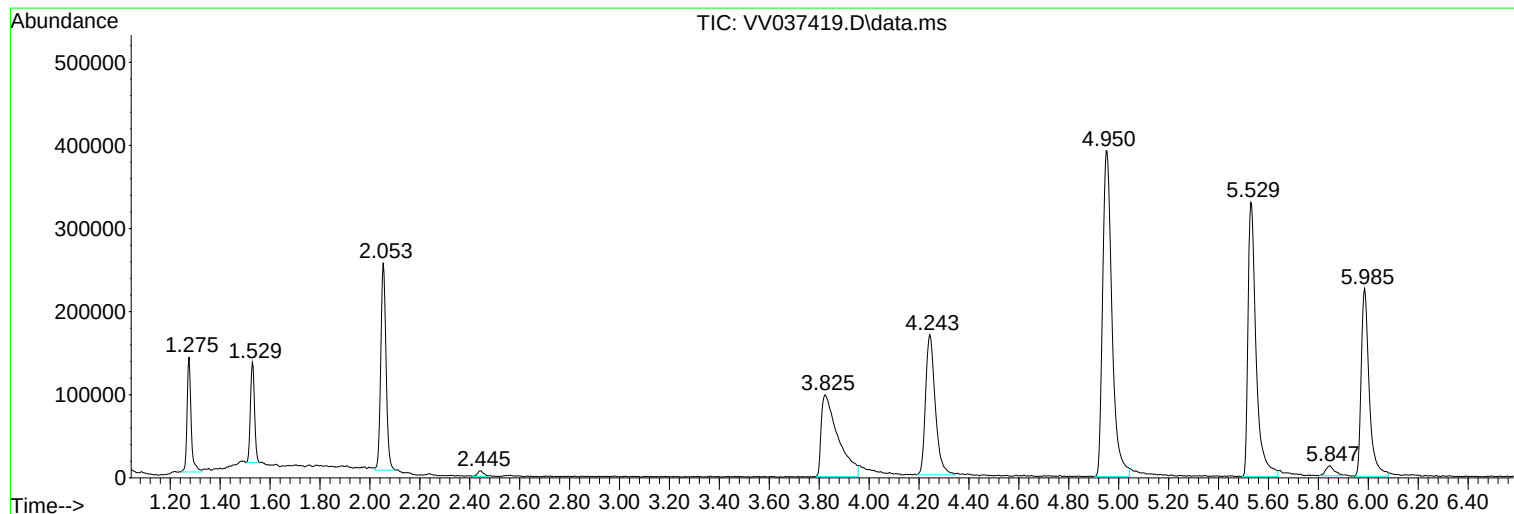

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV092024\
Data File : VV037419.D
Acq On : 20 Sep 2024 09:39
Operator : SY/MD
Sample : VV0920WBL01
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK245

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR091024WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV092024\
Data File : VV037419.D
Acq On : 20 Sep 2024 09:39
Operator : SY/MD
Sample : VV0920WBL01
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK245

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR091024WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
